


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047696.D
 Acq On : 26 Mar 2022 08:42
 Operator : SY/MD
 Sample : BFB055
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB055

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 30 01:20:49 2022

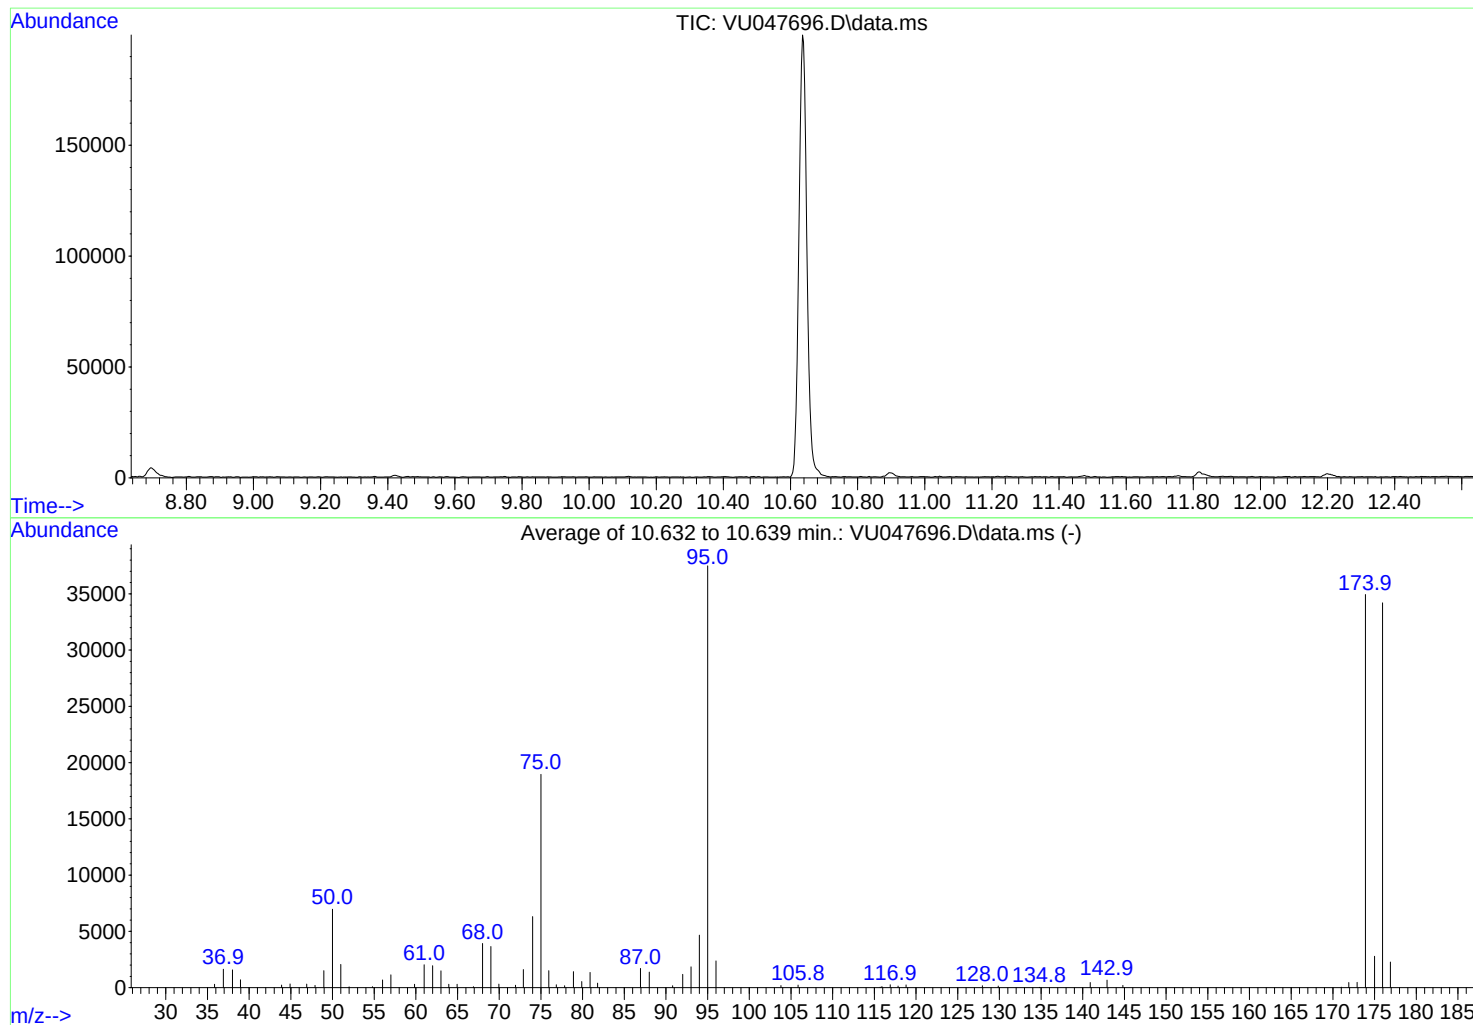

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	6971	PASS
75	95	30	80	50.6	18963	PASS
95	95	100	100	100.0	37488	PASS
96	95	5	9	6.3	2371	PASS
173	174	0.00	2	1.4	477	PASS
174	95	50	120	93.2	34936	PASS
175	174	5	9	8.0	2787	PASS
176	174	95	101	97.9	34195	PASS
177	176	5	9	6.6	2270	PASS

m/z	Abundance
39.80	174.0
43.90	210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
35.80	276.0
36.90	1646.0
38.00	1573.0
38.90	723.0
40.00	131.0
43.90	464.0
44.90	298.0
46.90	371.0
47.90	231.0
49.00	1413.0
50.00	6982.0
51.00	2077.0
54.80	146.0
56.00	567.0
57.00	1142.0
59.90	305.0
61.00	1941.0
62.00	1766.0
63.00	1431.0
63.90	275.0
64.90	257.0
68.00	3841.0
69.00	3472.0
70.00	326.0
71.90	239.0
72.90	1602.0
74.00	5933.0
75.00	18360.0
75.90	1523.0
76.80	253.0
77.80	145.0
78.90	1408.0
79.90	513.0
80.90	1266.0
81.80	419.0
87.00	1572.0
88.00	1413.0
90.80	162.0
92.00	1138.0
93.00	1839.0
94.00	4463.0
95.00	36376.0
96.00	2366.0
103.80	164.0
105.80	206.0
115.70	126.0
116.90	275.0
117.90	118.0
118.80	197.0
128.00	126.0
129.80	128.0
140.90	441.0
142.90	616.0
144.80	177.0
171.90	412.0
172.90	420.0
173.90	32952.0
175.00	2682.0
175.90	32248.0
176.90	2200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
35.90	327.0
36.90	1655.0
38.00	1643.0
38.90	714.0
39.90	152.0
43.90	429.0
44.90	344.0
46.90	311.0
47.90	214.0
49.00	1512.0
50.00	7118.0
51.00	2120.0
52.00	104.0
54.80	119.0
56.00	727.0
57.00	1172.0
59.80	291.0
61.00	2077.0
62.00	2002.0
63.00	1537.0
63.90	306.0
64.90	295.0
66.90	116.0
68.00	4021.0
69.00	3755.0
70.00	312.0
72.00	221.0
72.90	1675.0
74.00	6520.0
75.00	19544.0
76.00	1551.0
76.90	254.0
77.80	165.0
78.90	1483.0
79.90	563.0
80.90	1360.0
81.80	417.0
86.90	1752.0
88.00	1423.0
90.80	174.0
92.00	1230.0
93.00	1915.0
94.00	4822.0
95.00	38552.0
96.00	2432.0
103.80	188.0
105.90	240.0
115.90	144.0
116.90	248.0
117.80	139.0
118.80	248.0
127.90	173.0
129.90	142.0
140.90	494.0
142.90	688.0
144.80	203.0
171.90	441.0
172.90	511.0
173.90	35944.0
175.00	2887.0
175.90	35264.0
176.90	2289.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
35.90	315.0
36.90	1591.0
38.00	1544.0
39.00	656.0
39.90	172.0
43.90	412.0
44.90	333.0
46.90	258.0
47.90	167.0
48.90	1590.0
50.00	6812.0
51.00	1972.0
52.00	122.0
56.00	757.0
57.00	1084.0
59.80	290.0
61.00	2105.0
62.00	2057.0
63.00	1513.0
64.00	307.0
65.00	348.0
66.90	140.0
68.00	3899.0
69.00	3762.0
69.90	287.0
72.00	187.0
72.90	1559.0
74.00	6499.0
75.00	18984.0
76.00	1459.0
76.90	279.0
77.90	185.0
78.90	1397.0
79.90	552.0
80.90	1422.0
81.80	366.0
86.90	1780.0
88.00	1308.0
90.80	159.0
92.00	1188.0
93.00	1808.0
94.00	4719.0
95.00	37536.0
96.00	2314.0
103.80	188.0
105.90	249.0
115.90	143.0
116.90	229.0
117.80	151.0
118.80	281.0
127.90	193.0
129.90	160.0
134.80	103.0
140.90	455.0
142.90	688.0
144.80	207.0
171.00	109.0
171.90	521.0
172.90	500.0
173.90	35912.0
175.00	2793.0
176.00	35072.0
176.90	2321.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055