


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032724\
Data File : VU058220.D
Acq On : 27 Mar 2024 10:57
Operator : MD/SY
Sample : BFB130
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB130

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Mar 28 04:46:03 2024

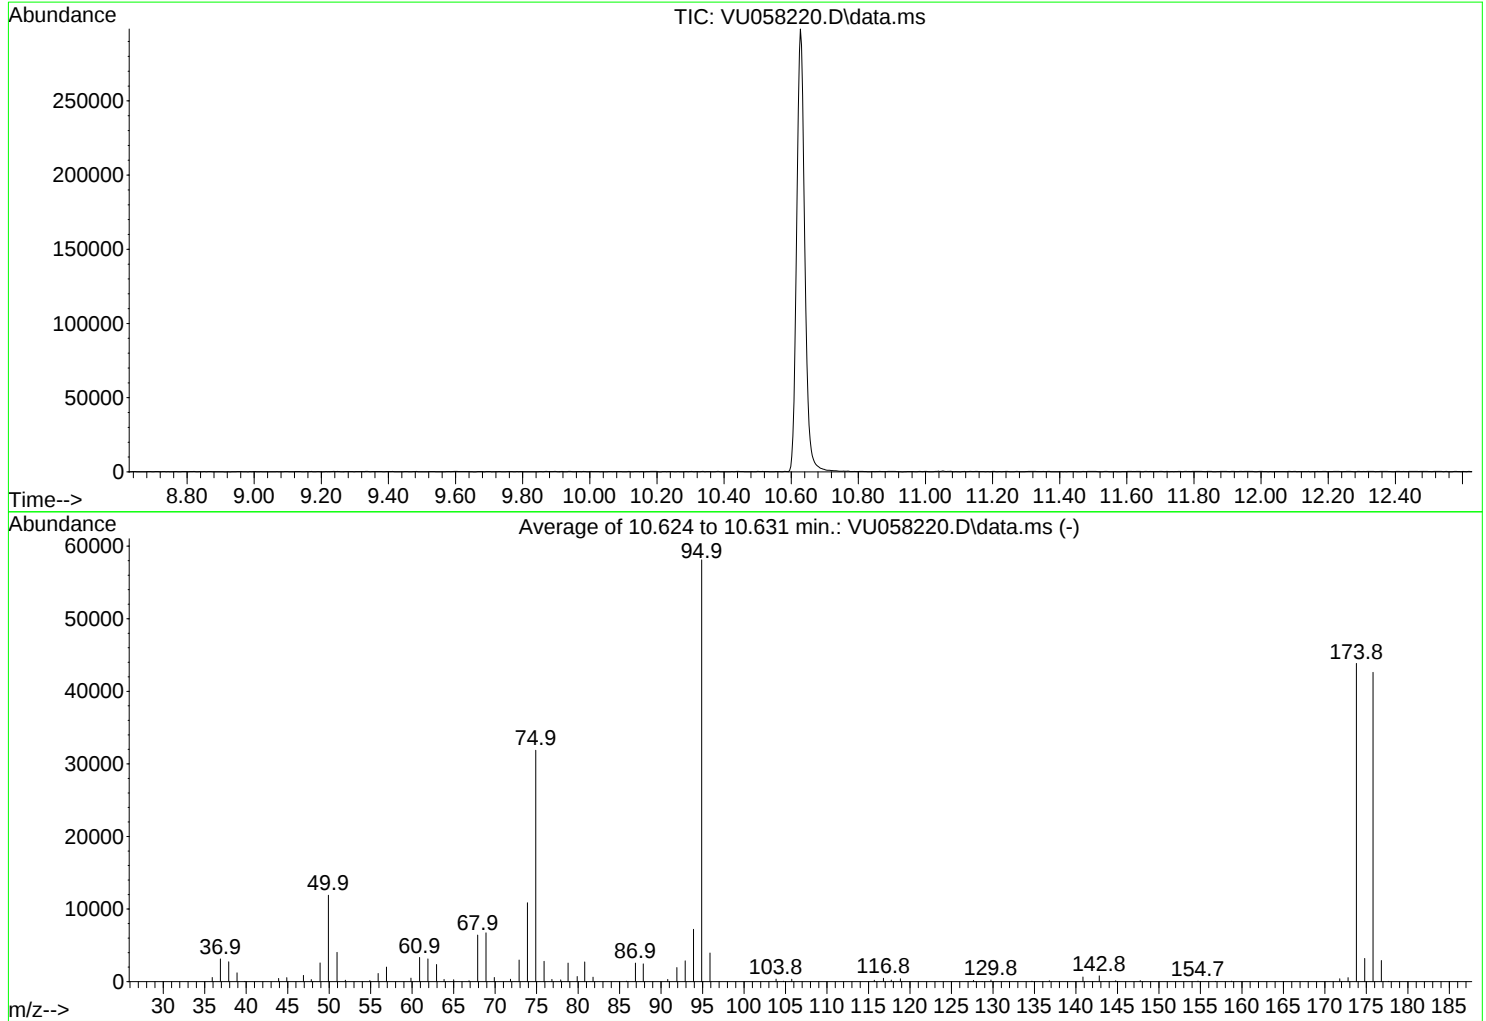

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	11906	PASS
75	95	30	80	54.8	31872	PASS
95	95	100	100	100.0	58115	PASS
96	95	5	9	6.8	3944	PASS
173	174	0.00	2	1.2	547	PASS
174	95	50	120	75.4	43840	PASS
175	174	5	9	7.3	3190	PASS
176	174	95	101	97.2	42611	PASS
177	176	5	9	6.8	2904	PASS

Scan 2891 (10.586 min): VU058220.D\data.ms
BFB130

m/z	Abundance
39.90	114.0
43.90	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB130

m/z	Abundance
35.90	594.0
36.90	3208.0
37.90	2682.0
38.90	1239.0
39.80	149.0
43.90	566.0
44.90	573.0
46.90	831.0
47.90	280.0
48.90	2634.0
49.90	11749.0
51.00	4046.0
52.00	185.0
54.90	161.0
55.90	1135.0
56.90	1903.0
59.80	487.0
60.90	3339.0
61.90	3210.0
63.00	2226.0
63.80	281.0
65.00	258.0
66.90	151.0
67.90	6352.0
68.90	6579.0
69.90	605.0
71.80	355.0
72.90	2829.0
73.90	10710.0
74.90	31584.0
75.90	2685.0
76.80	281.0
77.90	239.0
78.80	2506.0
79.90	638.0
80.80	2640.0
81.80	607.0
85.80	103.0
86.90	2526.0
87.90	2394.0
90.80	290.0
91.90	1864.0
92.90	2718.0
93.90	6997.0
94.90	57048.0
95.90	3911.0
103.90	322.0
105.70	355.0
115.70	188.0
116.80	494.0
117.70	224.0
118.80	395.0
127.60	211.0
129.80	196.0
136.80	130.0
140.90	585.0
142.80	842.0
144.80	130.0
147.70	144.0
154.70	149.0
156.80	105.0
171.80	338.0
172.80	548.0
173.80	42072.0
174.80	3109.0
175.80	40688.0
176.80	2901.0

Instrument :
MSVOA_U
ClientSampleId :
BFB130

m/z	Abundance
35.90	602.0
36.90	3187.0
37.90	2817.0
38.90	1251.0
39.90	163.0
43.90	611.0
44.90	572.0
46.90	915.0
47.90	289.0
48.90	2627.0
49.90	12273.0
51.00	4157.0
52.00	214.0
54.90	163.0
55.90	1154.0
56.90	2086.0
59.80	500.0
60.90	3434.0
61.90	3212.0
62.90	2444.0
63.90	319.0
65.00	286.0
66.80	135.0
67.90	6622.0
68.90	6942.0
69.90	596.0
71.90	321.0
72.90	3091.0
73.90	11211.0
74.90	32912.0
75.90	2868.0
76.90	311.0
77.90	260.0
78.80	2667.0
79.90	732.0
80.80	2801.0
81.80	642.0
85.90	103.0
86.90	2665.0
87.90	2441.0
90.80	313.0
91.90	2008.0
92.90	2966.0
93.90	7407.0
94.90	59784.0
95.90	4093.0
103.90	364.0
104.80	101.0
105.80	351.0
115.70	207.0
116.80	464.0
117.80	221.0
118.80	394.0
127.70	191.0
128.70	100.0
129.70	230.0
134.70	113.0
136.80	138.0
140.80	650.0
142.80	795.0
144.80	126.0
147.80	153.0
154.70	129.0
158.70	103.0
171.80	419.0
172.80	551.0
173.80	45216.0
174.80	3304.0
175.80	43840.0
176.80	2976.0
177.70	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB130

m/z	Abundance
35.90	557.0
36.90	2971.0
37.90	2687.0
38.90	1151.0
39.90	175.0
43.90	610.0
44.90	537.0
46.90	811.0
47.80	268.0
48.90	2467.0
49.90	11696.0
50.90	3890.0
51.90	206.0
54.90	151.0
55.90	1052.0
56.90	2009.0
59.90	500.0
60.90	3214.0
61.90	3008.0
62.90	2410.0
63.90	335.0
65.00	277.0
66.80	130.0
67.90	6280.0
68.90	6654.0
69.90	554.0
71.90	298.0
72.90	3031.0
73.90	10703.0
74.90	31120.0
75.90	2824.0
76.90	354.0
77.90	262.0
78.80	2521.0
79.90	769.0
80.80	2683.0
81.80	607.0
86.90	2463.0
87.80	2496.0
90.80	303.0
91.90	1922.0
92.90	2937.0
93.90	7202.0
94.90	57512.0
95.90	3829.0
103.80	360.0
104.70	102.0
105.80	317.0
115.70	222.0
116.80	441.0
117.80	223.0
118.90	383.0
127.70	165.0
129.70	255.0
134.70	119.0
136.80	110.0
140.80	687.0
142.80	727.0
144.80	115.0
147.80	154.0
158.80	104.0
171.80	465.0
172.80	543.0
173.80	44232.0
174.80	3157.0
175.80	43304.0
176.80	2836.0

Instrument :
MSVOA_U
ClientSampleId :
BFB130