

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032725\
 Data File : VU063314.D
 Acq On : 27 Mar 2025 10:45
 Operator : MD/SY
 Sample : VU0327WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK021

Quant Time: Mar 28 15:07:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM031925.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 28 15:05:02 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	10043	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	11408	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	4198	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.590	65	2382	0.37	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	74.00%		
4) 1,2-Dichloroethane-d4	5.685	65	2767	0.51	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.00%		
7) 1,2-Dichloropropane-d6	6.687	67	2534	0.68	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	136.00%		
8) Toluene-d8	7.888	98	4858	0.49	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.00%		
10) 1,1,2,2-Tetrachloroeth...	10.746	84	1502	0.47	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	94.00%		
Target Compounds						
6) Trichloroethene	6.544	95	179	0.02	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032725\
Data File : VU063314.D
Acq On : 27 Mar 2025 10:45
Operator : MD/SY
Sample : VU0327WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK021


Quant Time: Mar 28 15:07:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM031925.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 28 15:05:02 2025
Response via : Initial Calibration

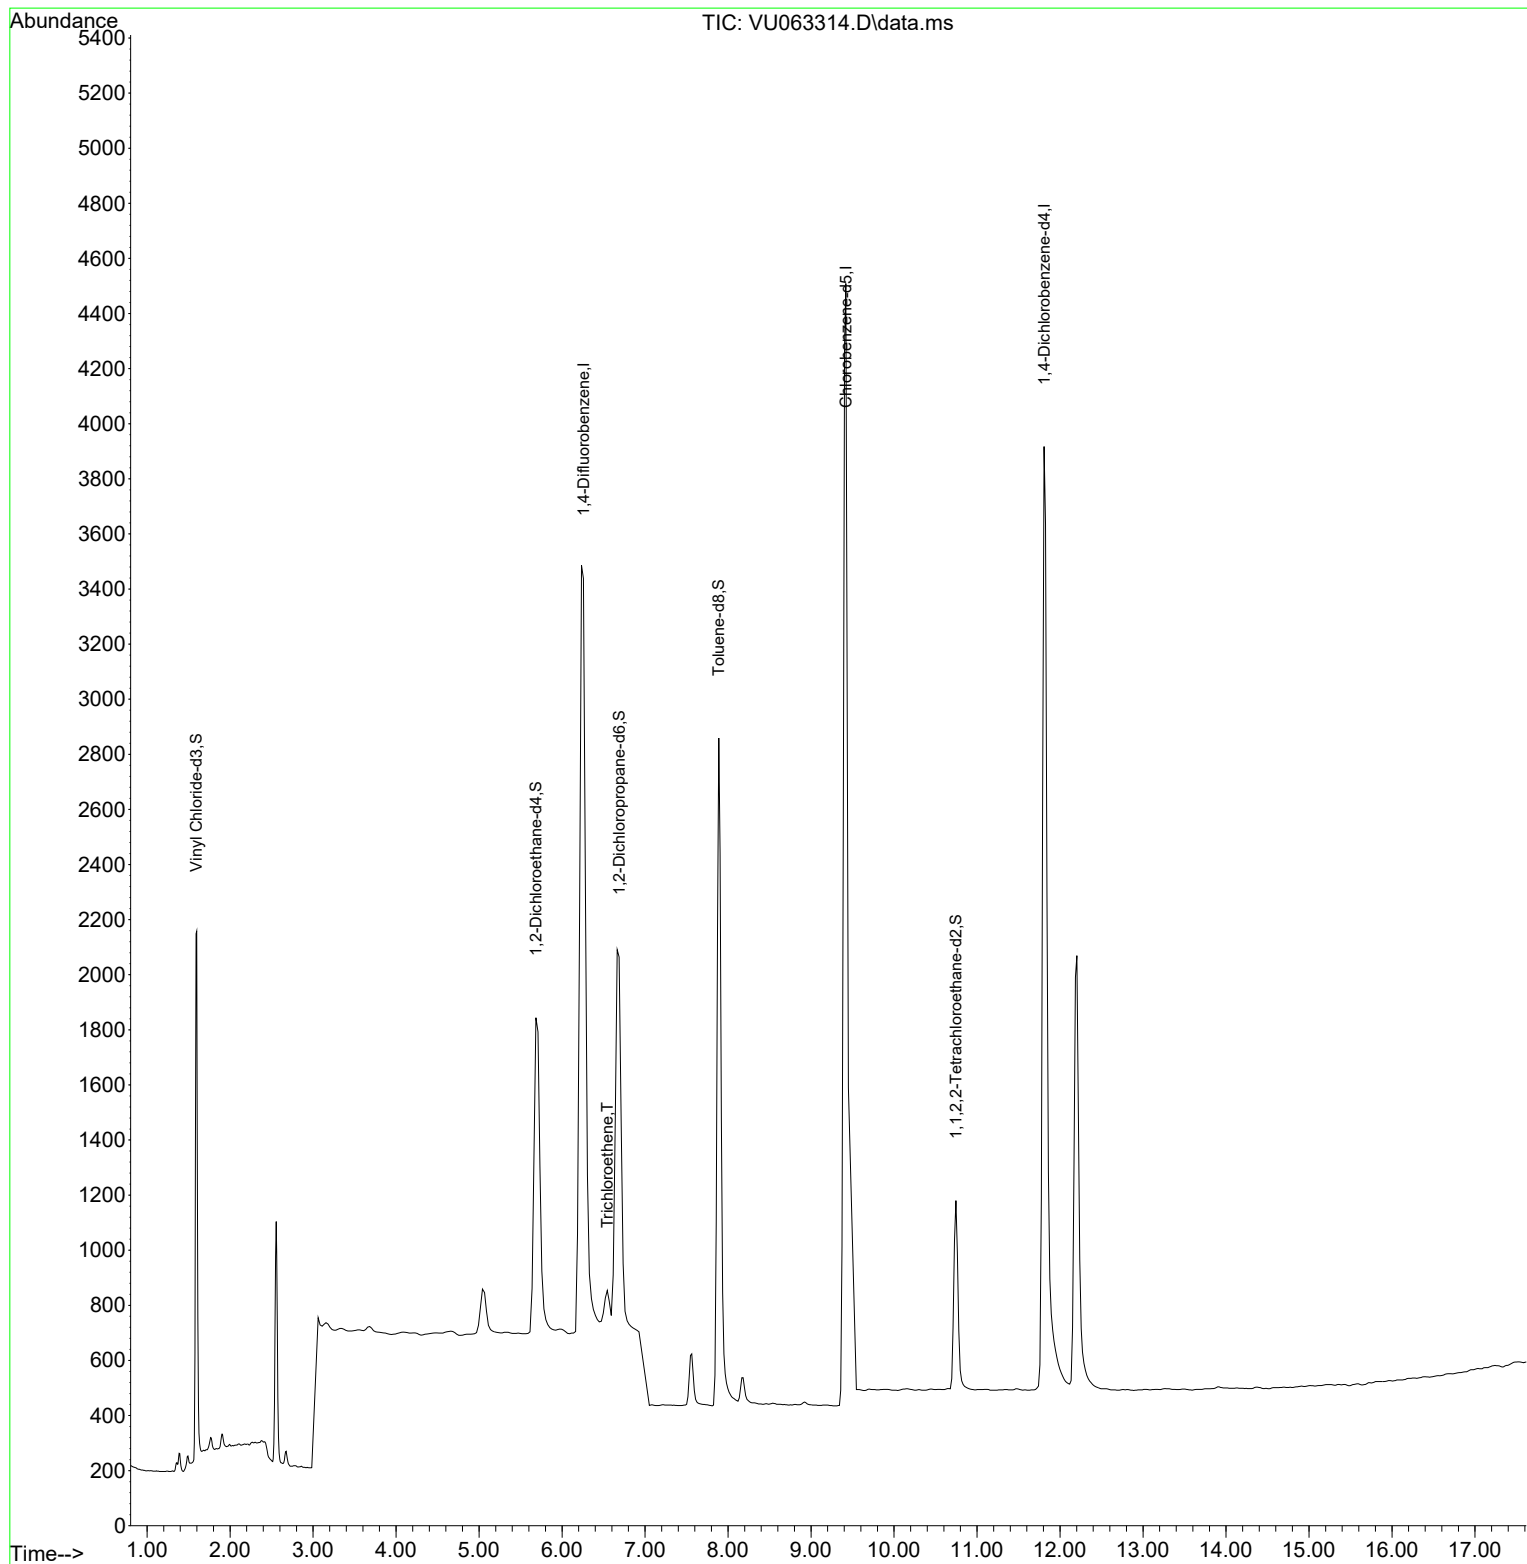

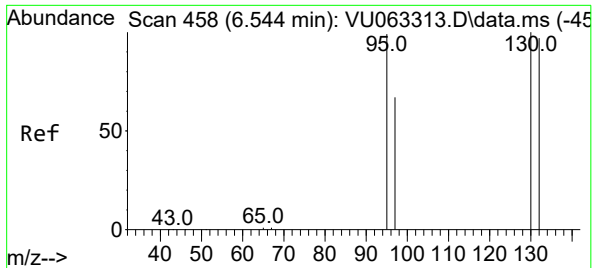

#6
 Trichloroethene
 Concen: 0.02 ug/L
 RT: 6.544 min Scan# 458
 Delta R.T. 0.000 min
 Lab File: VU063314.D
 Acq: 27 Mar 2025 10:45

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK021

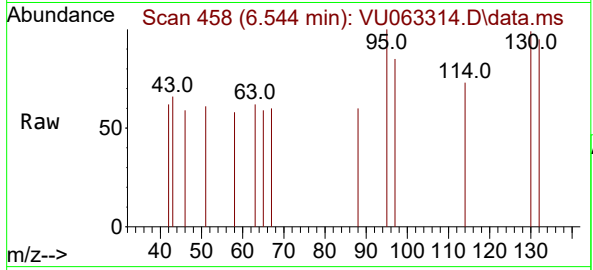

Tgt Ion: 95	Resp: 179
Ion Ratio	Lower Upper
95 100	
97 84.7	46.6 86.6
132 95.3	66.7 123.9
130 98.8	68.6 127.4

