


Data Path : D:\MassHunter\GCMS\1\data\VU032725\
Data File : VU063312.D
Acq On : 27 Mar 2025 09:18
Operator : MD/SY
Sample : BFB022
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB022

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM031925.M
Title : TRACE VOA SOM01.0
Last Update : Mon Mar 31 15:42:06 2025

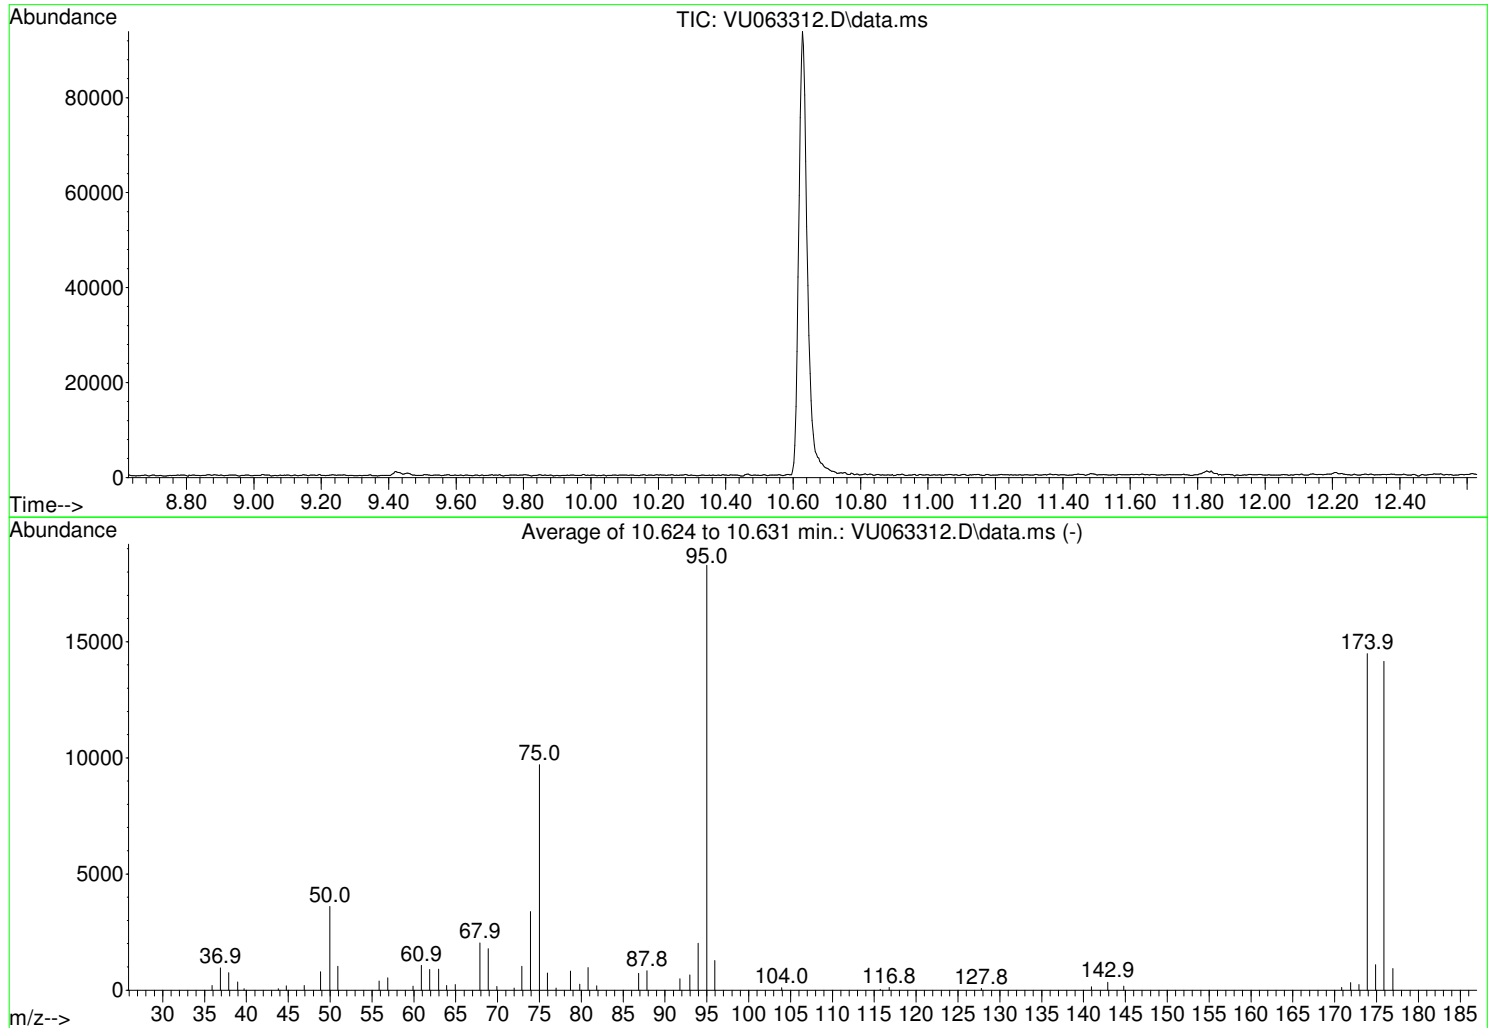

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	3599	PASS
75	95	30	80	53.1	9708	PASS
95	95	100	100	100.0	18291	PASS
96	95	5	9	7.0	1274	PASS
173	174	0.00	2	1.7	246	PASS
174	95	50	120	79.2	14484	PASS
175	174	5	9	7.5	1089	PASS
176	174	95	101	97.7	14152	PASS
177	176	5	9	6.5	924	PASS

m/z	Abundance
39.90	205.0
43.90	396.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	220.0
36.90	914.0
37.90	751.0
38.90	364.0
40.00	244.0
43.80	477.0
44.70	161.0
46.90	204.0
48.90	782.0
49.90	3481.0
50.90	1093.0
55.80	410.0
56.90	491.0
59.90	185.0
60.90	1044.0
61.90	865.0
62.90	867.0
63.90	205.0
64.90	209.0
67.90	2091.0
68.90	1790.0
69.90	186.0
72.00	150.0
72.90	992.0
73.90	3274.0
75.00	9408.0
76.00	705.0
77.00	147.0
78.70	849.0
79.80	251.0
80.80	975.0
81.80	172.0
86.80	655.0
87.90	826.0
91.80	519.0
93.00	668.0
93.90	1940.0
95.00	18048.0
95.90	1217.0
104.00	102.0
116.80	178.0
127.80	108.0
140.90	136.0
142.90	271.0
144.80	130.0
170.80	107.0
171.90	290.0
172.90	219.0
173.90	13614.0
174.90	1052.0
175.90	13266.0
176.90	875.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	204.0
36.90	996.0
37.90	757.0
38.90	360.0
39.90	208.0
43.80	486.0
44.80	193.0
46.90	213.0
48.90	825.0
49.90	3678.0
50.90	1040.0
55.90	421.0
56.90	550.0
59.90	185.0
60.90	1084.0
61.90	948.0
62.90	956.0
63.90	202.0
64.90	250.0
67.90	2118.0
68.90	1831.0
69.90	156.0
72.00	122.0
72.90	1084.0
74.00	3511.0
75.00	10003.0
75.90	753.0
77.00	111.0
78.70	828.0
79.80	249.0
80.80	1008.0
81.90	183.0
86.80	716.0
87.80	881.0
91.80	508.0
92.90	642.0
93.90	2075.0
95.00	18776.0
95.90	1321.0
103.90	117.0
116.80	162.0
127.80	122.0
140.90	143.0
142.90	341.0
144.80	165.0
170.80	137.0
171.90	349.0
172.90	261.0
173.90	14980.0
174.90	1098.0
175.90	14659.0
177.00	981.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	192.0
36.90	970.0
37.90	736.0
39.00	334.0
39.70	174.0
43.80	432.0
44.80	206.0
46.90	174.0
48.80	753.0
50.00	3638.0
50.90	933.0
55.90	365.0
56.90	560.0
59.90	157.0
60.90	1071.0
61.90	848.0
63.00	903.0
63.90	180.0
65.00	263.0
67.90	1900.0
68.90	1712.0
69.90	147.0
72.90	1012.0
74.00	3368.0
75.00	9714.0
75.90	734.0
78.70	771.0
79.80	262.0
80.80	925.0
81.90	216.0
86.90	810.0
87.80	807.0
91.80	436.0
92.90	661.0
94.00	2054.0
95.00	18048.0
96.00	1285.0
103.90	100.0
115.70	110.0
141.00	155.0
142.90	395.0
144.80	235.0
170.90	101.0
171.90	334.0
172.90	258.0
173.90	14859.0
174.90	1117.0
175.90	14532.0
177.00	915.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022