

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032820\
 Data File : VU037434.D
 Acq On : 28 Mar 2020 22:18
 Operator : JC/MD
 Sample : L2002-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 GAWH8

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 2:58:03 PM

Quant Time: Mar 30 00:25:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 30 00:15:54 2020
 Response via : Initial Calibration

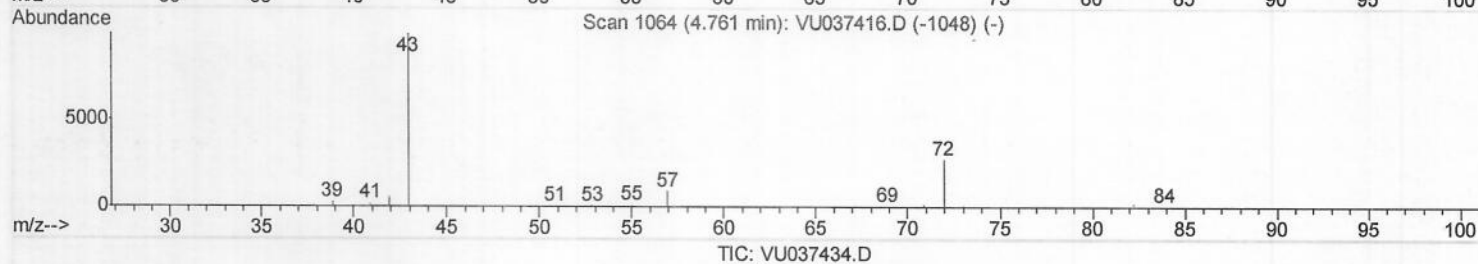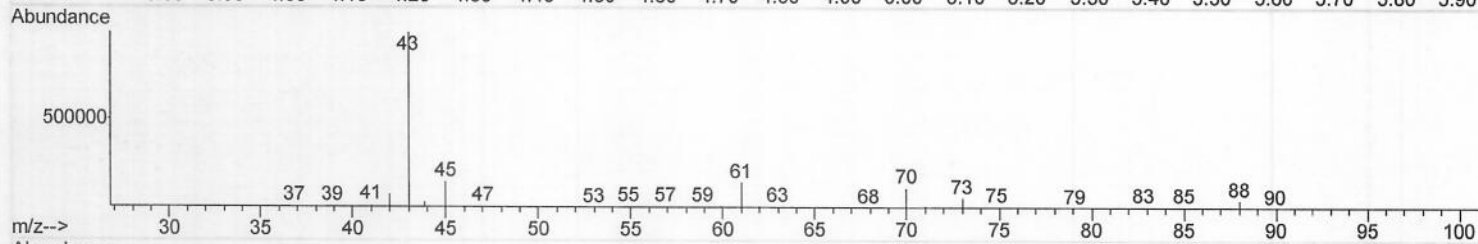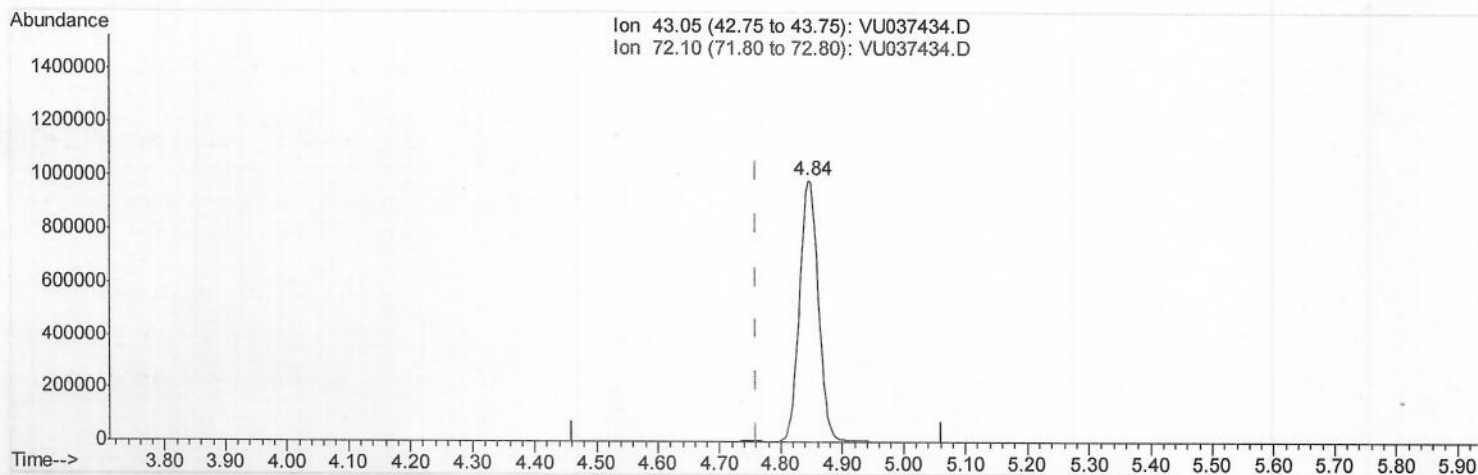

(21) 2-Butanone (T)

4.845min (+0.084) 952.46ug/L

response 2099145

Ion	Exp%	Act%
43.05	100	100
72.10	28.40	0.06#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032820\
 Data File : VU037434.D
 Acq On : 28 Mar 2020 22:18
 Operator : JC/MD
 Sample : L2002-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAWH8

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 2:58:03 PM

Quant Time: Mar 30 00:25:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 30 00:15:54 2020
 Response via : Initial Calibration

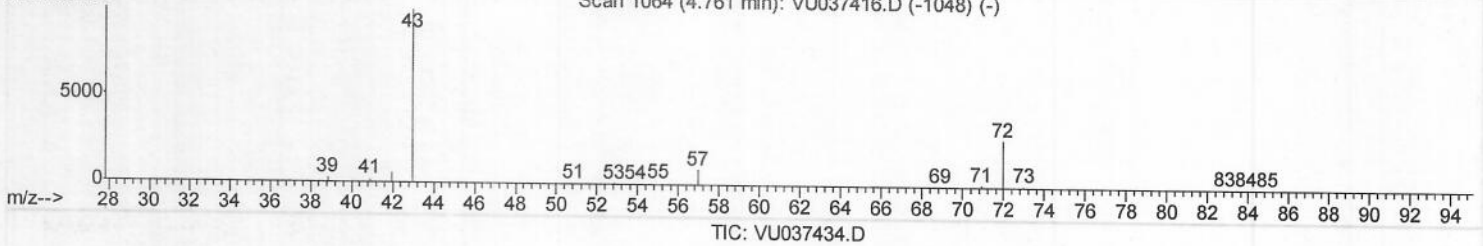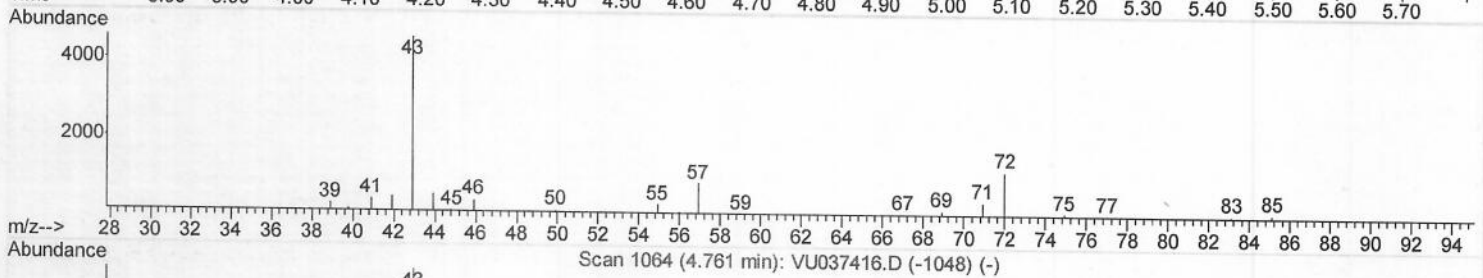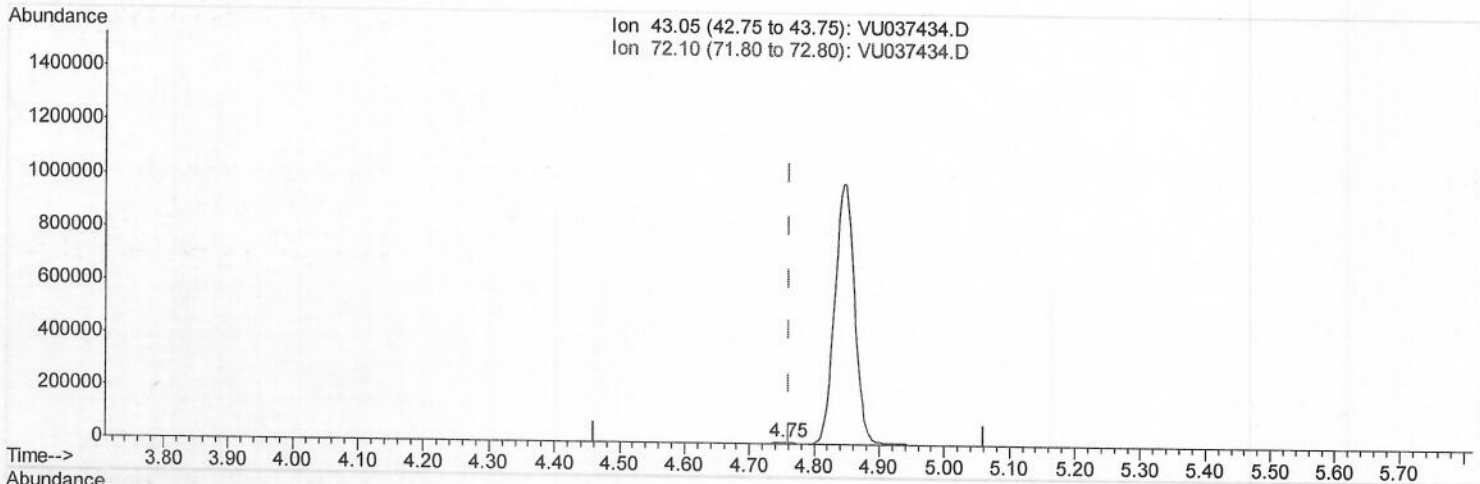

(21) 2-Butanone (T)

4.752min (-0.010) 5.01ug/L m

response 11034

Ion	Exp%	Act%
43.05	100	100
72.10	28.40	12.14#
0.00	0.00	0.00
0.00	0.00	0.00

SY
03/31/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032820\
 Data File : VU037434.D
 Acq On : 28 Mar 2020 22:18
 Operator : JC/MD
 Sample : L2002-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAWH8

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 2:58:03 PM

Quant Time: Mar 30 02:57:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 30 00:15:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	112139	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	104094	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	52893	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	36852	4.45	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.00%	
7) Chloroethane-d5	1.93	69	32186	5.19	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	103.80%	
11) 1,1-Dichloroethene-d2	2.59	63	58572	3.62	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.40%	
20) 2-Butanone-d5	4.67	46	109346	48.46	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	96.92%	
24) Chloroform-d	5.11	84	69074	4.22	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.40%	
26) 1,2-Dichloroethane-d4	5.74	65	43491	4.84	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.80%	
32) Benzene-d6	5.76	84	148535	4.94	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.80%	
36) 1,2-Dichloropropane-d6	6.72	67	48533	4.88	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.60%	
41) Toluene-d8	7.92	98	141311	4.95	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.00%	
43) trans-1,3-Dichloropropene-	8.20	79	21574	4.61	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	92.20%	
46) 2-Hexanone-d5	8.66	63	94307	50.68	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	101.36%	
57) 1,1,2,2-Tetrachloroethane-	10.77	84	39619	4.74	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.80%	
64) 1,2-Dichlorobenzene-d4	12.21	152	51204	4.92	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.40%	

Target Compounds

					Ovalue
13) Acetone	2.66	43	86643	66.833	ug/L 98
15) Methyl Acetate	2.98	43	168536	46.532	ug/L 97
21) 2-Butanone	4.75	43	11034m	5.007	ug/L
25) Chloroform	5.12	83	8825	0.582	ug/L 88
31) Carbon tetrachloride	5.56	117	36393	3.222	ug/L 100
42) Toluene	7.99	91	6830	0.206	ug/L 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SY
 03/31/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032820\
 Data File : VU037434.D
 Acq On : 28 Mar 2020 22:18
 Operator : JC/MD
 Sample : L2002-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAWH8

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 2:58:03 PM

Quant Time: Mar 30 02:57:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 30 00:15:54 2020
 Response via : Initial Calibration

