


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032820\
 Data File : VU037409.D
 Acq On : 28 Mar 2020 09:02
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB08

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Mar 28 11:41:38 2020

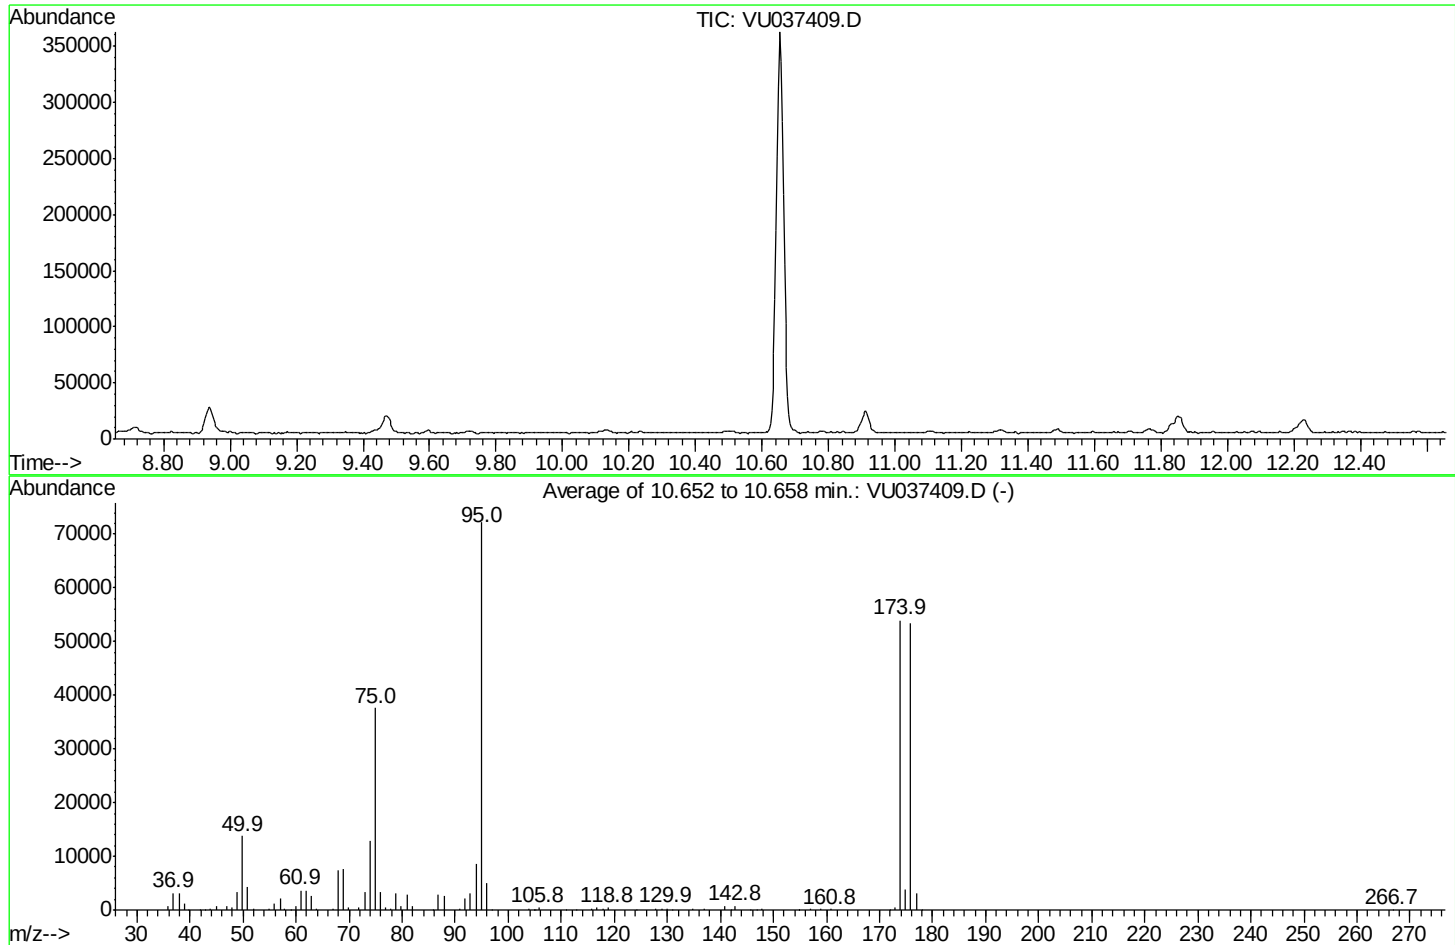

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	13732	PASS
75	95	30	80	52.2	37674	PASS
95	95	100	100	100.0	72224	PASS
96	95	5	9	6.8	4927	PASS
173	174	0.00	2	1.0	554	PASS
174	95	50	120	74.7	53928	PASS
175	174	5	9	7.2	3893	PASS
176	174	95	101	98.9	53333	PASS
177	176	5	9	5.9	3136	PASS

m/z	Abundance
35.90	652.0
36.90	3209.0
38.00	2967.0
38.90	1321.0
39.80	154.0
40.90	321.0
42.90	684.0
43.90	886.0
44.90	664.0
46.90	748.0
47.90	384.0
49.00	3556.0
49.90	13931.0
50.90	4414.0
52.00	247.0
55.00	734.0
55.90	1460.0
57.00	2845.0
57.80	192.0
58.90	111.0
59.90	799.0
60.90	3670.0
61.90	3456.0
62.90	2726.0
63.90	304.0
66.90	363.0
67.90	7711.0
68.90	7907.0
70.00	723.0
70.90	422.0
71.90	426.0
72.90	3426.0
73.90	12606.0
75.00	38872.0
75.90	3470.0
76.80	502.0
77.90	280.0
78.80	3231.0
79.80	739.0
80.80	3070.0
81.80	805.0
83.00	259.0
84.90	269.0
85.90	123.0
86.90	2817.0
87.90	2546.0
90.90	404.0
91.90	2075.0
92.90	3111.0
93.90	8727.0
95.00	74216.0
96.00	5099.0
97.10	277.0
103.90	389.0
105.10	110.0
105.80	478.0
111.00	213.0
112.90	144.0
115.80	246.0
116.70	445.0
117.80	274.0
118.80	429.0
124.00	117.0
127.60	228.0
129.00	124.0
129.90	238.0
130.80	177.0
134.70	222.0
136.90	182.0
140.90	741.0
142.80	762.0
146.80	106.0
147.80	185.0
154.70	195.0
156.90	123.0
158.90	155.0
160.80	184.0
171.90	165.0
172.90	519.0
173.90	53672.0
174.90	4023.0
175.90	52016.0
176.90	3119.0
178.00	106.0
266.70	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
35.90	644.0
36.90	3219.0
37.90	3131.0
38.90	1493.0
39.80	148.0
40.90	305.0
41.90	114.0
42.90	764.0
43.90	813.0
44.90	653.0
46.90	821.0
47.90	377.0
49.00	3557.0
49.90	14130.0
50.90	4429.0
52.00	255.0
55.00	713.0
55.90	1507.0
57.00	2978.0
57.90	160.0
59.90	824.0
60.90	3663.0
61.90	3630.0
62.90	2838.0
63.90	265.0
66.90	352.0
67.90	7716.0
68.90	8165.0
69.90	770.0
70.90	351.0
71.90	527.0
73.00	3406.0
73.90	13194.0
75.00	38944.0
75.90	3382.0
76.90	446.0
77.90	265.0
78.80	3276.0
79.80	719.0
80.90	2898.0
81.80	848.0
83.00	208.0
85.00	239.0
86.90	2997.0
87.90	2801.0
90.90	366.0
91.90	2143.0
92.90	3128.0
93.90	8831.0
95.00	74640.0
96.00	5095.0
97.00	270.0
103.90	377.0
104.70	118.0
105.10	123.0
105.80	468.0
111.00	173.0
112.90	146.0
115.70	261.0
116.70	441.0
117.80	289.0
118.80	448.0
124.10	116.0
127.60	248.0
128.90	136.0
129.90	331.0
130.90	119.0
134.80	213.0
136.90	174.0
140.90	691.0
142.70	748.0
147.80	233.0
154.90	186.0
156.80	141.0
158.90	187.0
160.80	197.0
171.90	146.0
172.90	577.0
173.90	55640.0
174.90	4002.0
175.90	55136.0
176.90	3197.0
177.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
36.00	614.0
36.90	2949.0
37.90	2964.0
38.90	1409.0
39.80	161.0
41.00	336.0
41.90	116.0
42.90	717.0
43.90	720.0
44.90	547.0
46.90	832.0
47.90	367.0
48.90	3031.0
49.90	13135.0
50.90	4023.0
51.90	225.0
55.00	665.0
56.00	1407.0
57.00	2644.0
57.90	150.0
59.90	761.0
60.90	3410.0
61.90	3531.0
62.90	2686.0
63.90	216.0
67.00	310.0
68.00	6946.0
68.90	7646.0
69.90	714.0
71.00	351.0
71.90	527.0
72.90	2933.0
73.90	12525.0
74.90	35208.0
75.90	3052.0
77.00	441.0
77.80	251.0
78.80	2946.0
79.80	697.0
80.90	2616.0
81.90	819.0
82.90	169.0
85.00	221.0
86.80	2693.0
87.90	2788.0
90.90	313.0
91.90	2030.0
92.90	2896.0
94.00	7979.0
95.00	67816.0
96.00	4589.0
96.90	228.0
98.00	100.0
103.90	320.0
104.80	168.0
105.80	390.0
110.90	138.0
112.90	112.0
115.70	243.0
116.80	423.0
117.80	271.0
118.80	447.0
127.70	255.0
128.80	145.0
129.90	324.0
134.80	178.0
136.80	169.0
140.90	616.0
141.90	122.0
142.80	707.0
145.70	112.0
147.80	241.0
154.90	186.0
156.80	136.0
158.90	162.0
160.80	147.0
172.90	567.0
173.90	52472.0
174.90	3656.0
175.90	52848.0
176.90	3092.0
267.00	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
38.90	181.0
39.90	127.0
40.90	385.0
43.00	616.0
43.80	467.0
54.90	386.0
55.80	203.0
57.00	676.0
67.00	101.0
68.00	122.0
68.90	253.0
69.90	145.0
71.00	541.0
81.90	147.0
82.90	220.0
84.10	121.0
84.90	346.0
96.80	137.0
97.90	125.0
110.80	121.0
113.00	103.0
267.00	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08