

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047722.D
 Acq On : 28 Mar 2022 12:55
 Operator : SY/MD
 Sample : VU0328WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	104	rVB	123519	148455	12.81%	1.533%
2	1.919	171	180	199	rBV	107428	147450	12.72%	1.522%
3	2.572	370	383	412	rBV	227172	388161	33.49%	4.007%
4	2.761	439	442	446	rVB	328	202	0.02%	0.002%
5	2.797	446	453	454	rBV3	950	935	0.08%	0.010%
6	2.851	462	470	475	rBV2	418	770	0.07%	0.008%
7	2.912	486	489	492	rBV	214	181	0.02%	0.002%
8	3.051	525	532	539	rVB4	813	1111	0.10%	0.011%
9	3.089	539	544	549	rBV3	263	255	0.02%	0.003%
10	3.356	623	627	630	rVV	288	192	0.02%	0.002%
11	3.424	643	648	651	rBV3	247	207	0.02%	0.002%
12	3.446	652	655	658	rVV2	248	196	0.02%	0.002%
13	3.488	666	668	675	rVB3	310	272	0.02%	0.003%
14	3.559	687	690	694	rBV2	284	240	0.02%	0.002%
15	3.623	707	710	714	rBV2	238	203	0.02%	0.002%
16	3.687	727	730	735	rBV2	279	289	0.02%	0.003%
17	3.954	808	813	816	rBV2	235	291	0.03%	0.003%
18	4.182	879	884	891	rBV3	202	213	0.02%	0.002%
19	4.346	931	935	942	rBV3	278	307	0.03%	0.003%
20	4.584	1003	1009	1012	rBV4	393	394	0.03%	0.004%
21	4.642	1012	1027	1066	rBV	120801	393580	33.96%	4.063%
22	4.871	1095	1098	1104	rVB3	636	558	0.05%	0.006%
23	4.986	1129	1134	1137	rBV3	208	229	0.02%	0.002%
24	5.067	1143	1159	1182	rBV	213888	468690	40.44%	4.838%
25	5.208	1200	1203	1206	rBV2	302	237	0.02%	0.002%
26	5.253	1213	1217	1222	rBV2	280	245	0.02%	0.003%
27	5.289	1222	1228	1229	rBV2	449	411	0.04%	0.004%
28	5.430	1270	1272	1277	rVB	235	182	0.02%	0.002%
29	5.729	1343	1365	1392	rBV2	427467	1159115	100.00%	11.966%
30	6.115	1482	1485	1488	rVB	314	197	0.02%	0.002%
31	6.173	1500	1503	1507	rBV2	276	221	0.02%	0.002%
32	6.250	1512	1527	1549	rBV	352096	671585	57.94%	6.933%
33	6.401	1572	1574	1577	rVB2	400	181	0.02%	0.002%
34	6.433	1579	1584	1585	rBV	316	220	0.02%	0.002%
35	6.472	1593	1596	1599	rBV3	353	313	0.03%	0.003%
36	6.533	1608	1615	1618	rBV4	1307	1692	0.15%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047722.D
 Acq On : 28 Mar 2022 12:55
 Operator : SY/MD
 Sample : VU0328WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1693	rBV	267353	529773	45.70%	5.469%
38	6.854	1711	1715	1723	rVB2	218	281	0.02%	0.003%
39	6.967	1747	1750	1758	rVB2	209	235	0.02%	0.002%
40	7.009	1758	1763	1769	rBV2	243	316	0.03%	0.003%
41	7.054	1774	1777	1783	rVB2	504	481	0.04%	0.005%
42	7.134	1800	1802	1809	rVB2	284	218	0.02%	0.002%
43	7.186	1809	1818	1827	rBV3	2185	3587	0.31%	0.037%
44	7.308	1851	1856	1859	rBV2	366	238	0.02%	0.002%
45	7.478	1901	1909	1912	rBV	474	645	0.06%	0.007%
46	7.565	1924	1936	1956	rBV	146660	260069	22.44%	2.685%
47	7.690	1968	1975	1986	rVV3	1655	2891	0.25%	0.030%
48	7.732	1986	1988	1992	rVB2	275	206	0.02%	0.002%
49	7.800	2003	2009	2014	rVV4	1305	1717	0.15%	0.018%
50	7.819	2014	2015	2018	rVB	641	255	0.02%	0.003%
51	7.899	2026	2040	2057	rBV	523120	911606	78.65%	9.411%
52	8.096	2099	2101	2105	rBV2	354	304	0.03%	0.003%
53	8.179	2115	2127	2152	rBV2	104503	185556	16.01%	1.916%
54	8.552	2238	2243	2244	rBV2	516	354	0.03%	0.004%
55	8.636	2256	2269	2301	rBV	453853	863979	74.54%	8.919%
56	8.954	2361	2368	2370	rBV3	162	213	0.02%	0.002%
57	9.018	2383	2388	2389	rBV	219	215	0.02%	0.002%
58	9.169	2433	2435	2439	rVV2	307	190	0.02%	0.002%
59	9.247	2453	2459	2462	rBV2	218	326	0.03%	0.003%
60	9.304	2474	2477	2483	rVB3	270	288	0.02%	0.003%
61	9.337	2483	2487	2488	rBV	396	249	0.02%	0.003%
62	9.417	2499	2512	2545	rBV	532564	896303	77.33%	9.253%
63	9.571	2554	2560	2568	rVB4	665	1044	0.09%	0.011%
64	9.700	2590	2600	2607	rVV4	1196	1976	0.17%	0.020%
65	9.880	2653	2656	2659	rBV2	214	190	0.02%	0.002%
66	10.108	2720	2727	2729	rBV2	973	1013	0.09%	0.010%
67	10.169	2739	2746	2747	rBV3	227	233	0.02%	0.002%
68	10.256	2770	2773	2778	rVB2	243	211	0.02%	0.002%
69	10.394	2812	2816	2819	rBV2	232	191	0.02%	0.002%
70	10.488	2839	2845	2853	rVB2	667	841	0.07%	0.009%
71	10.636	2885	2891	2895	rBV3	663	868	0.07%	0.009%
72	10.668	2898	2901	2906	rVB4	1003	1019	0.09%	0.011%
73	10.758	2916	2929	2946	rBV	439859	716856	61.85%	7.400%
74	10.822	2947	2949	2954	rVB3	449	380	0.03%	0.004%
75	11.015	3006	3009	3013	rVB3	331	252	0.02%	0.003%
76	11.092	3023	3033	3036	rBV4	641	974	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047722.D
 Acq On : 28 Mar 2022 12:55
 Operator : SY/MD
 Sample : VU0328WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.391	3122	3126	3130	rBV	326	267	0.02%	0.003%
78	11.417	3132	3134	3137	rVB	426	190	0.02%	0.002%
79	11.468	3139	3150	3161	rBV4	2209	3758	0.32%	0.039%
80	11.697	3216	3221	3225	rBV2	307	249	0.02%	0.003%
81	11.745	3229	3236	3244	rBV3	1391	2085	0.18%	0.022%
82	11.812	3244	3257	3275	rBV	581526	939281	81.03%	9.696%
83	11.941	3295	3297	3301	rVB2	617	356	0.03%	0.004%
84	11.970	3302	3306	3315	rVB3	897	1029	0.09%	0.011%
85	12.095	3340	3345	3347	rBV2	298	259	0.02%	0.003%
86	12.192	3360	3375	3395	rBV	576674	932563	80.45%	9.627%
87	12.340	3417	3421	3424	rBV2	386	319	0.03%	0.003%
88	12.616	3502	3507	3510	rBV2	321	357	0.03%	0.004%
89	12.658	3517	3520	3523	rBV2	288	221	0.02%	0.002%
90	12.857	3579	3582	3586	rBV2	194	189	0.02%	0.002%
91	12.999	3624	3626	3630	rVB2	640	365	0.03%	0.004%
92	13.070	3645	3648	3650	rBV	241	180	0.02%	0.002%
93	13.221	3689	3695	3703	rVB3	1963	2717	0.23%	0.028%
94	13.578	3804	3806	3808	rBV3	332	219	0.02%	0.002%
95	13.844	3882	3889	3890	rBV4	3331	3363	0.29%	0.035%
96	14.089	3955	3965	3986	rBV	10460	17614	1.52%	0.182%
97	14.330	4032	4040	4052	rVB4	3798	5849	0.50%	0.060%
98	14.996	4244	4247	4252	rBV3	495	411	0.04%	0.004%
99	15.018	4252	4254	4257	rBV	322	238	0.02%	0.002%
100	15.417	4376	4378	4383	rVB3	547	411	0.04%	0.004%




Sum of corrected areas: 9687013

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047722.D
Acq On : 28 Mar 2022 12:55
Operator : SY/MD
Sample : VU0328WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

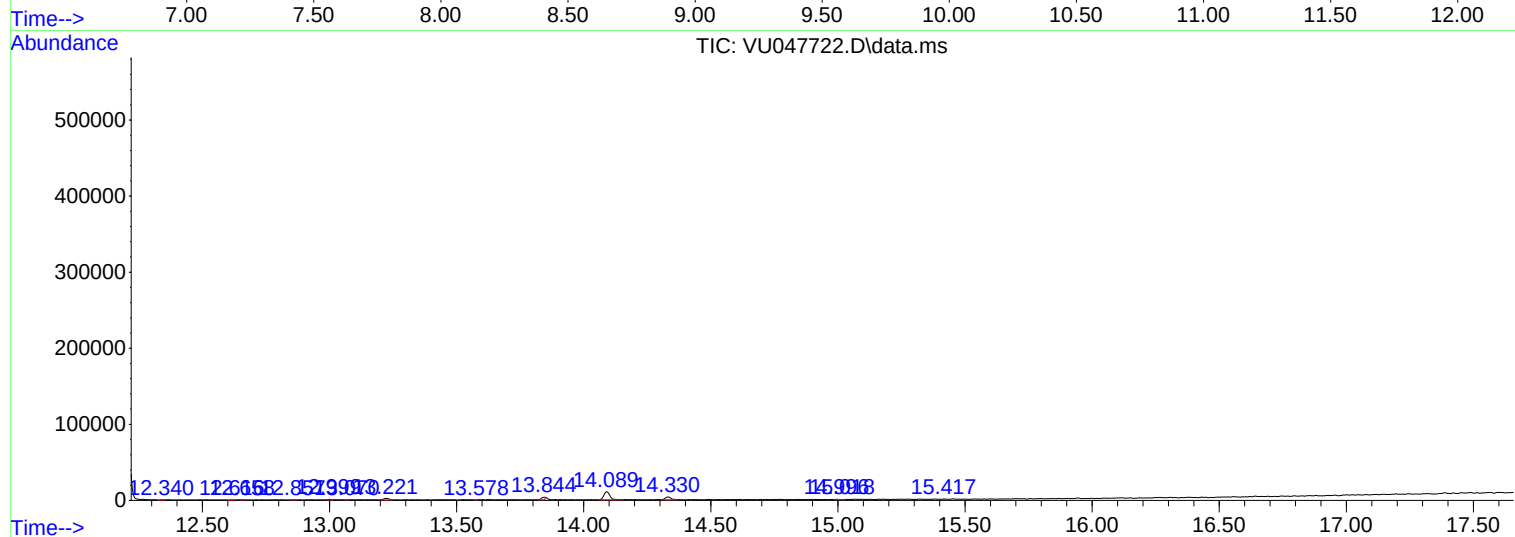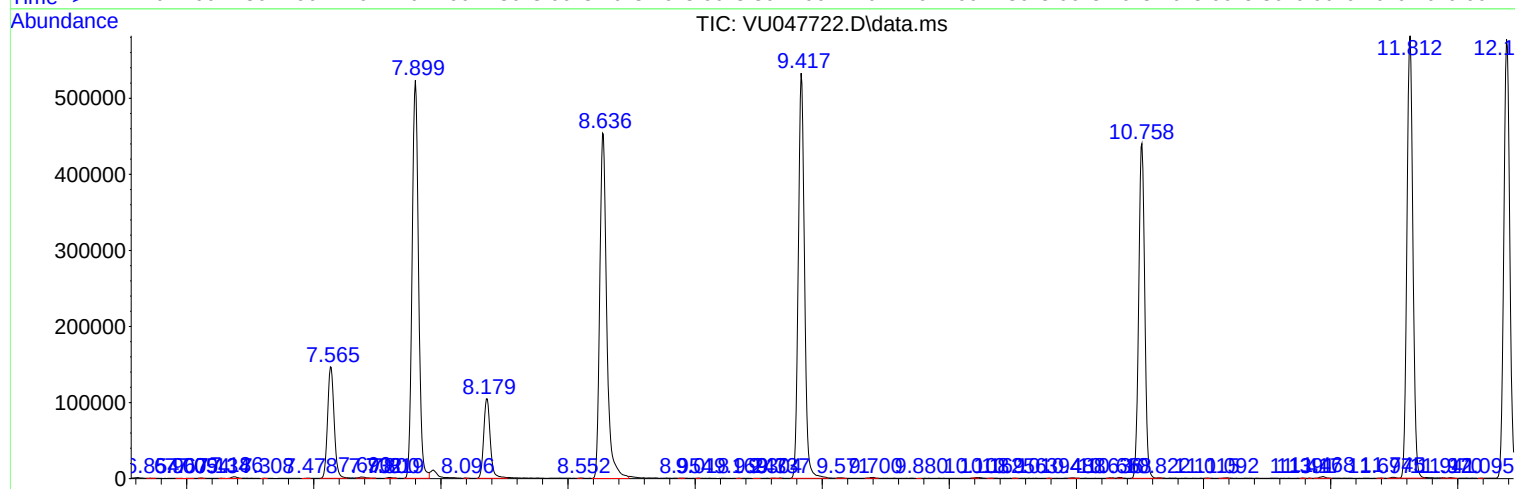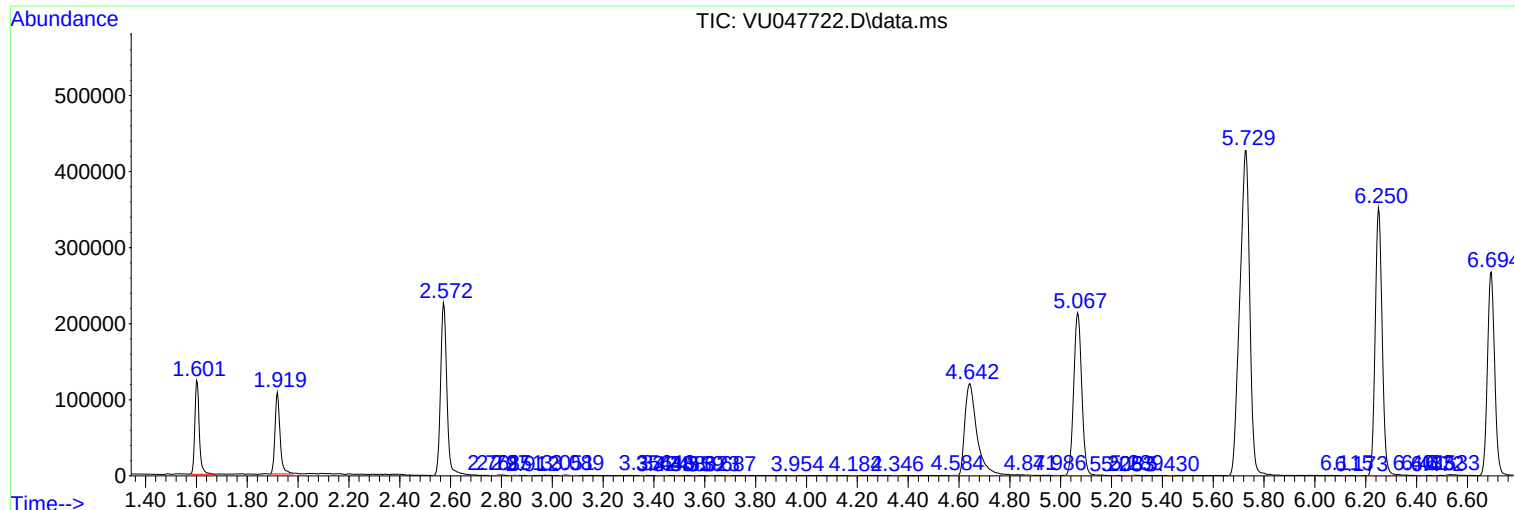

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047722.D
Acq On : 28 Mar 2022 12:55
Operator : SY/MD
Sample : VU0328WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047722.D
Acq On : 28 Mar 2022 12:55
Operator : SY/MD
Sample : VU0328WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK074

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------