

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047723.D
 Acq On : 28 Mar 2022 13:32
 Operator : SY/MD
 Sample : N2082-17DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW619DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	103	rVB2	102330	141168	13.65%	1.533%
2	1.919	171	180	208	rBV	71203	119851	11.59%	1.302%
3	2.568	369	382	394	rBV	181465	301049	29.10%	3.269%
4	2.790	444	451	460	rVB2	858	1554	0.15%	0.017%
5	2.929	491	494	501	rVB	221	200	0.02%	0.002%
6	3.047	524	531	537	rBV4	1983	2819	0.27%	0.031%
7	3.356	617	627	643	rVB2	6291	12058	1.17%	0.131%
8	3.427	643	649	656	rBV2	302	457	0.04%	0.005%
9	3.601	699	703	707	rVB2	290	280	0.03%	0.003%
10	3.633	707	713	714	rBV2	238	160	0.02%	0.002%
11	3.655	716	720	722	rBV	198	196	0.02%	0.002%
12	3.736	741	745	749	rVB2	257	259	0.03%	0.003%
13	3.874	769	788	811	rBV	115838	277103	26.79%	3.009%
14	4.154	871	875	877	rBV	209	191	0.02%	0.002%
15	4.276	910	913	919	rVB2	257	299	0.03%	0.003%
16	4.314	919	925	928	rBV	276	320	0.03%	0.003%
17	4.408	952	954	958	rBV	258	223	0.02%	0.002%
18	4.668	1011	1035	1084	rBV2	283587	811842	78.48%	8.817%
19	4.871	1096	1098	1104	rVB2	548	339	0.03%	0.004%
20	5.067	1142	1159	1181	rBV	162781	356487	34.46%	3.871%
21	5.321	1223	1238	1253	rVB3	10878	24605	2.38%	0.267%
22	5.375	1253	1255	1258	rBV	211	158	0.02%	0.002%
23	5.414	1264	1267	1274	rBV2	256	393	0.04%	0.004%
24	5.520	1297	1300	1304	rVB	194	147	0.01%	0.002%
25	5.584	1315	1320	1323	rBV2	130	144	0.01%	0.002%
26	5.610	1323	1328	1331	rBV2	136	140	0.01%	0.002%
27	5.726	1343	1364	1401	rBV2	330231	895987	86.61%	9.730%
28	5.980	1434	1443	1451	rVV5	1908	3656	0.35%	0.040%
29	6.025	1455	1457	1460	rBV2	308	227	0.02%	0.002%
30	6.080	1466	1474	1480	rBV2	368	726	0.07%	0.008%
31	6.189	1506	1508	1512	rVB3	238	145	0.01%	0.002%
32	6.250	1512	1527	1557	rBV	360976	689640	66.66%	7.489%
33	6.414	1576	1578	1582	rVB2	282	157	0.02%	0.002%
34	6.546	1607	1619	1631	rBV2	18485	34729	3.36%	0.377%
35	6.610	1631	1639	1641	rBV5	844	982	0.09%	0.011%
36	6.694	1650	1665	1688	rBV	205763	402844	38.94%	4.375%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047723.D
 Acq On : 28 Mar 2022 13:32
 Operator : SY/MD
 Sample : N2082-17DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW619DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.803	1696	1699	1700	rBV2	285	179	0.02%	0.002%
38	6.983	1752	1755	1758	rBV	233	149	0.01%	0.002%
39	7.192	1812	1820	1827	rBV6	1610	3151	0.30%	0.034%
40	7.452	1896	1901	1903	rBV2	321	255	0.02%	0.003%
41	7.485	1906	1911	1916	rVB3	369	385	0.04%	0.004%
42	7.568	1924	1937	1966	rVV	113117	203964	19.72%	2.215%
43	7.694	1968	1976	1986	rVB3	1202	2347	0.23%	0.025%
44	7.748	1991	1993	1998	rVB3	255	196	0.02%	0.002%
45	7.800	2005	2009	2011	rBV3	566	468	0.05%	0.005%
46	7.899	2026	2040	2056	rBV	404523	705076	68.16%	7.657%
47	8.089	2097	2099	2102	rVB	420	236	0.02%	0.003%
48	8.182	2116	2128	2143	rBV	82273	139865	13.52%	1.519%
49	8.372	2185	2187	2190	rBV2	223	175	0.02%	0.002%
50	8.401	2190	2196	2199	rBV5	1685	2095	0.20%	0.023%
51	8.555	2234	2244	2254	rBV4	3341	4574	0.44%	0.050%
52	8.649	2259	2273	2303	rBV	305690	661599	63.95%	7.185%
53	8.864	2335	2340	2345	rBV3	449	456	0.04%	0.005%
54	8.906	2350	2353	2355	rBV2	291	152	0.01%	0.002%
55	9.047	2394	2397	2402	rVB2	315	281	0.03%	0.003%
56	9.073	2402	2405	2407	rBV	266	159	0.02%	0.002%
57	9.166	2431	2434	2437	rVB2	264	215	0.02%	0.002%
58	9.420	2497	2513	2538	rBV	550989	932278	90.12%	10.125%
59	9.571	2553	2560	2570	rVB3	4201	6355	0.61%	0.069%
60	9.697	2590	2599	2607	rBV5	1652	2550	0.25%	0.028%
61	9.771	2619	2622	2628	rBV	163	149	0.01%	0.002%
62	9.816	2634	2636	2640	rBV2	213	171	0.02%	0.002%
63	9.973	2678	2685	2689	rBV3	274	305	0.03%	0.003%
64	10.102	2717	2725	2738	rVB5	5328	9296	0.90%	0.101%
65	10.491	2837	2846	2852	rVV3	2100	3084	0.30%	0.033%
66	10.565	2866	2869	2873	rVB	254	198	0.02%	0.002%
67	10.594	2873	2878	2881	rBV2	193	171	0.02%	0.002%
68	10.616	2881	2885	2887	rVV2	281	240	0.02%	0.003%
69	10.668	2895	2901	2908	rVB4	896	1225	0.12%	0.013%
70	10.761	2917	2930	2947	rBV	361851	582566	56.31%	6.327%
71	10.825	2948	2950	2954	rVB2	647	289	0.03%	0.003%
72	10.845	2954	2956	2960	rVB2	229	161	0.02%	0.002%
73	10.909	2966	2976	2983	rVV3	1820	2701	0.26%	0.029%
74	10.999	2997	3004	3008	rBV2	1553	2043	0.20%	0.022%
75	11.121	3039	3042	3044	rVB2	258	164	0.02%	0.002%
76	11.295	3087	3096	3106	rBV2	3629	5057	0.49%	0.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047723.D
 Acq On : 28 Mar 2022 13:32
 Operator : SY/MD
 Sample : N2082-17DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW619DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.369	3116	3119	3124	rBV2	237	246	0.02%	0.003%
78	11.468	3142	3150	3160	rVB3	5251	8073	0.78%	0.088%
79	11.517	3163	3165	3168	rVV2	234	163	0.02%	0.002%
80	11.607	3188	3193	3196	rBV3	410	342	0.03%	0.004%
81	11.697	3215	3221	3224	rBV5	535	461	0.04%	0.005%
82	11.751	3233	3238	3243	rVB4	1205	1166	0.11%	0.013%
83	11.816	3244	3258	3277	rBV	648666	1034493	100.00%	11.235%
84	11.931	3291	3294	3296	rBV2	276	223	0.02%	0.002%
85	12.092	3339	3344	3345	rBV3	1133	881	0.09%	0.010%
86	12.195	3363	3376	3396	rBV	473447	769029	74.34%	8.352%
87	12.378	3430	3433	3438	rBV3	347	342	0.03%	0.004%
88	12.488	3458	3467	3474	rVV3	5484	8402	0.81%	0.091%
89	12.732	3540	3543	3546	rVB2	301	221	0.02%	0.002%
90	12.771	3550	3555	3561	rVV3	621	773	0.07%	0.008%
91	12.809	3561	3567	3574	rVB5	1033	1604	0.16%	0.017%
92	12.841	3574	3577	3579	rBV2	430	290	0.03%	0.003%
93	12.918	3597	3601	3605	rVB3	403	392	0.04%	0.004%
94	13.224	3690	3696	3705	rVB2	1392	1858	0.18%	0.020%
95	13.590	3808	3810	3815	rVB2	337	241	0.02%	0.003%
96	13.844	3883	3889	3897	rVB3	2336	3102	0.30%	0.034%
97	14.018	3940	3943	3950	rVB4	707	690	0.07%	0.007%
98	14.089	3957	3965	3978	rVB3	9553	14699	1.42%	0.160%
99	14.333	4033	4041	4051	rVB3	2255	3626	0.35%	0.039%
100	15.050	4262	4264	4268	rBV2	428	300	0.03%	0.003%




Sum of corrected areas: 9208132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047723.D
Acq On : 28 Mar 2022 13:32
Operator : SY/MD
Sample : N2082-17DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW619DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

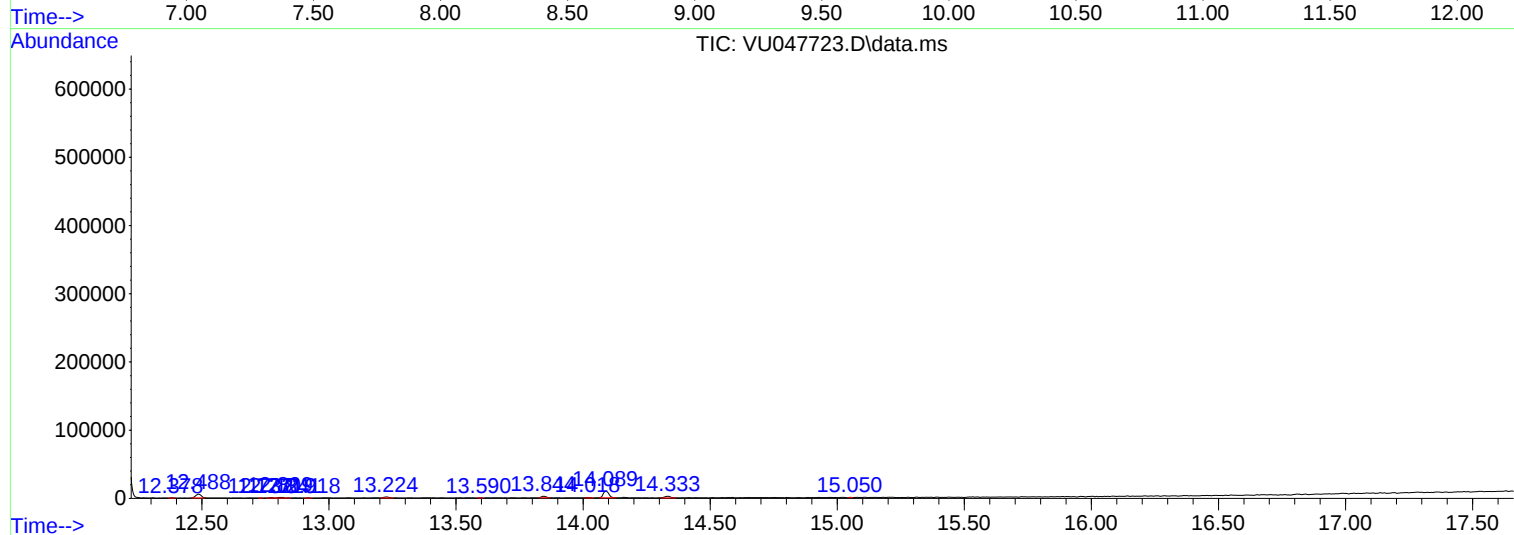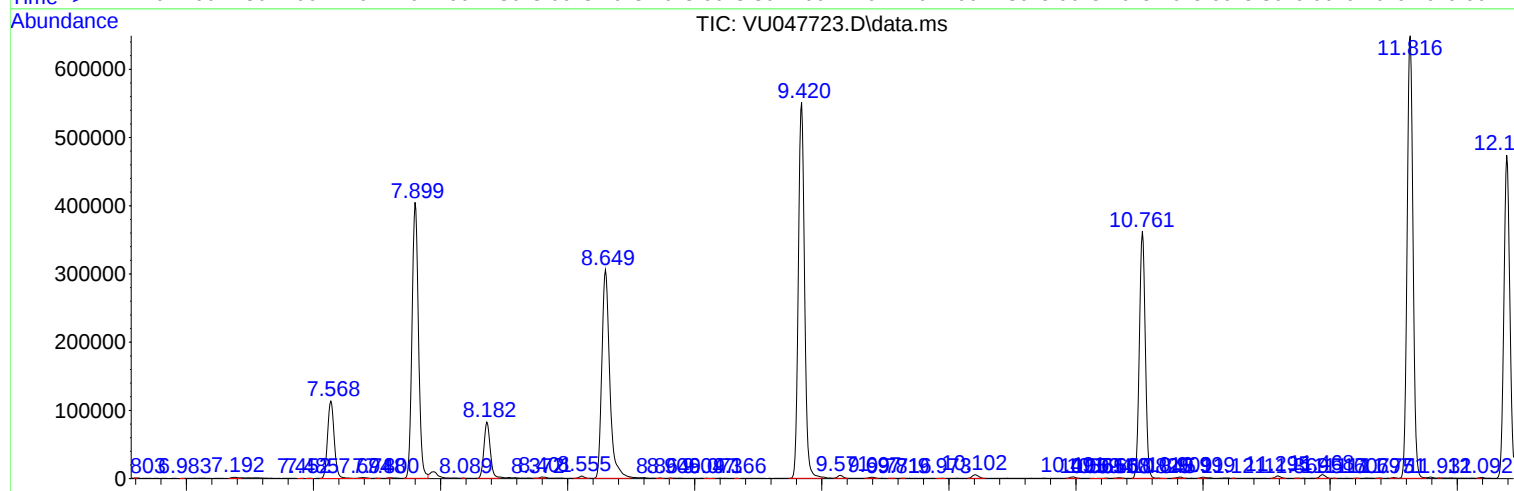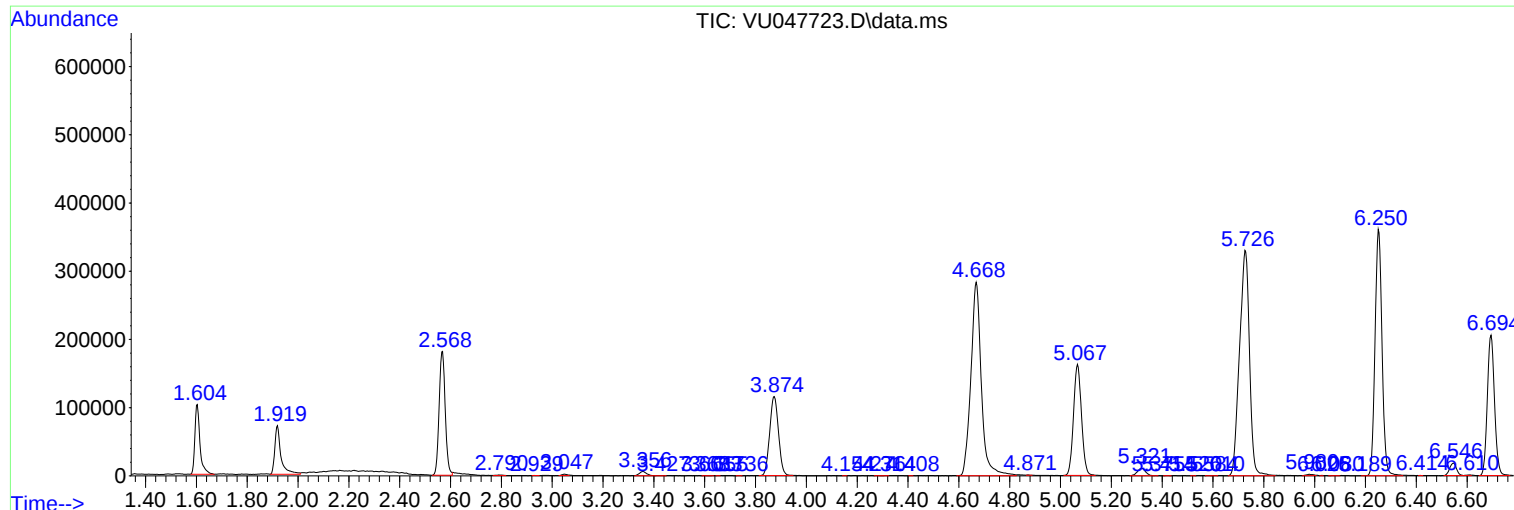

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047723.D
Acq On : 28 Mar 2022 13:32
Operator : SY/MD
Sample : N2082-17DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW619DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047723.D
Acq On : 28 Mar 2022 13:32
Operator : SY/MD
Sample : N2082-17DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW619DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------