

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047725.D
 Acq On : 28 Mar 2022 14:22
 Operator : SY/MD
 Sample : N2082-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	101	rVB	109496	131984	11.67%	1.394%
2	1.919	171	180	196	rBV	98154	136058	12.03%	1.437%
3	2.572	370	383	405	rBV	207331	349338	30.89%	3.690%
4	2.800	451	454	457	rVV2	328	273	0.02%	0.003%
5	2.867	470	475	479	rBV3	245	234	0.02%	0.002%
6	3.047	527	531	532	rBV2	585	426	0.04%	0.005%
7	3.096	543	546	550	rVB3	450	349	0.03%	0.004%
8	3.121	550	554	556	rBV2	370	282	0.02%	0.003%
9	3.160	564	566	571	rVB	429	271	0.02%	0.003%
10	3.334	614	620	622	rVV3	232	241	0.02%	0.003%
11	3.353	622	626	632	rVB2	396	355	0.03%	0.004%
12	3.417	640	646	652	rVB3	243	305	0.03%	0.003%
13	3.498	666	671	676	rBV2	250	330	0.03%	0.003%
14	3.581	695	697	700	rVV2	366	306	0.03%	0.003%
15	3.674	724	726	731	rVV2	269	215	0.02%	0.002%
16	3.742	744	747	751	rBV2	457	354	0.03%	0.004%
17	3.819	768	771	776	rBV2	388	363	0.03%	0.004%
18	3.973	814	819	824	rBV2	339	475	0.04%	0.005%
19	4.035	835	838	841	rBV2	290	222	0.02%	0.002%
20	4.356	936	938	944	rVV2	231	215	0.02%	0.002%
21	4.388	945	948	953	rVB2	307	211	0.02%	0.002%
22	4.498	977	982	985	rBV3	323	310	0.03%	0.003%
23	4.639	1012	1026	1068	rBV	122227	393016	34.75%	4.152%
24	5.067	1141	1159	1182	rBV	207248	454892	40.22%	4.805%
25	5.186	1194	1196	1200	rBV4	397	249	0.02%	0.003%
26	5.231	1206	1210	1216	rVB2	499	455	0.04%	0.005%
27	5.298	1224	1231	1238	rBV3	533	793	0.07%	0.008%
28	5.378	1253	1256	1258	rBV2	326	231	0.02%	0.002%
29	5.478	1283	1287	1291	rVB2	278	218	0.02%	0.002%
30	5.633	1332	1335	1339	rVB	245	208	0.02%	0.002%
31	5.729	1342	1365	1397	rBV2	414296	1130879	100.00%	11.946%
32	5.925	1424	1426	1434	rVB2	293	245	0.02%	0.003%
33	6.115	1482	1485	1489	rVV3	312	240	0.02%	0.003%
34	6.250	1512	1527	1558	rBV	347406	671936	59.42%	7.098%
35	6.526	1609	1613	1616	rBV4	912	870	0.08%	0.009%
36	6.559	1621	1623	1627	rVB3	336	218	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047725.D
 Acq On : 28 Mar 2022 14:22
 Operator : SY/MD
 Sample : N2082-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1691	rBV	266818	520178	46.00%	5.495%
38	6.803	1696	1699	1709	rVV4	1057	1286	0.11%	0.014%
39	7.047	1768	1775	1781	rBV3	587	653	0.06%	0.007%
40	7.186	1811	1818	1827	rVV3	2030	2987	0.26%	0.032%
41	7.417	1884	1890	1893	rBV2	275	270	0.02%	0.003%
42	7.510	1917	1919	1923	rVV	403	271	0.02%	0.003%
43	7.568	1923	1937	1956	rBV	143214	254466	22.50%	2.688%
44	7.690	1966	1975	1985	rVB4	1971	3059	0.27%	0.032%
45	7.899	2026	2040	2056	rBV	499632	871249	77.04%	9.204%
46	8.124	2107	2110	2115	rVB2	382	335	0.03%	0.004%
47	8.179	2115	2127	2145	rBV	103048	179504	15.87%	1.896%
48	8.346	2177	2179	2185	rVB4	376	314	0.03%	0.003%
49	8.407	2194	2198	2199	rBV2	315	242	0.02%	0.003%
50	8.472	2212	2218	2227	rVB2	1466	2156	0.19%	0.023%
51	8.581	2249	2252	2256	rBV	298	254	0.02%	0.003%
52	8.636	2256	2269	2305	rBV	449251	869583	76.89%	9.186%
53	8.841	2330	2333	2337	rVB2	500	341	0.03%	0.004%
54	9.134	2419	2424	2431	rBB3	257	309	0.03%	0.003%
55	9.243	2454	2458	2463	rBV3	365	423	0.04%	0.004%
56	9.369	2491	2497	2499	rVV3	279	249	0.02%	0.003%
57	9.417	2499	2512	2547	rVV	533118	897491	79.36%	9.481%
58	9.690	2592	2597	2605	rBV4	857	1248	0.11%	0.013%
59	9.767	2619	2621	2625	rBV2	259	238	0.02%	0.003%
60	9.809	2630	2634	2638	rVB2	307	296	0.03%	0.003%
61	9.986	2687	2689	2692	rBV2	306	243	0.02%	0.003%
62	10.102	2720	2725	2727	rVV2	295	262	0.02%	0.003%
63	10.365	2804	2807	2811	rBV3	267	242	0.02%	0.003%
64	10.491	2839	2846	2849	rVB3	307	358	0.03%	0.004%
65	10.642	2889	2893	2897	rBV	233	276	0.02%	0.003%
66	10.674	2897	2903	2908	rVV4	985	1206	0.11%	0.013%
67	10.758	2915	2929	2946	rBV	448313	717844	63.48%	7.583%
68	10.896	2960	2972	2984	rBV2	2557	4559	0.40%	0.048%
69	10.951	2986	2989	2995	rVB	380	357	0.03%	0.004%
70	10.999	3000	3004	3008	rVB2	253	215	0.02%	0.002%
71	11.095	3028	3034	3039	rBV4	605	677	0.06%	0.007%
72	11.227	3072	3075	3078	rBV	315	227	0.02%	0.002%
73	11.298	3093	3097	3099	rBV2	266	233	0.02%	0.002%
74	11.465	3142	3149	3158	rVB5	1280	2088	0.18%	0.022%
75	11.549	3171	3175	3180	rVB3	343	296	0.03%	0.003%
76	11.687	3216	3218	3224	rVB2	273	236	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047725.D
 Acq On : 28 Mar 2022 14:22
 Operator : SY/MD
 Sample : N2082-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.748	3233	3237	3241	rVB	371	365	0.03%	0.004%
78	11.812	3244	3257	3279	rVV	599274	938902	83.02%	9.918%
79	12.005	3312	3317	3320	rBV3	309	322	0.03%	0.003%
80	12.028	3321	3324	3328	rVB3	279	234	0.02%	0.002%
81	12.060	3331	3334	3338	rBV2	240	261	0.02%	0.003%
82	12.192	3363	3375	3398	rBV	553886	901974	79.76%	9.528%
83	12.385	3430	3435	3439	rBV3	236	268	0.02%	0.003%
84	12.417	3440	3445	3449	rBV3	375	469	0.04%	0.005%
85	12.497	3468	3470	3474	rVB2	510	288	0.03%	0.003%
86	12.529	3475	3480	3481	rBV2	272	226	0.02%	0.002%
87	12.584	3495	3497	3502	rBV2	491	419	0.04%	0.004%
88	12.658	3515	3520	3524	rBV3	266	305	0.03%	0.003%
89	12.758	3546	3551	3553	rBV2	447	454	0.04%	0.005%
90	12.925	3600	3603	3607	rVB2	443	331	0.03%	0.003%
91	12.957	3610	3613	3620	rVV3	267	280	0.02%	0.003%
92	13.118	3659	3663	3667	rBV3	266	287	0.03%	0.003%
93	13.211	3689	3692	3694	rBV2	320	234	0.02%	0.002%
94	13.420	3755	3757	3761	rBV2	351	235	0.02%	0.002%
95	13.568	3800	3803	3806	rBV3	313	253	0.02%	0.003%
96	13.844	3887	3889	3893	rBV2	496	314	0.03%	0.003%
97	14.095	3962	3967	3977	rVB	3012	3797	0.34%	0.040%
98	14.336	4035	4042	4048	rBV5	1129	1450	0.13%	0.015%
99	14.568	4112	4114	4116	rBV	360	245	0.02%	0.003%
100	15.089	4273	4276	4277	rBV	404	275	0.02%	0.003%


Sum of corrected areas: 9466476

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047725.D
Acq On : 28 Mar 2022 14:22
Operator : SY/MD
Sample : N2082-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

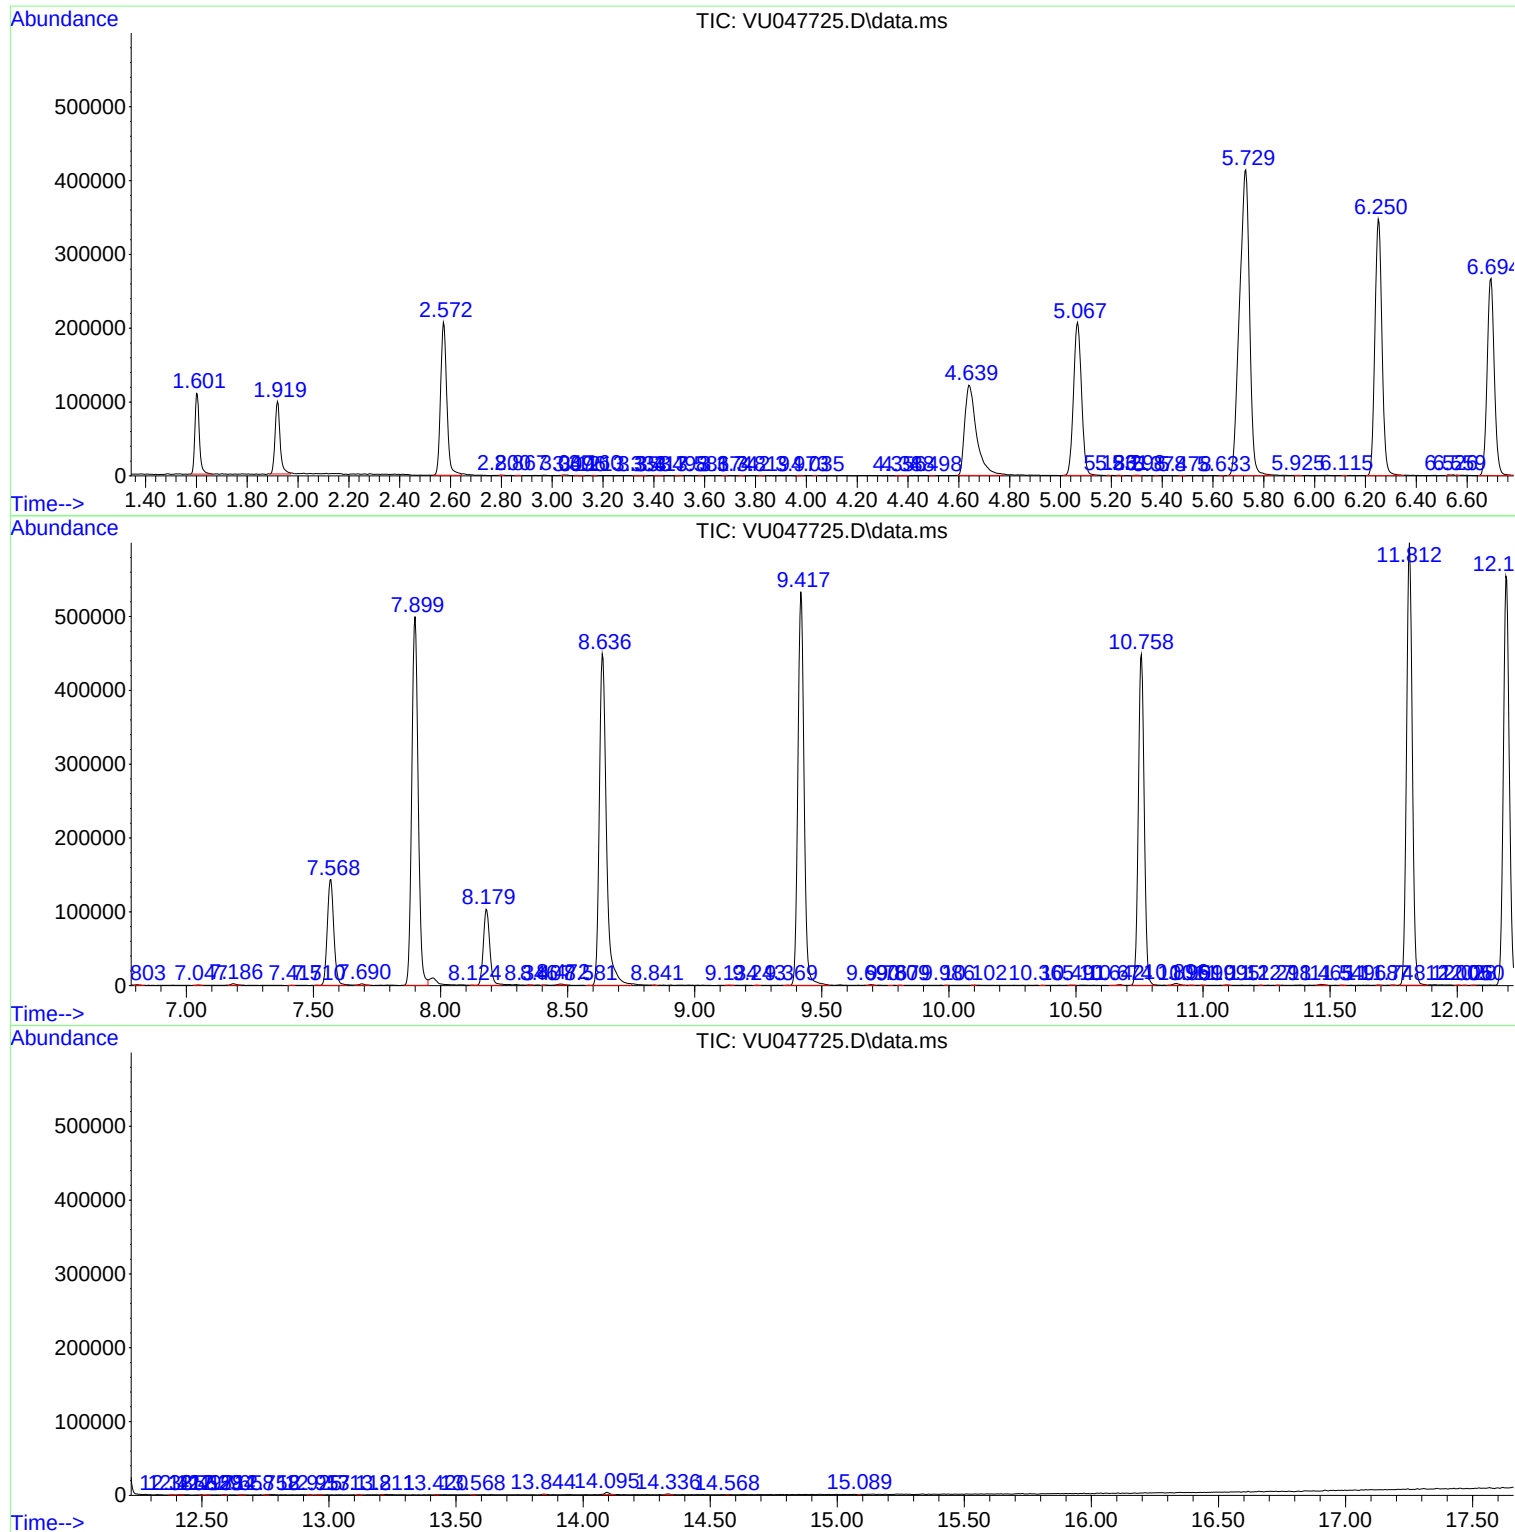

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047725.D
Acq On : 28 Mar 2022 14:22
Operator : SY/MD
Sample : N2082-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047725.D
Acq On : 28 Mar 2022 14:22
Operator : SY/MD
Sample : N2082-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------