

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047727.D
 Acq On : 28 Mar 2022 15:07
 Operator : SY/MD
 Sample : N2081-11DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	102	rBV	122307	143249	12.42%	1.371%
2	1.919	171	180	199	rBV	103163	142543	12.35%	1.364%
3	2.571	371	383	401	rBV	230721	392158	33.99%	3.753%
4	2.745	435	437	442	rVB4	468	344	0.03%	0.003%
5	2.793	444	452	454	rBV4	462	620	0.05%	0.006%
6	2.832	460	464	466	rBV2	168	168	0.01%	0.002%
7	2.916	488	490	494	rBV2	183	179	0.02%	0.002%
8	3.054	526	533	539	rVB4	982	1324	0.11%	0.013%
9	3.147	557	562	567	rBV3	366	370	0.03%	0.004%
10	3.227	584	587	593	rVB	273	301	0.03%	0.003%
11	3.359	615	628	629	rBV3	1626	1976	0.17%	0.019%
12	3.440	649	653	656	rBV2	281	243	0.02%	0.002%
13	3.706	732	736	739	rBV2	254	208	0.02%	0.002%
14	3.729	739	743	746	rBV2	286	263	0.02%	0.003%
15	3.793	759	763	767	rVB3	292	232	0.02%	0.002%
16	3.877	772	789	807	rVV	27497	63278	5.48%	0.606%
17	3.951	810	812	819	rVB2	395	310	0.03%	0.003%
18	4.160	873	877	880	rVB3	277	171	0.01%	0.002%
19	4.224	891	897	905	rVB3	375	472	0.04%	0.005%
20	4.276	910	913	918	rVV2	250	204	0.02%	0.002%
21	4.298	918	920	923	rVB2	311	199	0.02%	0.002%
22	4.369	940	942	948	rVV2	170	178	0.02%	0.002%
23	4.398	948	951	954	rVB2	260	202	0.02%	0.002%
24	4.430	959	961	964	rVV2	241	164	0.01%	0.002%
25	4.452	964	968	970	rVV2	239	165	0.01%	0.002%
26	4.517	985	988	995	rBV3	238	261	0.02%	0.002%
27	4.575	999	1006	1009	rBV3	272	292	0.03%	0.003%
28	4.665	1013	1034	1083	rBV2	151151	601220	52.11%	5.753%
29	5.067	1143	1159	1185	rBV	210923	465157	40.31%	4.451%
30	5.195	1195	1199	1203	rBV3	318	339	0.03%	0.003%
31	5.317	1221	1237	1262	rVB	146044	333021	28.86%	3.187%
32	5.726	1341	1364	1395	rBV2	423113	1153829	100.00%	11.042%
33	5.980	1440	1443	1448	rBV3	353	266	0.02%	0.003%
34	6.115	1482	1485	1489	rVB2	311	225	0.02%	0.002%
35	6.160	1496	1499	1506	rVB2	275	332	0.03%	0.003%
36	6.189	1506	1508	1511	rBV	304	178	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047727.D
 Acq On : 28 Mar 2022 15:07
 Operator : SY/MD
 Sample : N2081-11DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1551	rBV	370713	710316	61.56%	6.797%
38	6.546	1608	1619	1630	rBV6	4109	8319	0.72%	0.080%
39	6.600	1633	1636	1639	rBV3	484	360	0.03%	0.003%
40	6.693	1650	1665	1683	rBV	264414	521949	45.24%	4.995%
41	7.121	1796	1798	1799	rBV	336	170	0.01%	0.002%
42	7.131	1799	1801	1805	rVB2	253	176	0.02%	0.002%
43	7.185	1810	1818	1827	rBV3	2053	3354	0.29%	0.032%
44	7.275	1839	1846	1851	rBV2	270	349	0.03%	0.003%
45	7.375	1872	1877	1879	rVB3	220	193	0.02%	0.002%
46	7.565	1924	1936	1957	rVV	147203	262211	22.73%	2.509%
47	7.668	1965	1968	1969	rBV2	274	180	0.02%	0.002%
48	7.693	1970	1976	1983	rVB5	1563	2059	0.18%	0.020%
49	7.790	2003	2006	2010	rVV2	319	266	0.02%	0.003%
50	7.899	2025	2040	2056	rBV	522103	909201	78.80%	8.701%
51	8.179	2116	2127	2142	rBV	106581	183796	15.93%	1.759%
52	8.394	2191	2194	2197	rVB3	351	244	0.02%	0.002%
53	8.439	2205	2208	2209	rBV2	321	174	0.02%	0.002%
54	8.475	2210	2219	2233	rVB3	3376	6620	0.57%	0.063%
55	8.552	2233	2243	2255	rBV4	9765	16391	1.42%	0.157%
56	8.639	2256	2270	2303	rBV	446252	886080	76.79%	8.479%
57	8.906	2351	2353	2356	rVB3	420	215	0.02%	0.002%
58	8.928	2356	2360	2365	rVB3	342	224	0.02%	0.002%
59	9.073	2402	2405	2408	rVV	295	199	0.02%	0.002%
60	9.243	2455	2458	2462	rBV2	262	230	0.02%	0.002%
61	9.417	2499	2512	2549	rVB	550061	930891	80.68%	8.908%
62	9.571	2556	2560	2568	rVB3	530	684	0.06%	0.007%
63	9.629	2576	2578	2582	rVB2	322	191	0.02%	0.002%
64	9.693	2590	2598	2604	rBV3	1141	1753	0.15%	0.017%
65	9.771	2620	2622	2626	rVB3	303	202	0.02%	0.002%
66	9.796	2627	2630	2634	rBV2	237	160	0.01%	0.002%
67	9.960	2678	2681	2685	rBV	230	173	0.01%	0.002%
68	10.066	2708	2714	2715	rBV	207	175	0.02%	0.002%
69	10.098	2721	2724	2726	rBV2	468	343	0.03%	0.003%
70	10.311	2788	2790	2796	rVB3	197	181	0.02%	0.002%
71	10.488	2838	2845	2847	rBV2	416	442	0.04%	0.004%
72	10.555	2861	2866	2869	rBV2	295	362	0.03%	0.003%
73	10.648	2889	2895	2897	rBV2	363	489	0.04%	0.005%
74	10.671	2897	2902	2914	rVV5	1062	1562	0.14%	0.015%
75	10.758	2914	2929	2949	rVV	443922	724839	62.82%	6.936%
76	10.896	2962	2972	2982	rVB2	4445	6939	0.60%	0.066%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047727.D
 Acq On : 28 Mar 2022 15:07
 Operator : SY/MD
 Sample : N2081-11DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.086	3024	3031	3033	rBV3	682	758	0.07%	0.007%
78	11.153	3049	3052	3054	rBV2	249	174	0.02%	0.002%
79	11.468	3141	3150	3160	rVB2	5569	7717	0.67%	0.074%
80	11.606	3189	3193	3197	rVB3	242	232	0.02%	0.002%
81	11.690	3213	3219	3222	rBV3	491	405	0.04%	0.004%
82	11.738	3230	3234	3239	rBV3	394	377	0.03%	0.004%
83	11.812	3243	3257	3277	rBV	622134	1001343	86.78%	9.582%
84	11.889	3277	3281	3287	rVB5	990	1261	0.11%	0.012%
85	11.941	3295	3297	3303	rVB2	587	361	0.03%	0.003%
86	11.970	3303	3306	3307	rBV2	317	190	0.02%	0.002%
87	12.192	3362	3375	3394	rBV	579196	939962	81.46%	8.995%
88	12.375	3429	3432	3440	rBV2	504	533	0.05%	0.005%
89	12.420	3443	3446	3449	rBV	277	218	0.02%	0.002%
90	12.729	3539	3542	3544	rBV	218	170	0.01%	0.002%
91	12.770	3548	3555	3566	rVB5	1272	2111	0.18%	0.020%
92	12.825	3566	3572	3574	rBV3	288	311	0.03%	0.003%
93	12.883	3588	3590	3594	rVB	360	189	0.02%	0.002%
94	13.764	3861	3864	3867	rBV2	379	287	0.02%	0.003%
95	14.092	3958	3966	3975	rBV2	2526	4129	0.36%	0.040%
96	14.233	4008	4010	4016	rVB	288	217	0.02%	0.002%
97	14.330	4038	4040	4044	rBV2	425	355	0.03%	0.003%
98	15.150	4292	4295	4297	rBV3	564	319	0.03%	0.003%
99	15.349	4355	4357	4360	rBV3	518	279	0.02%	0.003%
100	15.716	4468	4471	4474	rBV3	760	563	0.05%	0.005%




Sum of corrected areas: 10449764

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047727.D
Acq On : 28 Mar 2022 15:07
Operator : SY/MD
Sample : N2081-11DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

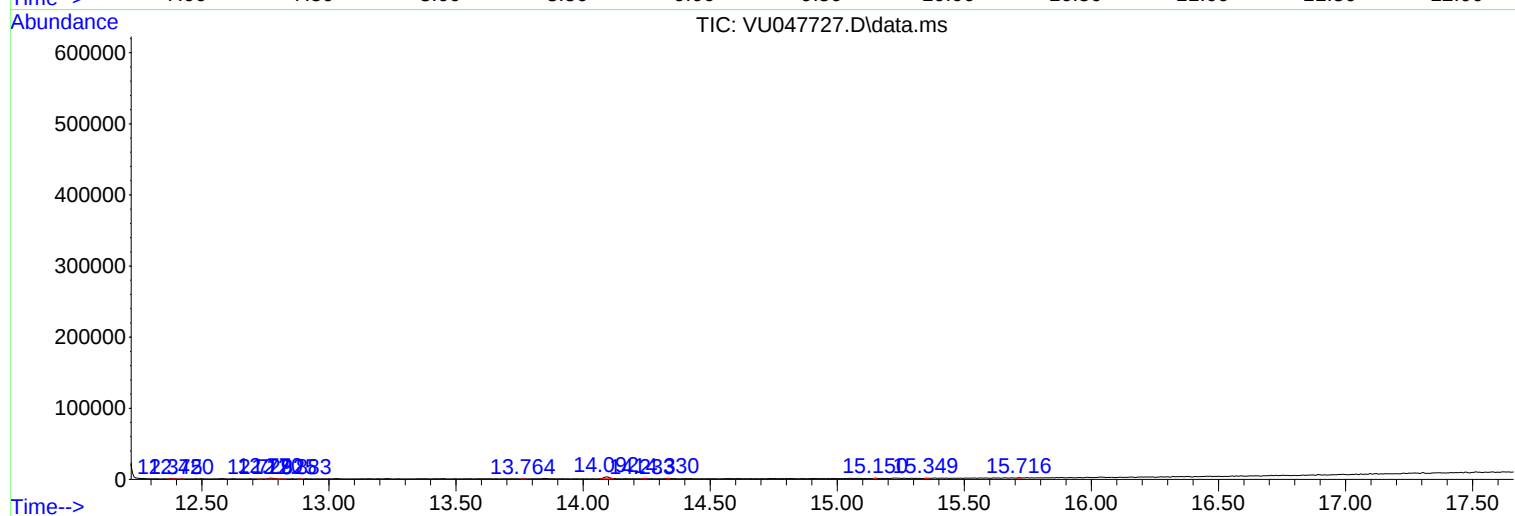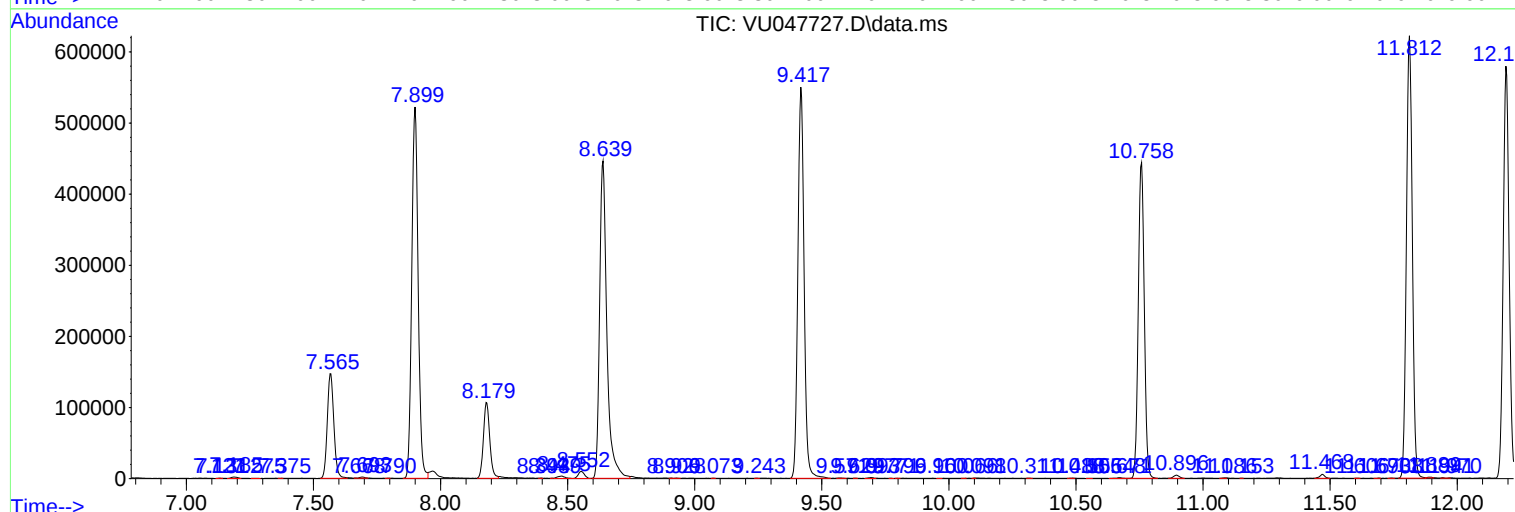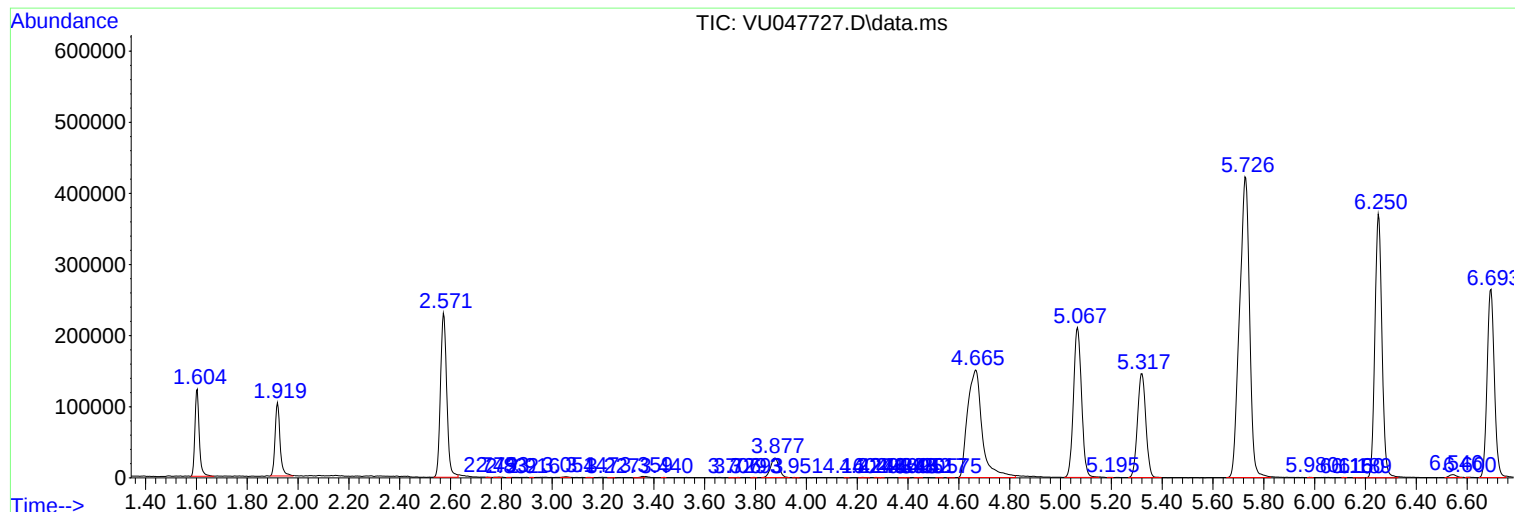

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047727.D
Acq On : 28 Mar 2022 15:07
Operator : SY/MD
Sample : N2081-11DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047727.D
Acq On : 28 Mar 2022 15:07
Operator : SY/MD
Sample : N2081-11DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------