

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047728.D
 Acq On : 28 Mar 2022 15:30
 Operator : SY/MD
 Sample : N2081-14DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047728.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rVB	113697	134469	12.35%	1.239%
2	1.919	170	180	197	rBV	100270	139651	12.82%	1.286%
3	2.517	363	366	369	rBV2	302	216	0.02%	0.002%
4	2.572	371	383	409	rBV2	218060	378549	34.75%	3.487%
5	2.774	441	446	447	rBV	207	178	0.02%	0.002%
6	2.945	497	499	502	rBV	237	176	0.02%	0.002%
7	3.054	525	533	542	rVB3	842	1312	0.12%	0.012%
8	3.183	569	573	577	rVV2	582	584	0.05%	0.005%
9	3.411	641	644	648	rVB3	272	196	0.02%	0.002%
10	3.437	648	652	654	rBV2	335	224	0.02%	0.002%
11	3.482	664	666	672	rVB2	345	274	0.03%	0.003%
12	3.511	672	675	677	rBV	299	224	0.02%	0.002%
13	3.697	729	733	736	rBV2	255	264	0.02%	0.002%
14	3.745	743	748	751	rBV2	223	211	0.02%	0.002%
15	3.874	774	788	804	rBV	14155	32966	3.03%	0.304%
16	4.073	844	850	854	rBV2	165	183	0.02%	0.002%
17	4.102	857	859	864	rVB2	206	177	0.02%	0.002%
18	4.189	881	886	888	rBV2	365	312	0.03%	0.003%
19	4.234	897	900	902	rVV	291	198	0.02%	0.002%
20	4.305	917	922	926	rVV3	310	333	0.03%	0.003%
21	4.588	1004	1010	1012	rBV	247	235	0.02%	0.002%
22	4.642	1012	1027	1065	rBV	118355	419193	38.48%	3.861%
23	4.922	1111	1114	1117	rBV2	324	231	0.02%	0.002%
24	5.067	1142	1159	1187	rBV	203341	441045	40.49%	4.063%
25	5.321	1218	1238	1260	rBV	240416	542410	49.80%	4.996%
26	5.536	1303	1305	1310	rVB	233	181	0.02%	0.002%
27	5.729	1339	1365	1390	rBV2	398953	1089258	100.00%	10.033%
28	5.928	1425	1427	1437	rVB2	292	274	0.03%	0.003%
29	6.044	1458	1463	1469	rVB4	612	631	0.06%	0.006%
30	6.070	1469	1471	1474	rBV2	338	277	0.03%	0.003%
31	6.137	1489	1492	1495	rVB2	302	220	0.02%	0.002%
32	6.166	1495	1501	1507	rVB	318	430	0.04%	0.004%
33	6.250	1511	1527	1556	rBV	372660	702286	64.47%	6.469%
34	6.382	1564	1568	1571	rVB3	486	310	0.03%	0.003%
35	6.462	1590	1593	1596	rVB2	346	197	0.02%	0.002%
36	6.481	1596	1599	1602	rVB3	316	216	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047728.D
 Acq On : 28 Mar 2022 15:30
 Operator : SY/MD
 Sample : N2081-14DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.543	1606	1618	1639	rVV	114850	215632	19.80%	1.986%
38	6.694	1649	1665	1688	rBV	255711	498603	45.77%	4.593%
39	7.047	1769	1775	1783	rVB3	557	751	0.07%	0.007%
40	7.182	1807	1817	1827	rBV5	2318	4345	0.40%	0.040%
41	7.510	1914	1919	1924	rBV3	298	355	0.03%	0.003%
42	7.565	1924	1936	1955	rBV	138240	248014	22.77%	2.285%
43	7.690	1968	1975	1988	rVB7	2040	4095	0.38%	0.038%
44	7.745	1988	1992	1996	rBV2	429	376	0.03%	0.003%
45	7.777	1996	2002	2004	rBV2	271	218	0.02%	0.002%
46	7.800	2004	2009	2013	rVB2	573	567	0.05%	0.005%
47	7.899	2023	2040	2055	rBV	495011	857571	78.73%	7.899%
48	8.179	2115	2127	2147	rBV	98907	171401	15.74%	1.579%
49	8.401	2191	2196	2204	rBB5	1370	1674	0.15%	0.015%
50	8.440	2204	2208	2209	rBV3	389	249	0.02%	0.002%
51	8.472	2210	2218	2231	rVB2	4700	8228	0.76%	0.076%
52	8.552	2231	2243	2257	rBV	349852	602646	55.33%	5.551%
53	8.636	2258	2269	2306	rVB	436092	832027	76.38%	7.664%
54	8.829	2327	2329	2333	rVB3	371	250	0.02%	0.002%
55	8.909	2350	2354	2357	rBV	382	298	0.03%	0.003%
56	9.083	2403	2408	2413	rBV2	203	269	0.02%	0.002%
57	9.105	2413	2415	2419	rBV	301	225	0.02%	0.002%
58	9.218	2447	2450	2451	rBV2	282	182	0.02%	0.002%
59	9.231	2452	2454	2457	rVV3	306	204	0.02%	0.002%
60	9.285	2468	2471	2477	rVB3	313	331	0.03%	0.003%
61	9.324	2477	2483	2486	rBV2	319	258	0.02%	0.002%
62	9.417	2499	2512	2550	rVV	552720	936170	85.95%	8.623%
63	9.681	2588	2594	2595	rBV	677	532	0.05%	0.005%
64	9.896	2658	2661	2664	rVB2	397	253	0.02%	0.002%
65	10.073	2711	2716	2718	rBV2	231	229	0.02%	0.002%
66	10.157	2739	2742	2745	rBV3	328	259	0.02%	0.002%
67	10.353	2796	2803	2807	rBV3	320	350	0.03%	0.003%
68	10.420	2821	2824	2830	rBV	257	192	0.02%	0.002%
69	10.488	2842	2845	2848	rVB2	311	232	0.02%	0.002%
70	10.587	2872	2876	2882	rVB2	293	289	0.03%	0.003%
71	10.616	2882	2885	2887	rBV	227	190	0.02%	0.002%
72	10.674	2895	2903	2909	rVB2	1118	1230	0.11%	0.011%
73	10.758	2916	2929	2951	rVB	420722	686128	62.99%	6.320%
74	10.893	2960	2971	2983	rBV	7187	11956	1.10%	0.110%
75	10.964	2990	2993	2998	rVB2	312	206	0.02%	0.002%
76	10.993	2999	3002	3005	rBV2	375	307	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047728.D
 Acq On : 28 Mar 2022 15:30
 Operator : SY/MD
 Sample : N2081-14DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.086	3028	3031	3037	rVB2	555	593	0.05%	0.005%
78	11.121	3040	3042	3045	rVB2	365	181	0.02%	0.002%
79	11.166	3052	3056	3057	rBV	303	199	0.02%	0.002%
80	11.237	3070	3078	3083	rBV3	454	636	0.06%	0.006%
81	11.472	3137	3151	3158	rBV6	1729	3294	0.30%	0.030%
82	11.523	3164	3167	3171	rBV3	282	259	0.02%	0.002%
83	11.748	3234	3237	3240	rVB2	396	227	0.02%	0.002%
84	11.812	3244	3257	3280	rBV	613453	982106	90.16%	9.046%
85	11.973	3301	3307	3314	rVB4	777	965	0.09%	0.009%
86	12.192	3362	3375	3394	rBV	543354	885017	81.25%	8.152%
87	12.314	3411	3413	3419	rVB3	510	412	0.04%	0.004%
88	12.346	3419	3423	3430	rVB4	464	612	0.06%	0.006%
89	12.378	3430	3433	3437	rBV3	315	263	0.02%	0.002%
90	12.774	3548	3556	3564	rBV2	1509	2642	0.24%	0.024%
91	13.028	3630	3635	3639	rBV2	441	408	0.04%	0.004%
92	13.208	3686	3691	3693	rBV2	500	460	0.04%	0.004%
93	13.256	3704	3706	3710	rBV2	217	199	0.02%	0.002%
94	13.298	3716	3719	3723	rBV	283	191	0.02%	0.002%
95	13.610	3812	3816	3821	rBV2	339	405	0.04%	0.004%
96	13.719	3846	3850	3852	rBV2	243	250	0.02%	0.002%
97	14.616	4123	4129	4133	rVB3	492	652	0.06%	0.006%
98	14.639	4133	4136	4137	rBV2	360	241	0.02%	0.002%
99	14.854	4199	4203	4206	rBV2	379	356	0.03%	0.003%
100	15.558	4420	4422	4427	rBV5	581	420	0.04%	0.004%


Sum of corrected areas: 10856371

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047728.D
Acq On : 28 Mar 2022 15:30
Operator : SY/MD
Sample : N2081-14DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

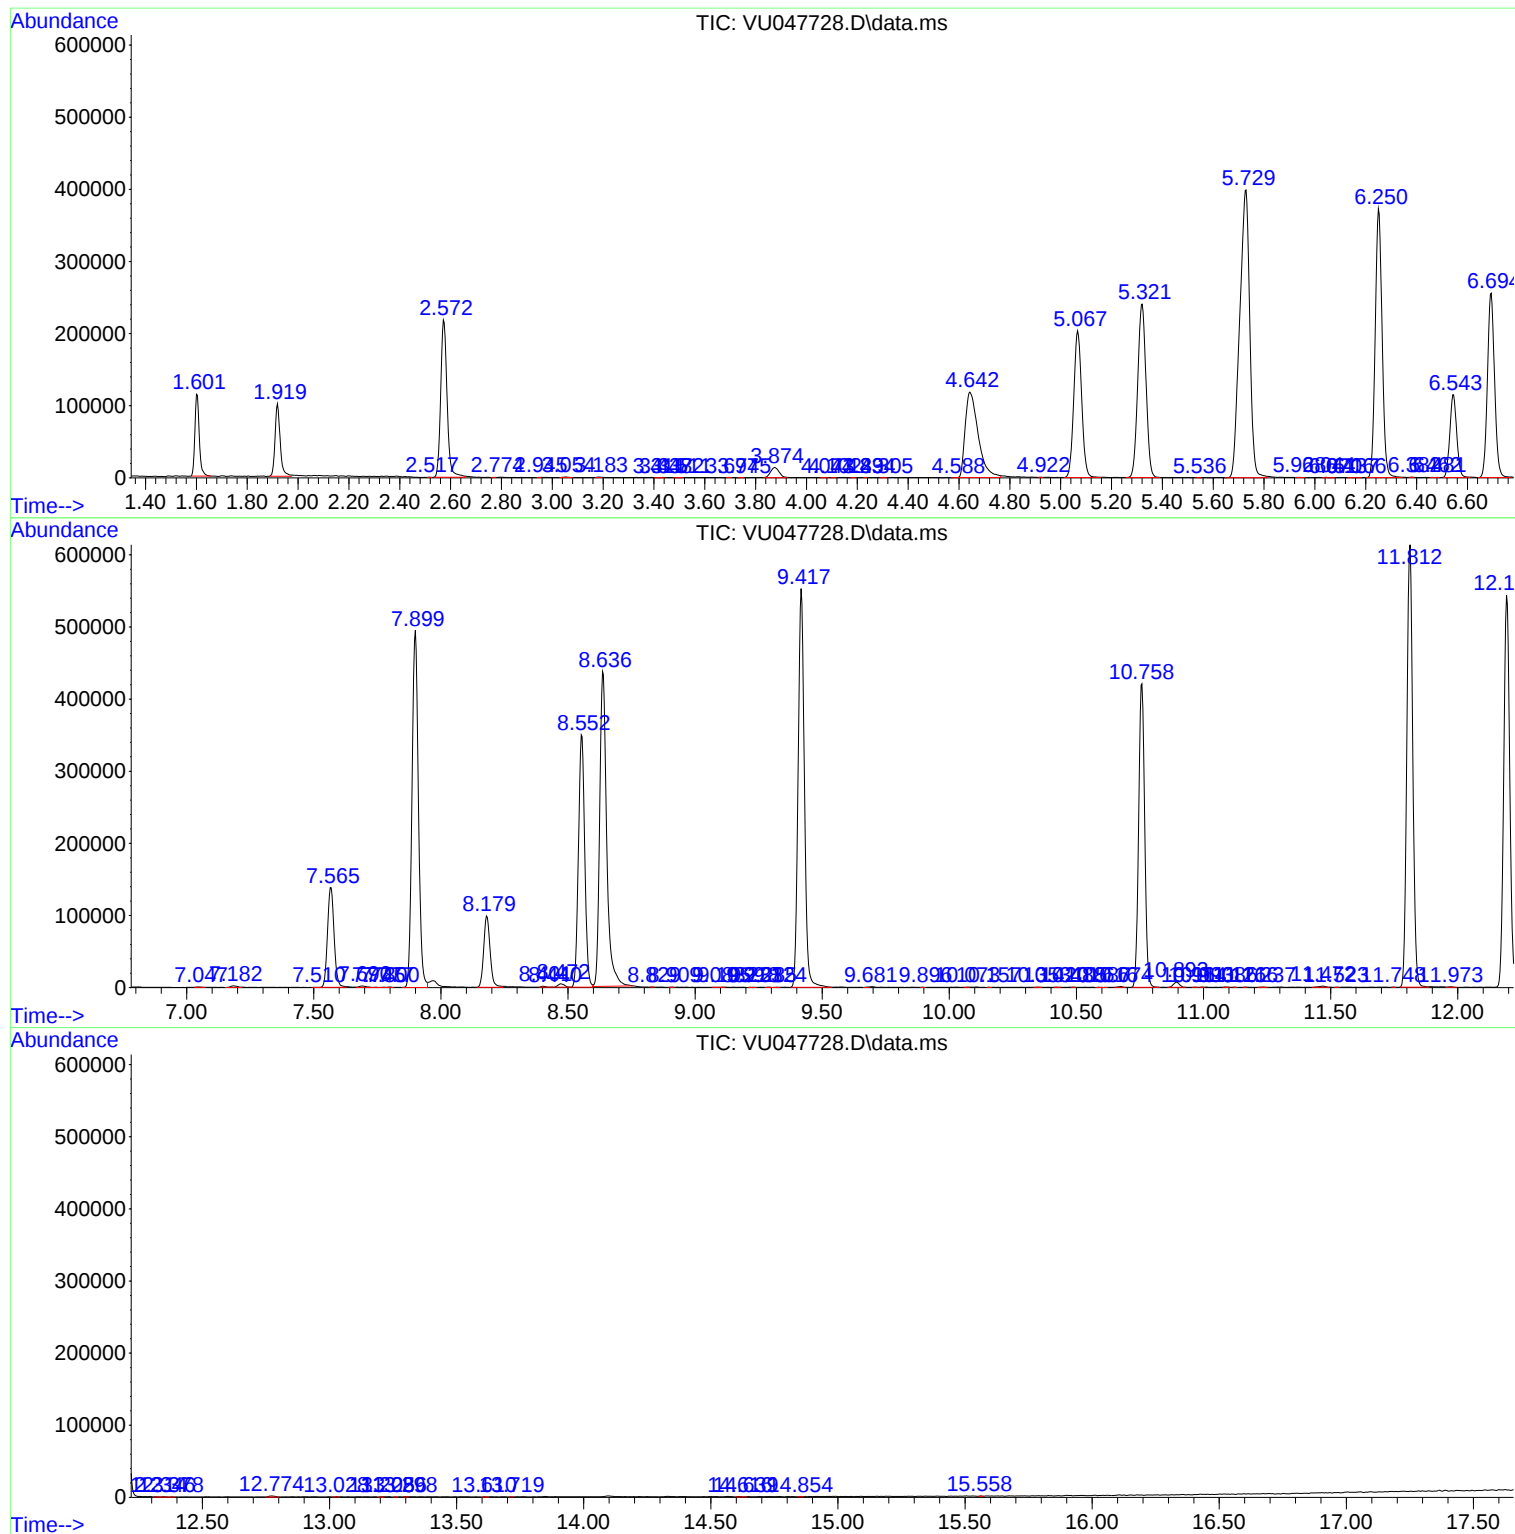

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047728.D
Acq On : 28 Mar 2022 15:30
Operator : SY/MD
Sample : N2081-14DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047728.D
Acq On : 28 Mar 2022 15:30
Operator : SY/MD
Sample : N2081-14DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------