

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047729.D
 Acq On : 28 Mar 2022 15:52
 Operator : SY/MD
 Sample : N2081-21DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rBV	114625	137767	12.30%	1.188%
2	1.919	171	180	201	rBV	100210	140634	12.55%	1.213%
3	2.578	371	385	412	rBV4	301035	599749	53.54%	5.173%
4	2.748	436	438	440	rBV	335	187	0.02%	0.002%
5	2.861	471	473	478	rVB2	357	233	0.02%	0.002%
6	2.890	478	482	486	rBV4	356	302	0.03%	0.003%
7	2.973	499	508	512	rBV4	460	875	0.08%	0.008%
8	3.054	526	533	540	rBV5	1051	1528	0.14%	0.013%
9	3.179	567	572	573	rBV	441	304	0.03%	0.003%
10	3.189	573	575	579	rVB2	537	382	0.03%	0.003%
11	3.237	588	590	595	rVB3	305	293	0.03%	0.003%
12	3.269	595	600	602	rBV2	203	212	0.02%	0.002%
13	3.362	620	629	639	rBV2	2850	5414	0.48%	0.047%
14	3.504	668	673	675	rBV	250	189	0.02%	0.002%
15	3.520	675	678	684	rVB3	270	284	0.03%	0.002%
16	3.559	686	690	691	rBV	246	162	0.01%	0.001%
17	3.594	695	701	702	rBV	357	240	0.02%	0.002%
18	3.697	730	733	735	rBV	208	171	0.02%	0.001%
19	3.761	749	753	757	rVV2	260	206	0.02%	0.002%
20	3.874	772	788	810	rBV	76532	183299	16.36%	1.581%
21	3.983	819	822	829	rBV3	222	262	0.02%	0.002%
22	4.022	832	834	839	rVB2	231	194	0.02%	0.002%
23	4.160	874	877	880	rBV3	270	202	0.02%	0.002%
24	4.189	882	886	892	rVB2	217	187	0.02%	0.002%
25	4.324	923	928	931	rBV2	349	257	0.02%	0.002%
26	4.475	969	975	980	rBV3	213	232	0.02%	0.002%
27	4.665	1011	1034	1071	rBV4	172766	648611	57.90%	5.594%
28	4.883	1100	1102	1105	rBV	272	217	0.02%	0.002%
29	4.999	1133	1138	1141	rBB3	247	251	0.02%	0.002%
30	5.067	1141	1159	1184	rBV	206609	461070	41.16%	3.977%
31	5.189	1195	1197	1200	rVB2	276	197	0.02%	0.002%
32	5.224	1202	1208	1210	rVB3	352	310	0.03%	0.003%
33	5.321	1220	1238	1259	rBV	353654	792848	70.78%	6.839%
34	5.517	1294	1299	1303	rBV4	597	694	0.06%	0.006%
35	5.729	1343	1365	1398	rVV2	412294	1120219	100.00%	9.662%
36	5.983	1442	1444	1448	rBV2	322	287	0.03%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047729.D
 Acq On : 28 Mar 2022 15:52
 Operator : SY/MD
 Sample : N2081-21DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.128	1485	1489	1495	rVB3	337	310	0.03%	0.003%
38	6.250	1512	1527	1550	rBV	376332	715184	63.84%	6.169%
39	6.542	1606	1618	1642	rBV	167937	319752	28.54%	2.758%
40	6.623	1642	1643	1647	rVB3	732	331	0.03%	0.003%
41	6.693	1647	1665	1694	rBV	261243	508959	45.43%	4.390%
42	6.796	1694	1697	1698	rBV2	451	233	0.02%	0.002%
43	6.941	1735	1742	1746	rBV2	299	455	0.04%	0.004%
44	7.060	1772	1779	1783	rBV2	348	509	0.05%	0.004%
45	7.147	1799	1806	1810	rBV3	236	273	0.02%	0.002%
46	7.185	1810	1818	1831	rVB3	2116	3582	0.32%	0.031%
47	7.301	1851	1854	1856	rBV2	288	220	0.02%	0.002%
48	7.423	1884	1892	1896	rBV2	218	296	0.03%	0.003%
49	7.452	1896	1901	1903	rBV	256	230	0.02%	0.002%
50	7.494	1910	1914	1919	rVB2	215	200	0.02%	0.002%
51	7.565	1921	1936	1958	rBV	141722	254660	22.73%	2.197%
52	7.655	1961	1964	1966	rBV2	301	173	0.02%	0.001%
53	7.761	1994	1997	2003	rVB2	322	253	0.02%	0.002%
54	7.790	2003	2006	2008	rBV2	499	345	0.03%	0.003%
55	7.803	2008	2010	2014	rVB3	340	286	0.03%	0.002%
56	7.899	2021	2040	2056	rBV	494347	872619	77.90%	7.527%
57	8.179	2115	2127	2151	rBV	102484	176444	15.75%	1.522%
58	8.353	2178	2181	2185	rVB	386	256	0.02%	0.002%
59	8.401	2189	2196	2207	rVB5	3795	6283	0.56%	0.054%
60	8.472	2208	2218	2230	rVB4	4405	8521	0.76%	0.073%
61	8.552	2231	2243	2257	rBV	136286	229532	20.49%	1.980%
62	8.636	2257	2269	2306	rVV	438057	829702	74.07%	7.156%
63	9.095	2409	2412	2414	rBV	262	180	0.02%	0.002%
64	9.137	2420	2425	2428	rBV	176	175	0.02%	0.002%
65	9.246	2456	2459	2461	rBV	250	210	0.02%	0.002%
66	9.263	2461	2464	2467	rVB2	281	215	0.02%	0.002%
67	9.320	2479	2482	2485	rVV	240	167	0.01%	0.001%
68	9.417	2499	2512	2552	rVB	567611	949675	84.78%	8.191%
69	9.555	2552	2555	2556	rBV2	343	165	0.01%	0.001%
70	9.581	2556	2563	2571	rVB2	537	900	0.08%	0.008%
71	9.697	2592	2599	2604	rBV3	998	1307	0.12%	0.011%
72	10.105	2723	2726	2728	rVV2	298	222	0.02%	0.002%
73	10.201	2752	2756	2761	rBV2	269	289	0.03%	0.002%
74	10.227	2761	2764	2772	rVB2	150	179	0.02%	0.002%
75	10.269	2773	2777	2783	rVB	302	338	0.03%	0.003%
76	10.320	2790	2793	2797	rVB	228	182	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047729.D
 Acq On : 28 Mar 2022 15:52
 Operator : SY/MD
 Sample : N2081-21DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.488	2842	2845	2850	rVB3	555	490	0.04%	0.004%
78	10.542	2859	2862	2865	rVB2	325	227	0.02%	0.002%
79	10.561	2865	2868	2871	rBV2	253	196	0.02%	0.002%
80	10.671	2894	2902	2908	rVV4	936	1396	0.12%	0.012%
81	10.758	2915	2929	2950	rBV	425086	689833	61.58%	5.950%
82	10.896	2961	2972	2981	rBV2	7117	11732	1.05%	0.101%
83	11.005	3002	3006	3009	rVB2	506	454	0.04%	0.004%
84	11.188	3060	3063	3067	rVV3	305	232	0.02%	0.002%
85	11.246	3078	3081	3085	rVB2	306	235	0.02%	0.002%
86	11.388	3123	3125	3131	rVB2	274	173	0.02%	0.001%
87	11.459	3141	3147	3148	rBV3	1171	918	0.08%	0.008%
88	11.696	3218	3221	3229	rVB3	631	590	0.05%	0.005%
89	11.751	3235	3238	3242	rVB3	377	317	0.03%	0.003%
90	11.812	3242	3257	3279	rBV	629613	1005877	89.79%	8.676%
91	11.918	3288	3290	3293	rBV3	539	384	0.03%	0.003%
92	11.996	3312	3314	3321	rVB2	230	215	0.02%	0.002%
93	12.192	3363	3375	3391	rBV	554339	892978	79.71%	7.702%
94	12.722	3536	3540	3543	rBV3	320	311	0.03%	0.003%
95	12.774	3549	3556	3565	rVV3	1817	2575	0.23%	0.022%
96	12.822	3569	3571	3575	rBV	320	246	0.02%	0.002%
97	13.227	3692	3697	3702	rBV3	548	637	0.06%	0.005%
98	13.510	3782	3785	3789	rBV3	234	190	0.02%	0.002%
99	13.841	3885	3888	3896	rVB4	764	988	0.09%	0.009%
100	14.986	4241	4244	4246	rBV	342	271	0.02%	0.002%


Sum of corrected areas: 11593746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047729.D
Acq On : 28 Mar 2022 15:52
Operator : SY/MD
Sample : N2081-21DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

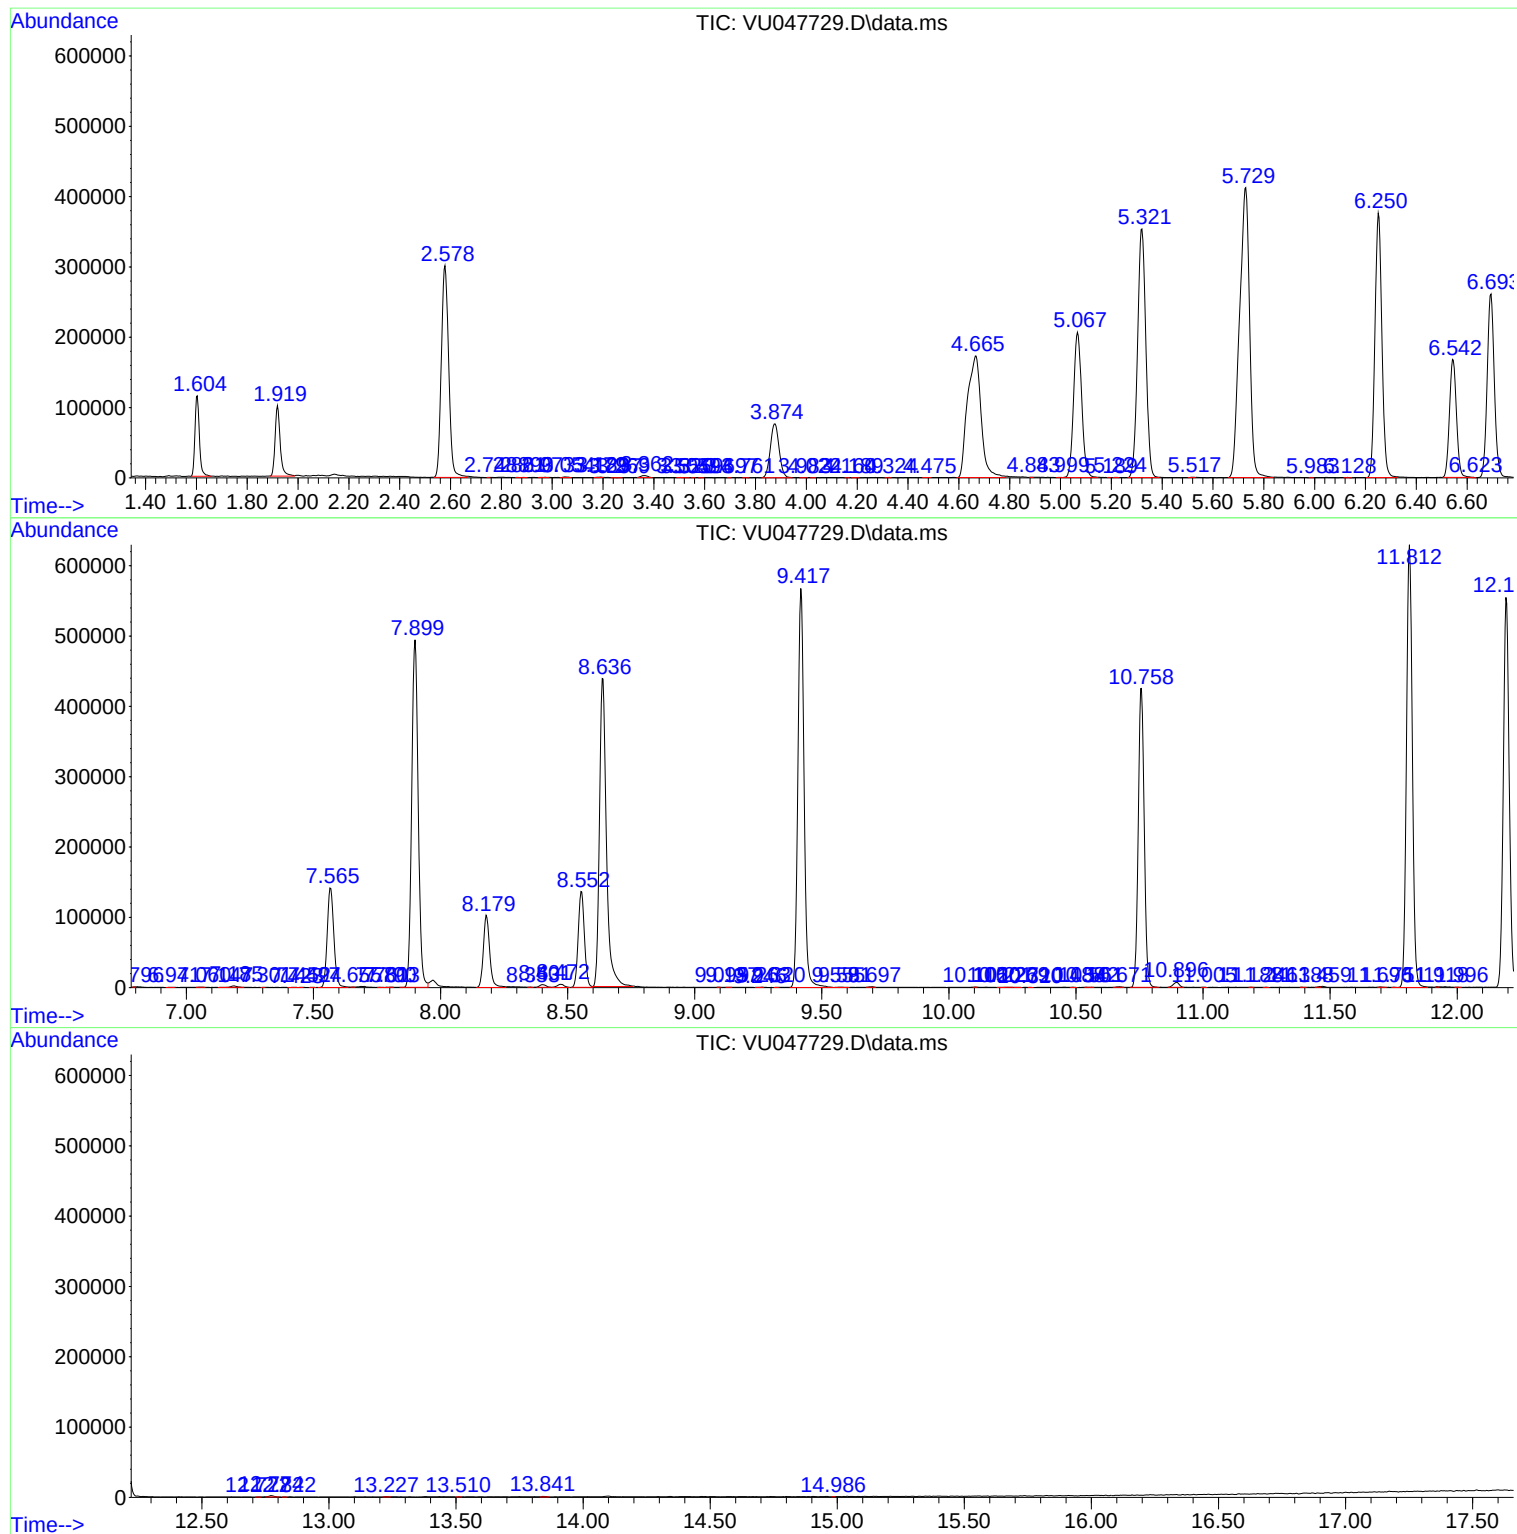

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047729.D
Acq On : 28 Mar 2022 15:52
Operator : SY/MD
Sample : N2081-21DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047729.D
Acq On : 28 Mar 2022 15:52
Operator : SY/MD
Sample : N2081-21DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------