

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047730.D
 Acq On : 28 Mar 2022 16:15
 Operator : SY/MD
 Sample : N2081-18DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047730.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rBV	118378	145779	12.70%	1.320%
2	1.919	171	180	198	rBV	100806	153794	13.40%	1.393%
3	2.485	353	356	360	rBV4	313	279	0.02%	0.003%
4	2.572	371	383	403	rBV	223131	379228	33.04%	3.434%
5	2.797	449	453	461	rVB3	523	539	0.05%	0.005%
6	2.974	505	508	513	rVB3	243	233	0.02%	0.002%
7	3.054	526	533	539	rVB3	1016	1425	0.12%	0.013%
8	3.173	567	570	572	rBV3	368	226	0.02%	0.002%
9	3.237	587	590	593	rBV	247	209	0.02%	0.002%
10	3.363	620	629	640	rVV4	2201	4299	0.37%	0.039%
11	3.443	649	654	658	rVB3	224	242	0.02%	0.002%
12	3.604	698	704	707	rBV2	281	316	0.03%	0.003%
13	3.874	772	788	809	rBV	79000	188796	16.45%	1.709%
14	3.999	822	827	829	rBV	198	189	0.02%	0.002%
15	4.067	845	848	851	rVB3	328	233	0.02%	0.002%
16	4.157	871	876	879	rBV2	278	303	0.03%	0.003%
17	4.212	890	893	901	rVV3	199	213	0.02%	0.002%
18	4.372	939	943	947	rBV2	253	243	0.02%	0.002%
19	4.446	962	966	969	rBV3	246	252	0.02%	0.002%
20	4.668	1012	1035	1063	rBV2	391743	1147829	100.00%	10.393%
21	5.067	1138	1159	1181	rBV	206720	452201	39.40%	4.094%
22	5.189	1194	1197	1199	rVB2	402	257	0.02%	0.002%
23	5.321	1218	1238	1256	rBV	126796	283879	24.73%	2.570%
24	5.398	1261	1262	1268	rVB2	396	251	0.02%	0.002%
25	5.462	1278	1282	1283	rBV	264	191	0.02%	0.002%
26	5.726	1340	1364	1396	rBV2	411775	1124084	97.93%	10.178%
27	6.047	1461	1464	1472	rVB2	591	504	0.04%	0.005%
28	6.118	1479	1486	1490	rVB3	412	622	0.05%	0.006%
29	6.250	1513	1527	1555	rBV	364982	701001	61.07%	6.347%
30	6.491	1598	1602	1605	rBV3	355	227	0.02%	0.002%
31	6.546	1609	1619	1631	rVV7	4792	9461	0.82%	0.086%
32	6.591	1631	1633	1635	rVV3	502	279	0.02%	0.003%
33	6.613	1638	1640	1644	rVB4	442	290	0.03%	0.003%
34	6.691	1647	1664	1691	rBV	256422	508517	44.30%	4.604%
35	6.797	1693	1697	1700	rBV4	501	372	0.03%	0.003%
36	6.848	1711	1713	1716	rVB2	303	190	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047730.D
 Acq On : 28 Mar 2022 16:15
 Operator : SY/MD
 Sample : N2081-18DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.880	1721	1723	1728	rVV2	278	213	0.02%	0.002%
38	7.009	1757	1763	1765	rBV	396	387	0.03%	0.004%
39	7.047	1772	1775	1782	rVB2	389	466	0.04%	0.004%
40	7.182	1810	1817	1830	rVV2	2126	3634	0.32%	0.033%
41	7.498	1910	1915	1917	rBV2	245	240	0.02%	0.002%
42	7.565	1924	1936	1966	rBV	142794	254547	22.18%	2.305%
43	7.694	1970	1976	1986	rVB5	2141	3359	0.29%	0.030%
44	7.742	1986	1991	1994	rBV2	400	374	0.03%	0.003%
45	7.797	2000	2008	2017	rBV3	1001	1455	0.13%	0.013%
46	7.900	2026	2040	2055	rBV	502852	876952	76.40%	7.940%
47	8.179	2115	2127	2142	rBV	101791	174882	15.24%	1.583%
48	8.472	2210	2218	2233	rVB3	2473	4579	0.40%	0.041%
49	8.555	2233	2244	2254	rVB4	11669	19634	1.71%	0.178%
50	8.636	2257	2269	2309	rBV	441155	851218	74.16%	7.707%
51	8.806	2320	2322	2331	rVB3	613	586	0.05%	0.005%
52	8.845	2331	2334	2336	rVB2	526	324	0.03%	0.003%
53	8.916	2353	2356	2358	rBV	360	188	0.02%	0.002%
54	9.009	2380	2385	2390	rBV2	415	454	0.04%	0.004%
55	9.044	2391	2396	2398	rBV2	243	191	0.02%	0.002%
56	9.417	2498	2512	2549	rBV	551135	927259	80.78%	8.396%
57	9.568	2552	2559	2567	rBV2	1531	1952	0.17%	0.018%
58	9.694	2590	2598	2609	rVV3	3752	5925	0.52%	0.054%
59	9.784	2623	2626	2631	rBV2	239	246	0.02%	0.002%
60	10.102	2714	2725	2739	rVV2	13696	22272	1.94%	0.202%
61	10.224	2755	2763	2765	rBV	223	279	0.02%	0.003%
62	10.298	2782	2786	2788	rBV2	290	216	0.02%	0.002%
63	10.485	2838	2844	2848	rBV3	507	657	0.06%	0.006%
64	10.671	2895	2902	2907	rVB3	1079	1090	0.09%	0.010%
65	10.703	2909	2912	2916	rVV2	222	192	0.02%	0.002%
66	10.758	2916	2929	2952	rVB	438201	705891	61.50%	6.392%
67	10.893	2964	2971	2983	rVB5	3225	5457	0.48%	0.049%
68	11.022	2995	3011	3022	rVV3	4792	11148	0.97%	0.101%
69	11.089	3022	3032	3046	rVB2	11570	18161	1.58%	0.164%
70	11.234	3071	3077	3078	rBV3	429	438	0.04%	0.004%
71	11.292	3084	3095	3105	rBV	13329	19986	1.74%	0.181%
72	11.468	3141	3150	3160	rVV2	8163	12004	1.05%	0.109%
73	11.645	3198	3205	3213	rBV3	490	723	0.06%	0.007%
74	11.700	3217	3222	3223	rBV2	485	331	0.03%	0.003%
75	11.748	3228	3237	3243	rVB5	1660	2371	0.21%	0.021%
76	11.813	3243	3257	3273	rBV	628337	1001579	87.26%	9.069%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047730.D
 Acq On : 28 Mar 2022 16:15
 Operator : SY/MD
 Sample : N2081-18DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.893	3274	3282	3294	rVB	21037	32661	2.85%	0.296%
78	12.009	3315	3318	3322	rBV3	318	333	0.03%	0.003%
79	12.095	3336	3345	3351	rBV2	7110	11061	0.96%	0.100%
80	12.192	3362	3375	3392	rBV	571652	927796	80.83%	8.401%
81	12.378	3425	3433	3441	rBV4	1826	2682	0.23%	0.024%
82	12.485	3455	3466	3478	rBV2	4489	8629	0.75%	0.078%
83	12.571	3488	3493	3504	rVB3	2715	3406	0.30%	0.031%
84	12.620	3506	3508	3513	rVV3	394	307	0.03%	0.003%
85	12.681	3522	3527	3529	rBV4	838	772	0.07%	0.007%
86	12.771	3547	3555	3563	rBV3	861	1392	0.12%	0.013%
87	12.861	3580	3583	3585	rBV2	387	262	0.02%	0.002%
88	12.912	3597	3599	3603	rBV2	322	288	0.03%	0.003%
89	12.973	3611	3618	3626	rBV3	1252	1814	0.16%	0.016%
90	13.028	3626	3635	3646	rVB3	2190	3234	0.28%	0.029%
91	13.169	3676	3679	3682	rBV3	295	234	0.02%	0.002%
92	13.221	3692	3695	3701	rVB3	438	465	0.04%	0.004%
93	13.446	3759	3765	3778	rVB6	2109	3570	0.31%	0.032%
94	13.629	3819	3822	3825	rVB2	534	379	0.03%	0.003%
95	13.841	3884	3888	3892	rBV3	872	886	0.08%	0.008%
96	14.095	3961	3967	3982	rVB2	2598	3669	0.32%	0.033%
97	14.632	4132	4134	4140	rBV2	339	236	0.02%	0.002%
98	15.128	4286	4288	4293	rBV2	430	420	0.04%	0.004%
99	15.317	4344	4347	4350	rBV2	484	404	0.04%	0.004%
100	15.372	4360	4364	4366	rBV3	541	489	0.04%	0.004%


Sum of corrected areas: 11044202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047730.D
Acq On : 28 Mar 2022 16:15
Operator : SY/MD
Sample : N2081-18DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

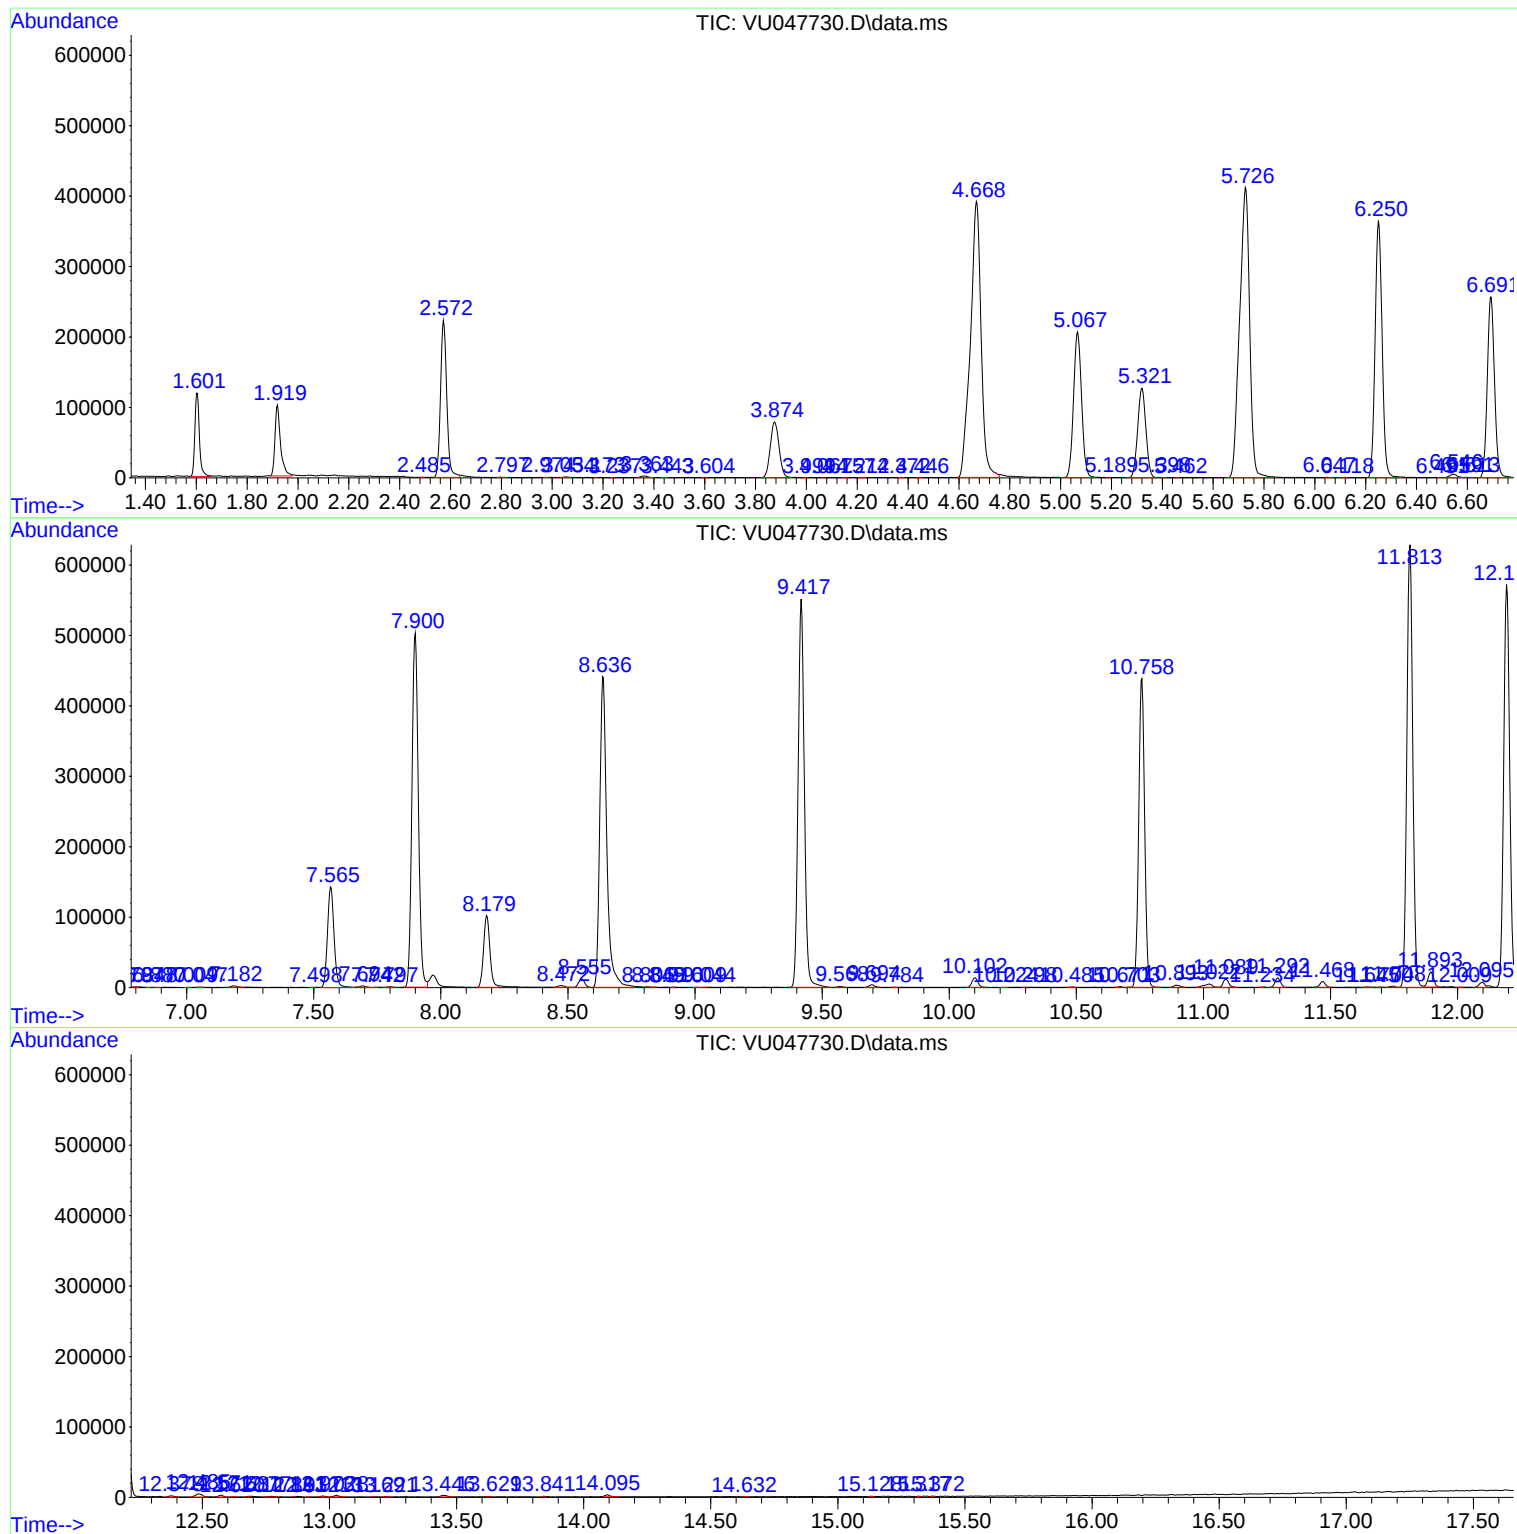

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047730.D
Acq On : 28 Mar 2022 16:15
Operator : SY/MD
Sample : N2081-18DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047730.D
Acq On : 28 Mar 2022 16:15
Operator : SY/MD
Sample : N2081-18DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------