

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047733.D
 Acq On : 28 Mar 2022 17:23
 Operator : SY/MD
 Sample : VIBLK053
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rVB	114833	136985	12.24%	1.433%
2	1.919	171	180	194	rBV	101767	140481	12.55%	1.469%
3	2.571	371	383	415	rBV	212608	371128	33.15%	3.881%
4	2.716	424	428	431	rVB2	396	308	0.03%	0.003%
5	2.745	435	437	441	rVB2	298	165	0.01%	0.002%
6	2.851	467	470	474	rVB3	236	190	0.02%	0.002%
7	2.903	481	486	488	rBV2	290	272	0.02%	0.003%
8	3.044	525	530	531	rVV	706	521	0.05%	0.005%
9	3.054	531	533	541	rVB2	934	888	0.08%	0.009%
10	3.166	565	568	572	rBV3	259	226	0.02%	0.002%
11	3.247	588	593	595	rBV3	256	222	0.02%	0.002%
12	3.462	655	660	664	rBV3	210	186	0.02%	0.002%
13	3.642	713	716	719	rBV2	219	158	0.01%	0.002%
14	3.681	723	728	730	rBV	253	186	0.02%	0.002%
15	3.880	777	790	796	rBV4	891	1778	0.16%	0.019%
16	4.012	825	831	835	rVB3	326	339	0.03%	0.004%
17	4.034	835	838	841	rBV2	230	172	0.02%	0.002%
18	4.192	884	887	892	rVB2	259	241	0.02%	0.003%
19	4.308	919	923	926	rBV3	273	210	0.02%	0.002%
20	4.359	936	939	943	rBV2	322	166	0.01%	0.002%
21	4.459	967	970	979	rVB2	223	201	0.02%	0.002%
22	4.549	996	998	1001	rVB	284	170	0.02%	0.002%
23	4.571	1001	1005	1006	rBV	289	219	0.02%	0.002%
24	4.642	1012	1027	1072	rBV	118077	398493	35.60%	4.168%
25	4.919	1111	1113	1116	rVB2	313	171	0.02%	0.002%
26	4.944	1117	1121	1124	rBV2	461	331	0.03%	0.003%
27	5.066	1142	1159	1182	rBV	207441	453667	40.52%	4.745%
28	5.211	1199	1204	1207	rBV5	365	347	0.03%	0.004%
29	5.224	1207	1208	1215	rVB2	330	259	0.02%	0.003%
30	5.320	1224	1238	1249	rBV6	3162	7360	0.66%	0.077%
31	5.591	1319	1322	1325	rBV	207	159	0.01%	0.002%
32	5.729	1342	1365	1388	rBV2	407986	1119493	100.00%	11.708%
33	5.883	1411	1413	1419	rVB2	544	412	0.04%	0.004%
34	5.938	1427	1430	1436	rVB2	192	173	0.02%	0.002%
35	6.038	1458	1461	1463	rBV	443	341	0.03%	0.004%
36	6.124	1482	1488	1492	rBV3	444	501	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047733.D
 Acq On : 28 Mar 2022 17:23
 Operator : SY/MD
 Sample : VIBLK053
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1554	rBV	365838	697696	62.32%	7.297%
38	6.417	1575	1579	1582	rVB2	261	237	0.02%	0.002%
39	6.465	1588	1594	1597	rBV3	242	266	0.02%	0.003%
40	6.536	1608	1616	1620	rBV5	1027	1540	0.14%	0.016%
41	6.693	1650	1665	1689	rBV	260387	512374	45.77%	5.358%
42	7.054	1771	1777	1779	rBV3	500	552	0.05%	0.006%
43	7.131	1793	1801	1802	rBB	30	159	0.01%	0.002%
44	7.182	1810	1817	1818	rBV3	1934	1559	0.14%	0.016%
45	7.221	1828	1829	1834	rVB2	449	200	0.02%	0.002%
46	7.565	1924	1936	1962	rVV	140849	253183	22.62%	2.648%
47	7.684	1968	1973	1984	rBV5	1529	2929	0.26%	0.031%
48	7.767	1994	1999	2001	rBV	195	161	0.01%	0.002%
49	7.796	2004	2008	2011	rBV	360	372	0.03%	0.004%
50	7.828	2015	2018	2023	rVB2	281	228	0.02%	0.002%
51	7.899	2025	2040	2056	rBV	505180	881010	78.70%	9.214%
52	8.179	2115	2127	2147	rBV	101269	175973	15.72%	1.840%
53	8.333	2172	2175	2180	rBV4	322	226	0.02%	0.002%
54	8.398	2192	2195	2199	rBV3	194	195	0.02%	0.002%
55	8.462	2213	2215	2217	rBV	328	177	0.02%	0.002%
56	8.552	2239	2243	2244	rBV3	718	532	0.05%	0.006%
57	8.635	2257	2269	2300	rBV	449845	858433	76.68%	8.978%
58	9.034	2390	2393	2397	rVB2	225	182	0.02%	0.002%
59	9.070	2402	2404	2408	rBV	282	231	0.02%	0.002%
60	9.147	2422	2428	2432	rVV3	293	310	0.03%	0.003%
61	9.201	2442	2445	2449	rVB3	267	238	0.02%	0.002%
62	9.320	2480	2482	2485	rVB	228	154	0.01%	0.002%
63	9.359	2491	2494	2497	rBV	292	168	0.02%	0.002%
64	9.417	2498	2512	2547	rVV	552118	926543	82.76%	9.690%
65	9.574	2556	2561	2565	rBV3	465	566	0.05%	0.006%
66	9.693	2591	2598	2606	rVB4	1567	2368	0.21%	0.025%
67	9.835	2640	2642	2649	rVB3	242	246	0.02%	0.003%
68	9.999	2689	2693	2696	rBV2	238	235	0.02%	0.002%
69	10.060	2709	2712	2715	rBV	221	169	0.02%	0.002%
70	10.102	2720	2725	2734	rVV4	713	1178	0.11%	0.012%
71	10.250	2767	2771	2775	rVB2	287	252	0.02%	0.003%
72	10.298	2784	2786	2790	rVB2	285	181	0.02%	0.002%
73	10.626	2884	2888	2893	rBV3	281	279	0.02%	0.003%
74	10.668	2898	2901	2908	rVB4	801	897	0.08%	0.009%
75	10.758	2916	2929	2947	rBV	433832	701318	62.65%	7.335%
76	10.873	2959	2965	2966	rBV3	474	395	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047733.D
 Acq On : 28 Mar 2022 17:23
 Operator : SY/MD
 Sample : VIBLK053
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.896	2966	2972	2978	rVV4	1332	1842	0.16%	0.019%
78	11.002	2998	3005	3010	rBV4	635	827	0.07%	0.009%
79	11.082	3026	3030	3034	rBV3	571	601	0.05%	0.006%
80	11.172	3054	3058	3060	rBV	391	246	0.02%	0.003%
81	11.278	3086	3091	3092	rBV2	241	174	0.02%	0.002%
82	11.291	3092	3095	3100	rVV2	520	470	0.04%	0.005%
83	11.468	3143	3150	3162	rVB4	3449	4928	0.44%	0.052%
84	11.529	3165	3169	3172	rVB2	291	201	0.02%	0.002%
85	11.664	3208	3211	3214	rBV	286	258	0.02%	0.003%
86	11.693	3217	3220	3223	rBV3	545	456	0.04%	0.005%
87	11.812	3244	3257	3276	rBV	609162	971983	86.82%	10.165%
88	11.976	3305	3308	3311	rVB	689	427	0.04%	0.004%
89	12.037	3322	3327	3333	rBV3	431	552	0.05%	0.006%
90	12.192	3363	3375	3392	rBV	559601	911583	81.43%	9.533%
91	12.732	3540	3543	3546	rBV2	517	499	0.04%	0.005%
92	12.777	3551	3557	3560	rVV2	603	746	0.07%	0.008%
93	12.851	3577	3580	3585	rBV	245	226	0.02%	0.002%
94	13.015	3628	3631	3632	rBV	288	169	0.02%	0.002%
95	13.204	3687	3690	3692	rBV	232	174	0.02%	0.002%
96	13.574	3803	3805	3811	rVB3	390	262	0.02%	0.003%
97	13.664	3829	3833	3837	rBV3	257	259	0.02%	0.003%
98	13.838	3884	3887	3888	rBV2	374	235	0.02%	0.002%
99	14.015	3939	3942	3948	rBV	366	372	0.03%	0.004%
100	14.095	3958	3967	3974	rBV	2108	3376	0.30%	0.035%




Sum of corrected areas: 9561897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047733.D
Acq On : 28 Mar 2022 17:23
Operator : SY/MD
Sample : VIBLK053
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK053

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

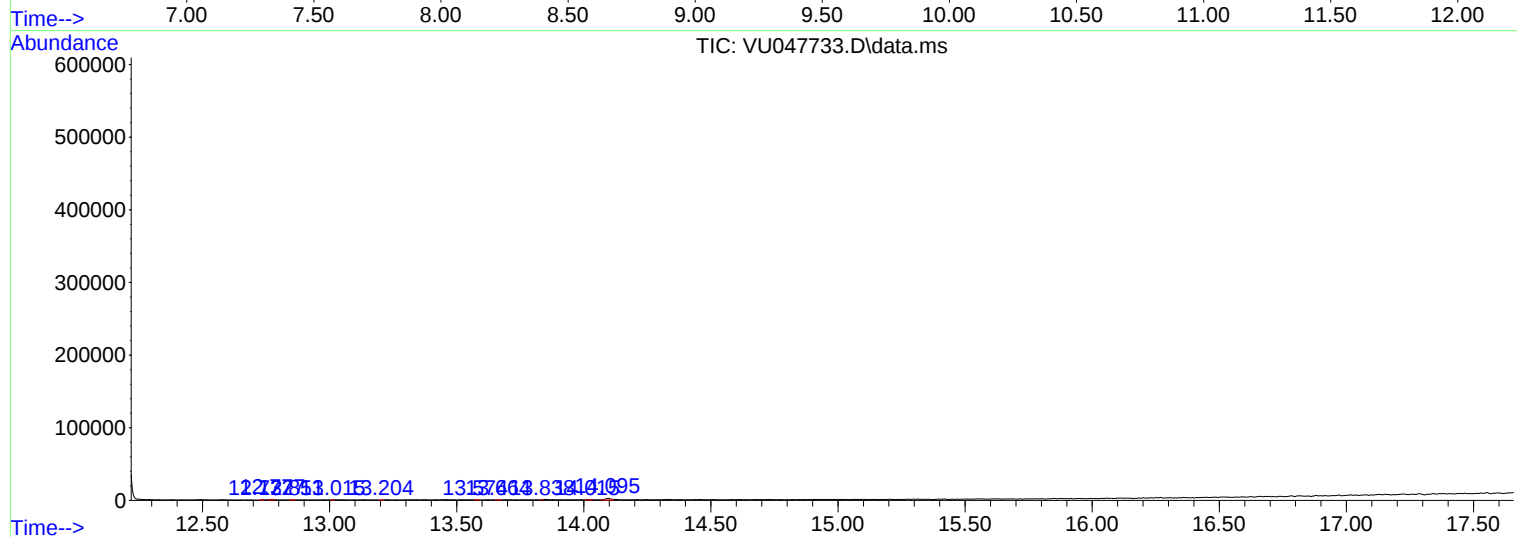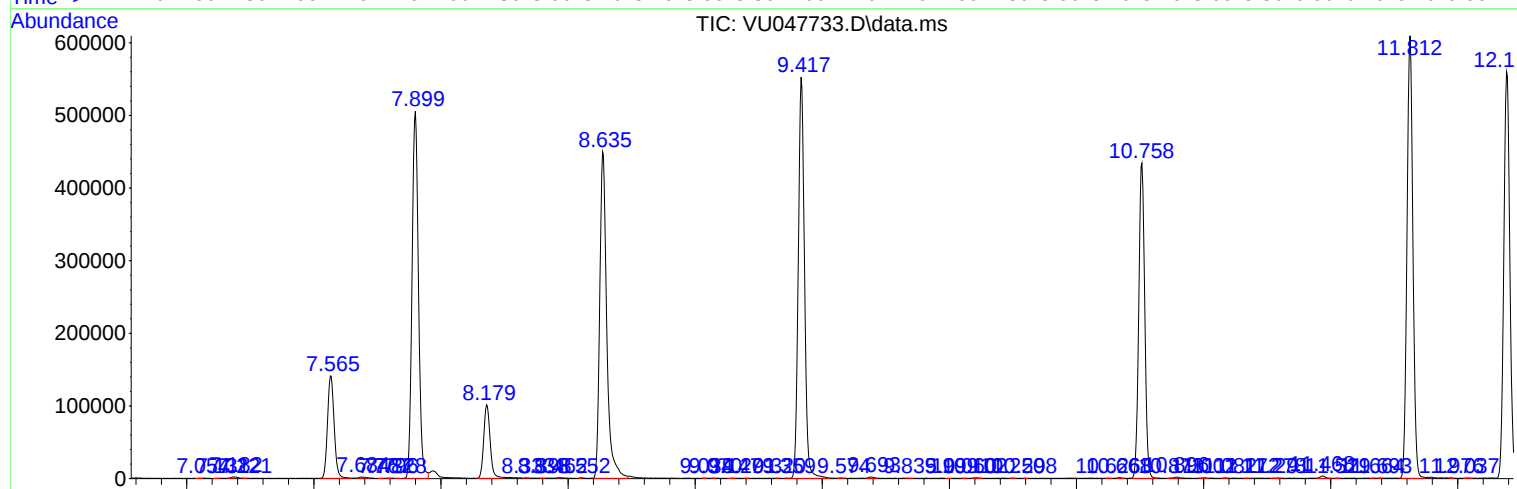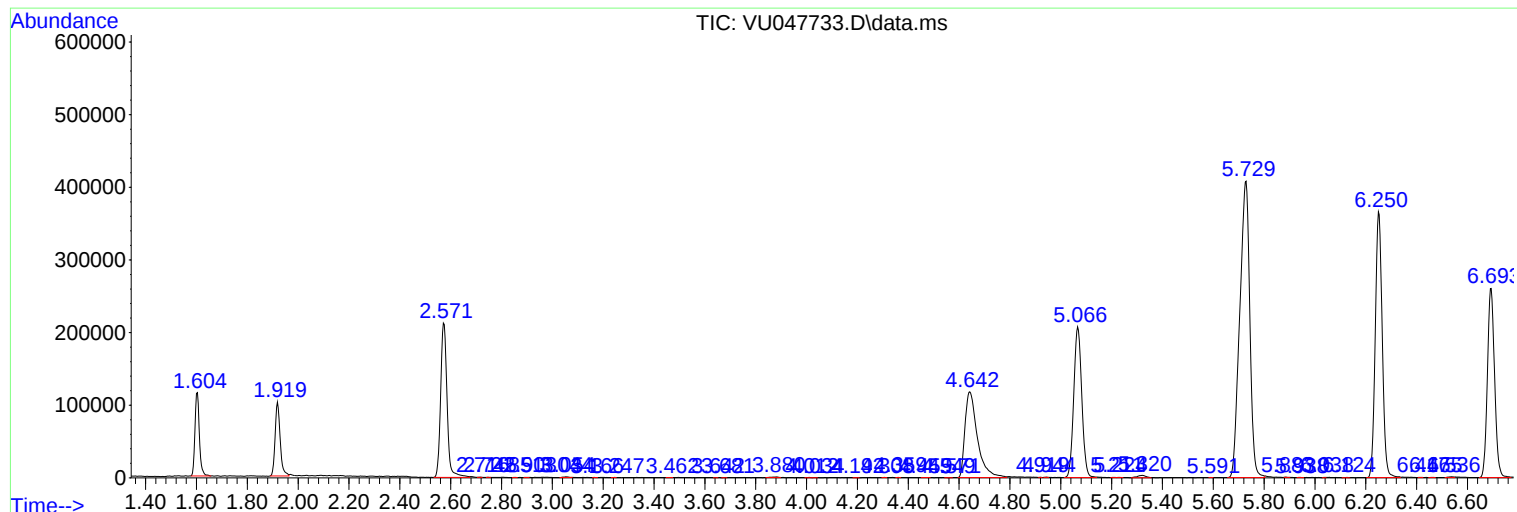

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047733.D
Acq On : 28 Mar 2022 17:23
Operator : SY/MD
Sample : VIBLK053
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK053

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047733.D
Acq On : 28 Mar 2022 17:23
Operator : SY/MD
Sample : VIBLK053
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK053

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------