

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047734.D
 Acq On : 28 Mar 2022 17:45
 Operator : SY/MD
 Sample : N2081-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rVB	115934	133445	12.20%	1.188%
2	1.694	105	110	129	rVB	5083	8953	0.82%	0.080%
3	1.919	171	180	205	rBV	98961	137853	12.60%	1.227%
4	2.575	370	384	401	rBV2	219124	389383	35.59%	3.465%
5	2.877	471	478	482	rBV3	537	669	0.06%	0.006%
6	2.903	483	486	488	rBV3	442	291	0.03%	0.003%
7	3.189	566	575	586	rVV4	1519	3086	0.28%	0.027%
8	3.311	612	613	616	rVV	326	210	0.02%	0.002%
9	3.366	619	630	638	rVB4	3294	5824	0.53%	0.052%
10	3.485	660	667	671	rBV2	382	483	0.04%	0.004%
11	3.510	671	675	678	rBV2	243	222	0.02%	0.002%
12	3.568	688	693	694	rBV2	333	222	0.02%	0.002%
13	3.623	708	710	712	rBV2	300	194	0.02%	0.002%
14	3.877	771	789	816	rVB	88204	209071	19.11%	1.861%
15	3.970	816	818	821	rBV	302	204	0.02%	0.002%
16	4.015	828	832	836	rBV2	263	209	0.02%	0.002%
17	4.452	964	968	970	rBV2	320	230	0.02%	0.002%
18	4.485	975	978	983	rVB2	461	330	0.03%	0.003%
19	4.661	1012	1033	1063	rBV2	154408	626186	57.24%	5.573%
20	5.067	1143	1159	1187	rBV	202572	450784	41.20%	4.012%
21	5.321	1216	1238	1261	rBV	433778	982558	89.81%	8.744%
22	5.497	1289	1293	1296	rBV	311	244	0.02%	0.002%
23	5.542	1305	1307	1311	rVB2	302	201	0.02%	0.002%
24	5.729	1343	1365	1394	rBV2	402244	1094007	100.00%	9.736%
25	5.915	1421	1423	1426	rBV3	252	174	0.02%	0.002%
26	6.105	1479	1482	1484	rBV2	217	165	0.02%	0.001%
27	6.166	1498	1501	1505	rBV	358	271	0.02%	0.002%
28	6.250	1513	1527	1555	rBV	363891	687892	62.88%	6.122%
29	6.391	1569	1571	1574	rVB2	387	221	0.02%	0.002%
30	6.410	1574	1577	1582	rVV2	216	165	0.02%	0.001%
31	6.546	1607	1619	1634	rVV2	29454	56583	5.17%	0.504%
32	6.693	1650	1665	1685	rBV	254040	498896	45.60%	4.440%
33	6.777	1687	1691	1695	rBV4	974	1026	0.09%	0.009%
34	6.893	1725	1727	1731	rVB2	317	193	0.02%	0.002%
35	7.009	1759	1763	1768	rBV3	340	330	0.03%	0.003%
36	7.041	1770	1773	1776	rBV2	251	229	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047734.D
 Acq On : 28 Mar 2022 17:45
 Operator : SY/MD
 Sample : N2081-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.086	1785	1787	1791	rVB	283	173	0.02%	0.002%
38	7.128	1796	1800	1810	rVB3	784	1048	0.10%	0.009%
39	7.185	1810	1818	1828	rBV2	2216	4035	0.37%	0.036%
40	7.423	1883	1892	1895	rBV3	358	507	0.05%	0.005%
41	7.446	1895	1899	1903	rVB2	320	294	0.03%	0.003%
42	7.568	1921	1937	1954	rBV	139650	248766	22.74%	2.214%
43	7.687	1969	1974	1983	rVB6	1576	2419	0.22%	0.022%
44	7.748	1989	1993	1998	rBV2	315	234	0.02%	0.002%
45	7.783	2002	2004	2005	rBV	345	173	0.02%	0.002%
46	7.796	2005	2008	2019	rVB2	494	660	0.06%	0.006%
47	7.899	2025	2040	2056	rBV	493691	858065	78.43%	7.636%
48	8.134	2109	2113	2115	rBV2	348	238	0.02%	0.002%
49	8.179	2115	2127	2146	rBV	102490	178890	16.35%	1.592%
50	8.330	2171	2174	2179	rVB3	487	403	0.04%	0.004%
51	8.401	2191	2196	2204	rVB5	920	1105	0.10%	0.010%
52	8.472	2206	2218	2230	rVB3	5241	9577	0.88%	0.085%
53	8.555	2232	2244	2257	rBV2	88283	149221	13.64%	1.328%
54	8.635	2257	2269	2316	rVB	497175	942575	86.16%	8.388%
55	8.922	2355	2358	2362	rVB3	360	306	0.03%	0.003%
56	8.944	2362	2365	2371	rBV3	230	326	0.03%	0.003%
57	9.095	2409	2412	2417	rBV3	189	175	0.02%	0.002%
58	9.121	2417	2420	2426	rVV3	287	294	0.03%	0.003%
59	9.291	2469	2473	2482	rBV5	793	857	0.08%	0.008%
60	9.417	2493	2512	2547	rBV	542877	911473	83.32%	8.112%
61	9.571	2557	2560	2569	rVB4	614	712	0.07%	0.006%
62	9.619	2569	2575	2578	rVB3	370	301	0.03%	0.003%
63	9.700	2591	2600	2604	rBV3	1366	1845	0.17%	0.016%
64	9.719	2604	2606	2608	rVB	447	198	0.02%	0.002%
65	9.767	2619	2621	2624	rBV	352	199	0.02%	0.002%
66	9.835	2639	2642	2647	rVB2	324	253	0.02%	0.002%
67	9.861	2647	2650	2653	rBV2	305	234	0.02%	0.002%
68	10.092	2719	2722	2724	rBV2	455	352	0.03%	0.003%
69	10.140	2734	2737	2739	rBV	252	174	0.02%	0.002%
70	10.372	2805	2809	2813	rBV	266	174	0.02%	0.002%
71	10.433	2825	2828	2831	rBV2	228	187	0.02%	0.002%
72	10.520	2851	2855	2857	rBV2	251	175	0.02%	0.002%
73	10.642	2888	2893	2896	rVV4	1014	943	0.09%	0.008%
74	10.671	2896	2902	2912	rVB3	1506	2149	0.20%	0.019%
75	10.758	2913	2929	2950	rVB	439370	712409	65.12%	6.340%
76	10.893	2961	2971	2986	rBV2	8417	14651	1.34%	0.130%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047734.D
 Acq On : 28 Mar 2022 17:45
 Operator : SY/MD
 Sample : N2081-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.079	3026	3029	3037	rVB4	641	731	0.07%	0.007%
78	11.166	3048	3056	3058	rBV4	1252	1499	0.14%	0.013%
79	11.346	3110	3112	3116	rVB2	248	171	0.02%	0.002%
80	11.397	3125	3128	3132	rBV	202	227	0.02%	0.002%
81	11.471	3138	3151	3157	rBV8	1817	3103	0.28%	0.028%
82	11.687	3213	3218	3219	rBV2	529	331	0.03%	0.003%
83	11.812	3244	3257	3275	rBV	611985	971939	88.84%	8.650%
84	11.938	3292	3296	3301	rBV5	1114	1076	0.10%	0.010%
85	11.963	3301	3304	3314	rVB6	1252	1601	0.15%	0.014%
86	12.057	3330	3333	3339	rBV4	402	454	0.04%	0.004%
87	12.192	3361	3375	3399	rBV	549735	907672	82.97%	8.078%
88	12.278	3399	3402	3408	rVB6	997	1032	0.09%	0.009%
89	12.436	3448	3451	3455	rVB3	236	232	0.02%	0.002%
90	12.584	3494	3497	3499	rBV2	216	176	0.02%	0.002%
91	12.706	3531	3535	3538	rBV2	227	173	0.02%	0.002%
92	12.725	3538	3541	3546	rVV3	252	237	0.02%	0.002%
93	12.774	3546	3556	3565	rVV2	4024	6118	0.56%	0.054%
94	12.844	3575	3578	3582	rBV2	203	192	0.02%	0.002%
95	12.941	3605	3608	3611	rVB	397	268	0.02%	0.002%
96	12.957	3611	3613	3617	rBV3	199	174	0.02%	0.002%
97	13.214	3691	3693	3695	rBV3	275	169	0.02%	0.002%
98	13.851	3888	3891	3896	rVB4	413	265	0.02%	0.002%
99	14.053	3950	3954	3958	rBV2	397	402	0.04%	0.004%
100	15.513	4405	4408	4410	rBV	709	513	0.05%	0.005%




Sum of corrected areas: 11236529

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047734.D
Acq On : 28 Mar 2022 17:45
Operator : SY/MD
Sample : N2081-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

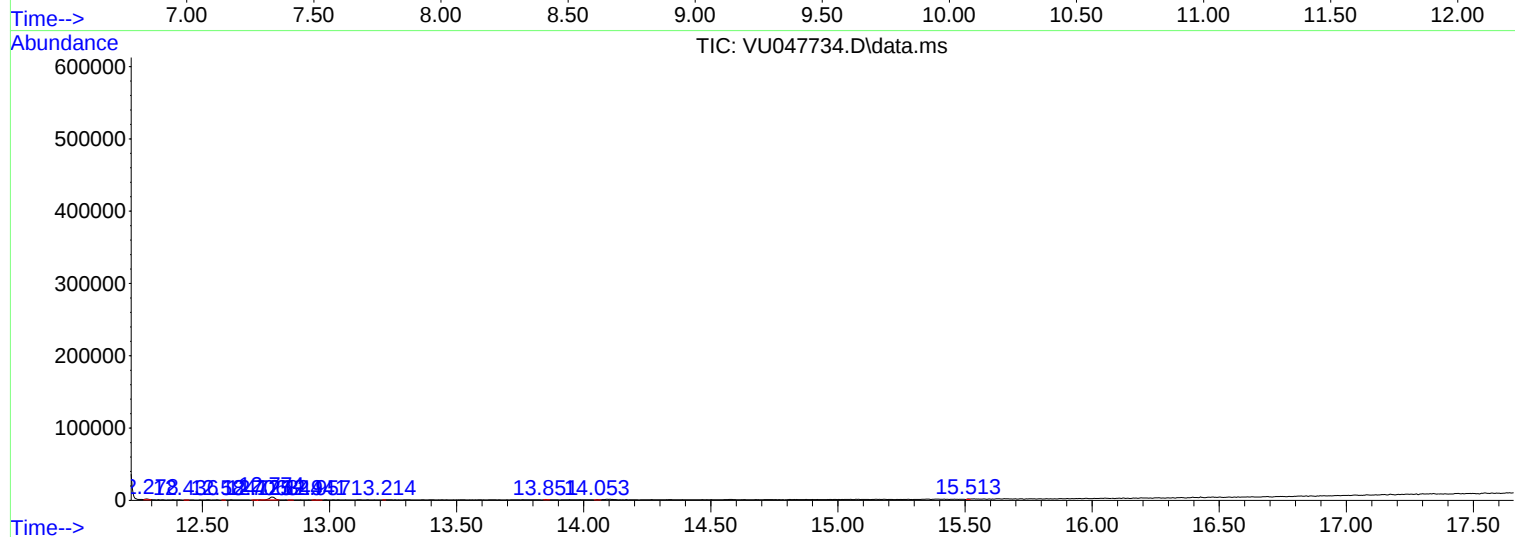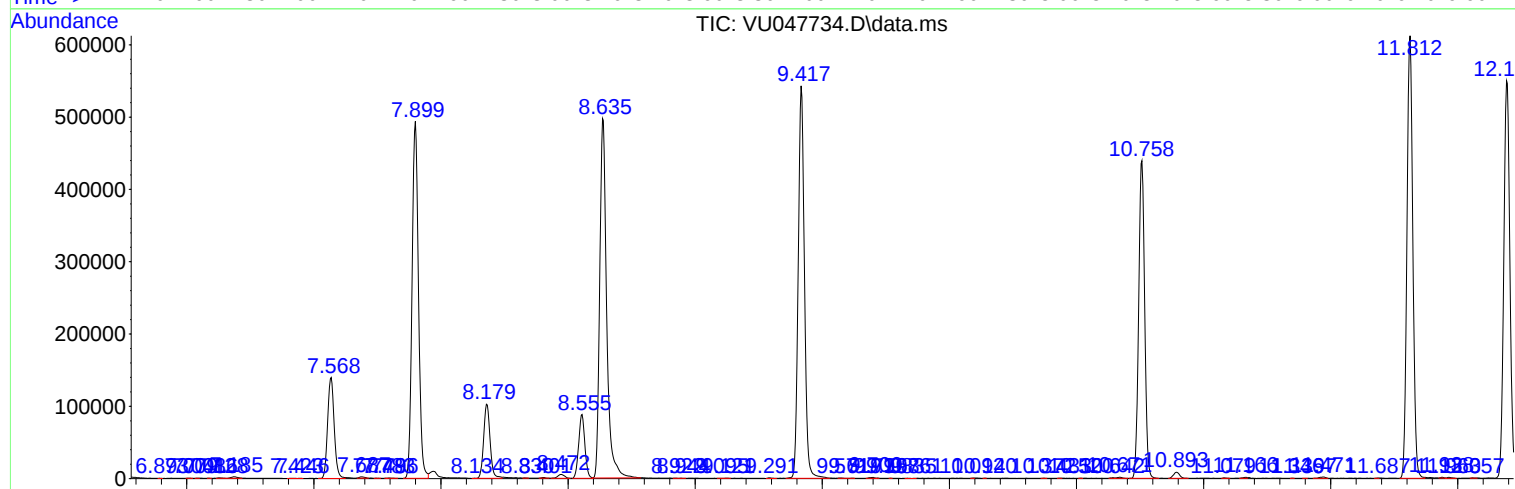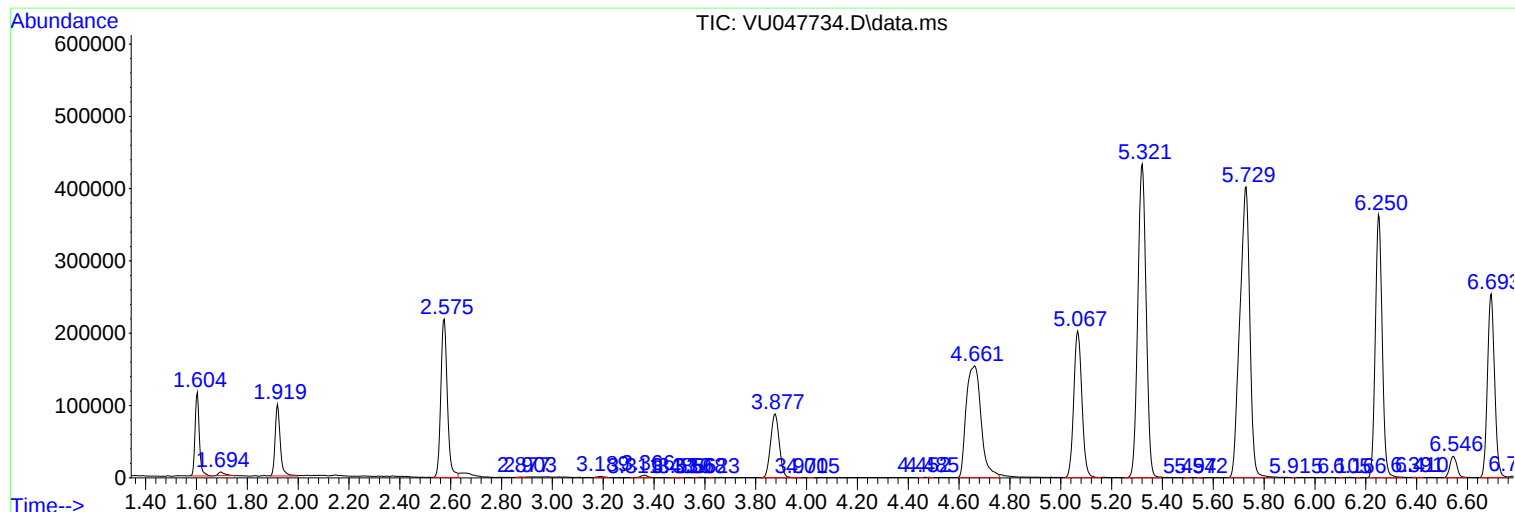

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047734.D
Acq On : 28 Mar 2022 17:45
Operator : SY/MD
Sample : N2081-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047734.D
Acq On : 28 Mar 2022 17:45
Operator : SY/MD
Sample : N2081-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------