

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047736.D
 Acq On : 28 Mar 2022 18:30
 Operator : SY/MD
 Sample : N2081-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rVB	127651	150445	3.76%	0.857%
2	1.919	170	180	202	rBV	113497	160464	4.01%	0.914%
3	2.147	244	251	258	rBV2	4024	5925	0.15%	0.034%
4	2.575	370	384	407	rBV3	254272	473707	11.83%	2.697%
5	2.710	424	426	433	rVB3	386	269	0.01%	0.002%
6	2.790	447	451	454	rBV4	410	397	0.01%	0.002%
7	2.883	477	480	483	rBV2	338	261	0.01%	0.001%
8	3.051	526	532	533	rBV2	616	689	0.02%	0.004%
9	3.186	567	574	576	rBV3	756	885	0.02%	0.005%
10	3.269	595	600	605	rBV	327	490	0.01%	0.003%
11	3.359	616	628	643	rBV2	19851	40149	1.00%	0.229%
12	3.475	660	664	666	rBV	431	335	0.01%	0.002%
13	3.523	674	679	682	rVB3	391	403	0.01%	0.002%
14	3.559	687	690	694	rVV2	275	258	0.01%	0.001%
15	3.604	701	704	708	rBV2	206	198	0.00%	0.001%
16	3.874	762	788	817	rBV	309341	743257	18.56%	4.232%
17	4.009	827	830	833	rVB2	377	220	0.01%	0.001%
18	4.044	838	841	844	rVB3	465	343	0.01%	0.002%
19	4.067	844	848	852	rBV3	441	450	0.01%	0.003%
20	4.305	917	922	925	rVB3	391	357	0.01%	0.002%
21	4.465	968	972	976	rBV2	297	228	0.01%	0.001%
22	4.671	1011	1036	1070	rBV2	1060591	2717369	67.85%	15.473%
23	5.006	1134	1140	1143	rBV4	443	484	0.01%	0.003%
24	5.067	1143	1159	1189	rVB	225951	499721	12.48%	2.845%
25	5.192	1196	1198	1200	rBV2	491	219	0.01%	0.001%
26	5.205	1200	1202	1207	rVB2	324	197	0.00%	0.001%
27	5.227	1207	1209	1212	rVB2	592	284	0.01%	0.002%
28	5.321	1218	1238	1261	rBV	1784764	4005226	100.00%	22.806%
29	5.729	1343	1365	1404	rBV2	440233	1215488	30.35%	6.921%
30	5.877	1408	1411	1414	rBV3	309	229	0.01%	0.001%
31	6.054	1460	1466	1469	rBV3	495	434	0.01%	0.002%
32	6.105	1476	1482	1483	rBV4	611	549	0.01%	0.003%
33	6.250	1511	1527	1555	rBV	362851	688105	17.18%	3.918%
34	6.546	1607	1619	1636	rBV2	44003	84769	2.12%	0.483%
35	6.623	1640	1643	1646	rVB	465	246	0.01%	0.001%
36	6.694	1650	1665	1687	rBV	276543	544143	13.59%	3.098%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047736.D
 Acq On : 28 Mar 2022 18:30
 Operator : SY/MD
 Sample : N2081-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.796	1695	1697	1698	rBV2	563	294	0.01%	0.002%
38	6.864	1714	1718	1721	rVB	241	205	0.01%	0.001%
39	6.976	1748	1753	1761	rBV3	434	680	0.02%	0.004%
40	7.044	1770	1774	1777	rBV2	438	469	0.01%	0.003%
41	7.108	1790	1794	1797	rBV2	325	242	0.01%	0.001%
42	7.185	1811	1818	1832	rVB3	2619	4351	0.11%	0.025%
43	7.247	1834	1837	1843	rVB2	219	213	0.01%	0.001%
44	7.282	1843	1848	1850	rBV	219	224	0.01%	0.001%
45	7.414	1886	1889	1893	rBV2	193	198	0.00%	0.001%
46	7.568	1923	1937	1960	rBV	141530	254802	6.36%	1.451%
47	7.693	1966	1976	1982	rBV6	1744	2915	0.07%	0.017%
48	7.739	1987	1990	1993	rVB3	460	275	0.01%	0.002%
49	7.764	1994	1998	2001	rBV2	284	257	0.01%	0.001%
50	7.841	2018	2022	2026	rBV3	352	331	0.01%	0.002%
51	7.899	2026	2040	2056	rBV	539679	941377	23.50%	5.360%
52	8.179	2112	2127	2150	rBV	116409	214982	5.37%	1.224%
53	8.401	2189	2196	2205	rVB5	2772	4548	0.11%	0.026%
54	8.472	2205	2218	2232	rBV2	7232	14148	0.35%	0.081%
55	8.555	2232	2244	2257	rBV	116146	197658	4.94%	1.125%
56	8.636	2257	2269	2306	rBV	485076	915671	22.86%	5.214%
57	8.809	2321	2323	2327	rVB3	572	391	0.01%	0.002%
58	8.828	2327	2329	2332	rBV2	499	300	0.01%	0.002%
59	8.951	2364	2367	2371	rBV2	380	308	0.01%	0.002%
60	9.018	2383	2388	2391	rVB4	305	241	0.01%	0.001%
61	9.089	2407	2410	2414	rBV2	275	290	0.01%	0.002%
62	9.166	2428	2434	2436	rBV	280	283	0.01%	0.002%
63	9.208	2442	2447	2450	rBV2	379	411	0.01%	0.002%
64	9.256	2458	2462	2464	rVB2	345	270	0.01%	0.002%
65	9.275	2464	2468	2471	rBV2	425	418	0.01%	0.002%
66	9.333	2479	2486	2488	rBV2	504	464	0.01%	0.003%
67	9.417	2499	2512	2547	rBV	528386	900977	22.50%	5.130%
68	9.693	2591	2598	2605	rBV3	1205	1670	0.04%	0.010%
69	10.041	2702	2706	2709	rBV	367	300	0.01%	0.002%
70	10.092	2719	2722	2724	rBV2	367	256	0.01%	0.001%
71	10.137	2733	2736	2744	rVB2	219	209	0.01%	0.001%
72	10.391	2811	2815	2822	rBV	236	198	0.00%	0.001%
73	10.455	2832	2835	2838	rVB2	304	206	0.01%	0.001%
74	10.497	2845	2848	2852	rVB3	448	329	0.01%	0.002%
75	10.632	2888	2890	2897	rVB2	376	300	0.01%	0.002%
76	10.671	2897	2902	2909	rBV3	1145	1288	0.03%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047736.D
 Acq On : 28 Mar 2022 18:30
 Operator : SY/MD
 Sample : N2081-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.758	2916	2929	2948	rBV	476511	767838	19.17%	4.372%
78	10.893	2961	2971	2984	rVB2	15530	25672	0.64%	0.146%
79	10.951	2984	2989	2991	rBV3	201	234	0.01%	0.001%
80	10.996	3000	3003	3007	rBV3	357	278	0.01%	0.002%
81	11.089	3027	3032	3036	rBV4	495	497	0.01%	0.003%
82	11.272	3085	3089	3091	rBV2	407	263	0.01%	0.001%
83	11.291	3091	3095	3097	rBV	310	230	0.01%	0.001%
84	11.423	3133	3136	3141	rVB	361	302	0.01%	0.002%
85	11.471	3141	3151	3161	rBV5	1677	2955	0.07%	0.017%
86	11.693	3217	3220	3223	rBV3	594	359	0.01%	0.002%
87	11.742	3232	3235	3244	rVB4	473	419	0.01%	0.002%
88	11.812	3244	3257	3277	rBV	600630	965578	24.11%	5.498%
89	11.944	3294	3298	3301	rVB3	681	573	0.01%	0.003%
90	11.976	3303	3308	3314	rVB4	820	808	0.02%	0.005%
91	12.095	3339	3345	3352	rVV6	3667	4207	0.11%	0.024%
92	12.192	3362	3375	3394	rBV	607329	983234	24.55%	5.599%
93	12.520	3474	3477	3481	rVB2	541	390	0.01%	0.002%
94	12.568	3490	3492	3497	rVV3	363	316	0.01%	0.002%
95	12.774	3547	3556	3564	rVB2	3963	5581	0.14%	0.032%
96	12.860	3579	3583	3586	rBV3	348	356	0.01%	0.002%
97	13.838	3885	3887	3889	rBV3	358	200	0.00%	0.001%
98	13.873	3895	3898	3902	rBV	368	241	0.01%	0.001%
99	14.089	3958	3965	3966	rBV3	1443	1134	0.03%	0.006%
100	14.343	4038	4044	4047	rBV4	571	646	0.02%	0.004%




Sum of corrected areas: 17562453

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047736.D
Acq On : 28 Mar 2022 18:30
Operator : SY/MD
Sample : N2081-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

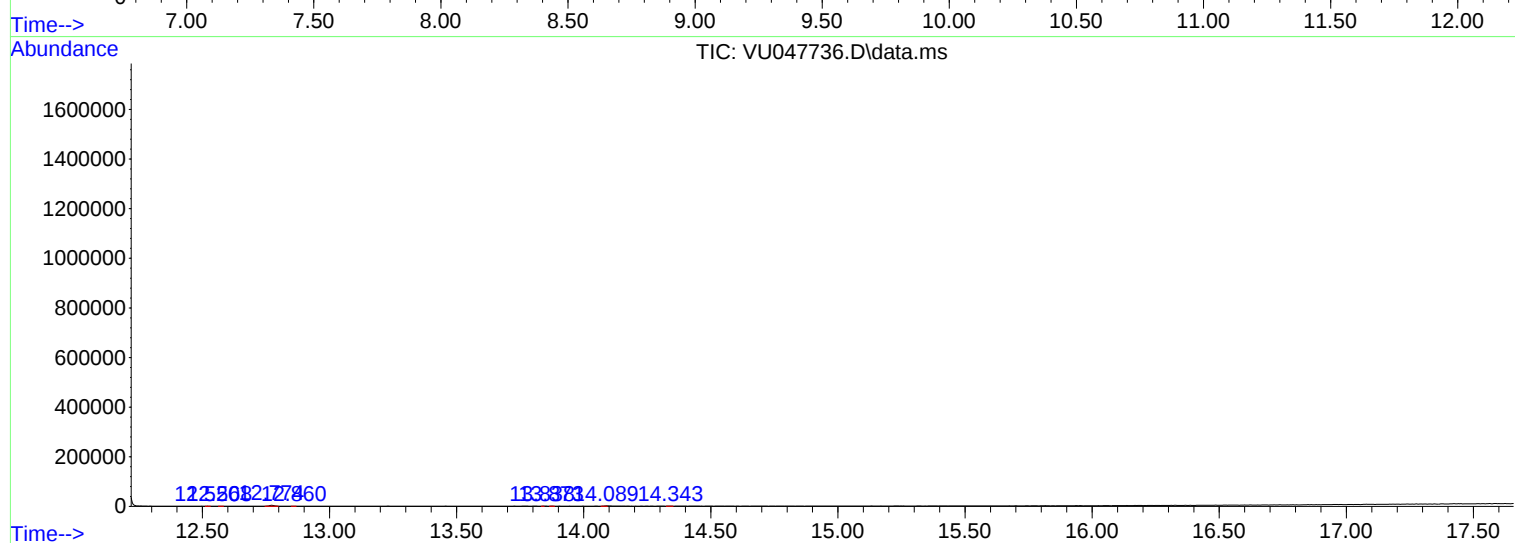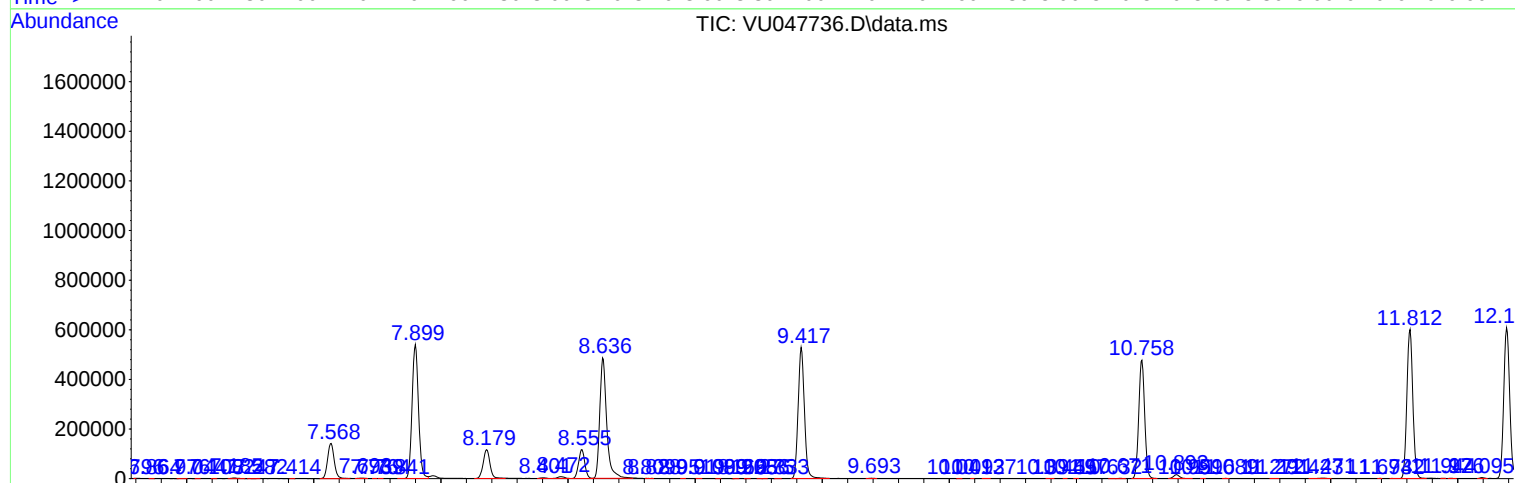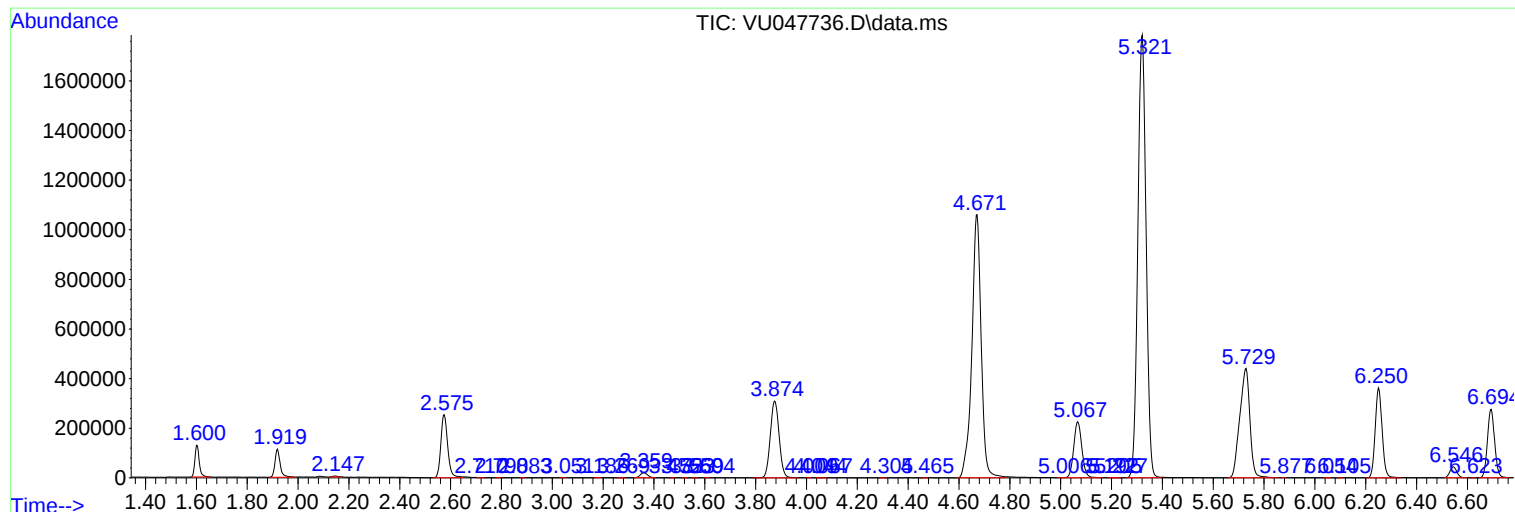

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047736.D
Acq On : 28 Mar 2022 18:30
Operator : SY/MD
Sample : N2081-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047736.D
Acq On : 28 Mar 2022 18:30
Operator : SY/MD
Sample : N2081-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------