

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047737.D
 Acq On : 28 Mar 2022 18:53
 Operator : SY/MD
 Sample : VIBLK054
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047737.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rBV	129524	153643	12.87%	1.543%
2	1.919	171	180	196	rBV	112003	155603	13.04%	1.562%
3	2.572	371	383	408	rBV	229097	388245	32.53%	3.899%
4	2.903	483	486	490	rBV3	305	275	0.02%	0.003%
5	3.054	526	533	540	rVV4	1312	2146	0.18%	0.022%
6	3.118	549	553	557	rBV3	282	269	0.02%	0.003%
7	3.202	573	579	580	rBV2	330	263	0.02%	0.003%
8	3.392	636	638	644	rVB3	429	374	0.03%	0.004%
9	3.427	645	649	652	rBV3	233	193	0.02%	0.002%
10	3.584	695	698	703	rVB	199	170	0.01%	0.002%
11	3.633	708	713	717	rBV2	230	271	0.02%	0.003%
12	3.700	729	734	737	rBV2	294	229	0.02%	0.002%
13	3.851	777	781	784	rBV2	210	244	0.02%	0.002%
14	3.977	813	820	824	rBV3	205	287	0.02%	0.003%
15	4.015	828	832	835	rBV3	209	218	0.02%	0.002%
16	4.067	845	848	854	rBV3	335	254	0.02%	0.003%
17	4.308	920	923	927	rVB2	212	182	0.02%	0.002%
18	4.356	935	938	940	rBV	263	181	0.02%	0.002%
19	4.427	955	960	963	rBV2	260	191	0.02%	0.002%
20	4.485	977	978	983	rVB	307	183	0.02%	0.002%
21	4.527	987	991	995	rBV2	309	284	0.02%	0.003%
22	4.642	1011	1027	1070	rBV	125938	425092	35.62%	4.269%
23	4.916	1110	1112	1114	rBV	232	161	0.01%	0.002%
24	5.067	1143	1159	1180	rBV	217970	479627	40.19%	4.816%
25	5.205	1198	1202	1203	rBV2	354	237	0.02%	0.002%
26	5.314	1226	1236	1237	rBV3	1598	2241	0.19%	0.023%
27	5.411	1262	1266	1271	rVB3	327	264	0.02%	0.003%
28	5.729	1342	1365	1402	rBV2	431670	1193463	100.00%	11.984%
29	5.871	1406	1409	1412	rBV	277	204	0.02%	0.002%
30	6.002	1446	1450	1453	rBV2	247	263	0.02%	0.003%
31	6.044	1457	1463	1468	rVB3	467	510	0.04%	0.005%
32	6.105	1477	1482	1483	rBV3	253	185	0.02%	0.002%
33	6.250	1512	1527	1555	rBV	400145	758300	63.54%	7.614%
34	6.388	1568	1570	1573	rBV	298	178	0.01%	0.002%
35	6.465	1589	1594	1597	rBV2	189	177	0.01%	0.002%
36	6.530	1609	1614	1615	rBV2	967	761	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047737.D
 Acq On : 28 Mar 2022 18:53
 Operator : SY/MD
 Sample : VIBLK054
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.594	1632	1634	1640	rVB4	480	399	0.03%	0.004%
38	6.690	1650	1664	1686	rBV	257224	501477	42.02%	5.036%
39	6.948	1739	1744	1747	rBV2	293	236	0.02%	0.002%
40	7.121	1794	1798	1800	rBV	255	215	0.02%	0.002%
41	7.186	1807	1818	1829	rVV3	2589	4493	0.38%	0.045%
42	7.237	1832	1834	1839	rVB2	208	158	0.01%	0.002%
43	7.340	1859	1866	1869	rBV	217	247	0.02%	0.002%
44	7.565	1923	1936	1954	rBV	138021	244834	20.51%	2.458%
45	7.687	1971	1974	1987	rVB4	1791	2787	0.23%	0.028%
46	7.739	1987	1990	1996	rBV3	535	337	0.03%	0.003%
47	7.793	2000	2007	2013	rBV3	380	517	0.04%	0.005%
48	7.899	2026	2040	2056	rBV	490400	855409	71.67%	8.590%
49	8.179	2116	2127	2147	rBV	97322	170439	14.28%	1.711%
50	8.478	2211	2220	2227	rVB3	1918	2657	0.22%	0.027%
51	8.555	2238	2244	2249	rBV4	1047	1157	0.10%	0.012%
52	8.636	2255	2269	2300	rBV	443931	851165	71.32%	8.547%
53	8.822	2323	2327	2330	rBV4	278	232	0.02%	0.002%
54	8.967	2369	2372	2378	rVV2	209	222	0.02%	0.002%
55	9.028	2388	2391	2396	rBV2	243	217	0.02%	0.002%
56	9.192	2439	2442	2446	rVB2	376	313	0.03%	0.003%
57	9.346	2484	2490	2493	rBV2	395	374	0.03%	0.004%
58	9.369	2494	2497	2499	rVV2	362	231	0.02%	0.002%
59	9.417	2499	2512	2547	rVV	548049	930246	77.95%	9.341%
60	9.571	2555	2560	2564	rVB5	539	632	0.05%	0.006%
61	9.591	2564	2566	2571	rVB2	264	219	0.02%	0.002%
62	9.616	2571	2574	2579	rBV2	326	350	0.03%	0.004%
63	9.697	2590	2599	2605	rVV2	767	1076	0.09%	0.011%
64	9.739	2608	2612	2616	rVB3	257	264	0.02%	0.003%
65	9.758	2616	2618	2622	rBV2	233	198	0.02%	0.002%
66	10.009	2693	2696	2701	rVB3	358	271	0.02%	0.003%
67	10.105	2716	2726	2731	rBV4	580	1010	0.08%	0.010%
68	10.211	2757	2759	2765	rVB3	323	295	0.02%	0.003%
69	10.243	2765	2769	2771	rBV	167	173	0.01%	0.002%
70	10.263	2772	2775	2780	rVV	336	270	0.02%	0.003%
71	10.321	2789	2793	2796	rBV2	323	253	0.02%	0.003%
72	10.475	2835	2841	2843	rBV2	396	337	0.03%	0.003%
73	10.668	2895	2901	2910	rBV4	892	1317	0.11%	0.013%
74	10.758	2916	2929	2949	rVB	471790	760107	63.69%	7.633%
75	10.893	2961	2971	2981	rVB2	3427	6154	0.52%	0.062%
76	10.938	2982	2985	2988	rVB2	263	190	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047737.D
 Acq On : 28 Mar 2022 18:53
 Operator : SY/MD
 Sample : VIBLK054
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.160	3050	3054	3057	rBV	236	185	0.02%	0.002%
78	11.414	3130	3133	3137	rVV2	420	254	0.02%	0.003%
79	11.468	3144	3150	3157	rVB4	1195	1555	0.13%	0.016%
80	11.536	3169	3171	3176	rVB2	431	322	0.03%	0.003%
81	11.565	3176	3180	3182	rBV	342	295	0.02%	0.003%
82	11.645	3202	3205	3208	rVB2	411	289	0.02%	0.003%
83	11.690	3213	3219	3222	rBV3	283	345	0.03%	0.003%
84	11.751	3231	3238	3243	rVB4	455	585	0.05%	0.006%
85	11.812	3243	3257	3277	rBV	674693	1065273	89.26%	10.697%
86	11.970	3301	3306	3312	rVB3	782	1019	0.09%	0.010%
87	11.996	3312	3314	3319	rVB2	357	259	0.02%	0.003%
88	12.021	3320	3322	3326	rBV2	225	187	0.02%	0.002%
89	12.128	3351	3355	3359	rBV2	291	259	0.02%	0.003%
90	12.192	3361	3375	3396	rBV	594389	975742	81.76%	9.798%
91	12.330	3414	3418	3421	rVB3	374	332	0.03%	0.003%
92	12.475	3460	3463	3466	rBV3	274	236	0.02%	0.002%
93	12.645	3512	3516	3520	rBV2	443	471	0.04%	0.005%
94	12.690	3527	3530	3533	rVB2	413	253	0.02%	0.003%
95	12.722	3533	3540	3541	rBV2	276	346	0.03%	0.003%
96	12.777	3551	3557	3562	rVB3	1047	1473	0.12%	0.015%
97	12.877	3582	3588	3592	rBV3	388	544	0.05%	0.005%
98	13.009	3625	3629	3633	rBV2	306	315	0.03%	0.003%
99	13.221	3692	3695	3698	rBV4	291	209	0.02%	0.002%
100	14.098	3961	3968	3974	rBV3	669	1129	0.09%	0.011%




Sum of corrected areas: 9958723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047737.D
Acq On : 28 Mar 2022 18:53
Operator : SY/MD
Sample : VIBLK054
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK054

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

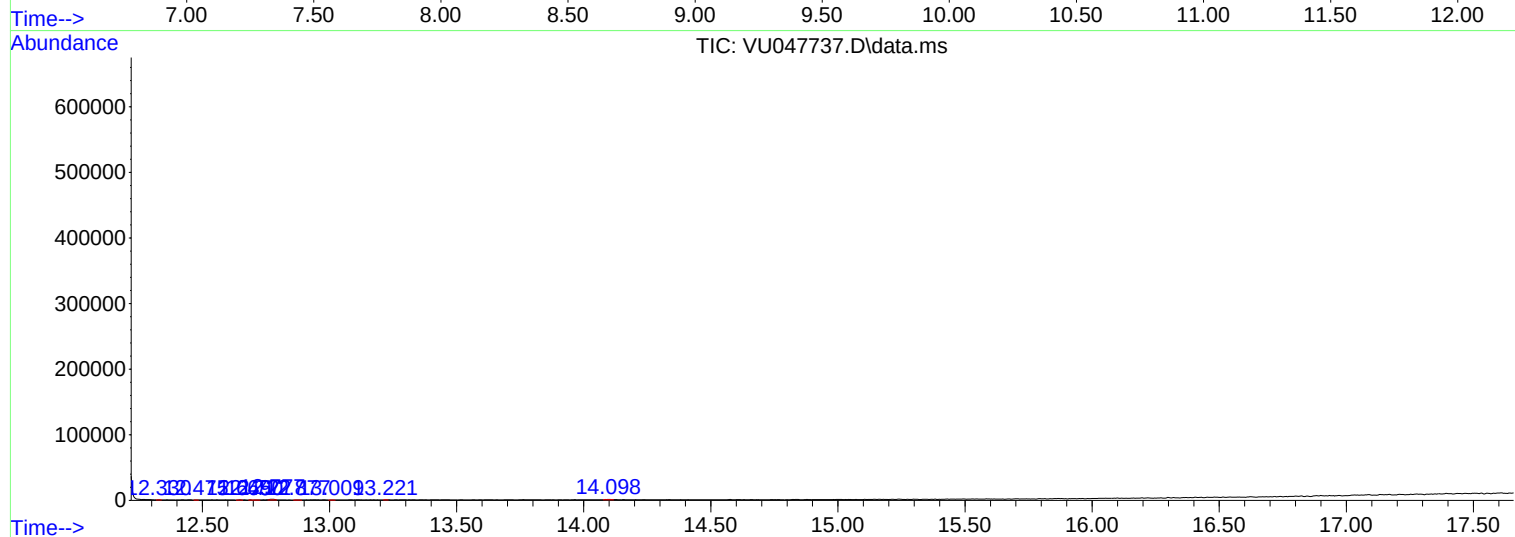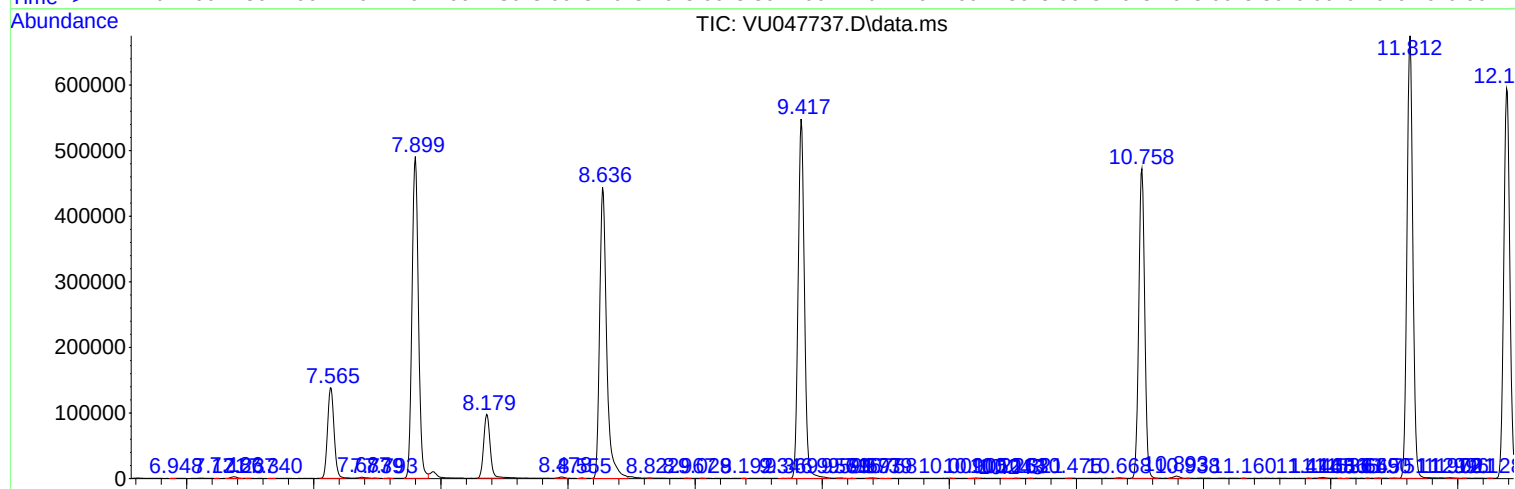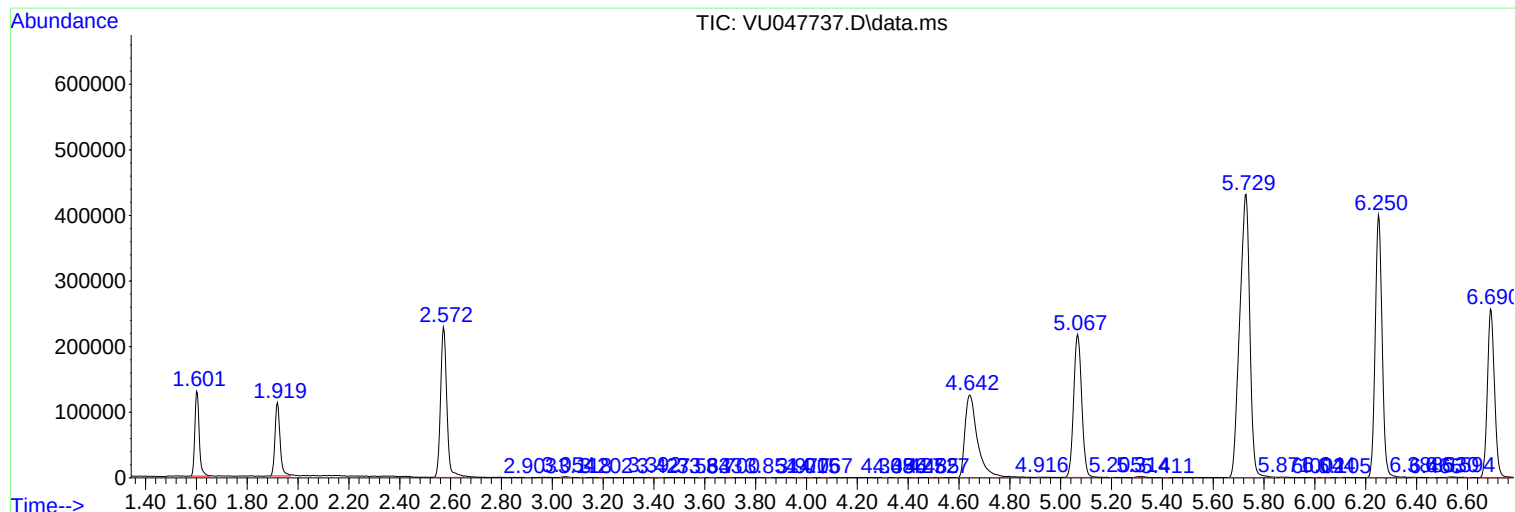

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047737.D
Acq On : 28 Mar 2022 18:53
Operator : SY/MD
Sample : VIBLK054
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK054

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047737.D
Acq On : 28 Mar 2022 18:53
Operator : SY/MD
Sample : VIBLK054
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK054

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------