

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047738.D
 Acq On : 28 Mar 2022 19:16
 Operator : SY/MD
 Sample : N2081-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rVB	123009	145661	3.72%	0.752%
2	1.919	171	180	200	rBV	107876	147861	3.78%	0.764%
3	2.359	314	317	326	rVB6	878	1161	0.03%	0.006%
4	2.459	346	348	350	rVB2	413	157	0.00%	0.001%
5	2.575	370	384	409	rBV3	272233	521145	13.31%	2.692%
6	2.896	479	484	486	rBV3	334	256	0.01%	0.001%
7	2.909	486	488	493	rBV2	263	267	0.01%	0.001%
8	2.964	501	505	507	rBV3	300	227	0.01%	0.001%
9	3.047	527	531	541	rVB3	764	1110	0.03%	0.006%
10	3.192	566	576	585	rBV3	1279	2297	0.06%	0.012%
11	3.285	601	605	608	rVV3	346	296	0.01%	0.002%
12	3.305	608	611	616	rVV3	278	264	0.01%	0.001%
13	3.356	621	627	637	rVB6	1267	2097	0.05%	0.011%
14	3.526	674	680	684	rBB2	189	252	0.01%	0.001%
15	3.555	686	689	693	rVB3	384	272	0.01%	0.001%
16	3.674	723	726	730	rVB	263	203	0.01%	0.001%
17	3.874	771	788	810	rBV	88344	209366	5.35%	1.081%
18	4.141	867	871	875	rVB3	250	248	0.01%	0.001%
19	4.231	895	899	902	rVV2	282	233	0.01%	0.001%
20	4.247	902	904	910	rVB3	295	313	0.01%	0.002%
21	4.282	913	915	919	rVB3	237	162	0.00%	0.001%
22	4.385	942	947	948	rBV	288	239	0.01%	0.001%
23	4.420	955	958	960	rBV2	250	160	0.00%	0.001%
24	4.481	969	977	979	rVB3	310	270	0.01%	0.001%
25	4.665	1013	1034	1064	rBV2	158895	610921	15.61%	3.156%
26	5.067	1142	1159	1187	rVV	220847	482314	12.32%	2.491%
27	5.163	1187	1189	1195	rVB4	590	380	0.01%	0.002%
28	5.221	1205	1207	1212	rVB2	268	198	0.01%	0.001%
29	5.321	1218	1238	1263	rBV	1529662	3442661	87.96%	17.783%
30	5.639	1333	1337	1339	rBV3	311	204	0.01%	0.001%
31	5.652	1339	1341	1343	rBV2	328	173	0.00%	0.001%
32	5.726	1343	1364	1394	rVV2	431947	1185192	30.28%	6.122%
33	5.938	1426	1430	1432	rBV2	237	171	0.00%	0.001%
34	6.044	1457	1463	1467	rBV4	680	765	0.02%	0.004%
35	6.105	1478	1482	1488	rBV3	334	344	0.01%	0.002%
36	6.250	1512	1527	1555	rBV	384678	735180	18.78%	3.798%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047738.D
 Acq On : 28 Mar 2022 19:16
 Operator : SY/MD
 Sample : N2081-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.440	1582	1586	1589	rVB3	311	290	0.01%	0.001%
38	6.459	1589	1592	1598	rBV3	412	300	0.01%	0.002%
39	6.542	1603	1618	1651	rBV	701875	1329738	33.97%	6.869%
40	6.694	1651	1665	1687	rVB	273537	537946	13.74%	2.779%
41	6.803	1695	1699	1705	rVB5	1145	1221	0.03%	0.006%
42	6.857	1714	1716	1725	rVB3	199	198	0.01%	0.001%
43	7.054	1769	1777	1782	rBV5	773	1004	0.03%	0.005%
44	7.073	1782	1783	1788	rVB3	338	201	0.01%	0.001%
45	7.150	1803	1807	1810	rBV2	190	208	0.01%	0.001%
46	7.189	1810	1819	1828	rVV6	2335	4306	0.11%	0.022%
47	7.240	1832	1835	1837	rBV2	307	247	0.01%	0.001%
48	7.311	1854	1857	1859	rBV	273	177	0.00%	0.001%
49	7.378	1872	1878	1881	rVV2	282	272	0.01%	0.001%
50	7.411	1884	1888	1892	rVV2	186	158	0.00%	0.001%
51	7.481	1907	1910	1916	rVB2	213	216	0.01%	0.001%
52	7.568	1924	1937	1956	rBV	138645	247997	6.34%	1.281%
53	7.690	1968	1975	1984	rBV5	1627	2614	0.07%	0.014%
54	7.803	2003	2010	2014	rBV2	552	583	0.01%	0.003%
55	7.899	2025	2040	2055	rBV	511254	891590	22.78%	4.605%
56	8.179	2115	2127	2142	rBV	109388	186621	4.77%	0.964%
57	8.404	2187	2197	2207	rBV3	6724	11483	0.29%	0.059%
58	8.472	2207	2218	2229	rVB3	7631	13224	0.34%	0.068%
59	8.552	2229	2243	2259	rBV	2295547	3913982	100.00%	20.217%
60	8.639	2259	2270	2304	rVB	475411	943532	24.11%	4.874%
61	8.893	2347	2349	2355	rBV4	435	320	0.01%	0.002%
62	8.986	2375	2378	2387	rVB2	500	491	0.01%	0.003%
63	9.028	2387	2391	2394	rVB4	352	300	0.01%	0.002%
64	9.176	2432	2437	2439	rBV	227	195	0.00%	0.001%
65	9.214	2446	2449	2453	rBV3	357	269	0.01%	0.001%
66	9.295	2470	2474	2476	rBV	255	174	0.00%	0.001%
67	9.340	2484	2488	2493	rVB3	347	443	0.01%	0.002%
68	9.417	2493	2512	2546	rBV	579364	969622	24.77%	5.008%
69	9.642	2578	2582	2583	rBV	242	171	0.00%	0.001%
70	9.693	2591	2598	2601	rBV4	1168	1496	0.04%	0.008%
71	9.883	2653	2657	2662	rVB3	236	234	0.01%	0.001%
72	9.938	2669	2674	2677	rBV3	260	279	0.01%	0.001%
73	10.034	2700	2704	2709	rVB3	389	405	0.01%	0.002%
74	10.066	2711	2714	2717	rBV3	280	190	0.00%	0.001%
75	10.108	2717	2727	2729	rBV3	592	658	0.02%	0.003%
76	10.484	2840	2844	2850	rVB2	454	415	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047738.D
 Acq On : 28 Mar 2022 19:16
 Operator : SY/MD
 Sample : N2081-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.574	2867	2872	2877	rVB2	300	282	0.01%	0.001%
78	10.664	2896	2900	2901	rBV2	847	638	0.02%	0.003%
79	10.758	2916	2929	2948	rBV	471204	768548	19.64%	3.970%
80	10.893	2959	2971	2984	rBB	12075	20108	0.51%	0.104%
81	11.070	3021	3026	3027	rBV	249	214	0.01%	0.001%
82	11.095	3032	3034	3039	rVB2	511	307	0.01%	0.002%
83	11.153	3045	3052	3056	rBV3	222	346	0.01%	0.002%
84	11.317	3099	3103	3106	rVB2	268	176	0.00%	0.001%
85	11.414	3130	3133	3135	rBV3	457	218	0.01%	0.001%
86	11.468	3143	3150	3158	rVB5	1673	2348	0.06%	0.012%
87	11.748	3233	3237	3241	rVB3	430	316	0.01%	0.002%
88	11.812	3244	3257	3279	rVV	650908	1027599	26.25%	5.308%
89	12.192	3362	3375	3396	rBV	592181	972060	24.84%	5.021%
90	12.317	3412	3414	3420	rVB2	382	271	0.01%	0.001%
91	12.462	3456	3459	3461	rBV2	265	166	0.00%	0.001%
92	12.661	3517	3521	3524	rBV2	273	301	0.01%	0.002%
93	12.741	3540	3546	3547	rBV	286	298	0.01%	0.002%
94	12.774	3549	3556	3567	rVB2	3486	5963	0.15%	0.031%
95	13.224	3694	3696	3700	rVB3	514	323	0.01%	0.002%
96	13.664	3828	3833	3838	rBV2	373	381	0.01%	0.002%
97	13.825	3878	3883	3889	rBV2	364	533	0.01%	0.003%
98	14.790	4179	4183	4187	rBV3	479	395	0.01%	0.002%
99	15.211	4311	4314	4322	rVB3	580	634	0.02%	0.003%
100	15.291	4337	4339	4341	rBV2	563	344	0.01%	0.002%




Sum of corrected areas: 19359559

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047738.D
Acq On : 28 Mar 2022 19:16
Operator : SY/MD
Sample : N2081-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

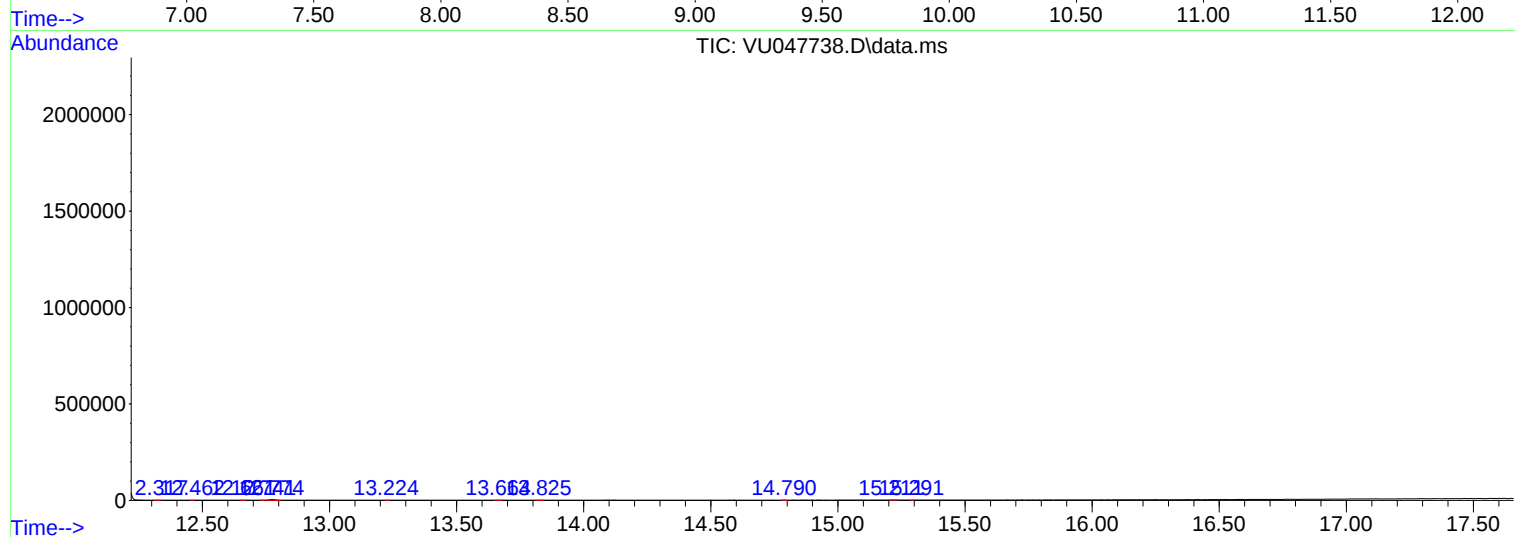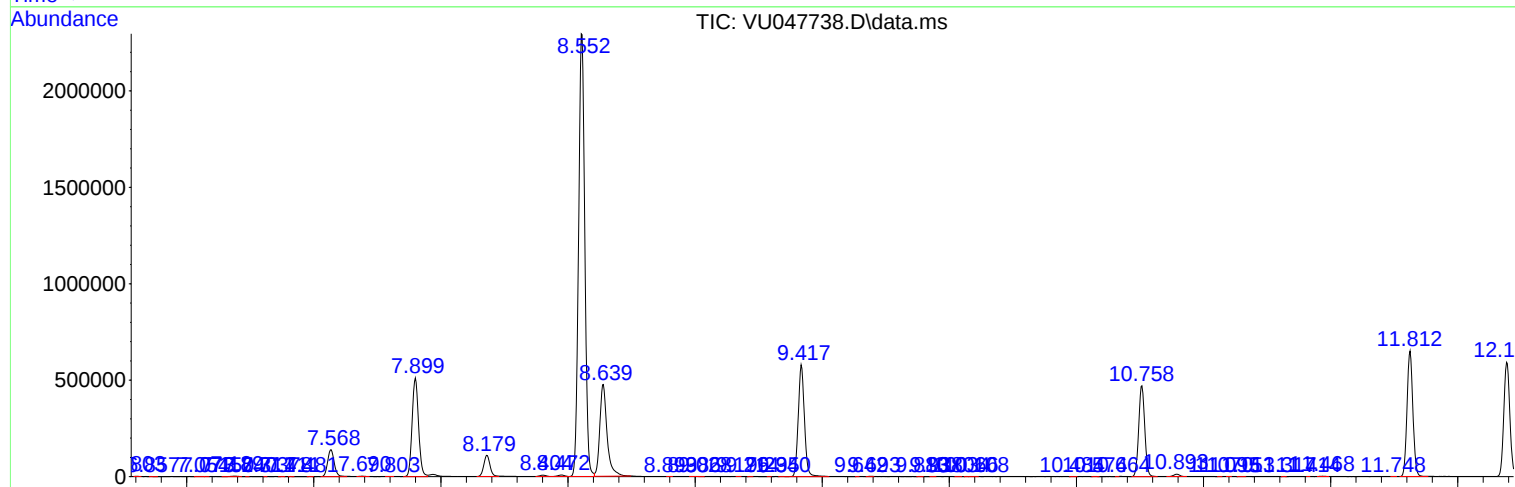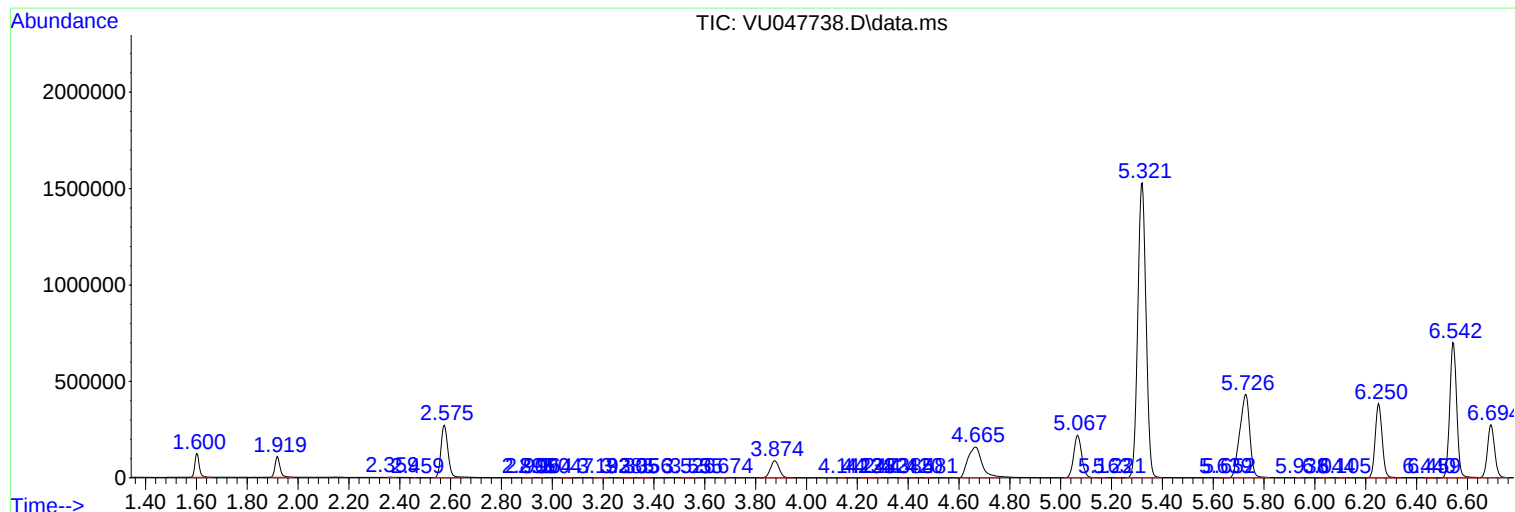

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047738.D
Acq On : 28 Mar 2022 19:16
Operator : SY/MD
Sample : N2081-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047738.D
Acq On : 28 Mar 2022 19:16
Operator : SY/MD
Sample : N2081-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------