

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047741.D
 Acq On : 28 Mar 2022 20:23
 Operator : SY/MD
 Sample : N2120-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rBV	122337	148327	12.72%	1.449%
2	1.736	116	123	134	rVB	10032	12304	1.06%	0.120%
3	1.919	171	180	197	rBV	105757	147733	12.67%	1.444%
4	2.572	371	383	406	rBV	218524	370958	31.81%	3.625%
5	2.800	448	454	459	rVB2	599	739	0.06%	0.007%
6	2.845	462	468	473	rBV2	239	309	0.03%	0.003%
7	2.867	473	475	479	rBV3	263	228	0.02%	0.002%
8	2.967	496	506	508	rBV2	555	826	0.07%	0.008%
9	3.044	527	530	532	rBV2	724	481	0.04%	0.005%
10	3.189	561	575	598	rVB	21498	49177	4.22%	0.481%
11	3.369	627	631	638	rBV2	597	515	0.04%	0.005%
12	3.591	696	700	706	rVB2	335	311	0.03%	0.003%
13	3.620	706	709	712	rVB2	326	223	0.02%	0.002%
14	3.646	712	717	720	rBV2	292	256	0.02%	0.003%
15	3.716	736	739	744	rVB2	333	296	0.03%	0.003%
16	3.745	744	748	751	rVB2	226	184	0.02%	0.002%
17	3.790	758	762	765	rBV	258	236	0.02%	0.002%
18	3.932	801	806	811	rBV2	338	352	0.03%	0.003%
19	4.083	848	853	856	rBV2	388	459	0.04%	0.004%
20	4.231	895	899	905	rVB3	280	334	0.03%	0.003%
21	4.311	920	924	928	rBV3	196	167	0.01%	0.002%
22	4.395	948	950	953	rVB	330	210	0.02%	0.002%
23	4.427	957	960	964	rBV2	194	204	0.02%	0.002%
24	4.491	970	980	983	rBV3	403	446	0.04%	0.004%
25	4.507	983	985	990	rVB3	304	233	0.02%	0.002%
26	4.642	1007	1027	1081	rBV2	159040	596469	51.14%	5.828%
27	5.067	1142	1159	1182	rBV	221212	500594	42.92%	4.892%
28	5.269	1218	1222	1224	rBV2	271	181	0.02%	0.002%
29	5.285	1224	1227	1230	rBV3	343	344	0.03%	0.003%
30	5.359	1244	1250	1253	rBV3	328	448	0.04%	0.004%
31	5.726	1343	1364	1399	rBV2	422747	1166245	100.00%	11.396%
32	6.044	1458	1463	1466	rBV2	480	457	0.04%	0.004%
33	6.115	1482	1485	1486	rBV	279	176	0.02%	0.002%
34	6.250	1513	1527	1552	rBV	400881	762059	65.34%	7.446%
35	6.446	1585	1588	1595	rVB2	419	480	0.04%	0.005%
36	6.478	1595	1598	1601	rBV3	347	245	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047741.D
 Acq On : 28 Mar 2022 20:23
 Operator : SY/MD
 Sample : N2120-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.530	1609	1614	1615	rBV3	1131	960	0.08%	0.009%
38	6.591	1629	1633	1635	rVB2	433	237	0.02%	0.002%
39	6.694	1649	1665	1688	rBV	268610	532676	45.67%	5.205%
40	6.806	1696	1700	1709	rVB4	1053	1355	0.12%	0.013%
41	6.871	1716	1720	1721	rBV2	296	176	0.02%	0.002%
42	6.912	1730	1733	1735	rBV3	299	195	0.02%	0.002%
43	7.038	1768	1772	1773	rBV2	334	219	0.02%	0.002%
44	7.131	1797	1801	1802	rBV2	259	167	0.01%	0.002%
45	7.182	1810	1817	1831	rBV5	2398	4417	0.38%	0.043%
46	7.240	1833	1835	1837	rBV	354	189	0.02%	0.002%
47	7.327	1859	1862	1869	rBV2	143	180	0.02%	0.002%
48	7.498	1911	1915	1918	rBV2	234	214	0.02%	0.002%
49	7.565	1924	1936	1954	rBV	148534	262056	22.47%	2.561%
50	7.690	1968	1975	1979	rBV6	1679	2386	0.20%	0.023%
51	7.806	2007	2011	2015	rBV3	381	414	0.04%	0.004%
52	7.899	2023	2040	2055	rBV	521406	904935	77.59%	8.843%
53	8.179	2115	2127	2147	rBV	103932	181225	15.54%	1.771%
54	8.475	2208	2219	2232	rVB3	14653	26124	2.24%	0.255%
55	8.552	2236	2243	2244	rBV4	1278	979	0.08%	0.010%
56	8.636	2256	2269	2301	rBV	469670	908164	77.87%	8.874%
57	8.790	2314	2317	2323	rVB5	613	462	0.04%	0.005%
58	9.118	2413	2419	2421	rBV2	282	329	0.03%	0.003%
59	9.176	2433	2437	2439	rBV2	279	259	0.02%	0.003%
60	9.253	2457	2461	2463	rBV2	260	195	0.02%	0.002%
61	9.362	2492	2495	2499	rVB3	341	258	0.02%	0.003%
62	9.417	2499	2512	2544	rBV	595729	1007410	86.38%	9.844%
63	9.571	2557	2560	2564	rVB2	641	429	0.04%	0.004%
64	9.668	2586	2590	2592	rVV	207	187	0.02%	0.002%
65	9.694	2594	2598	2607	rVB3	964	1134	0.10%	0.011%
66	9.784	2621	2626	2630	rBV3	268	263	0.02%	0.003%
67	9.967	2680	2683	2687	rBV	433	412	0.04%	0.004%
68	10.102	2720	2725	2728	rBV2	294	241	0.02%	0.002%
69	10.218	2757	2761	2764	rVB3	214	179	0.02%	0.002%
70	10.253	2768	2772	2777	rBV2	341	389	0.03%	0.004%
71	10.481	2840	2843	2847	rVB2	254	221	0.02%	0.002%
72	10.584	2872	2875	2877	rBV	337	170	0.01%	0.002%
73	10.600	2877	2880	2889	rVB2	303	306	0.03%	0.003%
74	10.668	2896	2901	2910	rVV4	704	915	0.08%	0.009%
75	10.706	2910	2913	2916	rVV2	212	211	0.02%	0.002%
76	10.758	2916	2929	2951	rVV	418266	690171	59.18%	6.744%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047741.D
 Acq On : 28 Mar 2022 20:23
 Operator : SY/MD
 Sample : N2120-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.893	2959	2971	2984	rBV	27249	44606	3.82%	0.436%
78	11.005	3003	3006	3010	rVB2	215	177	0.02%	0.002%
79	11.070	3022	3026	3029	rVB2	266	210	0.02%	0.002%
80	11.092	3029	3033	3041	rVB2	395	391	0.03%	0.004%
81	11.195	3060	3065	3070	rBV3	381	357	0.03%	0.003%
82	11.558	3175	3178	3181	rBV	265	187	0.02%	0.002%
83	11.703	3218	3223	3226	rBV3	444	466	0.04%	0.005%
84	11.748	3232	3237	3242	rBV3	513	547	0.05%	0.005%
85	11.812	3243	3257	3280	rVV	618257	974749	83.58%	9.525%
86	11.938	3291	3296	3300	rBV4	427	329	0.03%	0.003%
87	11.964	3302	3304	3310	rVB4	541	447	0.04%	0.004%
88	12.018	3318	3321	3325	rBV2	278	185	0.02%	0.002%
89	12.066	3328	3336	3352	rVB5	4177	8107	0.70%	0.079%
90	12.192	3359	3375	3393	rBV	547232	891785	76.47%	8.714%
91	12.333	3416	3419	3422	rVB2	343	206	0.02%	0.002%
92	12.636	3509	3513	3517	rBV3	283	311	0.03%	0.003%
93	12.774	3546	3556	3566	rVB2	7030	11475	0.98%	0.112%
94	13.047	3638	3641	3645	rBV3	340	306	0.03%	0.003%
95	13.748	3856	3859	3861	rBV2	260	192	0.02%	0.002%
96	13.841	3884	3888	3896	rBV4	1118	1494	0.13%	0.015%
97	14.330	4037	4040	4047	rVB2	597	808	0.07%	0.008%
98	15.092	4275	4277	4281	rBV3	541	412	0.04%	0.004%
99	15.436	4380	4384	4386	rBV3	503	414	0.04%	0.004%
100	15.658	4450	4453	4458	rBV4	936	1054	0.09%	0.010%




Sum of corrected areas: 10233830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047741.D
Acq On : 28 Mar 2022 20:23
Operator : SY/MD
Sample : N2120-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

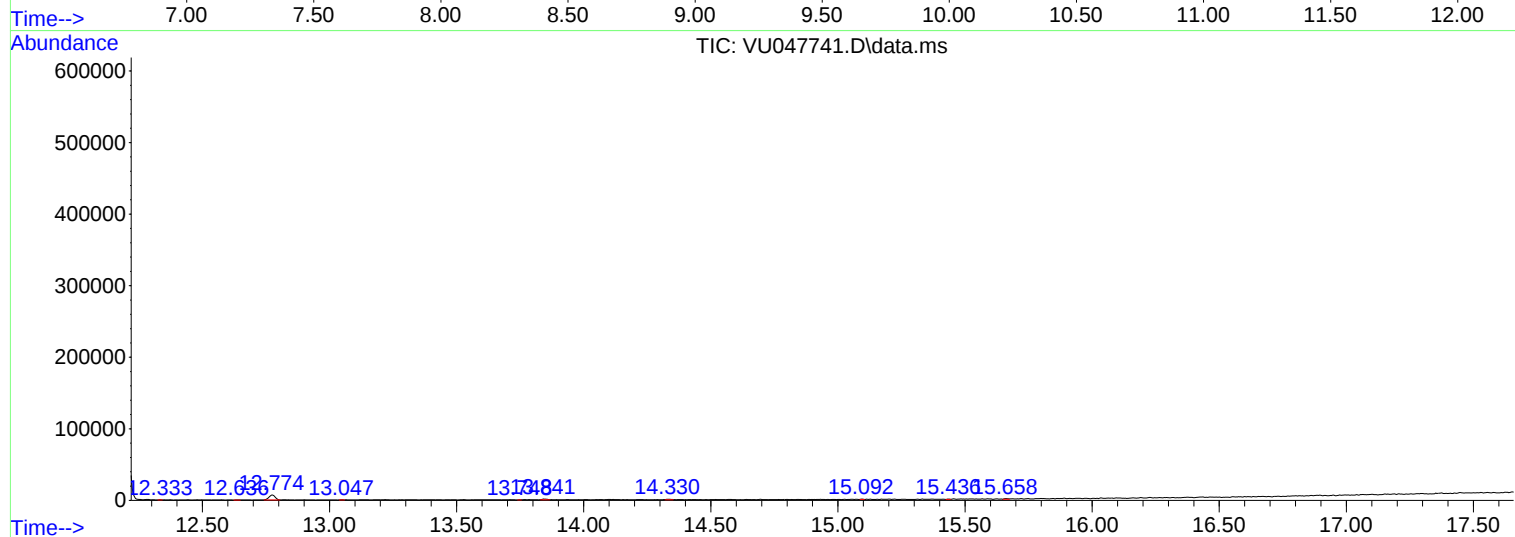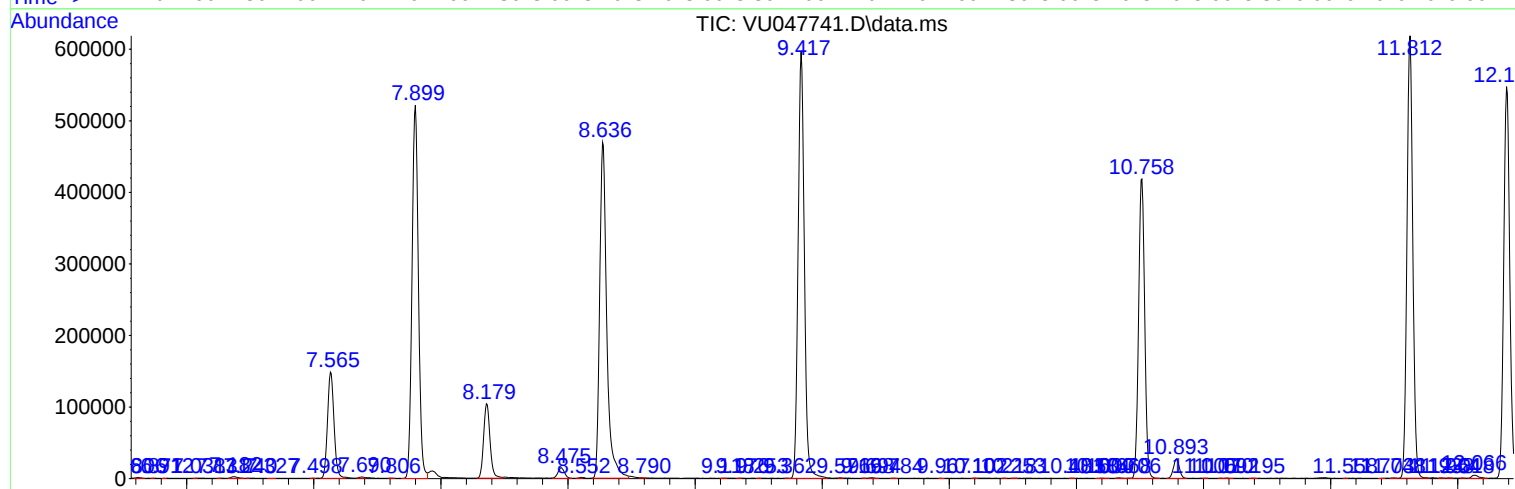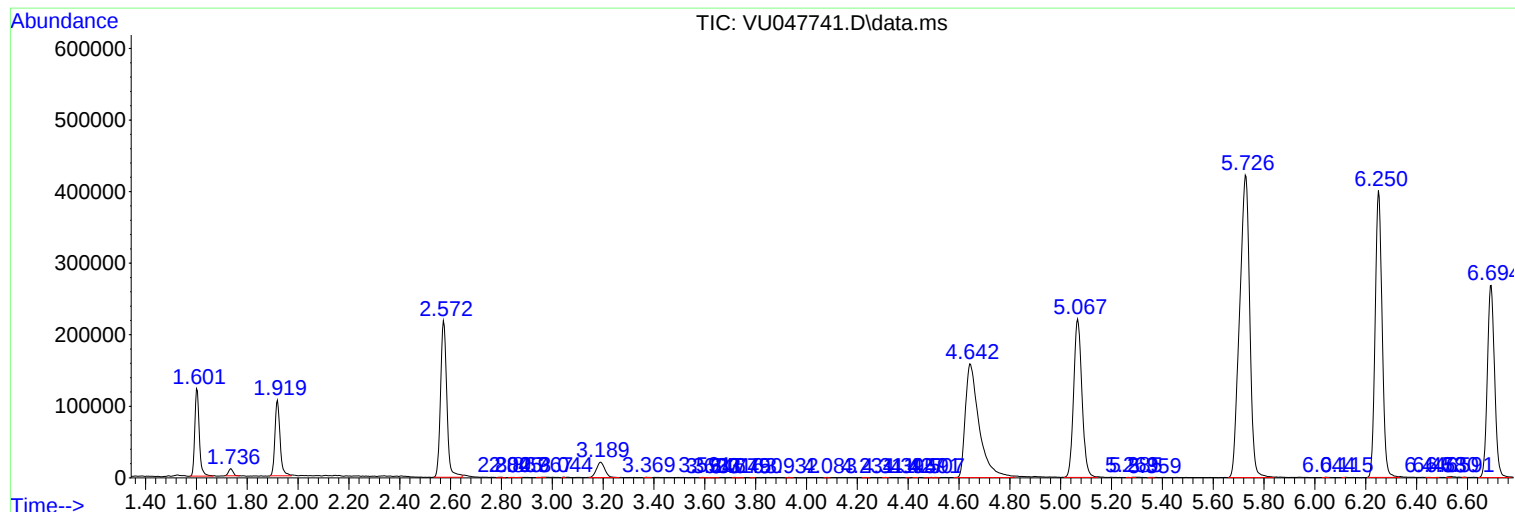

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047741.D
Acq On : 28 Mar 2022 20:23
Operator : SY/MD
Sample : N2120-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047741.D
Acq On : 28 Mar 2022 20:23
Operator : SY/MD
Sample : N2120-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc