

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047742.D
 Acq On : 28 Mar 2022 20:46
 Operator : SY/MD
 Sample : N2120-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rVB	121495	142628	12.27%	1.362%
2	1.735	117	123	130	rVB	11603	13099	1.13%	0.125%
3	1.919	171	180	199	rBV	107337	146498	12.61%	1.399%
4	2.571	371	383	408	rBV	219792	373856	32.17%	3.571%
5	2.800	450	454	461	rVB4	493	527	0.05%	0.005%
6	2.838	461	466	468	rBV3	329	280	0.02%	0.003%
7	2.854	468	471	473	rBV	357	218	0.02%	0.002%
8	3.044	526	530	533	rBV4	495	538	0.05%	0.005%
9	3.086	541	543	548	rVB2	356	249	0.02%	0.002%
10	3.189	561	575	595	rVV2	21658	51723	4.45%	0.494%
11	3.263	595	598	601	rVV	299	181	0.02%	0.002%
12	3.359	625	628	634	rVV4	518	449	0.04%	0.004%
13	3.462	657	660	667	rBV3	157	168	0.01%	0.002%
14	3.542	680	685	695	rVB3	225	414	0.04%	0.004%
15	3.607	699	705	711	rBV3	190	338	0.03%	0.003%
16	3.674	722	726	730	rVB2	284	295	0.03%	0.003%
17	3.755	746	751	754	rBV2	305	227	0.02%	0.002%
18	4.079	849	852	854	rVB2	262	170	0.01%	0.002%
19	4.099	854	858	861	rBV2	302	281	0.02%	0.003%
20	4.340	927	933	936	rBV	347	256	0.02%	0.002%
21	4.391	946	949	957	rBB3	197	193	0.02%	0.002%
22	4.443	962	965	969	rVB2	229	183	0.02%	0.002%
23	4.475	972	975	983	rVB2	266	277	0.02%	0.003%
24	4.642	1009	1027	1083	rBV2	167595	602130	51.82%	5.752%
25	4.909	1107	1110	1111	rBV	332	169	0.01%	0.002%
26	4.976	1129	1131	1136	rVB4	319	230	0.02%	0.002%
27	5.066	1143	1159	1185	rBV	219391	497615	42.82%	4.753%
28	5.295	1224	1230	1236	rBV3	445	538	0.05%	0.005%
29	5.456	1278	1280	1289	rVB2	327	258	0.02%	0.002%
30	5.494	1289	1292	1298	rBV3	310	280	0.02%	0.003%
31	5.729	1342	1365	1397	rBV2	424260	1162026	100.00%	11.100%
32	5.947	1429	1433	1436	rBV2	252	210	0.02%	0.002%
33	6.050	1456	1465	1472	rBV4	520	942	0.08%	0.009%
34	6.079	1472	1474	1477	rBV	329	196	0.02%	0.002%
35	6.198	1506	1511	1513	rBV2	294	272	0.02%	0.003%
36	6.250	1513	1527	1554	rBV	402610	770631	66.32%	7.361%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047742.D
 Acq On : 28 Mar 2022 20:46
 Operator : SY/MD
 Sample : N2120-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.539	1607	1617	1623	rBV7	1168	2267	0.20%	0.022%
38	6.693	1650	1665	1691	rVV	270909	530443	45.65%	5.067%
39	6.899	1727	1729	1733	rVB2	392	273	0.02%	0.003%
40	6.928	1733	1738	1740	rBV2	321	362	0.03%	0.003%
41	7.034	1766	1771	1772	rBV2	283	204	0.02%	0.002%
42	7.182	1810	1817	1818	rBV3	2276	2009	0.17%	0.019%
43	7.240	1832	1835	1839	rBV2	238	205	0.02%	0.002%
44	7.308	1854	1856	1859	rBV	321	193	0.02%	0.002%
45	7.401	1880	1885	1887	rBV3	233	231	0.02%	0.002%
46	7.568	1921	1937	1958	rBV	145436	258715	22.26%	2.471%
47	7.690	1968	1975	1988	rVB6	1981	3928	0.34%	0.038%
48	7.748	1988	1993	1996	rVB2	379	377	0.03%	0.004%
49	7.899	2026	2040	2056	rBV	523950	901476	77.58%	8.611%
50	8.179	2115	2127	2146	rBV	101629	178549	15.37%	1.706%
51	8.330	2172	2174	2179	rVB2	424	281	0.02%	0.003%
52	8.472	2207	2218	2233	rVB2	14037	25689	2.21%	0.245%
53	8.552	2239	2243	2252	rVB5	907	1039	0.09%	0.010%
54	8.635	2254	2269	2310	rBV	467603	906673	78.03%	8.661%
55	8.861	2336	2339	2342	rBV2	354	301	0.03%	0.003%
56	8.973	2370	2374	2376	rBV2	226	199	0.02%	0.002%
57	9.086	2406	2409	2414	rVV2	242	214	0.02%	0.002%
58	9.160	2428	2432	2435	rBV	180	168	0.01%	0.002%
59	9.201	2440	2445	2447	rBV3	304	230	0.02%	0.002%
60	9.224	2448	2452	2456	rBV2	225	237	0.02%	0.002%
61	9.295	2469	2474	2476	rBV	177	175	0.02%	0.002%
62	9.343	2486	2489	2494	rVB3	258	219	0.02%	0.002%
63	9.417	2498	2512	2550	rBV	612175	1027166	88.39%	9.812%
64	9.565	2555	2558	2559	rBV2	345	246	0.02%	0.002%
65	9.600	2566	2569	2572	rBV2	311	241	0.02%	0.002%
66	9.693	2590	2598	2603	rBV4	898	1155	0.10%	0.011%
67	10.095	2719	2723	2728	rBV4	356	362	0.03%	0.003%
68	10.340	2793	2799	2804	rBV3	197	280	0.02%	0.003%
69	10.549	2861	2864	2869	rVV2	341	266	0.02%	0.003%
70	10.668	2897	2901	2903	rBV4	834	577	0.05%	0.006%
71	10.680	2903	2905	2908	rVB2	537	279	0.02%	0.003%
72	10.758	2916	2929	2946	rBV	459151	747087	64.29%	7.136%
73	10.893	2960	2971	2985	rBV	29172	47707	4.11%	0.456%
74	10.957	2988	2991	2995	rVB2	304	263	0.02%	0.003%
75	11.002	3001	3005	3008	rBV3	249	198	0.02%	0.002%
76	11.079	3025	3029	3031	rBV2	288	219	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047742.D
 Acq On : 28 Mar 2022 20:46
 Operator : SY/MD
 Sample : N2120-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.134	3043	3046	3049	rBV2	330	253	0.02%	0.002%
78	11.394	3121	3127	3131	rBV3	273	350	0.03%	0.003%
79	11.465	3144	3149	3150	rBV2	973	678	0.06%	0.006%
80	11.745	3231	3236	3237	rBV2	476	344	0.03%	0.003%
81	11.812	3244	3257	3283	rBV	683130	1074819	92.50%	10.267%
82	11.915	3287	3289	3292	rVV2	536	408	0.04%	0.004%
83	11.950	3296	3300	3303	rVB2	558	431	0.04%	0.004%
84	12.005	3314	3317	3322	rBV2	266	260	0.02%	0.002%
85	12.066	3328	3336	3347	rBV5	4010	6474	0.56%	0.062%
86	12.192	3358	3375	3393	rBV	586683	958819	82.51%	9.159%
87	12.385	3430	3435	3439	rVB4	360	367	0.03%	0.004%
88	12.404	3439	3441	3445	rBV3	200	184	0.02%	0.002%
89	12.430	3445	3449	3453	rVB3	389	297	0.03%	0.003%
90	12.587	3496	3498	3503	rBV2	260	171	0.01%	0.002%
91	12.632	3508	3512	3515	rBV	314	227	0.02%	0.002%
92	12.674	3522	3525	3527	rBV2	284	198	0.02%	0.002%
93	12.774	3545	3556	3567	rBV3	7420	11600	1.00%	0.111%
94	13.847	3883	3890	3894	rBV3	1242	1458	0.13%	0.014%
95	14.085	3962	3964	3968	rBV3	387	353	0.03%	0.003%
96	14.182	3991	3994	3996	rBV2	363	260	0.02%	0.002%
97	14.327	4036	4039	4042	rBV2	589	505	0.04%	0.005%
98	14.664	4142	4144	4148	rBV2	313	191	0.02%	0.002%
99	14.963	4234	4237	4241	rBV4	481	377	0.03%	0.004%
100	15.140	4289	4292	4296	rVB3	530	327	0.03%	0.003%


Sum of corrected areas: 10468599

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047742.D
Acq On : 28 Mar 2022 20:46
Operator : SY/MD
Sample : N2120-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

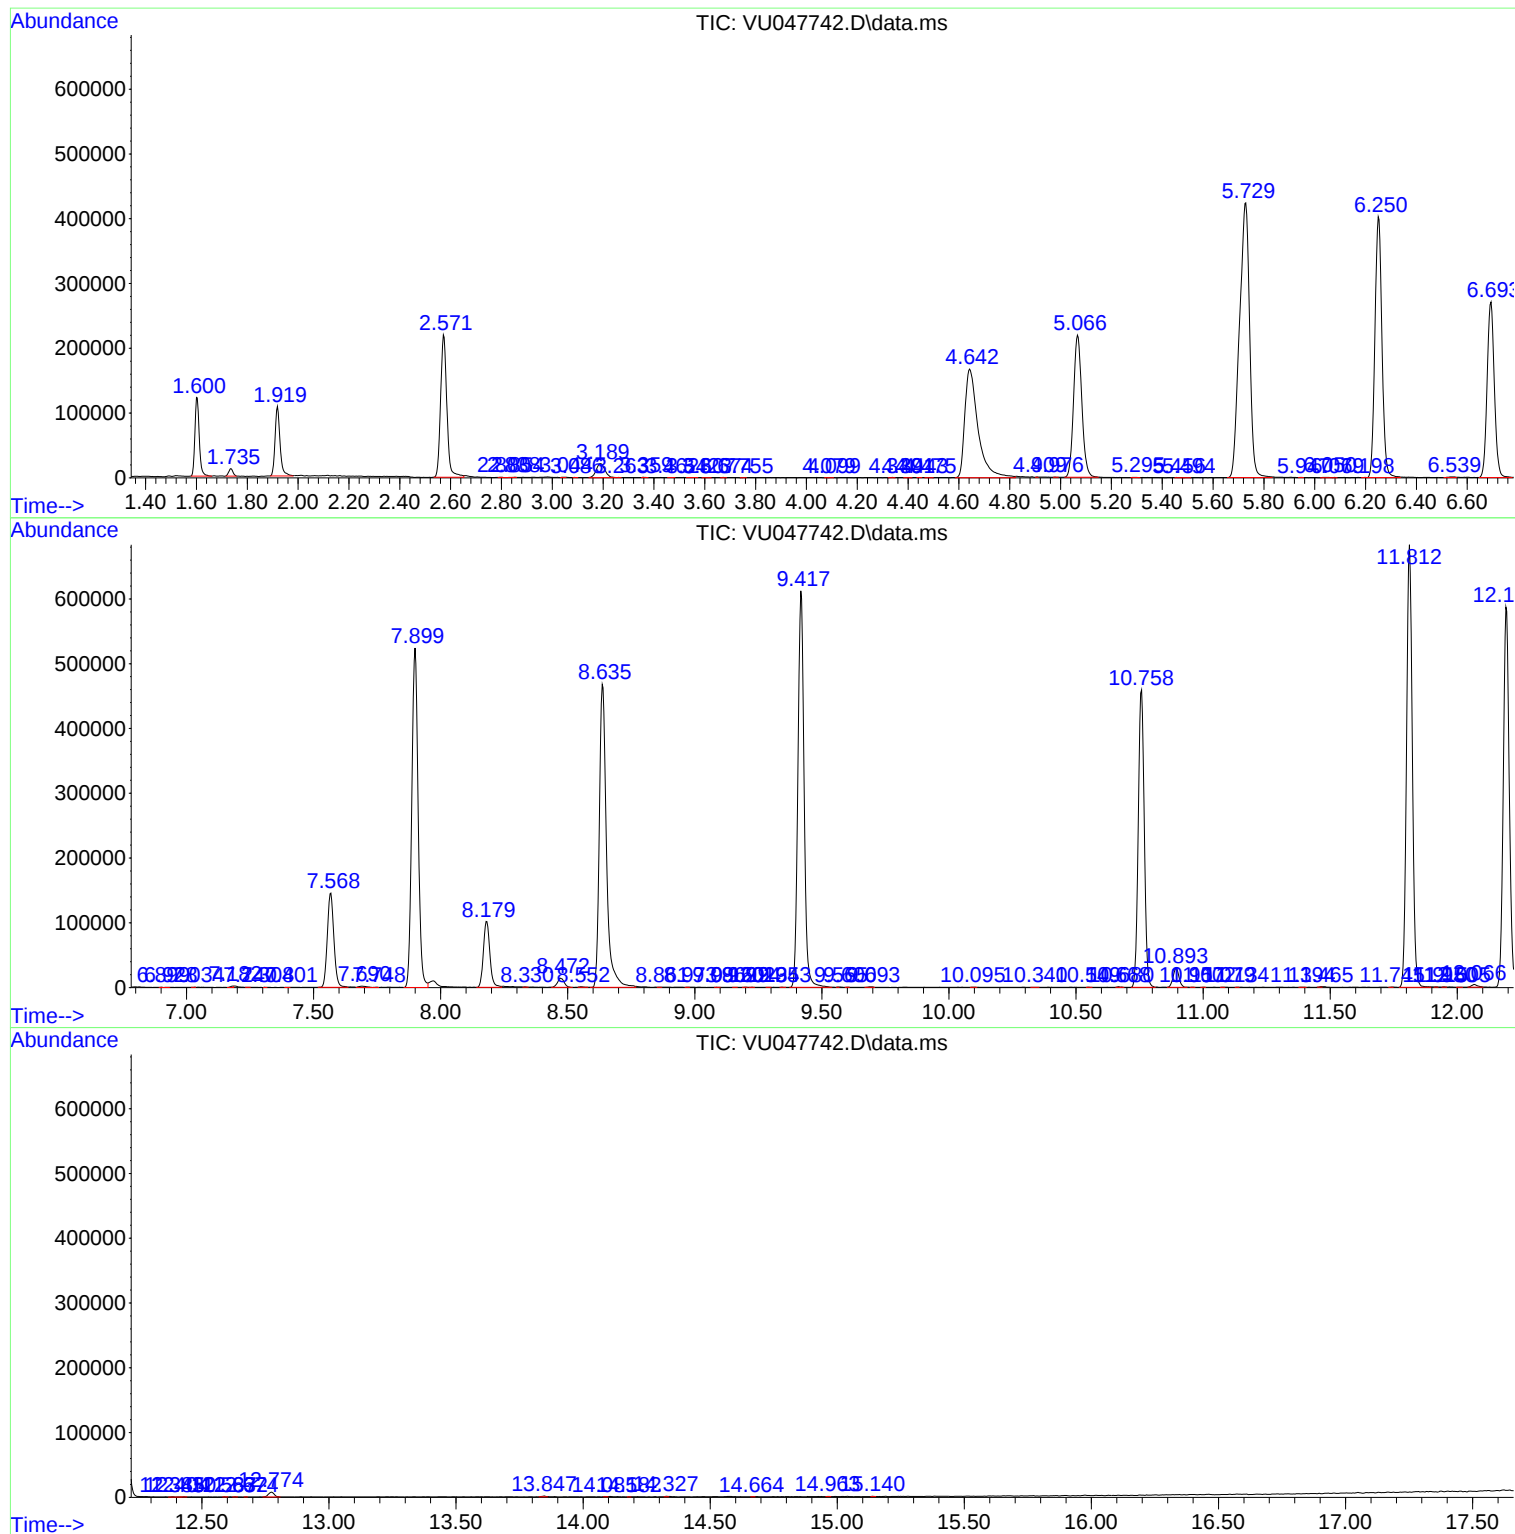

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047742.D
Acq On : 28 Mar 2022 20:46
Operator : SY/MD
Sample : N2120-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
Data File : VU047742.D
Acq On : 28 Mar 2022 20:46
Operator : SY/MD
Sample : N2120-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc