


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032822\
 Data File : VU047720.D
 Acq On : 28 Mar 2022 10:49
 Operator : SY/MD
 Sample : BFB056
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB056

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 30 01:20:49 2022

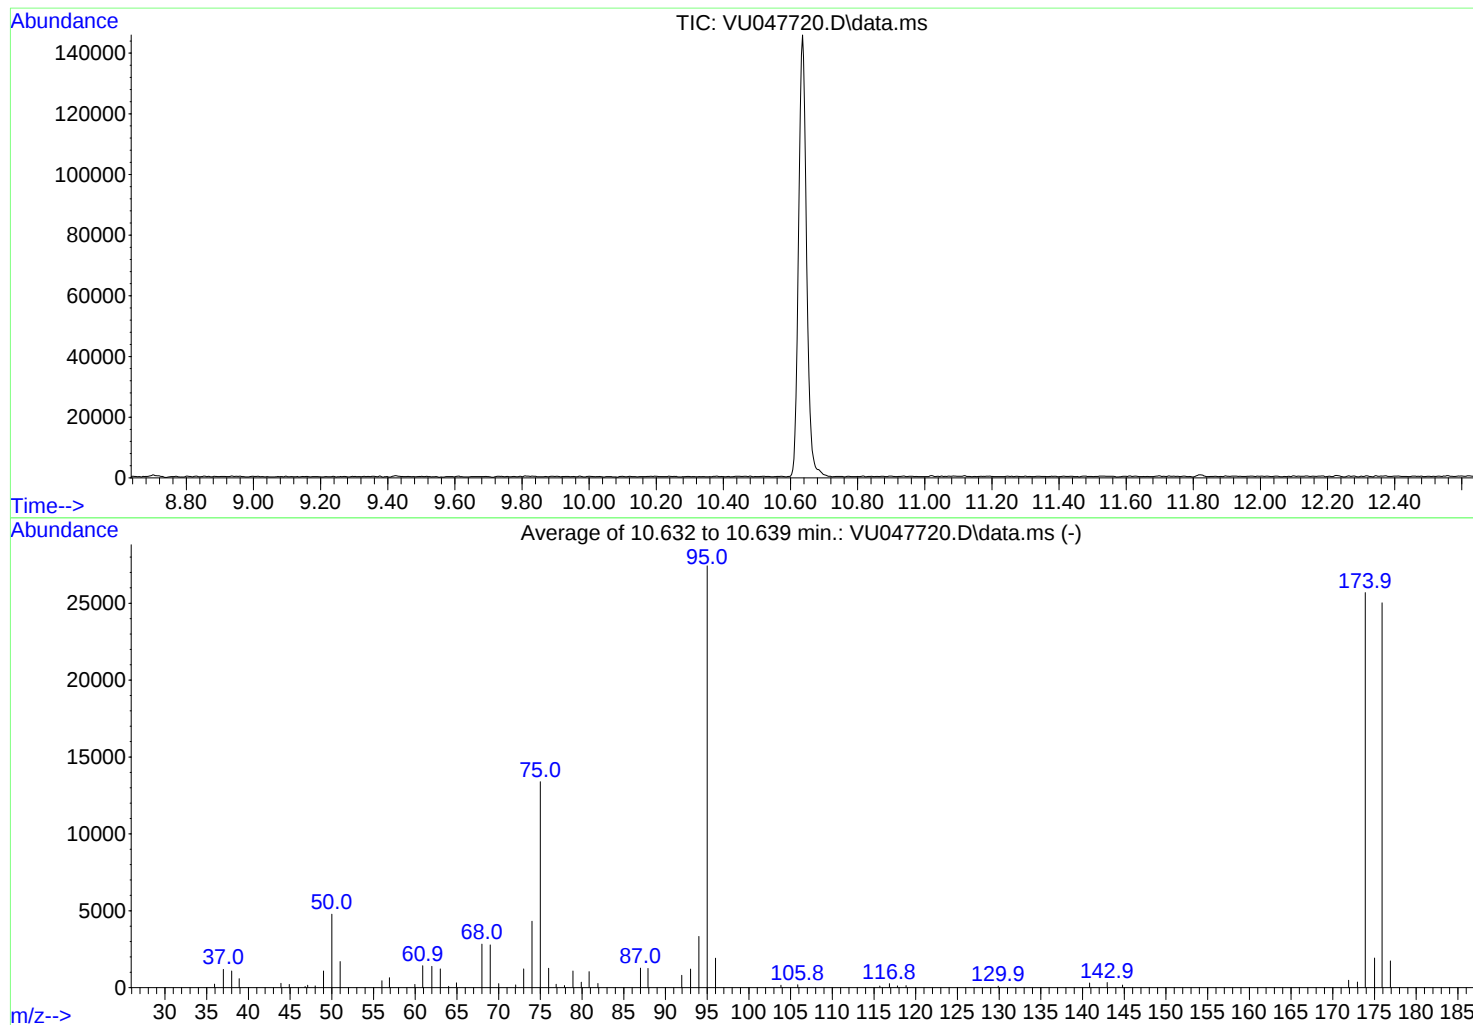

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	4774	PASS
75	95	30	80	48.8	13392	PASS
95	95	100	100	100.0	27432	PASS
96	95	5	9	7.0	1914	PASS
173	174	0.00	2	1.4	366	PASS
174	95	50	120	93.7	25696	PASS
175	174	5	9	7.5	1922	PASS
176	174	95	101	97.4	25029	PASS
177	176	5	9	6.9	1735	PASS

Scan 2878 (10.594 min): VU047720.D\data.ms
BFB056

m/z	Abundance
39.90	188.0
43.90	290.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
35.90	181.0
37.00	1167.0
38.00	1112.0
38.90	589.0
39.80	153.0
44.00	633.0
44.90	205.0
47.10	260.0
48.00	102.0
49.00	1125.0
50.00	4787.0
51.00	1698.0
56.00	454.0
56.90	640.0
60.00	185.0
60.90	1430.0
62.00	1454.0
63.00	1212.0
64.00	139.0
65.00	290.0
68.00	2909.0
69.00	2768.0
70.00	237.0
72.00	197.0
73.00	1223.0
74.00	4160.0
75.00	13421.0
76.00	1306.0
76.90	229.0
77.90	120.0
78.90	1099.0
79.90	383.0
80.80	1053.0
81.90	254.0
87.00	1317.0
87.90	1181.0
92.00	839.0
93.00	1186.0
94.00	3397.0
95.00	26720.0
96.00	1972.0
103.80	141.0
105.80	180.0
115.80	105.0
116.90	291.0
117.80	105.0
118.80	152.0
140.80	281.0
143.00	331.0
144.80	151.0
171.90	469.0
172.90	349.0
173.90	24808.0
175.00	1890.0
175.90	24584.0
176.90	1809.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
36.00	241.0
37.00	1247.0
38.00	1117.0
38.90	616.0
39.80	137.0
43.90	592.0
44.90	200.0
47.10	214.0
48.00	117.0
49.00	1081.0
50.00	4939.0
51.00	1756.0
56.00	473.0
56.90	667.0
59.90	207.0
60.90	1472.0
62.00	1435.0
63.00	1266.0
64.00	119.0
64.90	319.0
68.00	2943.0
69.00	2874.0
70.00	273.0
72.10	196.0
73.00	1243.0
74.00	4319.0
75.00	13794.0
76.00	1315.0
76.90	230.0
77.90	145.0
78.90	1112.0
79.90	361.0
80.90	1087.0
81.90	282.0
87.00	1341.0
87.90	1288.0
92.00	834.0
93.00	1209.0
94.00	3450.0
95.00	28392.0
96.00	1957.0
103.90	166.0
105.80	197.0
115.70	100.0
116.90	270.0
117.80	120.0
118.90	128.0
129.90	139.0
140.80	324.0
143.00	333.0
144.80	178.0
171.90	504.0
172.90	385.0
173.90	26480.0
175.00	1999.0
175.90	25944.0
176.90	1808.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056

m/z	Abundance
36.00	274.0
37.00	1158.0
38.00	1026.0
38.90	529.0
39.80	129.0
43.90	495.0
44.90	217.0
46.80	215.0
48.00	125.0
49.00	1037.0
50.00	4595.0
51.00	1630.0
56.00	427.0
56.90	632.0
59.90	222.0
60.90	1378.0
62.00	1279.0
63.00	1185.0
64.90	329.0
68.00	2645.0
69.00	2693.0
70.00	282.0
72.10	146.0
73.00	1194.0
74.00	4493.0
75.00	12962.0
76.00	1165.0
76.90	196.0
77.90	134.0
78.90	1051.0
79.90	317.0
80.90	989.0
81.90	285.0
87.00	1149.0
87.90	1264.0
91.90	745.0
93.00	1216.0
94.00	3147.0
95.00	27184.0
96.00	1813.0
103.90	176.0
105.90	175.0
115.60	102.0
116.80	220.0
117.80	120.0
118.90	124.0
129.90	156.0
140.90	313.0
142.90	324.0
144.80	181.0
171.90	478.0
173.00	363.0
173.90	25800.0
175.00	1876.0
175.90	24560.0
176.90	1587.0

Instrument :
MSVOA_U
ClientSampleId :
BFB056