


Data Path : D:\MassHunter\GCMS\1\data\VU032825\
Data File : VU063317.D
Acq On : 28 Mar 2025 09:36
Operator : MD/SY
Sample : BFB023
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB023

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM031925.M
Title : TRACE VOA SOM01.0
Last Update : Mon Mar 31 15:42:06 2025

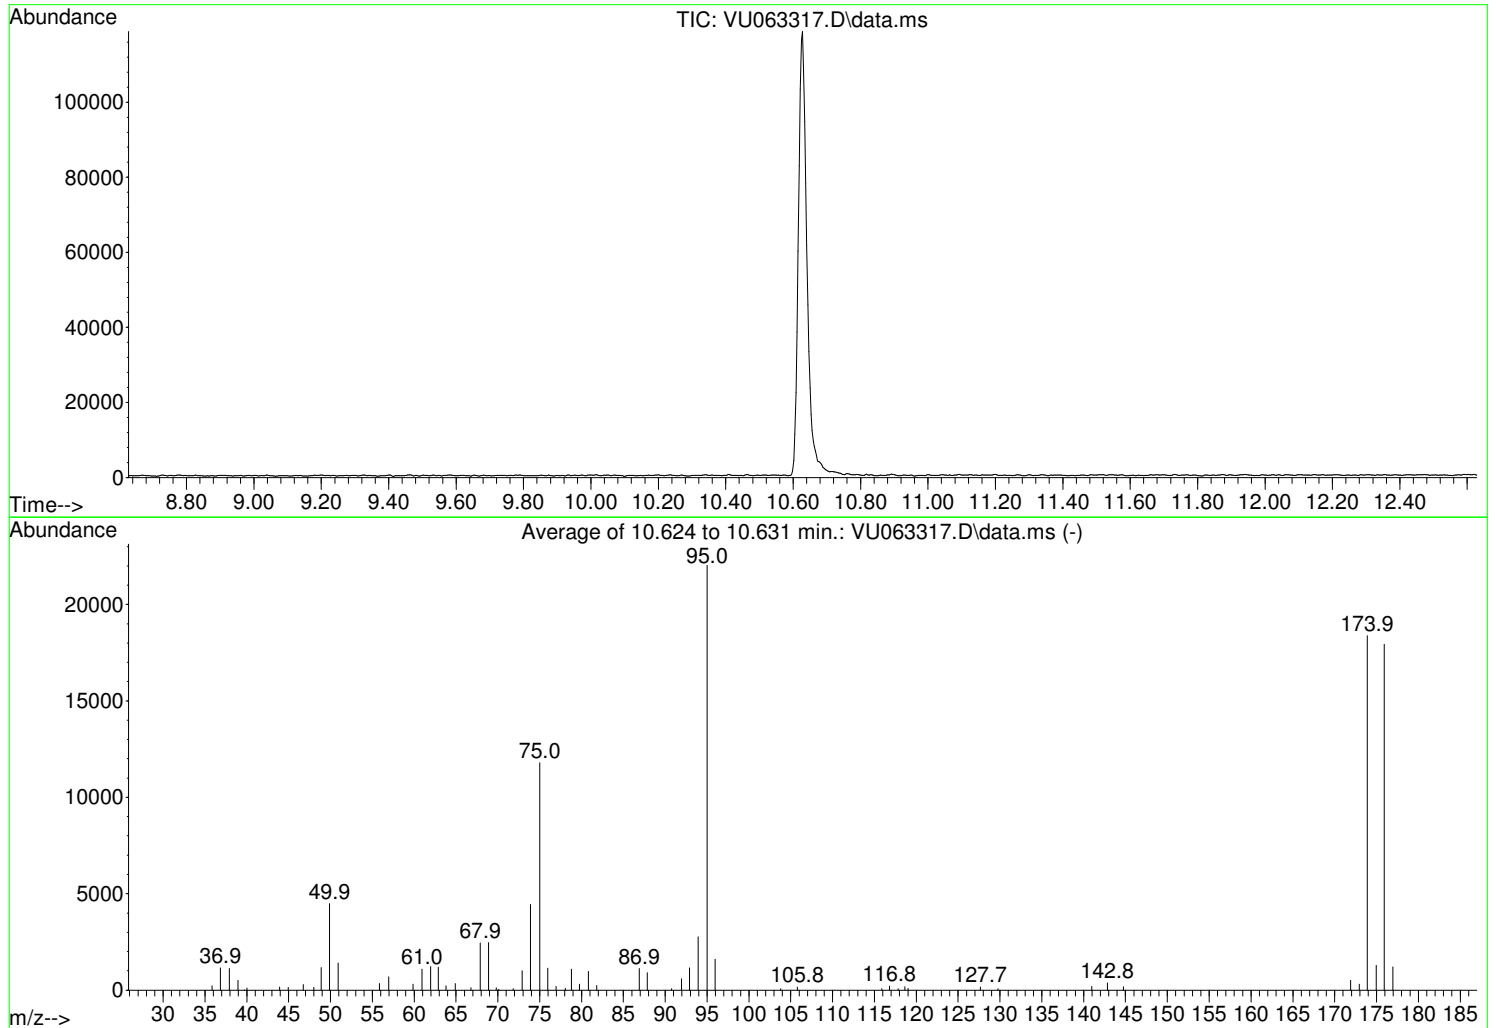

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	4492	PASS
75	95	30	80	53.5	11789	PASS
95	95	100	100	100.0	22032	PASS
96	95	5	9	7.3	1605	PASS
173	174	0.00	2	1.7	312	PASS
174	95	50	120	83.5	18387	PASS
175	174	5	9	7.0	1286	PASS
176	174	95	101	97.5	17936	PASS
177	176	5	9	6.7	1207	PASS

Scan 2891 (10.586 min): VU063317.D\data.ms
BFB023

m/z	Abundance
39.80	113.0
43.90	373.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
35.80	195.0
36.80	1261.0
37.90	1185.0
39.00	526.0
39.70	188.0
43.90	529.0
45.00	158.0
46.70	263.0
48.00	187.0
48.90	1277.0
49.90	4719.0
50.90	1405.0
55.80	342.0
57.00	684.0
59.90	232.0
60.90	1164.0
62.00	1225.0
62.90	1202.0
63.80	239.0
64.90	329.0
66.80	129.0
67.90	2626.0
68.90	2405.0
70.10	109.0
72.90	1123.0
73.90	4573.0
75.00	12134.0
76.00	1074.0
76.90	219.0
78.80	1133.0
79.80	314.0
80.80	955.0
81.80	230.0
86.90	1305.0
87.90	928.0
92.00	610.0
92.90	1029.0
93.90	2911.0
95.00	22624.0
96.00	1662.0
103.80	106.0
105.80	122.0
115.90	104.0
116.80	191.0
117.80	132.0
118.60	140.0
119.00	130.0
127.70	152.0
129.80	129.0
141.00	217.0
142.80	385.0
144.80	146.0
171.90	476.0
172.90	271.0
173.90	18216.0
174.90	1318.0
175.90	17704.0
176.90	1327.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
35.80	239.0
36.90	1164.0
37.90	1155.0
38.90	507.0
39.70	156.0
40.00	155.0
43.90	532.0
44.90	141.0
46.70	309.0
48.00	147.0
48.90	1221.0
49.90	4685.0
50.90	1449.0
55.80	343.0
56.90	708.0
59.80	319.0
60.90	1104.0
62.00	1245.0
62.90	1245.0
63.80	243.0
64.90	367.0
66.80	148.0
67.90	2499.0
68.90	2524.0
69.80	167.0
71.80	105.0
72.90	998.0
73.90	4554.0
75.00	12119.0
76.00	1156.0
77.00	199.0
78.10	159.0
78.80	1127.0
79.70	326.0
80.80	993.0
81.80	247.0
86.90	1155.0
87.80	940.0
90.80	106.0
92.00	571.0
92.90	1192.0
94.00	2875.0
95.00	22688.0
95.90	1638.0
103.80	101.0
105.80	151.0
115.90	102.0
116.80	219.0
117.90	104.0
118.60	187.0
119.00	158.0
127.60	171.0
129.70	116.0
141.00	186.0
142.90	389.0
144.80	187.0
171.90	549.0
173.00	323.0
173.90	18976.0
175.00	1286.0
175.90	18456.0
177.00	1236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
35.90	233.0
36.90	1032.0
37.90	999.0
38.90	477.0
40.00	163.0
43.90	520.0
44.90	131.0
46.80	288.0
47.90	111.0
48.90	1027.0
49.90	4073.0
50.90	1352.0
55.90	330.0
56.90	683.0
59.80	384.0
61.00	976.0
61.90	1205.0
62.90	1104.0
63.80	211.0
64.90	333.0
66.80	106.0
67.90	2202.0
68.90	2475.0
69.80	198.0
71.90	129.0
72.90	908.0
73.90	4185.0
75.00	11113.0
75.90	1178.0
77.00	180.0
78.00	109.0
78.80	983.0
79.70	274.0
80.80	950.0
81.80	270.0
86.90	914.0
87.80	863.0
90.70	112.0
91.90	587.0
92.90	1224.0
94.00	2483.0
95.00	20784.0
95.90	1515.0
105.80	189.0
116.80	217.0
118.70	212.0
127.70	127.0
140.90	162.0
142.90	364.0
144.70	187.0
171.90	503.0
173.00	343.0
173.90	17968.0
175.00	1253.0
175.90	17648.0
176.90	1059.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023