

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
 Data File : VU047752.D
 Acq On : 29 Mar 2022 16:26
 Operator : SY/MD
 Sample : N2081-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	102	rVB	136783	164607	14.68%	1.788%
2	1.919	171	180	206	rBV	107391	149919	13.37%	1.629%
3	2.572	370	383	415	rBV	238346	404047	36.04%	4.390%
4	2.906	483	487	490	rBV2	273	197	0.02%	0.002%
5	2.948	496	500	504	rBV2	314	390	0.03%	0.004%
6	3.047	525	531	539	rVB5	767	1059	0.09%	0.012%
7	3.182	570	573	577	rVB3	316	217	0.02%	0.002%
8	3.260	594	597	601	rBV	214	189	0.02%	0.002%
9	3.510	671	675	677	rBV2	274	238	0.02%	0.003%
10	3.826	770	773	776	rVV	355	240	0.02%	0.003%
11	3.887	788	792	795	rBV3	348	269	0.02%	0.003%
12	3.912	795	800	805	rVB2	322	393	0.04%	0.004%
13	3.944	807	810	814	rBV2	302	223	0.02%	0.002%
14	4.147	863	873	876	rVV2	249	363	0.03%	0.004%
15	4.192	884	887	891	rBV	232	187	0.02%	0.002%
16	4.282	910	915	919	rVB	296	221	0.02%	0.002%
17	4.407	951	954	958	rVV2	269	213	0.02%	0.002%
18	4.430	958	961	968	rVV2	175	232	0.02%	0.003%
19	4.520	984	989	991	rVB	228	194	0.02%	0.002%
20	4.571	998	1005	1007	rVB3	239	181	0.02%	0.002%
21	4.642	1007	1027	1062	rBV	103799	342795	30.57%	3.724%
22	5.067	1142	1159	1184	rBV	202660	442767	39.49%	4.810%
23	5.176	1190	1193	1202	rVB4	533	649	0.06%	0.007%
24	5.231	1202	1210	1214	rBV3	255	374	0.03%	0.004%
25	5.292	1222	1229	1235	rBV4	521	775	0.07%	0.008%
26	5.375	1249	1255	1256	rBV	223	187	0.02%	0.002%
27	5.597	1320	1324	1327	rBV	392	290	0.03%	0.003%
28	5.729	1342	1365	1398	rBV2	415516	1121224	100.00%	12.181%
29	6.038	1455	1461	1462	rBV2	446	405	0.04%	0.004%
30	6.054	1462	1466	1471	rVV3	684	748	0.07%	0.008%
31	6.076	1471	1473	1477	rVV	309	256	0.02%	0.003%
32	6.121	1484	1487	1494	rVB2	300	267	0.02%	0.003%
33	6.250	1512	1527	1558	rVV	328084	626318	55.86%	6.804%
34	6.356	1558	1560	1565	rVB2	556	377	0.03%	0.004%
35	6.494	1598	1603	1605	rBV3	253	238	0.02%	0.003%
36	6.533	1608	1615	1622	rBV6	1190	1704	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
 Data File : VU047752.D
 Acq On : 29 Mar 2022 16:26
 Operator : SY/MD
 Sample : N2081-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.694	1649	1665	1694	rBV	257022	499363	44.54%	5.425%
38	6.809	1694	1701	1704	rBV	632	687	0.06%	0.007%
39	6.941	1741	1742	1752	rVB	242	241	0.02%	0.003%
40	7.047	1769	1775	1780	rBV4	585	748	0.07%	0.008%
41	7.092	1787	1789	1796	rVB3	228	214	0.02%	0.002%
42	7.182	1808	1817	1825	rBV5	1481	2585	0.23%	0.028%
43	7.272	1841	1845	1850	rVB3	176	239	0.02%	0.003%
44	7.330	1856	1863	1864	rBV	242	241	0.02%	0.003%
45	7.430	1890	1894	1897	rBV2	277	196	0.02%	0.002%
46	7.504	1912	1917	1922	rBV2	283	273	0.02%	0.003%
47	7.568	1922	1937	1953	rBV	141066	250027	22.30%	2.716%
48	7.690	1969	1975	1983	rVB4	1269	1516	0.14%	0.016%
49	7.899	2022	2040	2056	rBV	517133	902408	80.48%	9.804%
50	8.179	2115	2127	2143	rBV	98997	171138	15.26%	1.859%
51	8.472	2207	2218	2221	rBV4	858	1336	0.12%	0.015%
52	8.636	2256	2269	2304	rBV	394164	775261	69.14%	8.422%
53	8.861	2334	2339	2345	rVB3	361	467	0.04%	0.005%
54	9.047	2393	2397	2400	rVB3	266	196	0.02%	0.002%
55	9.079	2400	2407	2409	rBV2	273	338	0.03%	0.004%
56	9.121	2417	2420	2426	rVB2	401	301	0.03%	0.003%
57	9.192	2440	2442	2448	rVB2	251	193	0.02%	0.002%
58	9.301	2472	2476	2479	rBV	212	192	0.02%	0.002%
59	9.417	2497	2512	2536	rBV	497108	846897	75.53%	9.201%
60	9.568	2556	2559	2566	rVV2	455	490	0.04%	0.005%
61	9.693	2590	2598	2603	rBV3	1386	1589	0.14%	0.017%
62	9.751	2613	2616	2620	rBV2	208	191	0.02%	0.002%
63	9.970	2680	2684	2688	rVB2	232	190	0.02%	0.002%
64	10.102	2721	2725	2726	rBV	338	265	0.02%	0.003%
65	10.626	2884	2888	2891	rBV2	225	190	0.02%	0.002%
66	10.671	2895	2902	2909	rBV8	2612	4036	0.36%	0.044%
67	10.758	2916	2929	2948	rBV	406787	656244	58.53%	7.129%
68	10.870	2956	2964	2965	rBV3	822	931	0.08%	0.010%
69	10.896	2966	2972	2981	rVV3	2074	2985	0.27%	0.032%
70	10.938	2981	2985	2992	rVB2	256	374	0.03%	0.004%
71	10.980	2995	2998	3001	rVB2	321	229	0.02%	0.002%
72	11.008	3001	3007	3009	rBV2	309	207	0.02%	0.002%
73	11.044	3014	3018	3023	rVB3	373	389	0.03%	0.004%
74	11.086	3023	3031	3034	rBV3	424	546	0.05%	0.006%
75	11.414	3131	3133	3136	rVV2	343	210	0.02%	0.002%
76	11.459	3139	3147	3159	rBV5	2344	4201	0.37%	0.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
 Data File : VU047752.D
 Acq On : 29 Mar 2022 16:26
 Operator : SY/MD
 Sample : N2081-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.568	3176	3181	3183	rBV2	364	362	0.03%	0.004%
78	11.623	3194	3198	3202	rBV2	295	207	0.02%	0.002%
79	11.697	3215	3221	3228	rBV4	1389	1659	0.15%	0.018%
80	11.742	3228	3235	3236	rBV3	753	621	0.06%	0.007%
81	11.812	3244	3257	3279	rBV	574121	902677	80.51%	9.807%
82	11.909	3285	3287	3289	rBV3	482	302	0.03%	0.003%
83	11.944	3292	3298	3302	rVV4	1269	1646	0.15%	0.018%
84	11.973	3303	3307	3315	rVB5	1917	2324	0.21%	0.025%
85	12.192	3360	3375	3393	rVV	543084	889067	79.29%	9.659%
86	12.336	3414	3420	3424	rBV4	797	765	0.07%	0.008%
87	12.381	3429	3434	3438	rVB3	361	389	0.03%	0.004%
88	12.404	3438	3441	3443	rBV2	305	187	0.02%	0.002%
89	12.471	3458	3462	3467	rVB3	356	342	0.03%	0.004%
90	12.507	3468	3473	3476	rBV2	222	244	0.02%	0.003%
91	12.642	3507	3515	3519	rBV3	752	934	0.08%	0.010%
92	12.777	3551	3557	3562	rVB3	891	1222	0.11%	0.013%
93	12.851	3573	3580	3584	rBV3	293	483	0.04%	0.005%
94	13.143	3667	3671	3680	rVB3	427	557	0.05%	0.006%
95	13.497	3776	3781	3784	rBV3	410	409	0.04%	0.004%
96	13.520	3785	3788	3791	rVV	276	201	0.02%	0.002%
97	13.844	3882	3889	3898	rVB3	4221	5865	0.52%	0.064%
98	14.095	3963	3967	3976	rVB3	744	1195	0.11%	0.013%
99	14.336	4039	4042	4052	rVB4	1413	1514	0.14%	0.016%
100	15.143	4291	4293	4295	rBV2	426	231	0.02%	0.003%




Sum of corrected areas: 9204680

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
Data File : VU047752.D
Acq On : 29 Mar 2022 16:26
Operator : SY/MD
Sample : N2081-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

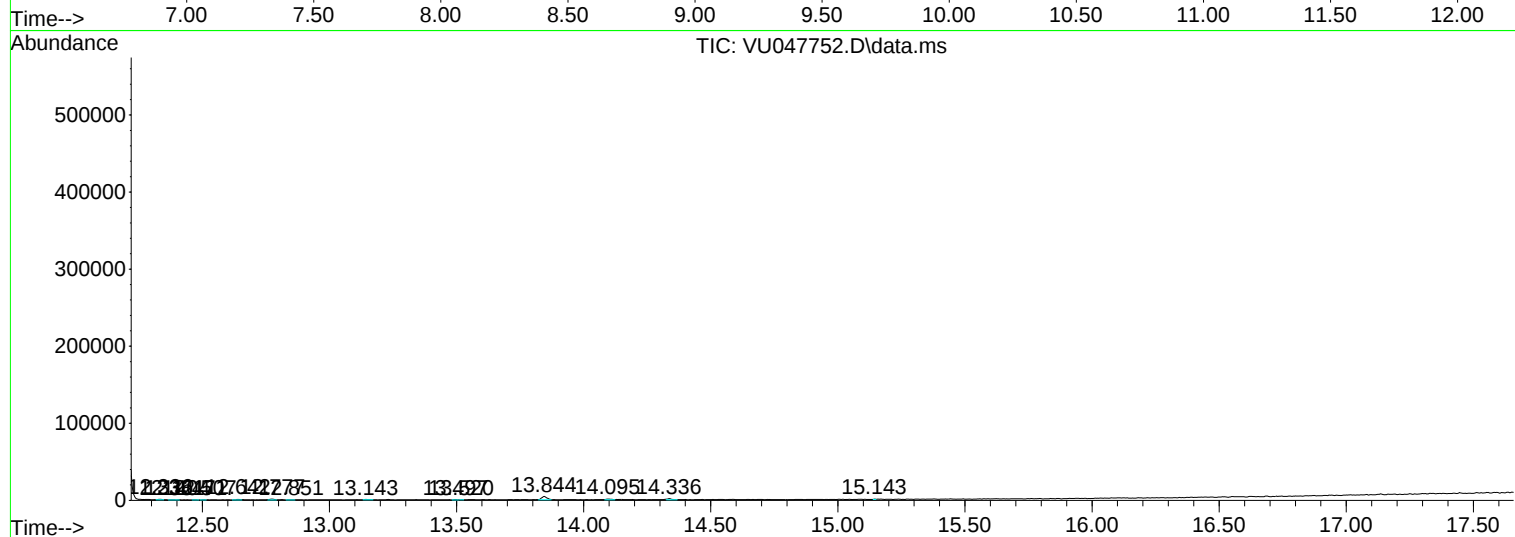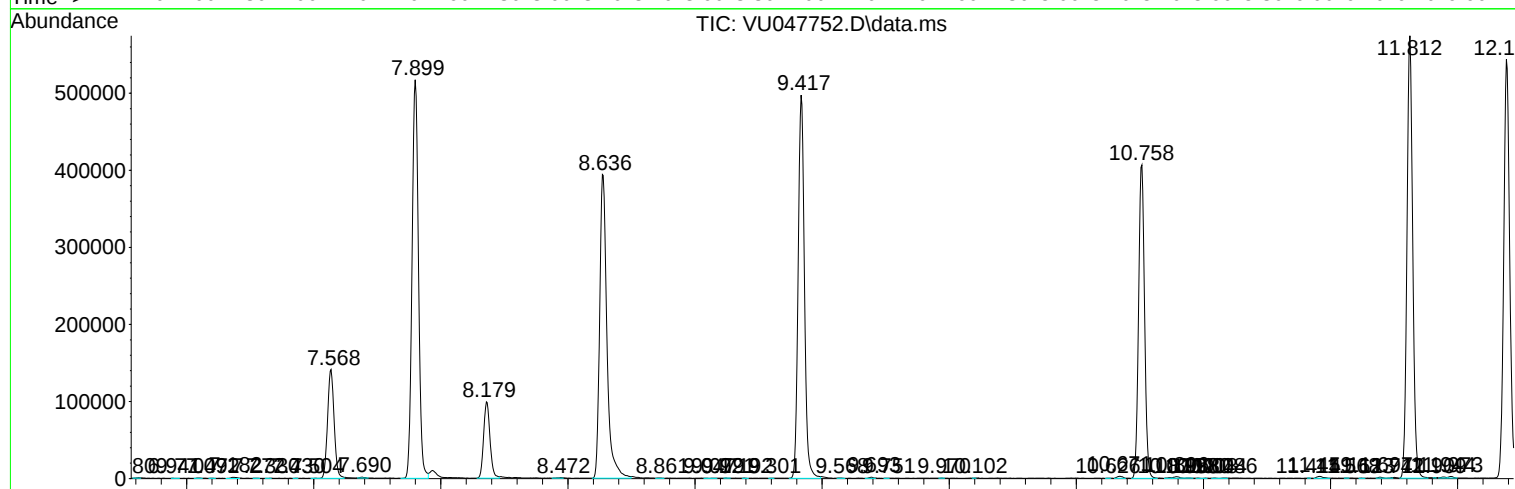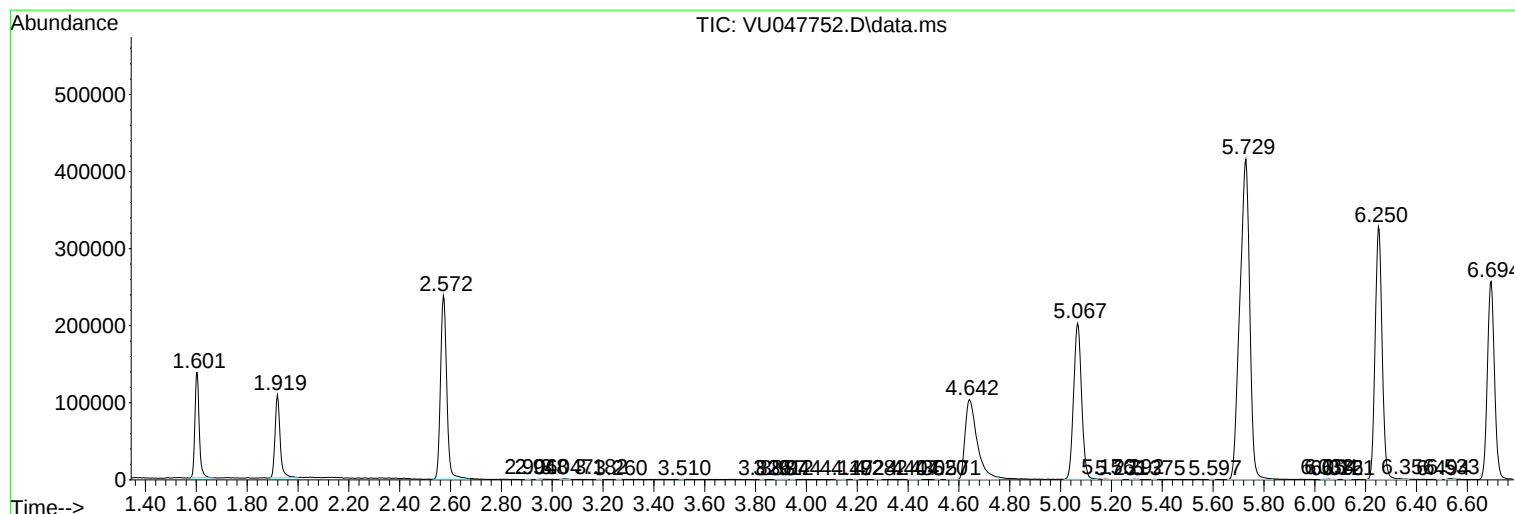

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
Data File : VU047752.D
Acq On : 29 Mar 2022 16:26
Operator : SY/MD
Sample : N2081-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
Data File : VU047752.D
Acq On : 29 Mar 2022 16:26
Operator : SY/MD
Sample : N2081-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc