

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
 Data File : VU047754.D
 Acq On : 29 Mar 2022 17:11
 Operator : SY/MD
 Sample : N2120-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	100	rVB	125337	148941	13.88%	1.704%
2	1.919	171	180	200	rBV	102049	142094	13.24%	1.625%
3	2.572	371	383	420	rBV	220097	373617	34.82%	4.274%
4	2.729	429	432	435	rBV2	267	182	0.02%	0.002%
5	2.954	498	502	503	rBV2	287	208	0.02%	0.002%
6	3.047	525	531	532	rBV2	798	705	0.07%	0.008%
7	3.092	542	545	548	rVB3	262	218	0.02%	0.002%
8	3.160	561	566	569	rVB2	219	190	0.02%	0.002%
9	3.272	596	601	605	rVV3	312	334	0.03%	0.004%
10	3.292	605	607	612	rVB2	237	189	0.02%	0.002%
11	3.372	629	632	635	rVB2	238	163	0.02%	0.002%
12	3.465	657	661	665	rBV2	254	221	0.02%	0.003%
13	4.076	846	851	853	rBV3	263	276	0.03%	0.003%
14	4.250	902	905	910	rVB2	298	254	0.02%	0.003%
15	4.285	910	916	921	rBV2	182	225	0.02%	0.003%
16	4.642	1009	1027	1072	rBV	103737	342326	31.91%	3.916%
17	5.067	1142	1159	1181	rBV	194597	424561	39.57%	4.857%
18	5.192	1195	1198	1201	rVB2	383	252	0.02%	0.003%
19	5.221	1205	1207	1209	rBV	357	203	0.02%	0.002%
20	5.298	1224	1231	1236	rBV3	586	894	0.08%	0.010%
21	5.391	1258	1260	1265	rVB2	333	167	0.02%	0.002%
22	5.571	1313	1316	1321	rBV2	228	173	0.02%	0.002%
23	5.616	1327	1330	1333	rBV2	297	291	0.03%	0.003%
24	5.726	1343	1364	1402	rVV2	394234	1072944	100.00%	12.273%
25	5.893	1413	1416	1419	rBV2	252	166	0.02%	0.002%
26	6.018	1451	1455	1458	rBV2	239	220	0.02%	0.003%
27	6.128	1486	1489	1494	rVB2	438	365	0.03%	0.004%
28	6.195	1505	1510	1512	rBV2	167	161	0.02%	0.002%
29	6.250	1512	1527	1552	rBV	311398	593943	55.36%	6.794%
30	6.481	1597	1599	1603	rVV2	287	163	0.02%	0.002%
31	6.536	1606	1616	1624	rBV4	894	1596	0.15%	0.018%
32	6.565	1624	1625	1629	rVB2	337	165	0.02%	0.002%
33	6.694	1649	1665	1687	rBV	242521	480498	44.78%	5.496%
34	6.915	1728	1734	1736	rBV	172	187	0.02%	0.002%
35	7.047	1772	1775	1777	rBV3	267	202	0.02%	0.002%
36	7.115	1791	1796	1798	rBV2	211	177	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
 Data File : VU047754.D
 Acq On : 29 Mar 2022 17:11
 Operator : SY/MD
 Sample : N2120-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.189	1811	1819	1825	rBV4	1468	2443	0.23%	0.028%
38	7.250	1832	1838	1841	rBV3	286	254	0.02%	0.003%
39	7.417	1886	1890	1894	rVB2	283	219	0.02%	0.003%
40	7.507	1913	1918	1919	rBV2	251	197	0.02%	0.002%
41	7.568	1923	1937	1963	rVV	137312	242423	22.59%	2.773%
42	7.690	1967	1975	1987	rVB5	1132	2212	0.21%	0.025%
43	7.742	1987	1991	1993	rBV2	267	208	0.02%	0.002%
44	7.784	2001	2004	2011	rBV2	441	558	0.05%	0.006%
45	7.838	2016	2021	2026	rBV2	394	391	0.04%	0.004%
46	7.899	2026	2040	2056	rBV	488500	846724	78.92%	9.686%
47	8.182	2115	2128	2143	rBV	95886	166927	15.56%	1.909%
48	8.385	2188	2191	2193	rBV3	297	215	0.02%	0.002%
49	8.436	2203	2207	2210	rBV2	511	398	0.04%	0.005%
50	8.472	2210	2218	2222	rBV3	1062	1320	0.12%	0.015%
51	8.533	2232	2237	2239	rBV2	199	188	0.02%	0.002%
52	8.636	2257	2269	2303	rBV	387672	760457	70.88%	8.699%
53	8.848	2332	2335	2337	rVB3	383	200	0.02%	0.002%
54	8.922	2351	2358	2361	rBV3	231	305	0.03%	0.003%
55	9.156	2428	2431	2435	rVB3	255	172	0.02%	0.002%
56	9.263	2461	2464	2467	rVB2	300	196	0.02%	0.002%
57	9.417	2498	2512	2545	rBV	471055	796658	74.25%	9.113%
58	9.571	2555	2560	2566	rBV4	519	448	0.04%	0.005%
59	9.690	2595	2597	2605	rVB2	635	779	0.07%	0.009%
60	9.767	2617	2621	2623	rBV	217	161	0.02%	0.002%
61	9.906	2660	2664	2667	rBV2	232	204	0.02%	0.002%
62	9.928	2667	2671	2674	rVV2	306	220	0.02%	0.003%
63	10.063	2706	2713	2716	rBV	406	393	0.04%	0.004%
64	10.099	2719	2724	2728	rVV4	531	520	0.05%	0.006%
65	10.128	2731	2733	2737	rVB3	316	196	0.02%	0.002%
66	10.304	2783	2788	2792	rBV2	354	391	0.04%	0.004%
67	10.407	2818	2820	2823	rVB2	308	172	0.02%	0.002%
68	10.475	2836	2841	2842	rBV2	308	247	0.02%	0.003%
69	10.539	2858	2861	2866	rVB2	305	274	0.03%	0.003%
70	10.671	2895	2902	2910	rVB4	2569	3859	0.36%	0.044%
71	10.709	2910	2914	2916	rBV3	252	193	0.02%	0.002%
72	10.758	2916	2929	2949	rVV	395819	643540	59.98%	7.361%
73	10.864	2959	2962	2964	rBV2	348	277	0.03%	0.003%
74	10.883	2964	2968	2969	rBV2	961	648	0.06%	0.007%
75	11.288	3091	3094	3098	rVB2	261	165	0.02%	0.002%
76	11.459	3137	3147	3155	rBV7	2061	3238	0.30%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
 Data File : VU047754.D
 Acq On : 29 Mar 2022 17:11
 Operator : SY/MD
 Sample : N2120-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.513	3161	3164	3167	rBV	353	204	0.02%	0.002%
78	11.574	3179	3183	3185	rBV3	232	192	0.02%	0.002%
79	11.693	3213	3220	3221	rBV2	884	801	0.07%	0.009%
80	11.745	3232	3236	3238	rBV	452	414	0.04%	0.005%
81	11.812	3242	3257	3278	rBV	522570	833161	77.65%	9.530%
82	11.970	3301	3306	3316	rVB4	2160	3206	0.30%	0.037%
83	12.082	3339	3341	3345	rVV2	364	228	0.02%	0.003%
84	12.121	3348	3353	3357	rBV2	281	373	0.03%	0.004%
85	12.192	3361	3375	3397	rVV	502198	830188	77.37%	9.496%
86	12.327	3415	3417	3422	rVV5	694	367	0.03%	0.004%
87	12.352	3422	3425	3430	rVB3	393	314	0.03%	0.004%
88	12.398	3435	3439	3442	rBV3	518	410	0.04%	0.005%
89	12.590	3495	3499	3500	rBV2	253	172	0.02%	0.002%
90	12.635	3507	3513	3514	rBV2	409	400	0.04%	0.005%
91	12.706	3533	3535	3540	rVB	456	348	0.03%	0.004%
92	12.735	3540	3544	3546	rBV2	322	312	0.03%	0.004%
93	12.999	3622	3626	3631	rBV2	392	429	0.04%	0.005%
94	13.156	3669	3675	3677	rBV2	498	477	0.04%	0.005%
95	13.230	3693	3698	3702	rBV3	525	610	0.06%	0.007%
96	13.513	3783	3786	3791	rVB3	341	252	0.02%	0.003%
97	13.848	3887	3890	3899	rVB5	1533	1738	0.16%	0.020%
98	14.092	3963	3966	3967	rBV2	418	258	0.02%	0.003%
99	14.340	4037	4043	4047	rBV3	557	728	0.07%	0.008%
100	15.147	4292	4294	4299	rBV2	553	449	0.04%	0.005%




Sum of corrected areas: 8742092

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
Data File : VU047754.D
Acq On : 29 Mar 2022 17:11
Operator : SY/MD
Sample : N2120-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

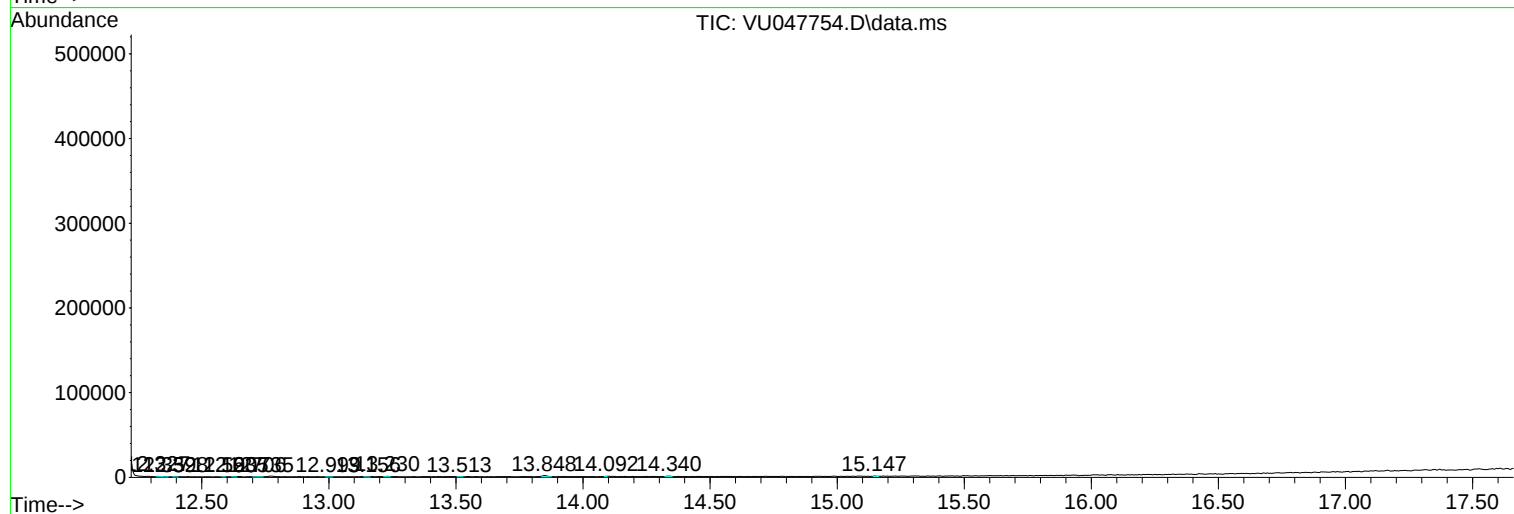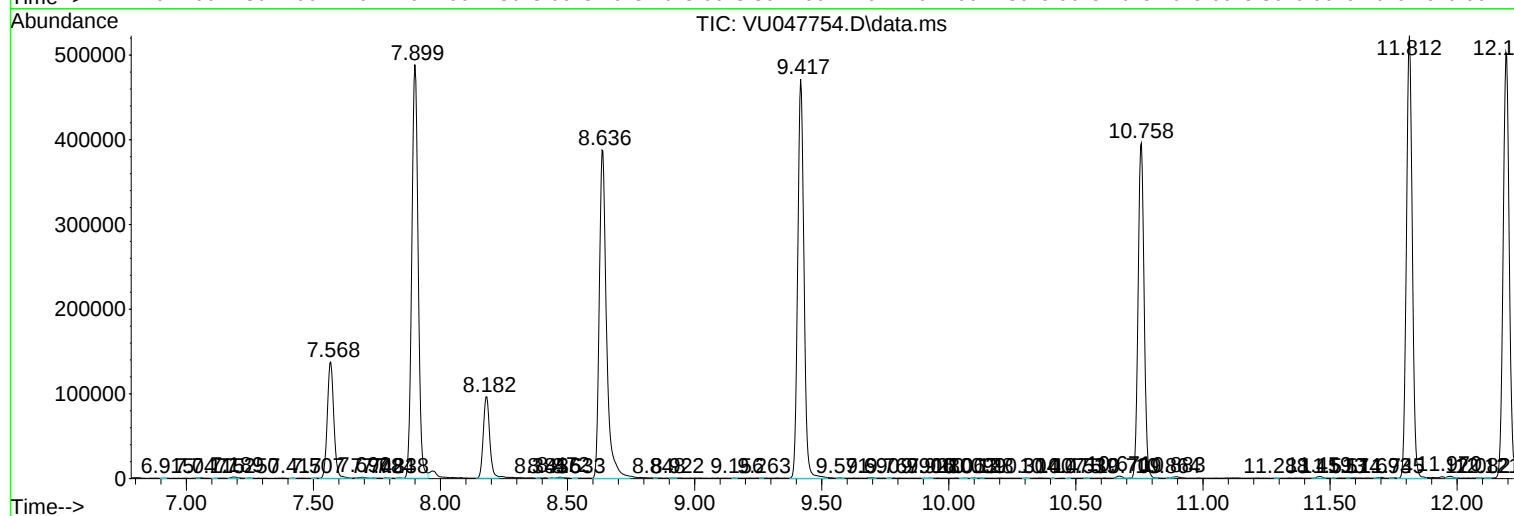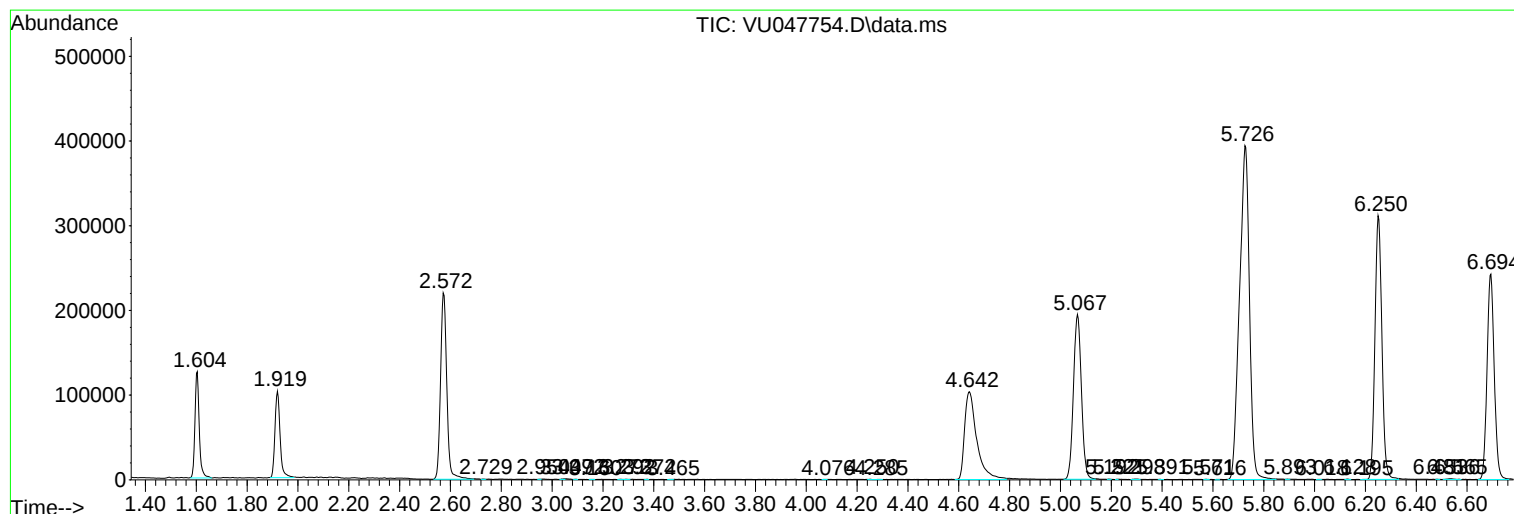

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
Data File : VU047754.D
Acq On : 29 Mar 2022 17:11
Operator : SY/MD
Sample : N2120-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
Data File : VU047754.D
Acq On : 29 Mar 2022 17:11
Operator : SY/MD
Sample : N2120-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------