


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032922\
 Data File : VU047744.D
 Acq On : 29 Mar 2022 09:03
 Operator : SY/MD
 Sample : BFB057
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB057

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 30 01:20:49 2022

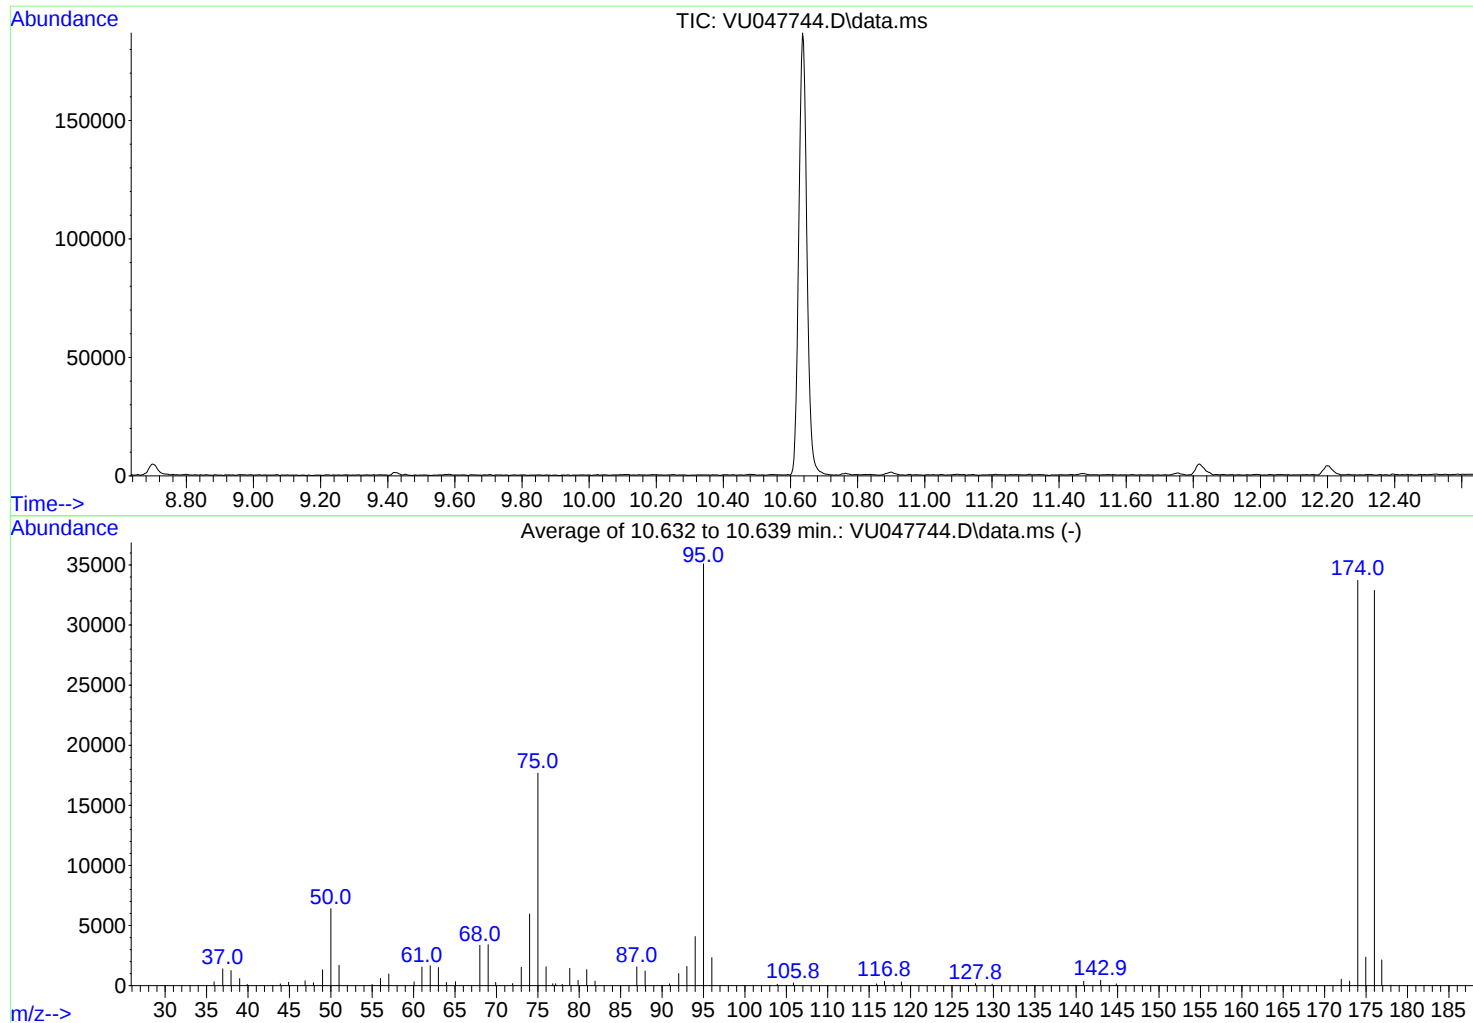

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	6405	PASS
75	95	30	80	50.4	17680	PASS
95	95	100	100	100.0	35091	PASS
96	95	5	9	6.6	2328	PASS
173	174	0.00	2	1.1	376	PASS
174	95	50	120	96.1	33725	PASS
175	174	5	9	7.0	2368	PASS
176	174	95	101	97.5	32877	PASS
177	176	5	9	6.5	2143	PASS

m/z	Abundance
35.90	333.0
37.00	1445.0
38.00	1256.0
39.00	594.0
40.00	227.0
44.00	472.0
44.90	293.0
46.90	404.0
47.90	245.0
49.00	1367.0
50.00	6623.0
51.00	1732.0
55.00	113.0
56.00	616.0
57.00	1013.0
60.10	328.0
61.00	1604.0
62.00	1736.0
63.00	1537.0
64.00	281.0
65.10	338.0
68.00	3454.0
69.00	3543.0
69.90	266.0
72.00	185.0
73.00	1562.0
74.00	6135.0
75.00	18176.0
76.00	1651.0
76.80	216.0
77.10	242.0
77.90	118.0
78.80	1479.0
79.80	450.0
80.90	1370.0
81.90	381.0
86.90	1599.0
87.90	1230.0
90.90	156.0
92.00	1051.0
93.00	1643.0
94.00	4216.0
95.00	36112.0
96.00	2393.0
103.90	119.0
105.90	233.0
115.90	152.0
116.80	389.0
117.90	109.0
118.90	322.0
127.80	179.0
129.90	131.0
140.90	383.0
142.90	461.0
144.80	159.0
172.00	558.0
173.00	403.0
174.00	34672.0
175.00	2392.0
176.00	33824.0
176.90	2214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
35.90	338.0
37.00	1409.0
37.90	1295.0
39.00	624.0
40.00	192.0
43.90	452.0
44.90	267.0
46.90	445.0
48.00	252.0
49.00	1240.0
50.00	6339.0
51.00	1756.0
55.00	104.0
56.00	592.0
57.00	887.0
60.00	323.0
61.00	1528.0
62.00	1686.0
63.00	1455.0
64.00	289.0
65.00	353.0
68.00	3348.0
69.00	3414.0
69.90	260.0
72.00	182.0
73.00	1515.0
74.00	5911.0
75.00	17720.0
76.00	1572.0
76.80	273.0
78.00	103.0
78.90	1419.0
79.90	446.0
80.90	1370.0
81.90	352.0
87.00	1500.0
88.00	1209.0
91.00	141.0
92.00	1037.0
93.00	1646.0
94.00	4317.0
95.00	35000.0
96.00	2304.0
103.90	141.0
105.80	242.0
115.90	151.0
116.90	323.0
117.90	110.0
118.90	316.0
127.90	138.0
129.80	124.0
140.90	404.0
143.00	469.0
144.90	147.0
172.00	552.0
173.00	329.0
174.00	34664.0
174.90	2458.0
176.00	33640.0
176.90	2159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
39.80	111.0
43.90	316.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
39.80	111.0
43.90	316.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
35.90	287.0
36.90	1341.0
38.00	1194.0
39.00	558.0
40.00	225.0
44.00	480.0
44.90	266.0
46.90	362.0
47.80	226.0
49.00	1349.0
50.00	6252.0
51.00	1580.0
55.00	105.0
56.00	597.0
57.00	999.0
60.00	326.0
61.00	1520.0
62.00	1545.0
63.00	1515.0
63.90	238.0
65.10	295.0
68.00	3253.0
69.00	3281.0
69.90	285.0
71.90	159.0
73.00	1516.0
74.00	5830.0
75.00	17144.0
76.00	1482.0
77.20	219.0
77.90	112.0
78.80	1435.0
79.80	442.0
80.90	1248.0
81.90	381.0
87.00	1559.0
87.90	1218.0
90.80	138.0
92.00	941.0
93.00	1493.0
94.00	3745.0
95.00	34160.0
96.00	2288.0
103.90	110.0
105.90	194.0
115.90	141.0
116.80	378.0
118.90	284.0
127.80	193.0
129.90	145.0
140.90	314.0
142.90	444.0
144.80	152.0
172.00	492.0
173.00	396.0
174.00	31840.0
174.90	2253.0
176.00	31168.0
176.90	2055.0
178.00	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057