

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU033020\
 Data File : VU037458.D
 Acq On : 30 Mar 2020 13:04
 Operator : JC/MD
 Sample : L2001-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 GAWF9

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 6:12:25 PM

Quant Time: Mar 31 01:49:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 31 01:26:39 2020
 Response via : Initial Calibration

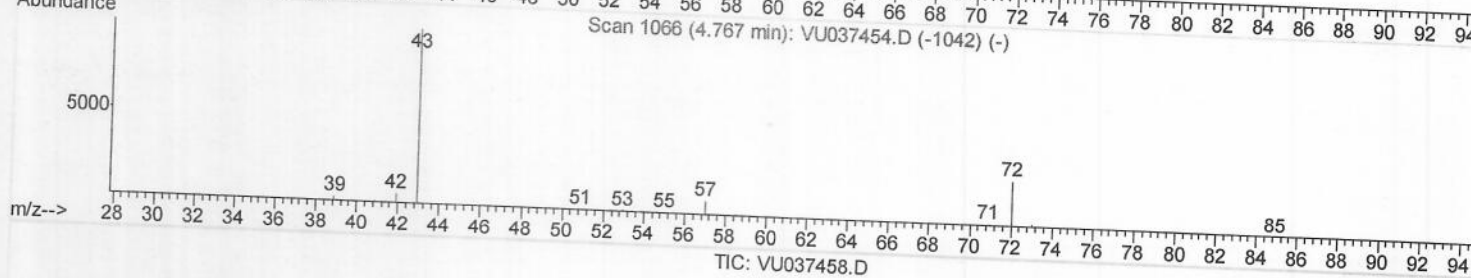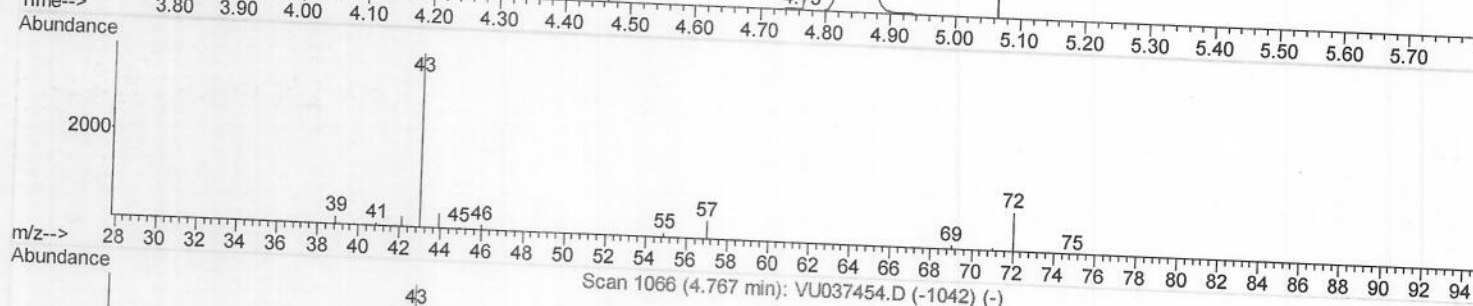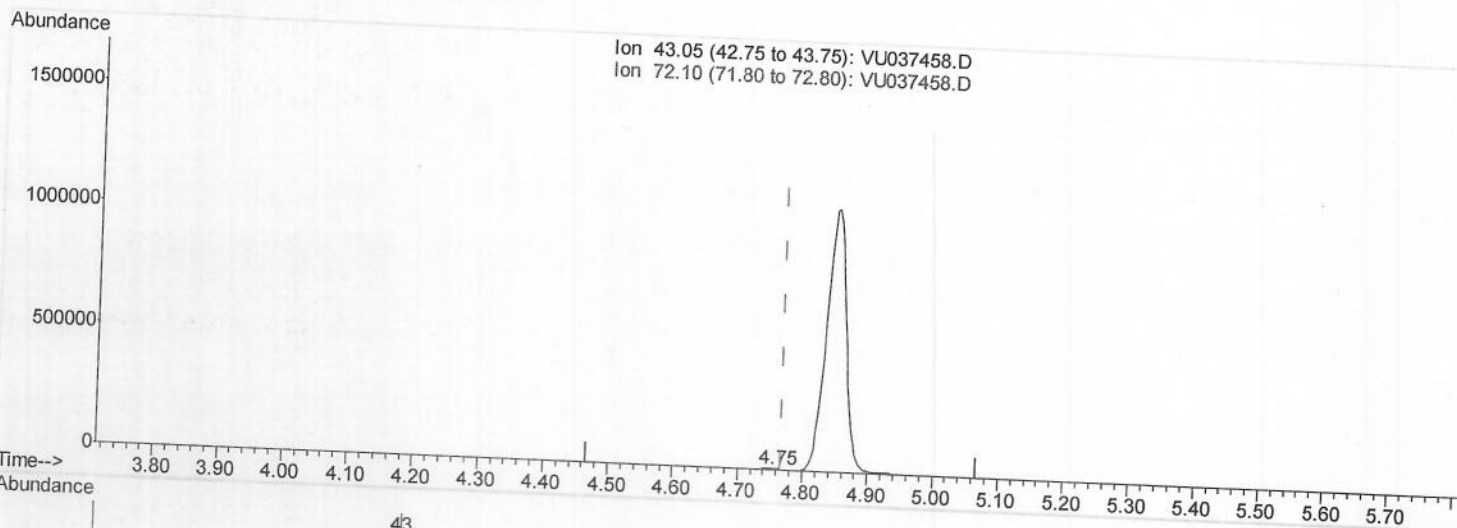

(21) 2-Butanone (T)

4.755min (-0.013) 5.27ug/L m

response 9698

Ion Exp% Act%

43.05 100 100

72.10 28.40 11.87#

0.00 0.00 0.00

0.00 0.00 0.00

SY
 03/31/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU033020\
 Data File : VU037458.D
 Acq On : 30 Mar 2020 13:04
 Operator : JC/MD
 Sample : L2001-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 GAWF9

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 6:12:25 PM

Quant Time: Mar 31 01:54:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 31 01:26:39 2020
 Response via : Initial Calibration

Internal Standards		R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene		6.28	114	93718	5.00	ug/L	0.00
28) Chlorobenzene-d5		9.44	117	87852	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4		11.83	152	43705	5.00	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.61	65	28885	4.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.60%	
7) Chloroethane-d5		1.93	69	27850	5.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.40%	
11) 1,1-Dichloroethene-d2		2.59	63	44991	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%	
20) 2-Butanone-d5		4.67	46	105671	56.04	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.08%	
24) Chloroform-d		5.11	84	61706	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%	
26) 1,2-Dichloroethane-d4		5.74	65	38021	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.20%	
32) Benzene-d6		5.76	84	123077	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%	
36) 1,2-Dichloropropane-d6		6.72	67	42134	5.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.40%	
41) Toluene-d8		7.92	98	111193	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%	
43) trans-1,3-Dichloropropene-		8.20	79	16811	4.26	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.20%	
46) 2-Hexanone-d5		8.66	63	88697	56.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.96%	
57) 1,1,2,2-Tetrachloroethane-		10.77	84	35511	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.80%	
64) 1,2-Dichlorobenzene-d4		12.21	152	41695	4.84	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.80%	
Target Compounds							
13) Acetone		2.66	43	82890	76.506	ug/L	Ovalue 99
15) Methyl Acetate		2.98	43	89893	29.697	ug/L	97
21) 2-Butanone		4.75	43	9698m	5.265	ug/L	
25) Chloroform		5.13	83	3480	0.275	ug/L #	69
31) Carbon tetrachloride		5.56	117	169787	17.809	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SY
 03/31/2020

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU033020\
 Data File : VU037458.D
 Acq On : 30 Mar 2020 13:04
 Operator : JC/MD
 Sample : L2001-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAWF9

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 6:12:25 PM

Quant Time: Mar 31 01:54:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 31 01:26:39 2020
 Response via : Initial Calibration

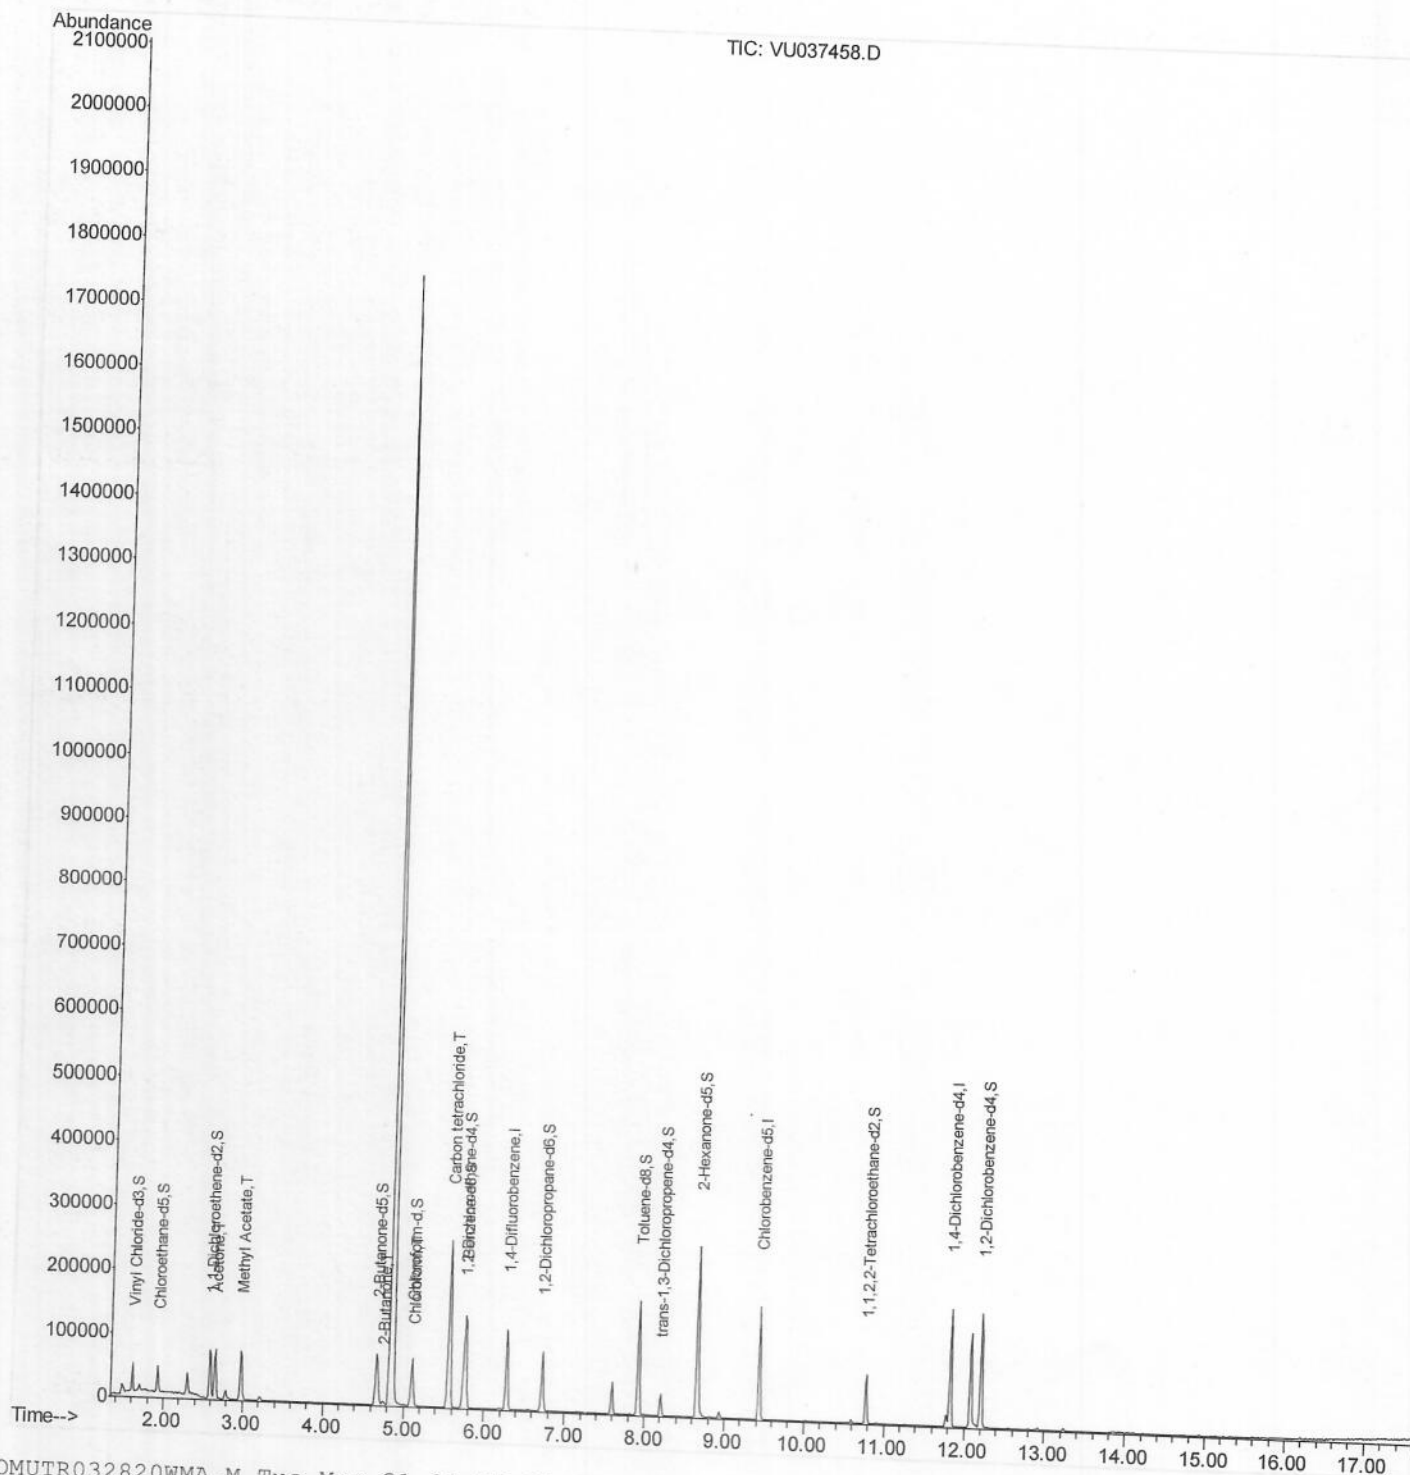

SOMUTR032820WMA.M Tue Mar 31 01:53:21 2020

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU033020\
 Data File : VU037458.D
 Acq On : 30 Mar 2020 13:04
 Operator : JC/MD
 Sample : L2001-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 GAWF9

Manual Integrations
 APPROVED

MMDadoda
 3/31/2020 6:12:25 PM

Quant Time: Mar 31 01:49:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 31 01:26:39 2020
 Response via : Initial Calibration

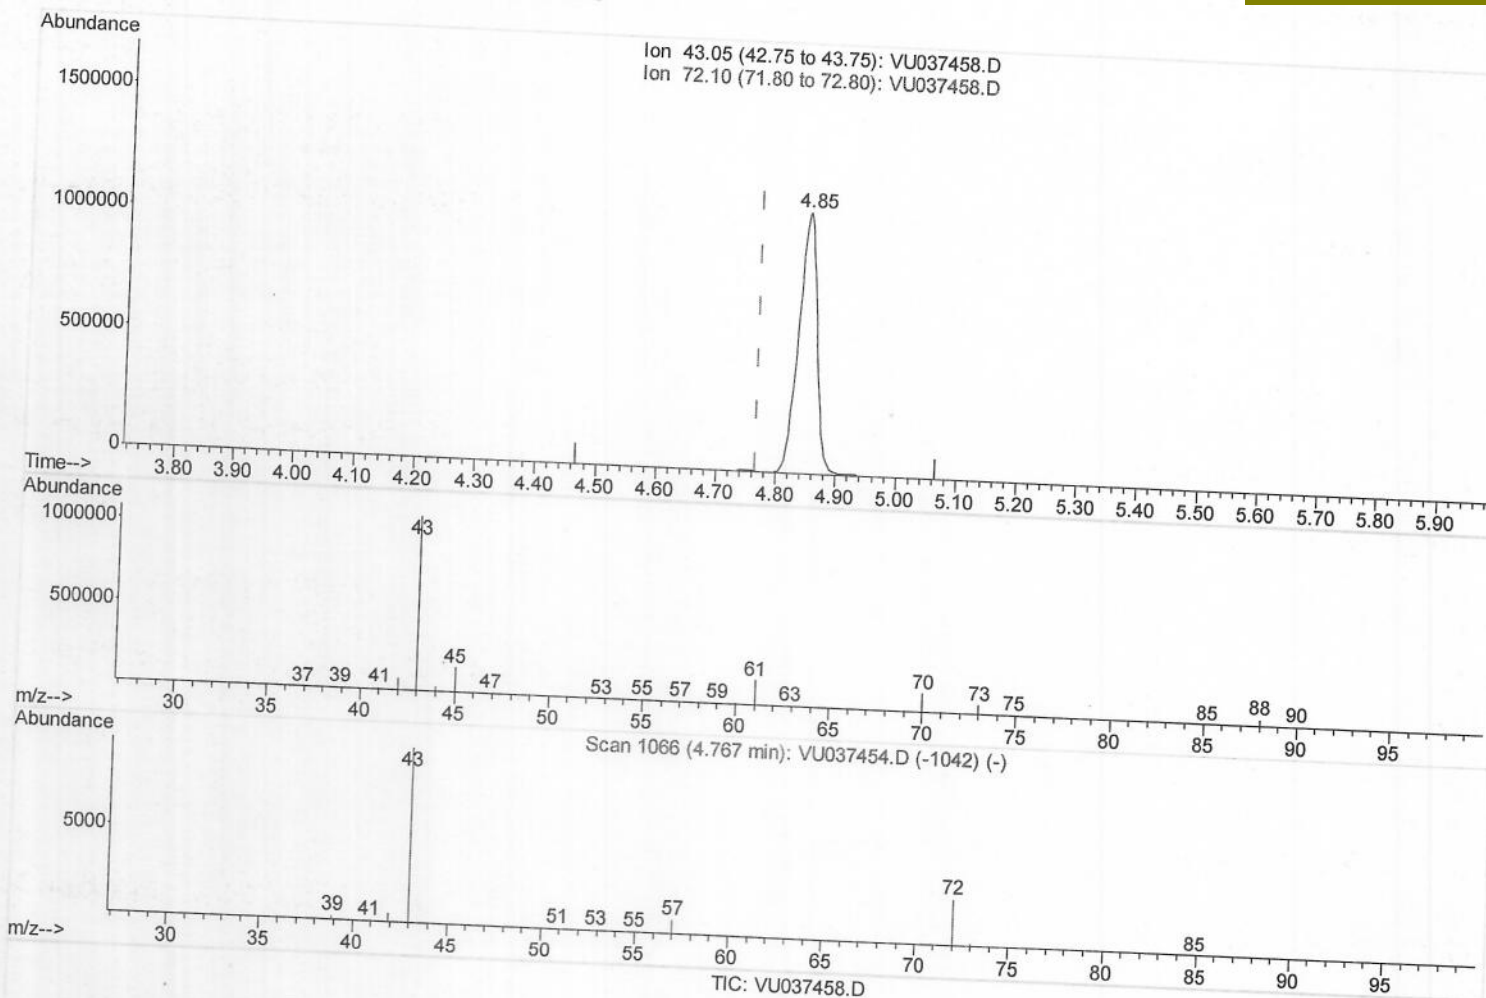

(21) 2-Butanone (T)

4.848min (+0.080) 1247.03ug/L

response 2296884

Ion	Exp%	Act%
43.05	100	100
72.10	28.40	0.05#
0.00	0.00	0.00
0.00	0.00	0.00