

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU033020\
 Data File : VU037480.D
 Acq On : 31 Mar 2020 00:20
 Operator : JC/MD
 Sample : L2002-10DL 40X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAWH2DL

Quant Time: Mar 31 05:09:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 31 04:01:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	91640	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	85582	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	40385	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	27553	4.07	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.40%
7) Chloroethane-d5	1.93	69	26127	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.20%
11) 1,1-Dichloroethene-d2	2.59	63	42874	3.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.00%
20) 2-Butanone-d5	4.67	46	105720	57.34	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.68%
24) Chloroform-d	5.10	84	59067	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.40%
26) 1,2-Dichloroethane-d4	5.74	65	34257	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
32) Benzene-d6	5.76	84	117836	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
36) 1,2-Dichloropropane-d6	6.72	67	40571	4.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.20%
41) Toluene-d8	7.93	98	106143	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	8.20	79	17826	4.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.60%
46) 2-Hexanone-d5	8.66	63	86728	56.69	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.38%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	34194	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.60%
64) 1,2-Dichlorobenzene-d4	12.21	152	39012	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds					Ovalue
31) Carbon tetrachloride	5.56	117	99674	10.732 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU033020\
Data File : VU037480.D
Acq On : 31 Mar 2020 00:20
Operator : JC/MD
Sample : L2002-10DL 40X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAWH2DL

Quant Time: Mar 31 05:09:20 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Mar 31 04:01:00 2020
Response via : Initial Calibration

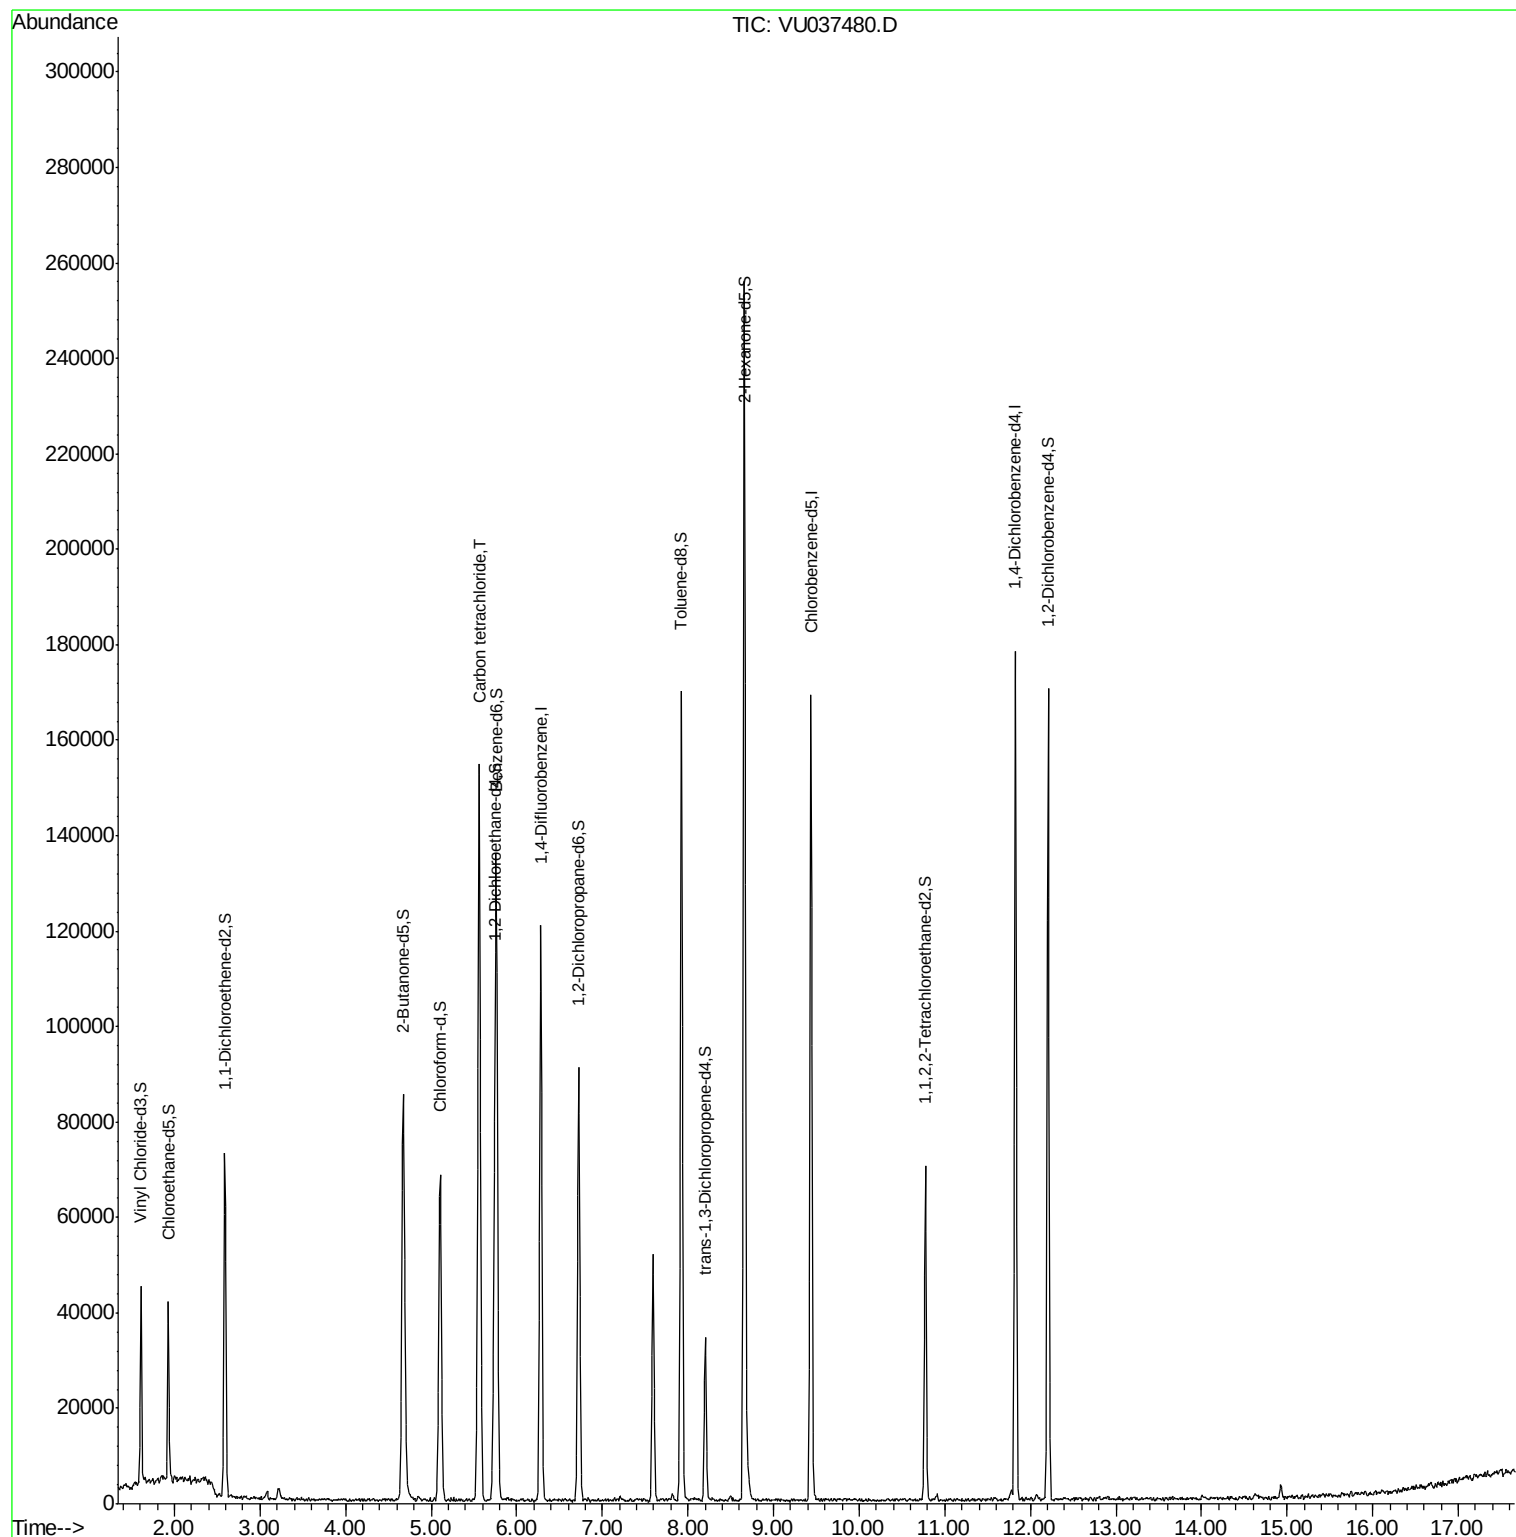

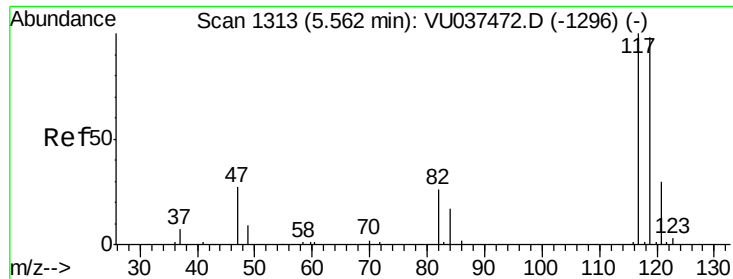

#31

Carbon tetrachloride

Concen: 10.732 ug/L

RT: 5.56 min Scan# 1313

Delta R.T. 0.00 min

Lab File: VU037480.D

Acq: 31 Mar 2020 00:20

Instrument :

MSVOA_U

ClientSampleId :

GAWH2DL

Tot Ion:117 Resp: 99674

Ion Ratio Lower Upper

117 100

119 96.8 77.7 116.5

