


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU033020\
 Data File : VU037453.D
 Acq On : 30 Mar 2020 08:18
 Operator : JC/MD
 Sample : BFB09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB09

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Mar 31 16:20:39 2020

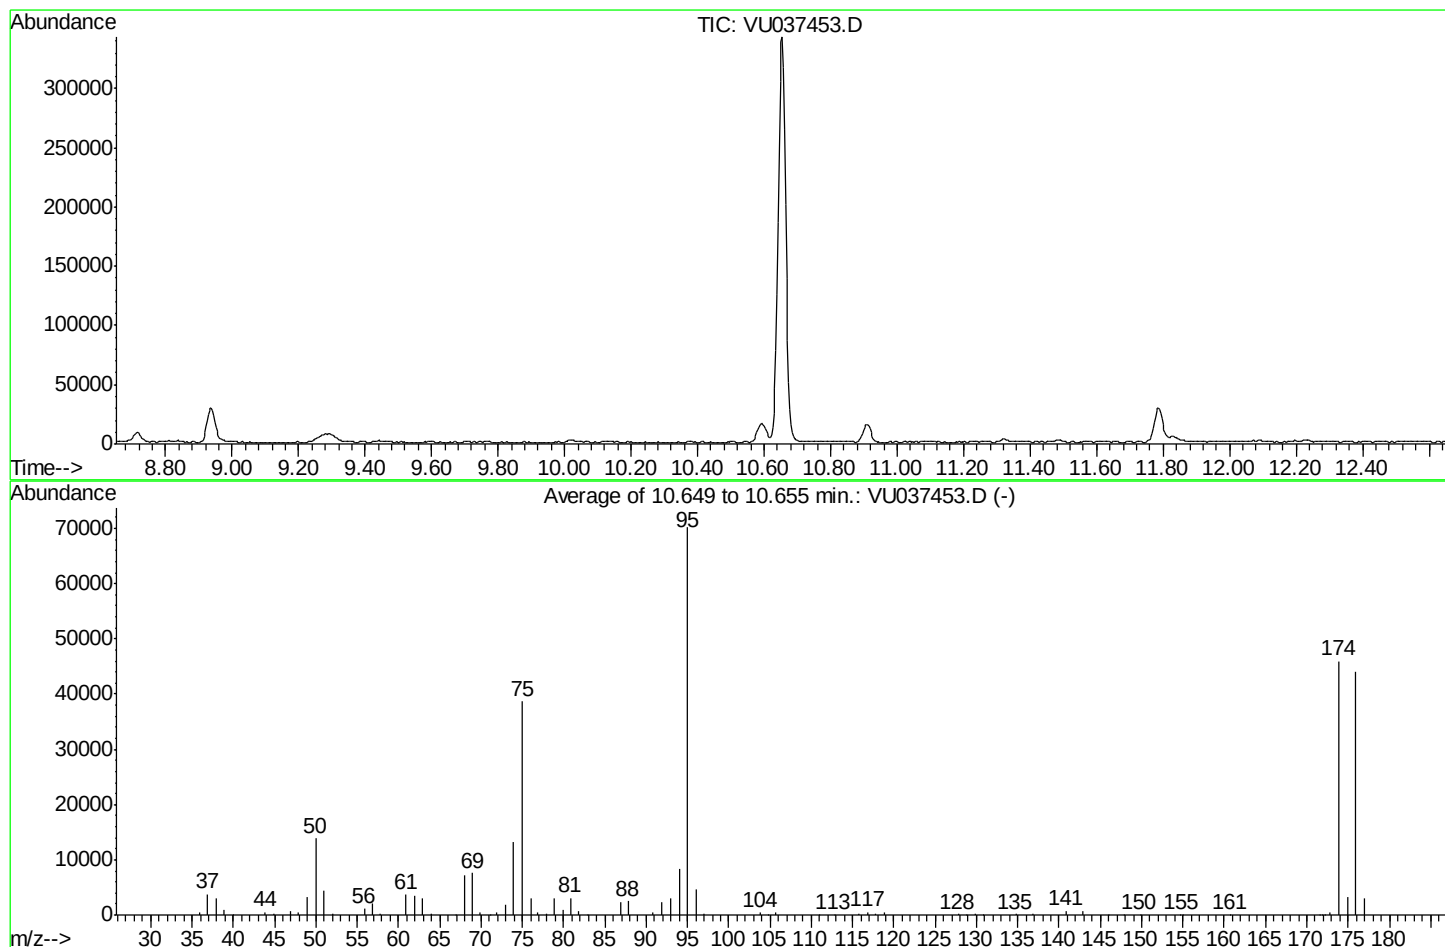

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	13871	PASS
75	95	30	80	55.1	38714	PASS
95	95	100	100	100.0	70213	PASS
96	95	5	9	6.7	4702	PASS
173	174	0.00	2	0.9	428	PASS
174	95	50	120	65.6	46026	PASS
175	174	5	9	7.3	3370	PASS
176	174	95	101	95.9	44117	PASS
177	176	5	9	6.7	2973	PASS

m/z	Abundance
35.90	714.0
36.90	3567.0
37.90	2884.0
39.00	1226.0
39.90	164.0
40.90	185.0
42.00	104.0
42.90	272.0
44.00	905.0
44.90	752.0
47.00	783.0
47.90	367.0
48.90	3029.0
49.90	12897.0
51.00	4428.0
52.00	251.0
54.90	449.0
55.90	1108.0
56.90	2140.0
57.80	131.0
59.90	815.0
61.00	3730.0
61.90	3333.0
62.90	2691.0
63.90	245.0
66.80	282.0
68.00	6770.0
69.00	7217.0
69.90	484.0
70.90	155.0
71.90	364.0
72.90	3129.0
74.00	12360.0
75.00	36536.0
76.00	2785.0
76.90	346.0
77.80	166.0
78.90	2868.0
79.90	769.0
80.80	2775.0
81.80	640.0
82.90	126.0
86.90	2531.0
87.90	2189.0
90.80	460.0
91.90	2282.0
92.90	2939.0
94.00	7862.0
95.00	65448.0
96.00	4433.0
97.00	178.0
103.80	319.0
105.70	336.0
111.00	117.0
112.80	128.0
115.80	305.0
116.90	455.0
117.80	236.0
118.80	431.0
127.80	196.0
128.80	147.0
129.80	187.0
130.70	119.0
134.80	158.0
136.90	117.0
140.90	747.0
142.90	762.0
154.70	108.0
160.80	120.0
171.90	151.0
172.90	397.0
173.90	41960.0
174.90	2920.0
175.90	39648.0
176.90	2736.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
35.90	718.0
36.90	3881.0
37.90	3161.0
39.00	1528.0
39.90	203.0
40.90	178.0
41.90	122.0
43.00	299.0
44.00	883.0
44.90	754.0
47.00	730.0
47.90	481.0
48.90	3291.0
50.00	14241.0
51.00	4554.0
52.00	221.0
54.90	476.0
55.90	1357.0
56.90	2485.0
57.80	147.0
59.90	800.0
61.00	4000.0
61.90	3627.0
63.00	3051.0
64.00	252.0
66.90	229.0
68.00	7404.0
69.00	7992.0
69.90	513.0
71.10	156.0
71.90	404.0
72.90	3282.0
74.00	13681.0
75.00	39784.0
76.00	3020.0
76.90	371.0
77.80	216.0
78.90	3147.0
79.90	897.0
80.90	3159.0
81.80	690.0
82.90	180.0
86.90	2458.0
87.80	2545.0
90.80	454.0
91.90	2433.0
93.00	3148.0
94.00	8743.0
95.00	72664.0
96.00	4958.0
97.00	200.0
103.90	419.0
105.70	396.0
115.80	310.0
116.90	544.0
117.80	283.0
118.80	427.0
127.80	218.0
128.80	143.0
129.80	211.0
130.70	123.0
134.70	145.0
136.90	148.0
140.90	803.0
142.90	756.0
147.80	103.0
154.90	108.0
160.70	102.0
172.10	165.0
172.90	458.0
173.90	47184.0
174.90	3479.0
175.90	45264.0
176.90	3047.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
35.90	760.0
36.90	3773.0
38.00	3229.0
38.90	1629.0
39.90	194.0
41.00	196.0
41.90	125.0
43.00	365.0
43.90	822.0
44.90	713.0
47.00	730.0
47.90	557.0
48.90	3216.0
50.00	14476.0
50.90	4248.0
52.00	196.0
54.90	477.0
55.90	1448.0
57.00	2572.0
57.80	158.0
60.00	786.0
61.00	3895.0
61.90	3641.0
63.00	2987.0
64.00	237.0
66.90	209.0
68.00	7465.0
69.00	8054.0
69.90	522.0
71.10	157.0
71.90	381.0
72.90	3233.0
74.00	13805.0
75.00	39824.0
76.00	3165.0
76.90	421.0
77.90	287.0
78.80	3218.0
79.90	870.0
80.90	3303.0
81.80	687.0
83.00	202.0
85.20	128.0
86.90	2414.0
87.80	2751.0
90.90	438.0
91.90	2183.0
93.00	3050.0
94.00	8758.0
95.00	72528.0
96.00	4716.0
96.90	210.0
103.90	453.0
104.80	110.0
105.80	405.0
115.80	270.0
116.90	562.0
117.80	289.0
118.80	375.0
127.80	273.0
129.80	242.0
130.80	115.0
134.90	122.0
136.80	158.0
140.90	743.0
142.80	737.0
145.90	127.0
149.80	149.0
154.90	154.0
171.60	148.0
172.80	431.0
173.90	48936.0
174.90	3712.0
175.90	47440.0
176.90	3137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
35.90	205.0
37.80	120.0
38.90	438.0
39.90	141.0
41.00	694.0
41.90	487.0
42.90	632.0
43.90	296.0
44.90	540.0
53.00	119.0
54.90	577.0
56.00	224.0
56.90	273.0
58.10	131.0
58.90	107.0
59.90	3311.0
60.90	184.0
66.90	125.0
68.90	156.0
71.00	205.0
72.90	1414.0
73.80	147.0
82.90	114.0
85.00	146.0
86.90	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09