


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040224\
Data File : VU058324.D
Acq On : 02 Apr 2024 08:29
Operator : MD/SY
Sample : BFB134
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB134

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 03 01:56:26 2024

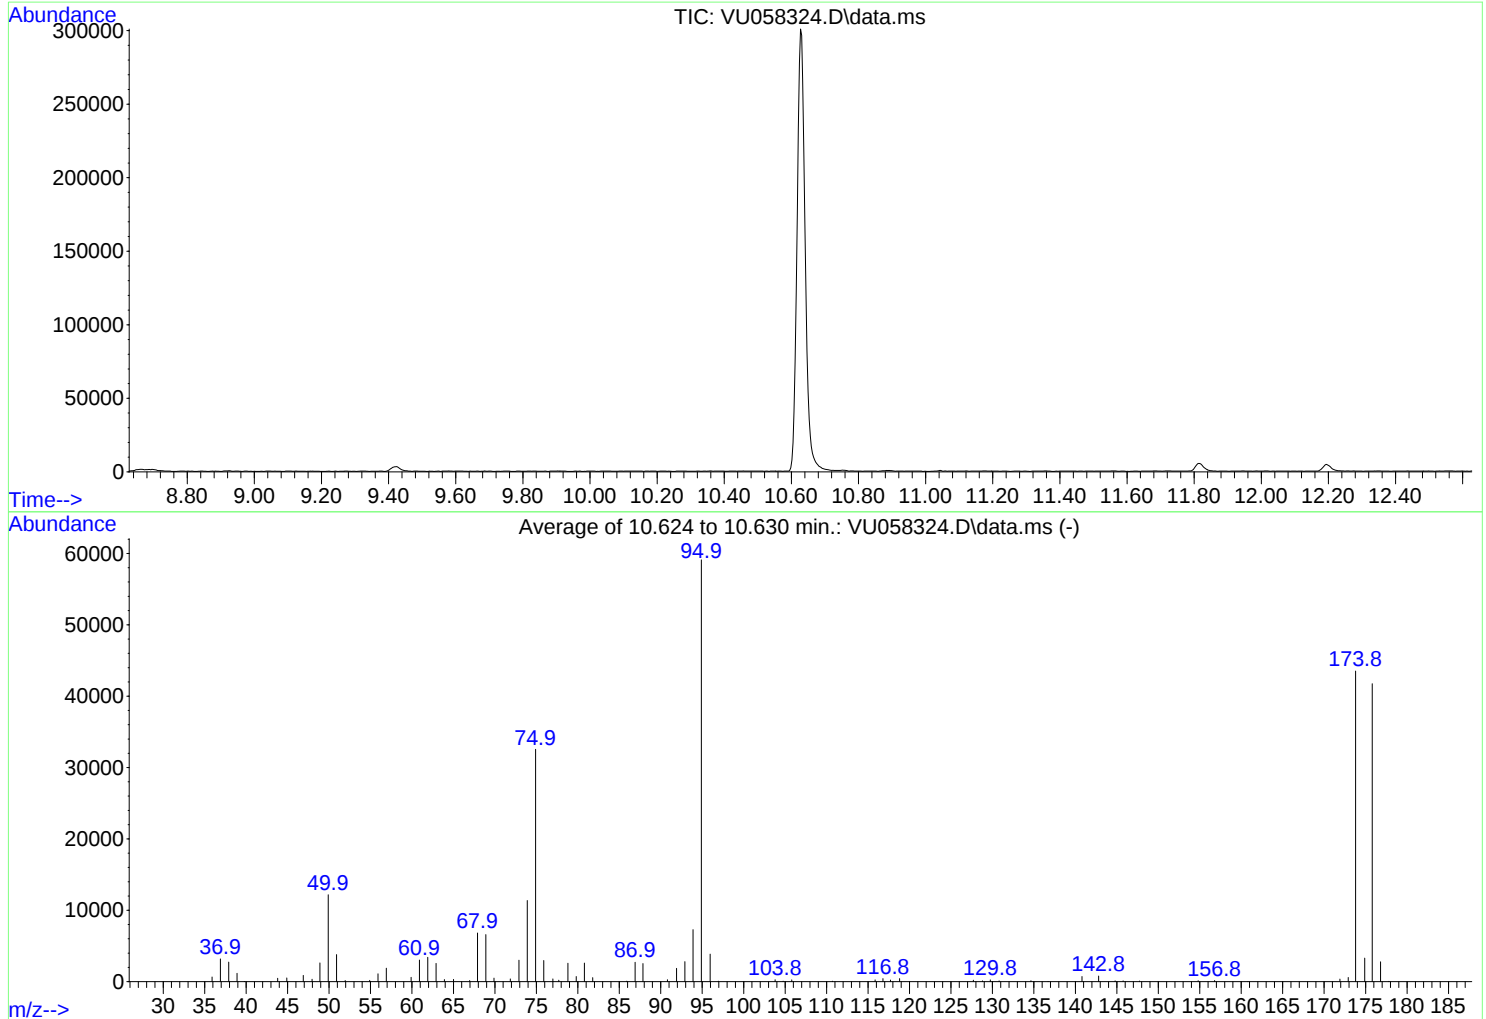

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	12167	PASS
75	95	30	80	55.1	32549	PASS
95	95	100	100	100.0	59107	PASS
96	95	5	9	6.5	3860	PASS
173	174	0.00	2	1.3	574	PASS
174	95	50	120	73.6	43517	PASS
175	174	5	9	7.6	3292	PASS
176	174	95	101	96.0	41755	PASS
177	176	5	9	6.7	2788	PASS

m/z	Abundance
39.80	386.0
43.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

m/z	Abundance
35.90	668.0
36.90	3163.0
37.90	2668.0
38.90	1143.0
39.80	367.0
43.80	583.0
44.90	545.0
46.90	886.0
48.00	336.0
48.90	2663.0
49.90	11986.0
50.90	3711.0
51.90	151.0
54.90	171.0
55.90	1073.0
56.90	1751.0
59.80	628.0
60.90	2995.0
61.90	3378.0
62.90	2490.0
63.90	265.0
65.00	319.0
66.90	145.0
67.90	6705.0
68.90	6237.0
69.90	412.0
71.80	363.0
72.90	2902.0
73.90	11072.0
74.90	31256.0
75.90	2834.0
77.00	404.0
77.70	144.0
78.80	2377.0
79.80	694.0
80.80	2538.0
81.80	578.0
86.90	2521.0
87.80	2340.0
90.80	270.0
91.90	1785.0
92.90	2664.0
93.90	6911.0
94.90	56464.0
95.90	3672.0
103.80	275.0
104.70	109.0
105.80	212.0
115.80	249.0
116.80	407.0
117.60	224.0
118.80	406.0
127.70	182.0
128.80	116.0
129.80	203.0
130.80	127.0
134.60	145.0
140.80	617.0
142.80	758.0
144.80	107.0
145.70	121.0
154.90	143.0
156.80	157.0
171.90	338.0
172.90	571.0
173.80	40208.0
174.90	3209.0
175.80	39096.0
176.80	2684.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

m/z	Abundance
35.90	676.0
36.90	3278.0
37.90	2814.0
38.90	1235.0
39.80	415.0
43.80	604.0
44.90	527.0
46.90	930.0
48.00	326.0
48.90	2723.0
49.90	12509.0
50.90	3909.0
51.90	165.0
54.90	179.0
55.90	1128.0
56.90	1927.0
59.90	634.0
60.90	3125.0
61.90	3531.0
62.90	2611.0
63.90	306.0
65.00	320.0
67.00	157.0
67.90	7031.0
68.90	6818.0
69.90	494.0
71.90	409.0
72.90	3062.0
73.90	11679.0
74.90	33536.0
75.90	3056.0
77.00	396.0
77.70	204.0
78.80	2659.0
79.80	756.0
80.80	2709.0
81.80	598.0
85.90	115.0
86.90	2788.0
87.90	2613.0
90.80	286.0
91.90	1927.0
92.90	2933.0
93.90	7548.0
94.90	60992.0
96.00	3968.0
97.00	102.0
103.80	284.0
104.80	111.0
105.80	253.0
110.70	100.0
115.90	250.0
116.80	463.0
117.70	239.0
118.80	434.0
127.70	199.0
128.80	108.0
129.70	249.0
130.80	135.0
134.70	137.0
140.80	727.0
142.80	807.0
144.80	117.0
145.80	121.0
147.80	134.0
154.80	142.0
156.80	166.0
171.90	369.0
172.90	594.0
173.80	44800.0
174.90	3374.0
175.80	43056.0
176.80	2878.0
177.80	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

m/z	Abundance
35.90	588.0
36.90	3127.0
37.90	2707.0
38.90	1143.0
39.80	450.0
43.80	575.0
44.90	499.0
46.90	824.0
47.90	328.0
48.90	2509.0
49.90	12005.0
50.90	3747.0
52.00	178.0
54.90	168.0
55.90	1115.0
56.90	1947.0
60.00	587.0
60.90	2990.0
61.90	3312.0
62.90	2539.0
63.90	305.0
65.00	306.0
67.00	178.0
67.90	6699.0
68.90	6726.0
69.90	580.0
71.90	392.0
72.90	3047.0
73.90	11322.0
74.90	32856.0
75.90	3001.0
77.00	333.0
77.70	259.0
78.80	2698.0
79.80	732.0
80.80	2589.0
81.80	525.0
85.90	120.0
86.90	2815.0
87.90	2672.0
90.80	267.0
91.90	1890.0
92.90	2818.0
93.90	7401.0
94.90	59864.0
96.00	3939.0
96.90	120.0
103.80	270.0
105.80	283.0
110.70	114.0
115.90	220.0
116.80	440.0
117.80	243.0
118.80	412.0
127.70	210.0
128.80	102.0
129.70	287.0
130.80	112.0
134.70	129.0
136.70	104.0
140.80	784.0
142.80	799.0
144.80	134.0
145.80	115.0
147.70	155.0
154.70	142.0
156.80	123.0
160.80	100.0
171.90	373.0
172.90	556.0
173.80	45544.0
174.90	3292.0
175.80	43112.0
176.80	2803.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134