
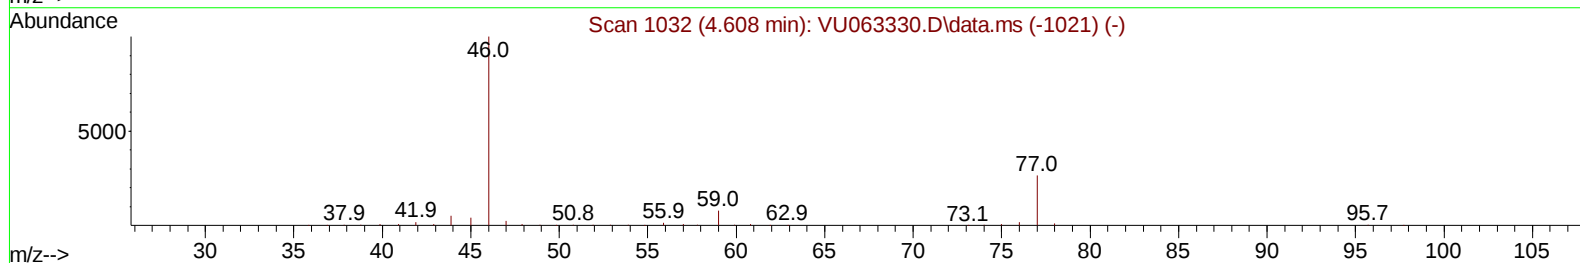
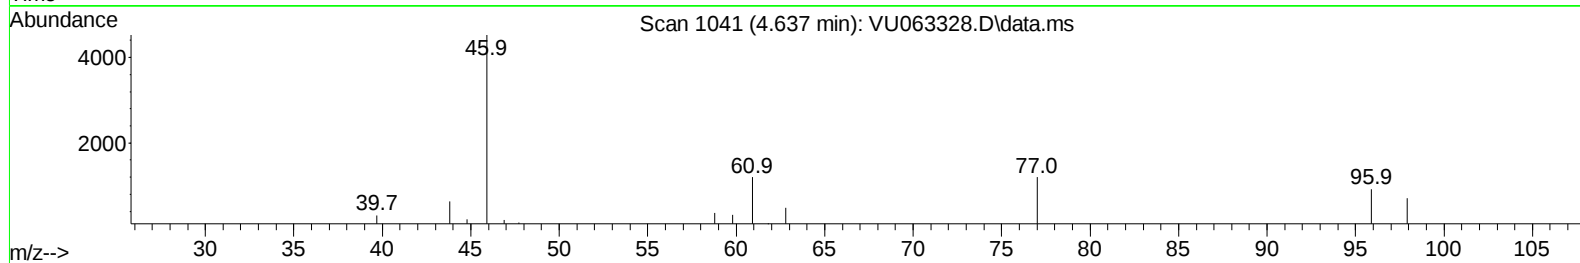


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

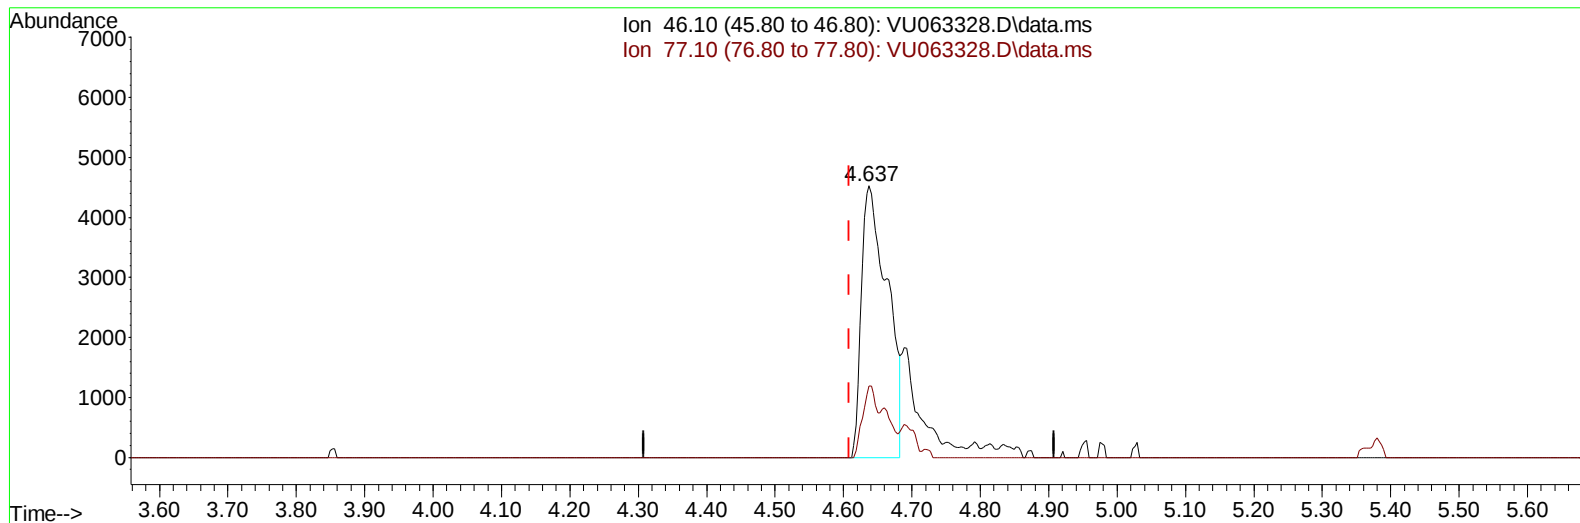

TIC: VU063328.D\data.ms

(20) 2-Butanone-d5 (S)




4.637min (+ 0.029) 3.45 ug/L

response 11915

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.20	15.01#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

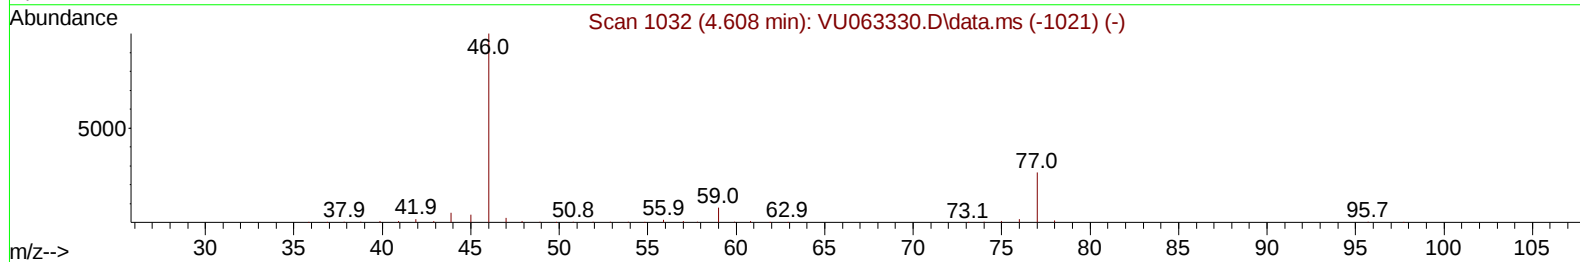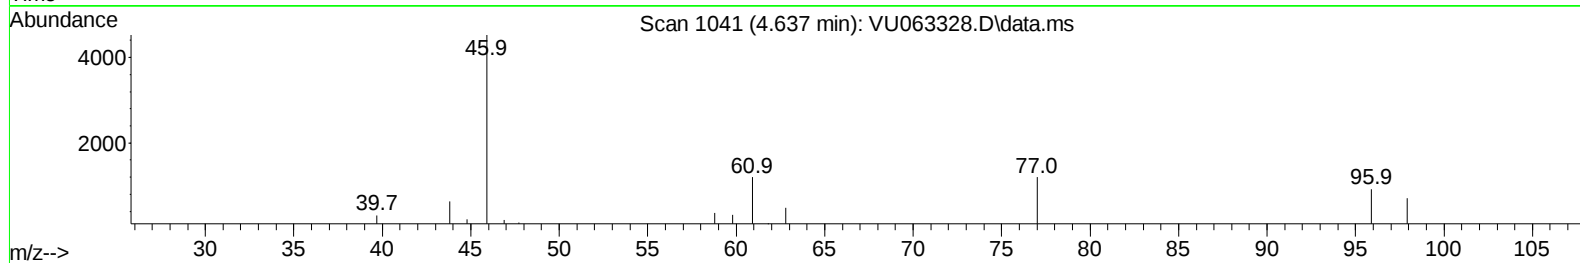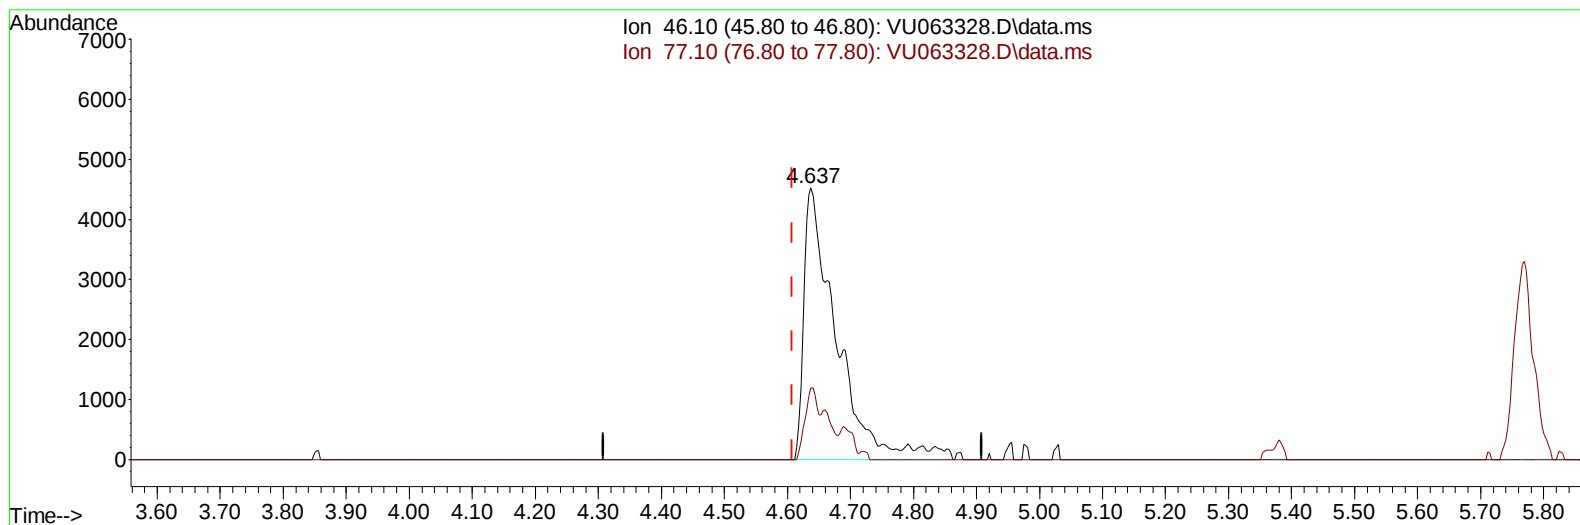

TIC: VU063328.D\data.ms

(20) 2-Butanone-d5 (S)




4.637min (+ 0.029) 4.71 ug/L m

response 16274

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.20	10.99#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

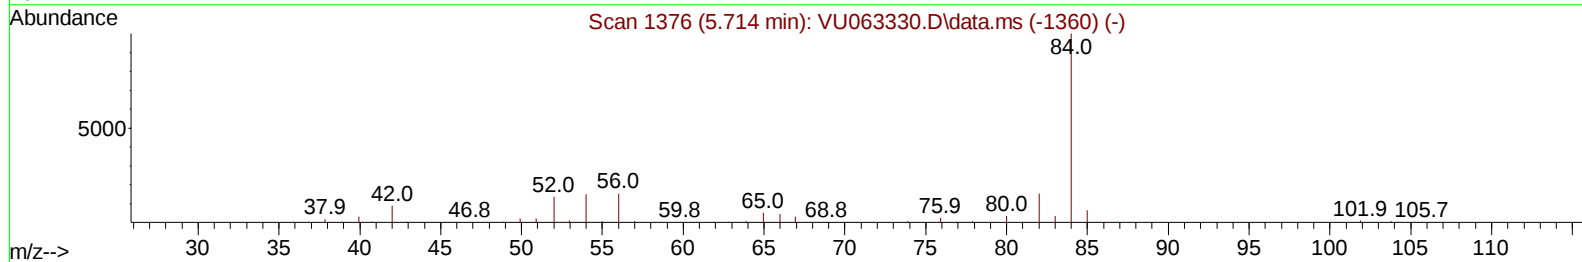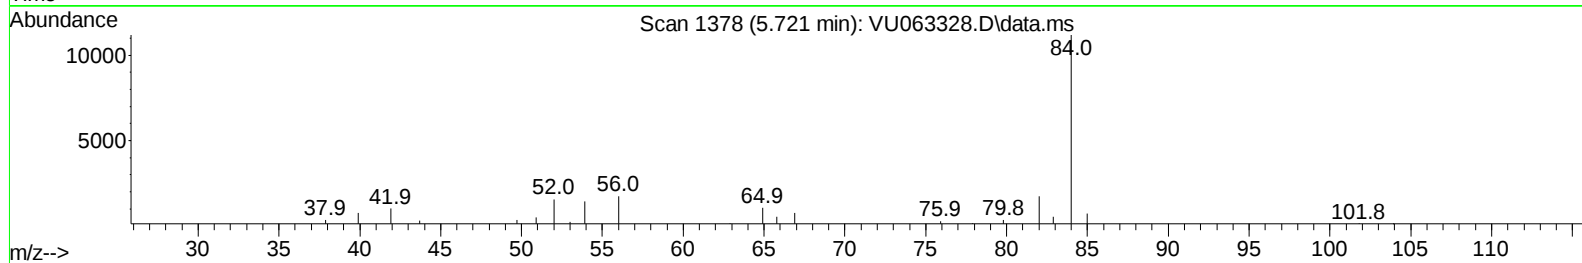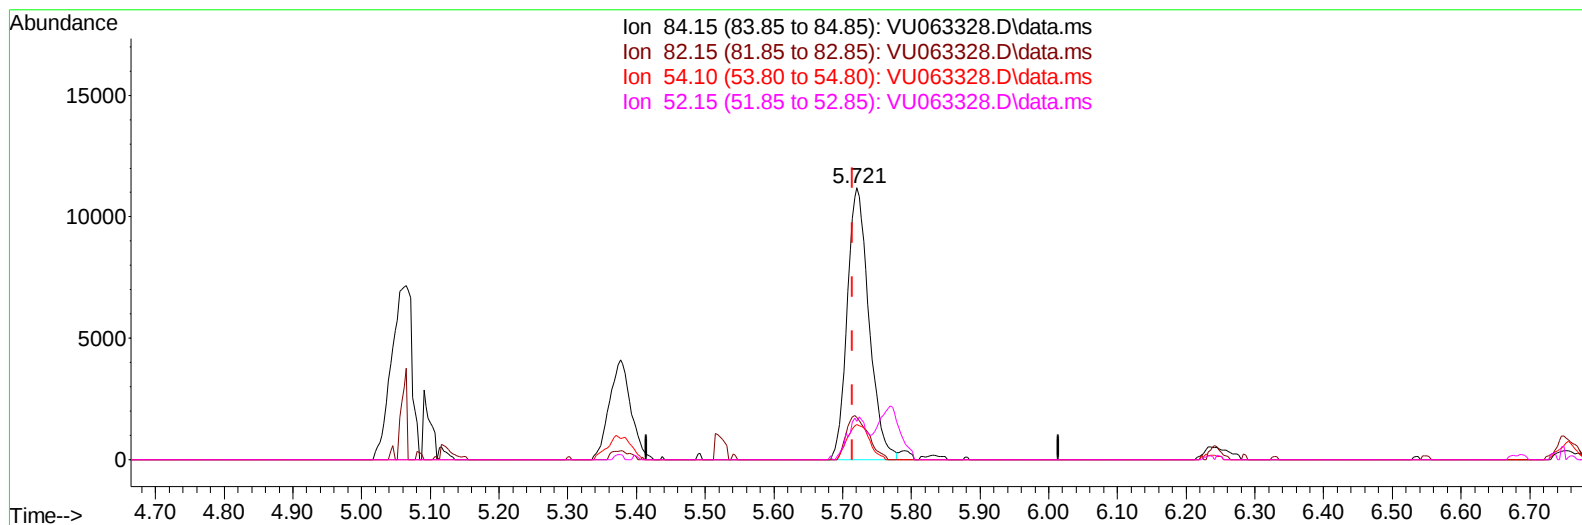

TIC: VU063328.D\data.ms

(32) Benzene-d6 (S)




5.721min (+ 0.006) 0.47 ug/L

response 24613

Ion	Exp%	Act%
84.15	100.00	100.00
82.15	15.40	16.25
54.10	14.70	12.94
52.15	12.80	13.70

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

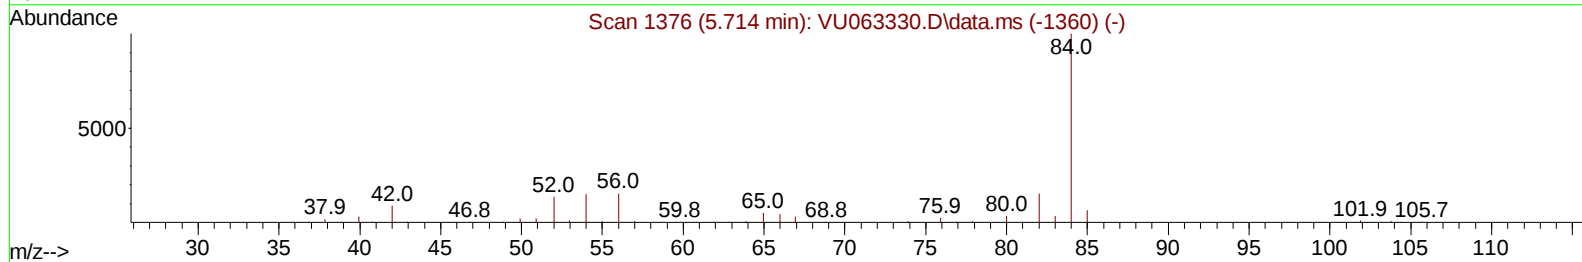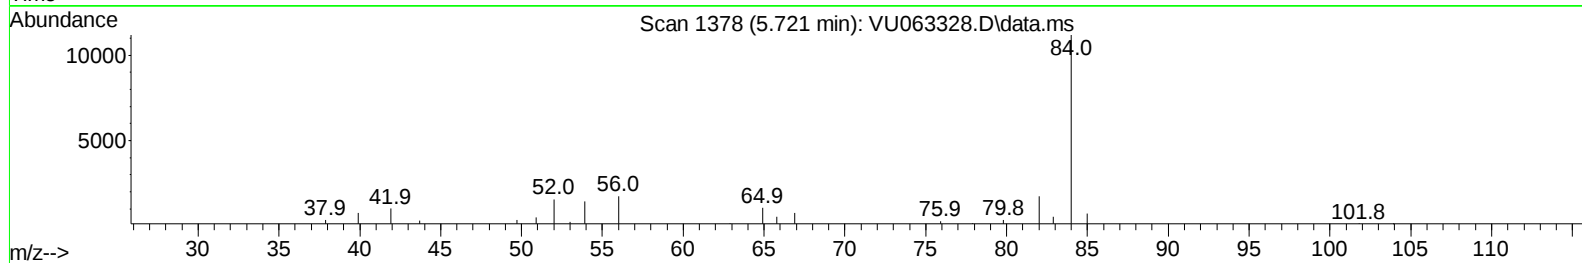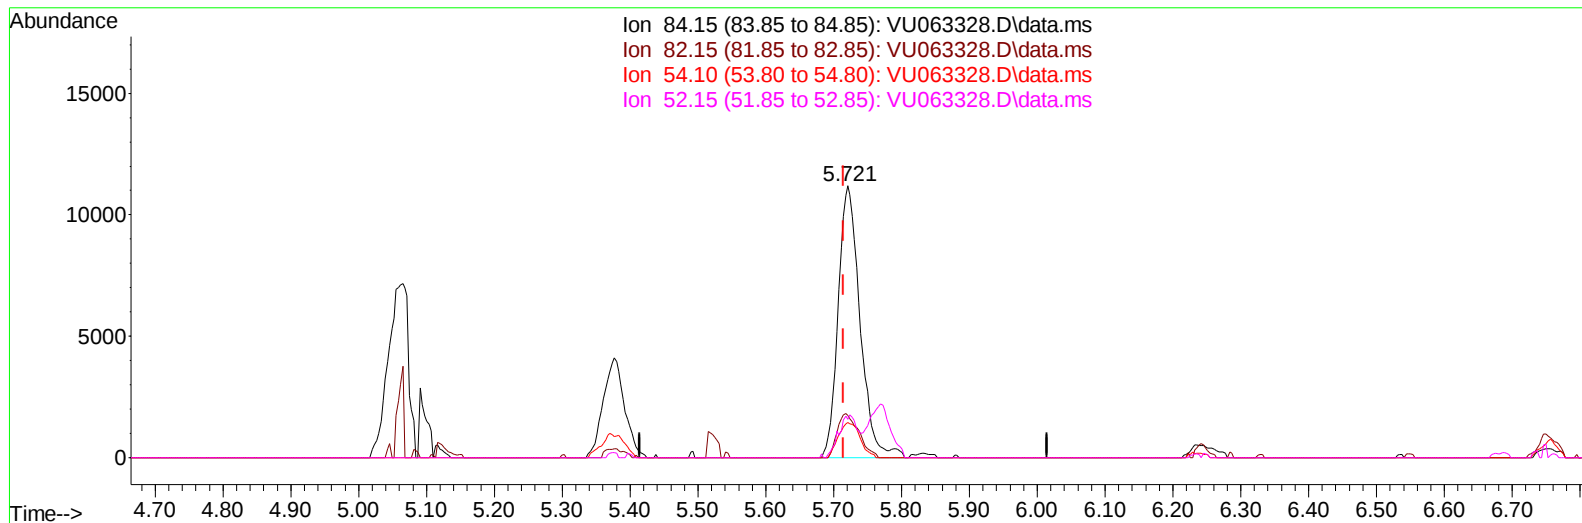

TIC: VU063328.D\data.ms

(32) Benzene-d6 (S)




5.721min (+ 0.006) 0.47 ug/L m

response 25016

Ion	Exp%	Act%
84.15	100.00	100.00
82.15	15.40	15.99
54.10	14.70	12.73
52.15	12.80	13.48

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

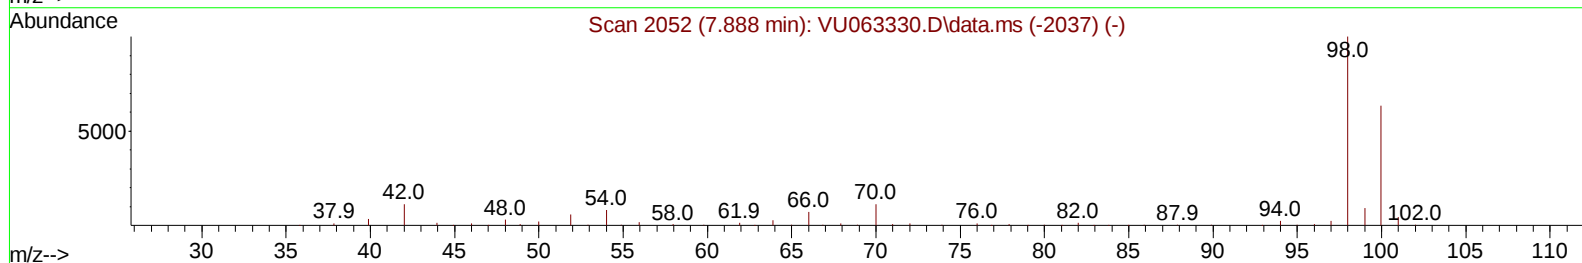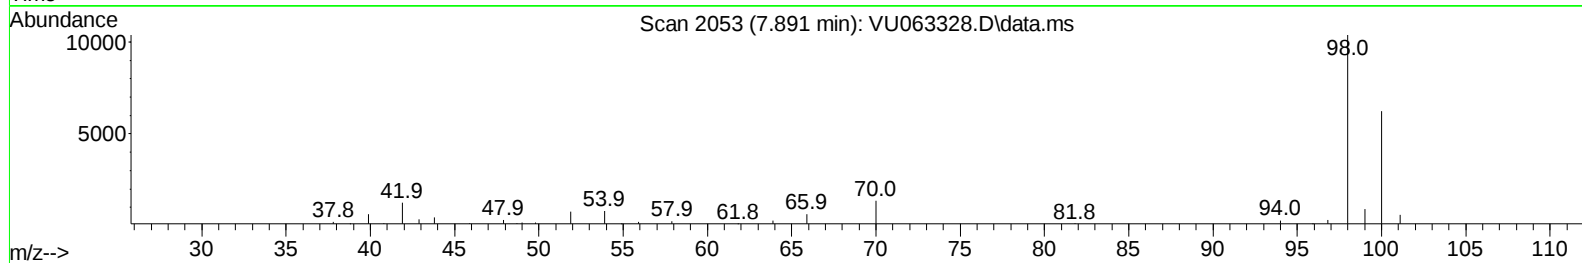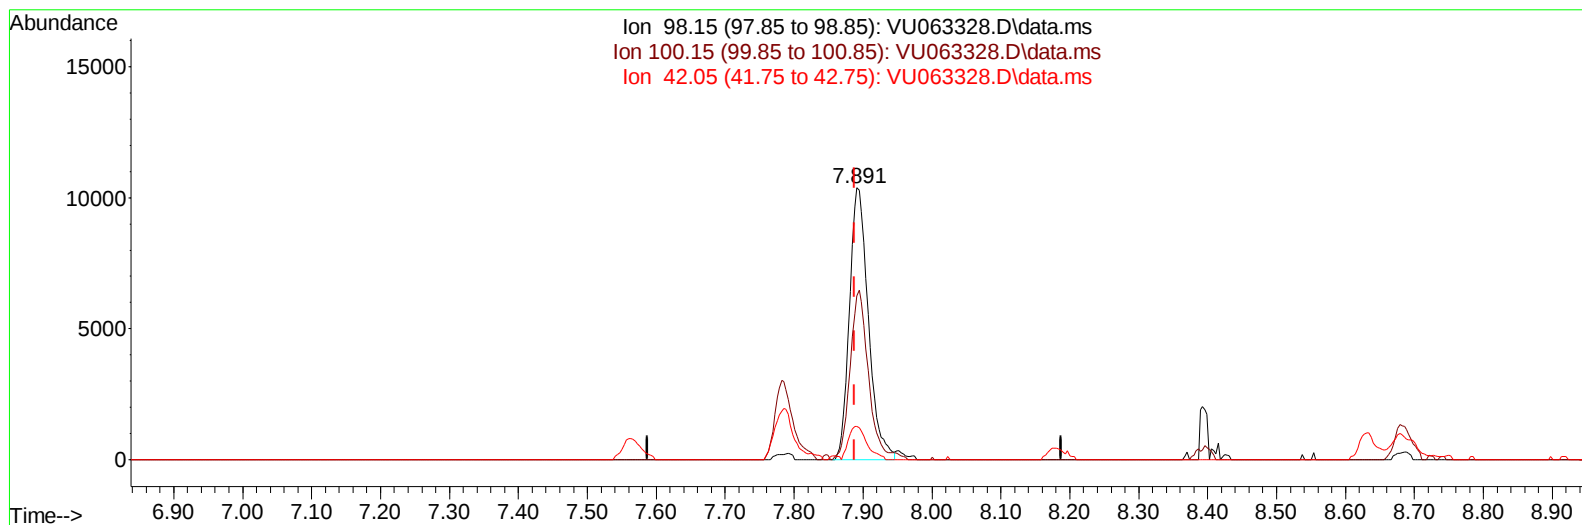

TIC: VU063328.D\data.ms

(41) Toluene-d8 (S)




7.891min (+ 0.003) 0.43 ug/L

response 19691

Ion	Exp%	Act%
98.15	100.00	100.00
100.15	62.10	60.99
42.05	11.00	11.78
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

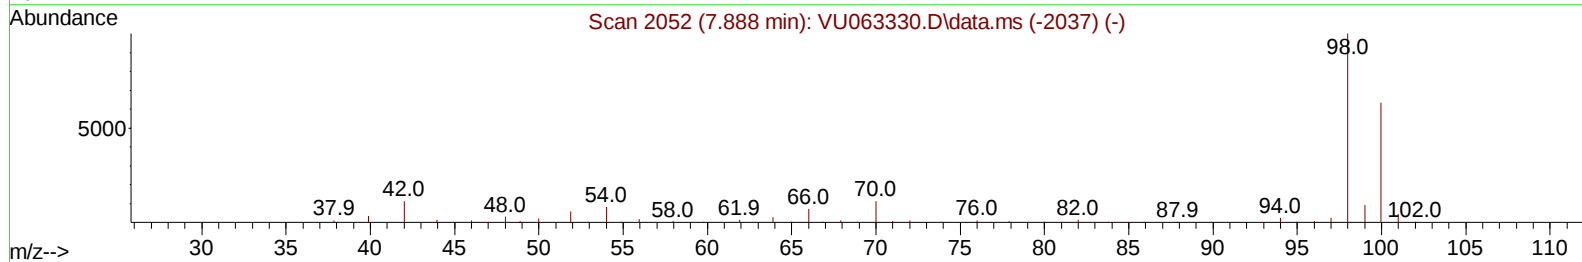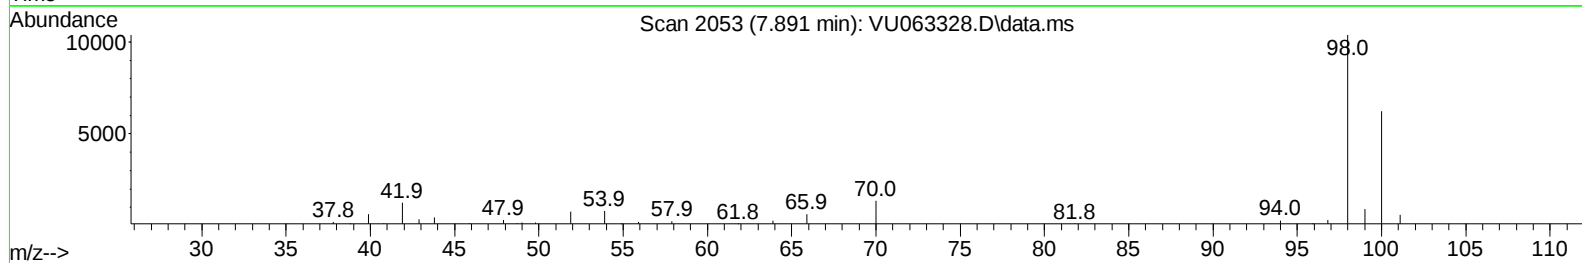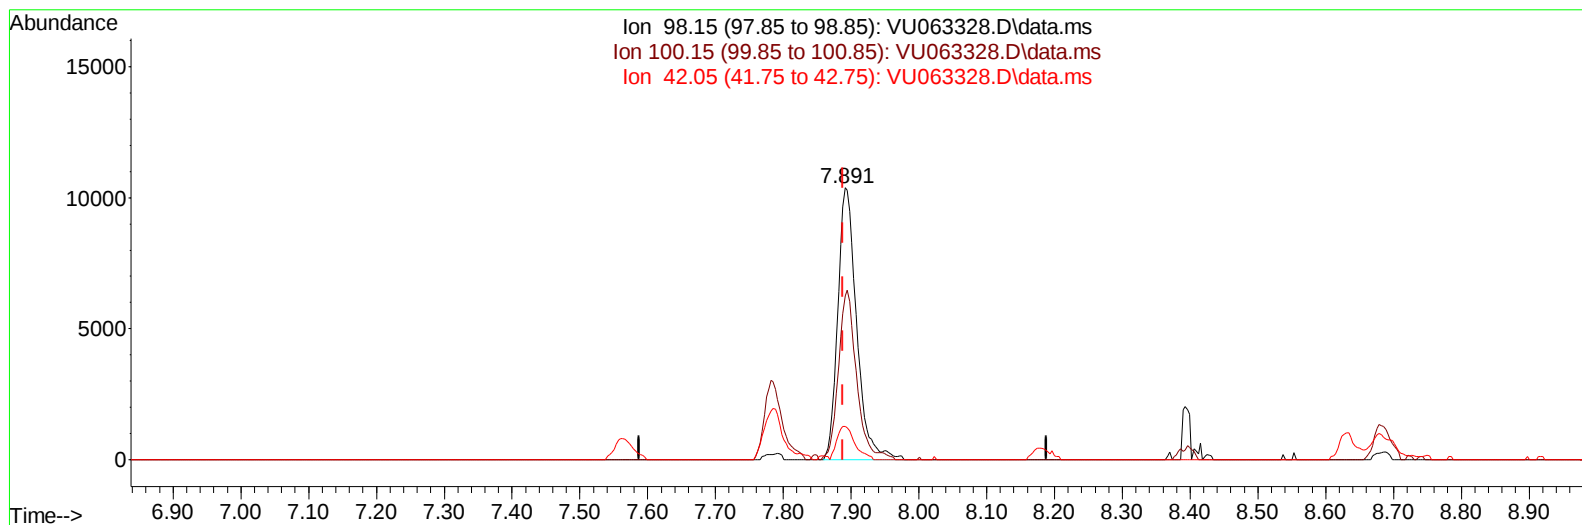

TIC: VU063328.D\data.ms

(41) Toluene-d8 (S)




7.891min (+ 0.003) 0.44 ug/L m

response 20039

Ion	Exp%	Act%
98.15	100.00	100.00
100.15	62.10	59.93
42.05	11.00	11.58
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

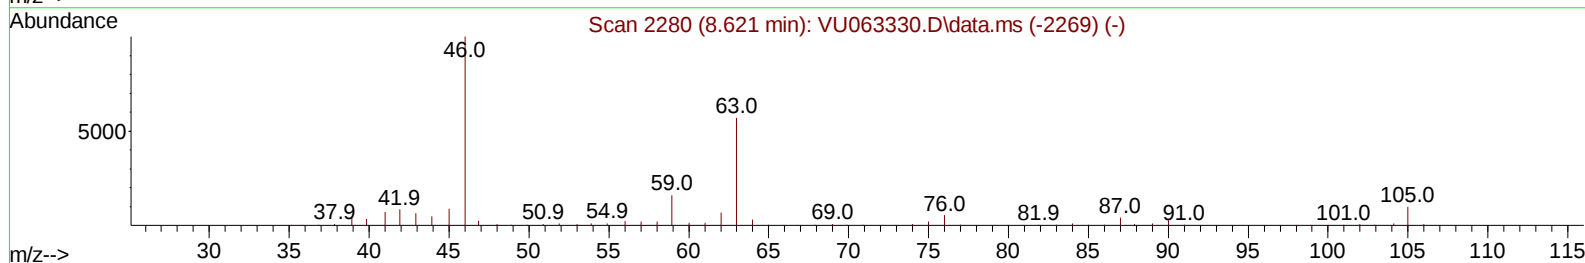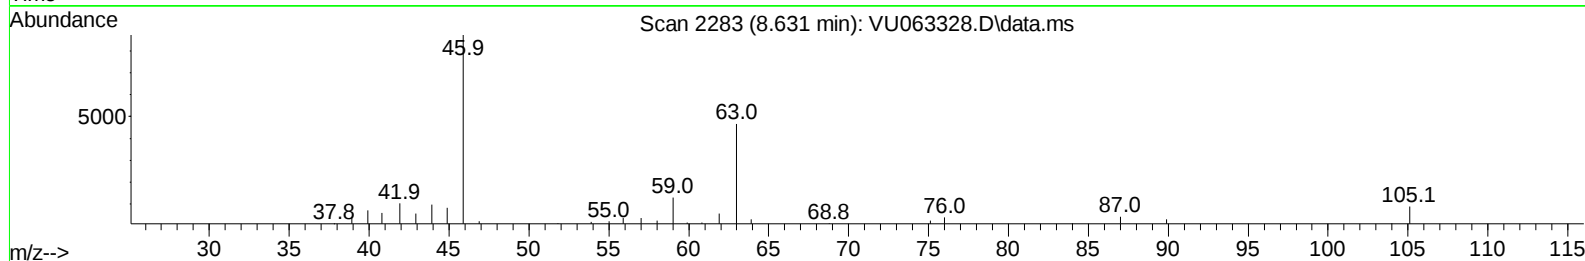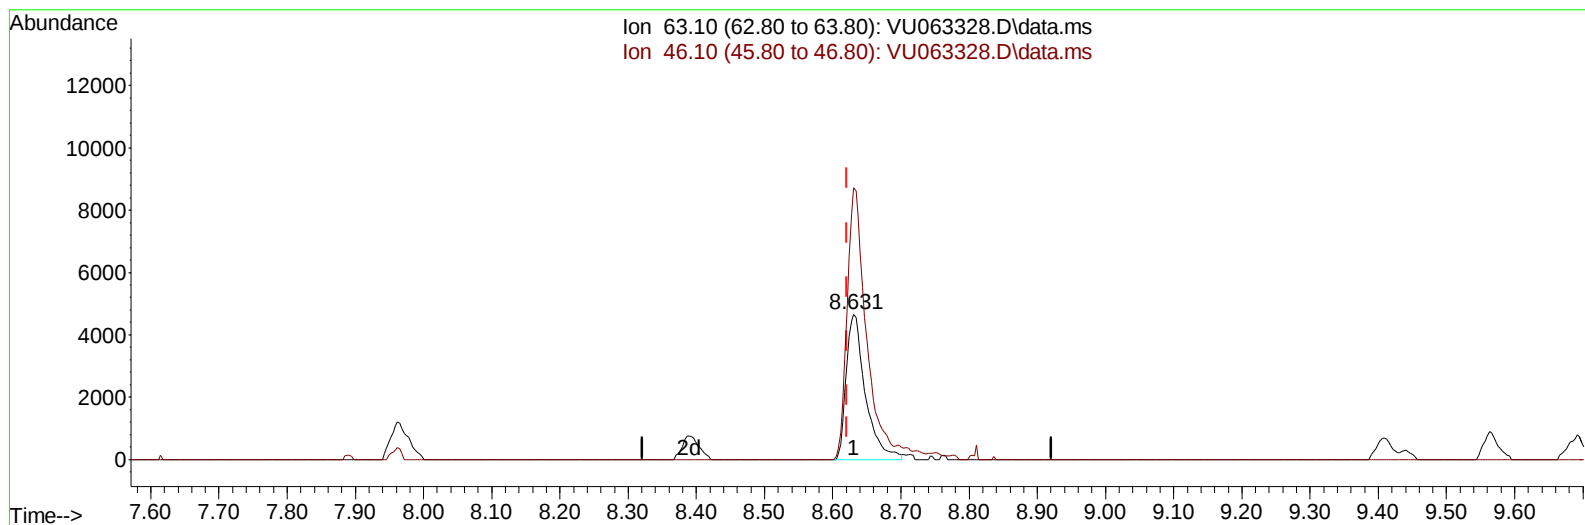

TIC: VU063328.D\data.ms

(46) 2-Hexanone-d5 (S)




8.631min (+ 0.010) 3.49 ug/L

response 9083

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	177.60	185.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

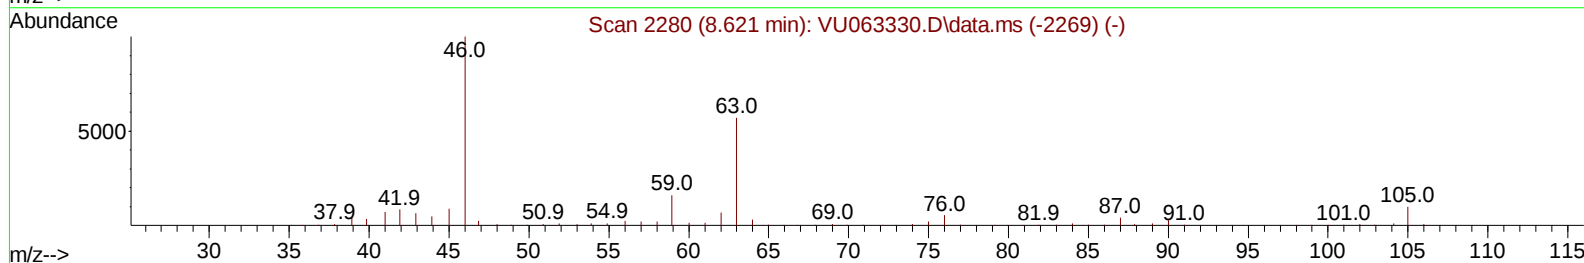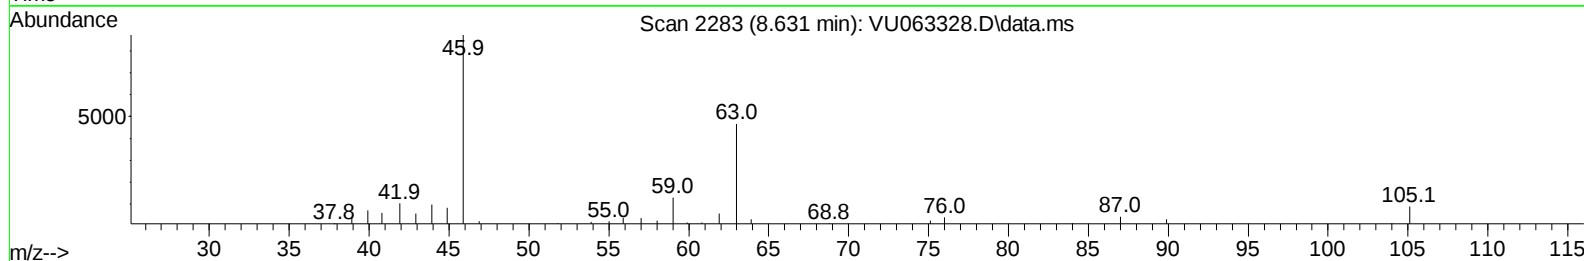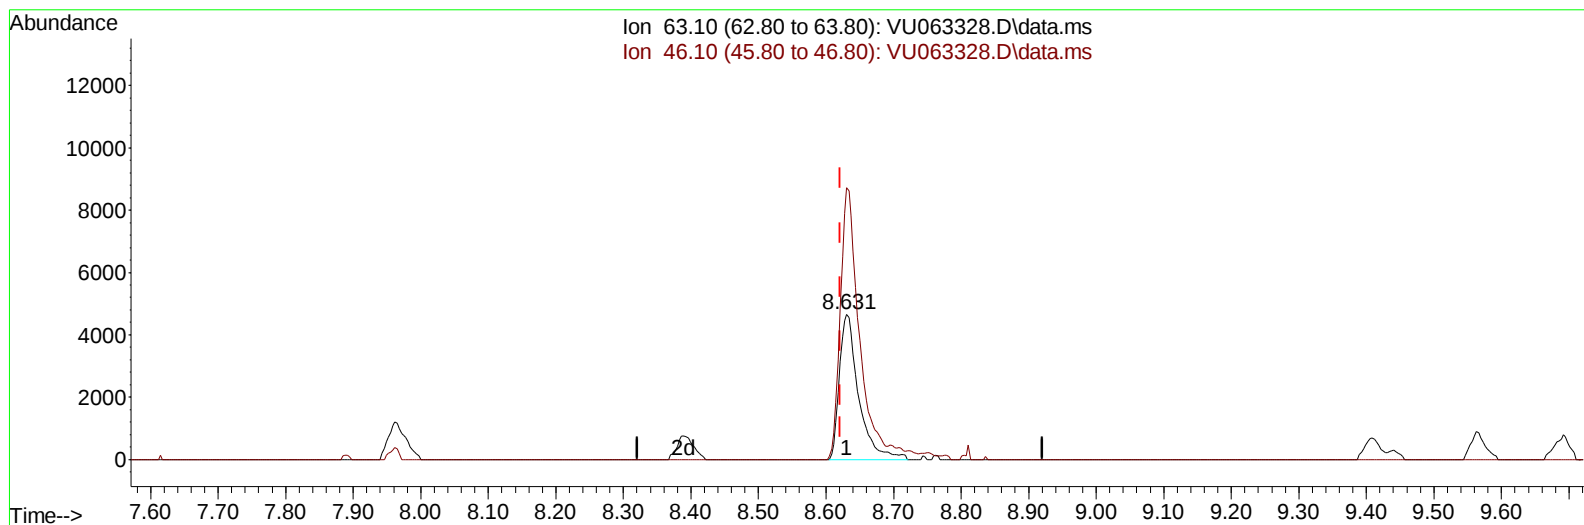

TIC: VU063328.D\data.ms

(46) 2-Hexanone-d5 (S)




8.631min (+ 0.010) 3.55 ug/L m

response 9230

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	177.60	182.58
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

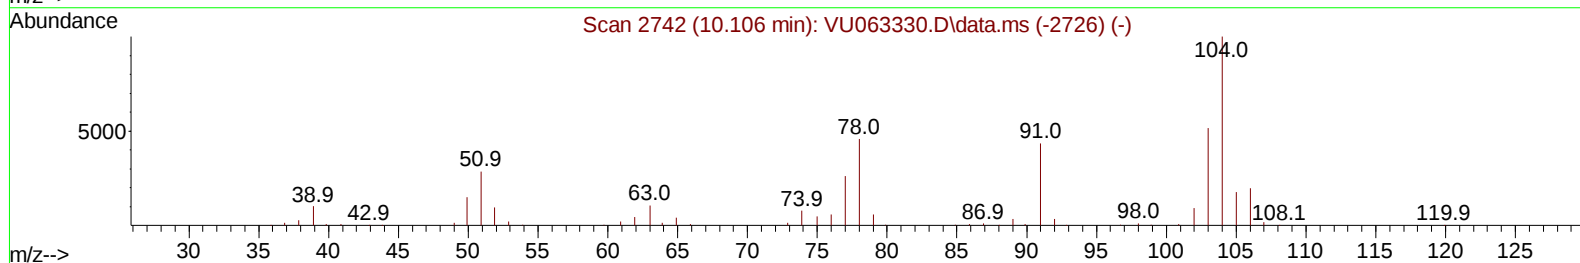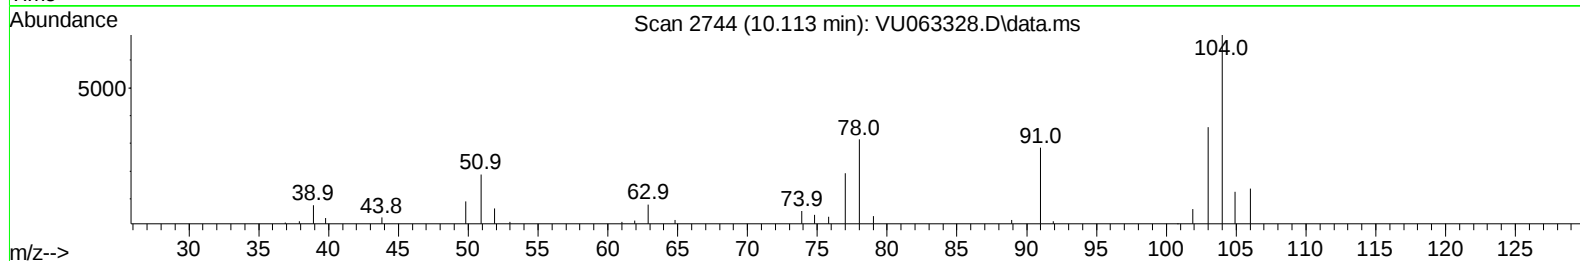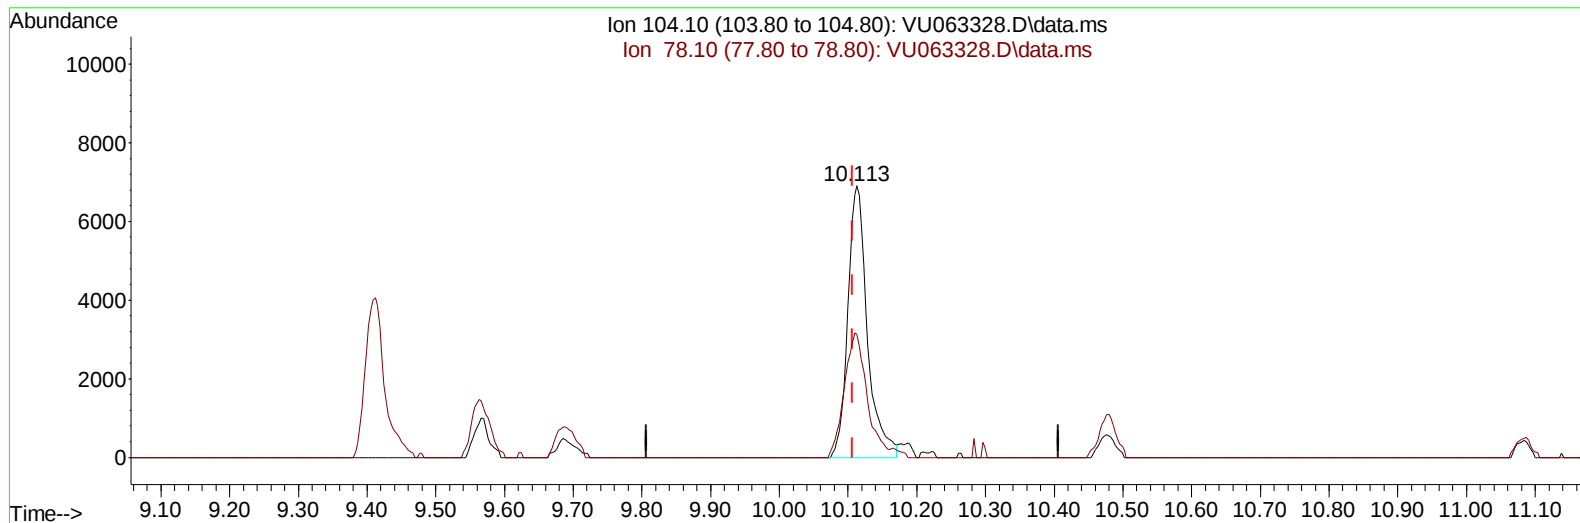

TIC: VU063328.D\data.ms

(55) Styrene (T)




10.113min (+ 0.006) 0.37 ug/L

response 13622

Ion	Exp%	Act%
104.10	100.00	100.00
78.10	45.80	45.42
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040325\
Data File : VU063328.D
Acq On : 03 Apr 2025 14:46
Operator : MD/SY
Sample : VSTD0.512
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 04 09:11:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 04 09:10:38 2025
Response via : Initial Calibration

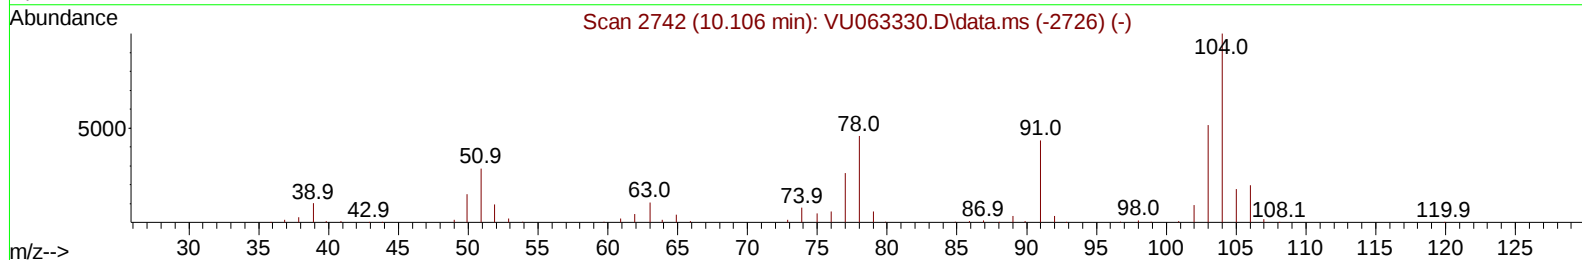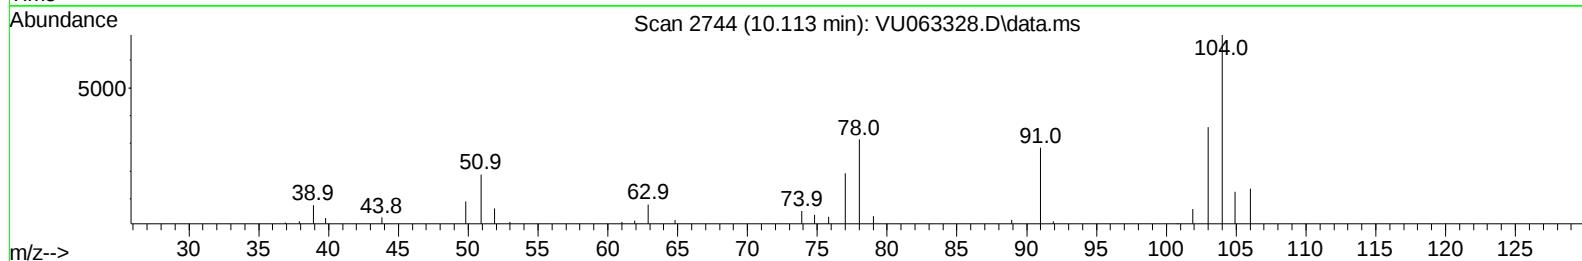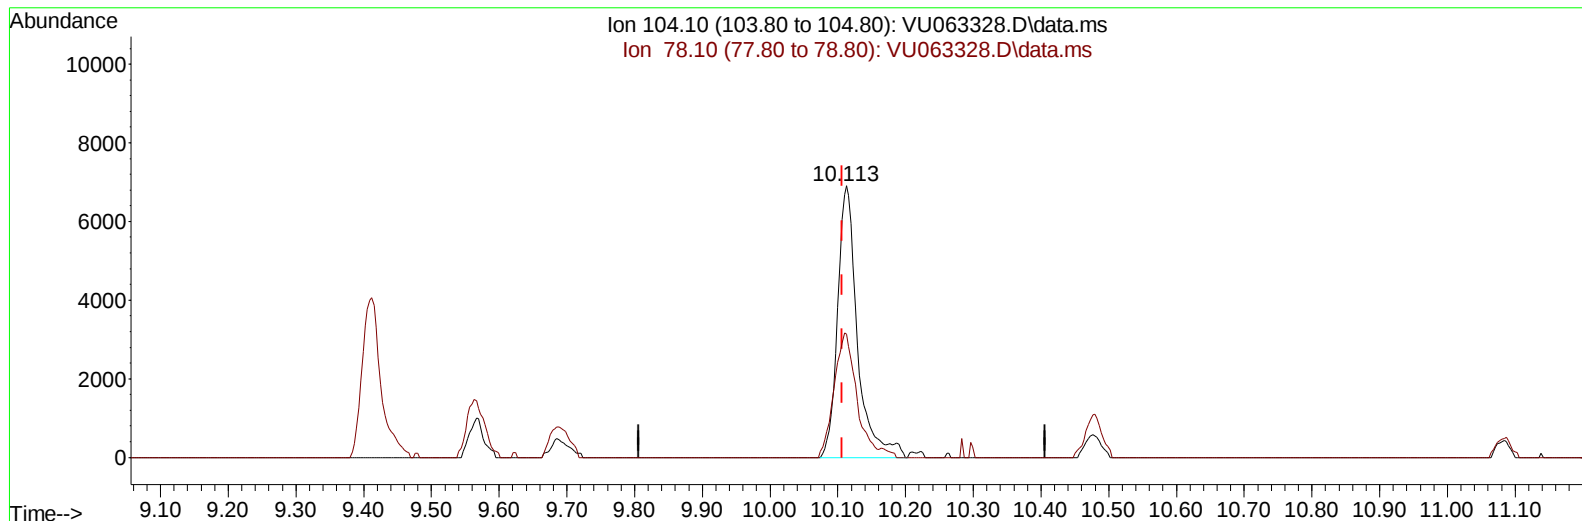

TIC: VU063328.D\data.ms

(55) Styrene (T)

10.113min (+ 0.006) 0.38 ug/L m

response 14076

Ion	Exp%	Act%
104.10	100.00	100.00
78.10	45.80	45.42
0.00	0.00	0.00
0.00	0.00	0.00