
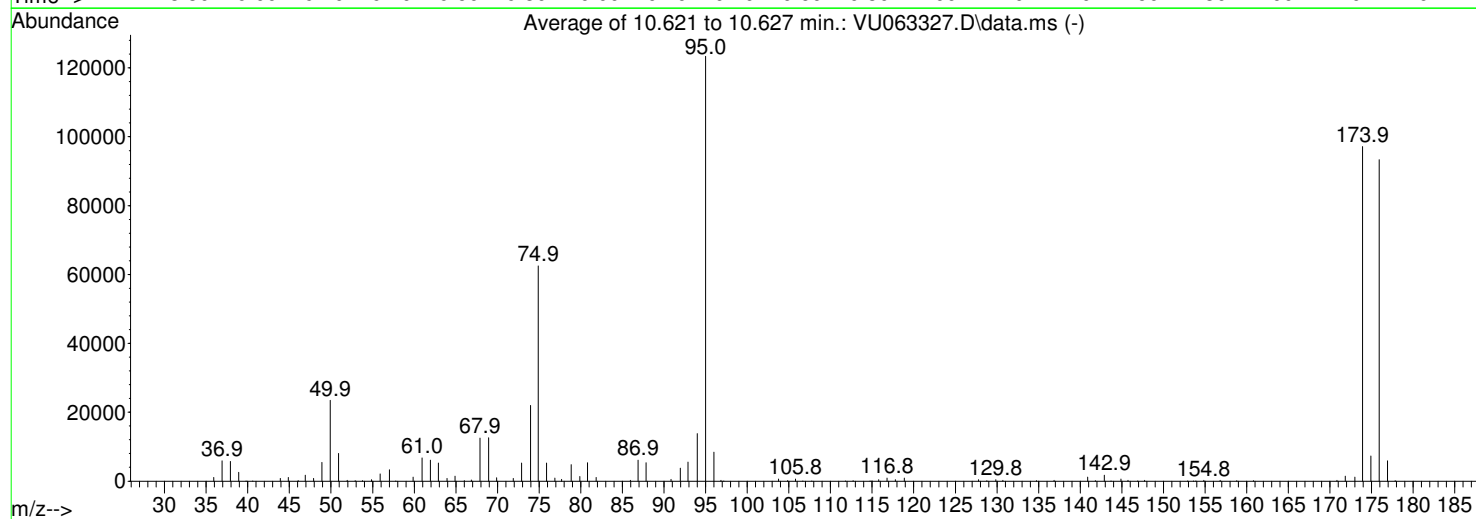


Data Path : D:\MassHunter\GCMS\1\data\VU040325\
Data File : VU063327.D
Acq On : 03 Apr 2025 13:52
Operator : MD/SY
Sample : BFB079
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB079

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Apr 04 09:52:11 2025

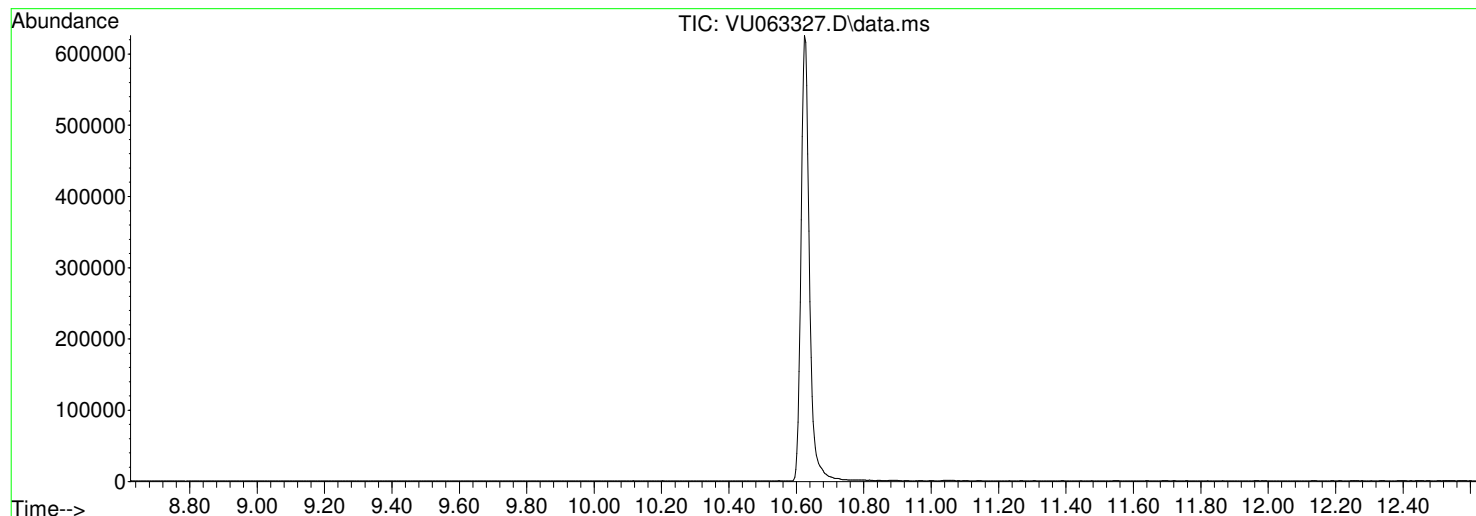

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	23437	PASS
75	95	30	80	50.7	62493	PASS
95	95	100	100	100.0	123381	PASS
96	95	5	9	6.9	8454	PASS
173	174	0.00	2	1.2	1154	PASS
174	95	50	120	78.8	97181	PASS
175	174	5	9	7.5	7286	PASS
176	174	95	101	96.1	93365	PASS
177	176	5	9	6.3	5913	PASS

m/z	Abundance
39.90	296.0
43.90	436.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	1081.0
36.90	5874.0
37.90	5794.0
38.90	2684.0
39.80	360.0
43.90	1268.0
44.90	1116.0
46.10	204.0
46.90	1662.0
47.90	695.0
48.90	5371.0
49.90	22496.0
50.90	7605.0
52.00	243.0
52.90	142.0
53.80	152.0
54.80	348.0
55.90	2078.0
57.00	3014.0
57.80	105.0
59.80	1167.0
61.00	6451.0
62.00	5864.0
62.90	5108.0
64.00	833.0
64.90	1327.0
66.00	152.0
66.90	287.0
67.90	11906.0
69.00	12251.0
69.90	1040.0
71.90	676.0
72.90	4996.0
73.90	21440.0
74.90	60584.0
75.90	5312.0
76.90	839.0
77.70	501.0
78.80	4630.0
79.90	1292.0
80.80	5041.0
81.90	1139.0
86.00	147.0
86.90	6038.0
87.80	4887.0
90.90	538.0
91.90	3749.0
92.90	5081.0
94.00	13440.0
95.00	117584.0
96.00	8388.0
96.80	179.0
97.20	158.0
103.70	538.0
104.80	133.0
105.80	640.0
106.70	103.0
107.80	123.0
112.60	112.0
114.70	140.0
115.80	350.0
116.80	844.0
117.80	403.0
118.80	759.0
127.80	382.0
128.80	183.0
129.90	435.0
130.70	180.0
134.70	168.0
136.80	192.0
140.90	1281.0
141.80	183.0
142.90	1674.0
143.70	137.0
144.90	616.0
145.80	201.0
147.80	211.0
152.90	106.0
153.60	110.0
154.80	242.0
156.80	261.0
158.80	145.0
160.80	120.0
170.80	264.0
171.80	1358.0
173.00	1000.0
173.90	89928.0
174.90	6864.0
175.90	87176.0
176.90	5681.0
177.80	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	1170.0
36.90	6016.0
37.90	5968.0
38.90	2697.0
39.80	370.0
40.60	103.0
43.90	1242.0
44.90	1096.0
46.10	184.0
46.90	1771.0
47.90	769.0
48.90	5590.0
49.90	24080.0
50.90	8268.0
51.90	275.0
52.90	151.0
53.80	137.0
54.90	441.0
55.90	2125.0
57.00	3332.0
57.80	105.0
59.90	1204.0
61.00	6941.0
62.00	6189.0
62.90	5485.0
64.00	849.0
64.90	1477.0
66.00	140.0
66.90	292.0
67.90	12917.0
69.00	12989.0
69.90	1042.0
71.90	811.0
72.90	5326.0
74.00	22672.0
74.90	64304.0
75.90	5434.0
76.90	877.0
77.70	565.0
78.80	4846.0
79.90	1416.0
80.80	5543.0
81.90	1125.0
85.90	213.0
86.90	6336.0
87.80	5465.0
90.80	573.0
92.00	3931.0
92.90	5532.0
94.00	14191.0
95.00	127584.0
96.00	8804.0
96.90	232.0
103.80	595.0
104.90	129.0
105.80	664.0
107.70	141.0
112.70	123.0
114.80	114.0
115.80	412.0
116.80	942.0
117.80	423.0
118.90	878.0
127.80	408.0
128.80	158.0
129.80	458.0
130.70	223.0
134.80	187.0
136.80	221.0
140.90	1275.0
141.80	177.0
142.90	1759.0
143.70	127.0
144.90	638.0
145.70	233.0
146.90	108.0
147.80	272.0
153.60	113.0
153.90	113.0
154.90	287.0
156.80	287.0
158.80	172.0
160.80	143.0
170.90	238.0
171.90	1434.0
173.00	1205.0
173.90	99944.0
174.90	7553.0
175.90	96480.0
176.90	6100.0
177.90	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	1058.0
36.90	5698.0
37.90	5496.0
38.90	2411.0
39.80	403.0
43.90	1182.0
44.80	1083.0
46.00	144.0
46.90	1705.0
47.90	789.0
48.90	5293.0
49.90	23736.0
50.90	8179.0
51.90	306.0
52.90	148.0
54.90	429.0
55.90	2026.0
57.00	3432.0
59.90	1192.0
60.90	6721.0
61.90	6098.0
62.90	5289.0
63.90	816.0
64.90	1458.0
66.00	113.0
66.80	323.0
67.90	12800.0
68.90	12521.0
69.90	931.0
71.90	764.0
72.90	5322.0
74.00	21696.0
74.90	62592.0
75.90	5154.0
76.90	831.0
77.70	587.0
78.90	4755.0
79.90	1384.0
80.80	5465.0
81.80	1040.0
86.00	244.0
86.90	6024.0
87.90	5575.0
90.80	532.0
92.00	3703.0
92.90	5890.0
94.00	13878.0
95.00	124976.0
96.00	8171.0
96.90	246.0
103.80	672.0
104.90	149.0
105.80	638.0
111.80	106.0
112.80	139.0
115.00	109.0
115.80	456.0
116.80	1008.0
117.80	405.0
118.90	897.0
127.80	454.0
128.80	171.0
129.80	422.0
130.70	251.0
134.80	201.0
136.90	257.0
140.90	1061.0
141.80	149.0
142.90	1766.0
144.90	543.0
145.70	243.0
146.90	111.0
147.70	275.0
153.90	104.0
154.90	296.0
156.80	256.0
158.80	165.0
160.80	133.0
170.80	227.0
171.80	1489.0
173.00	1257.0
173.90	101672.0
174.90	7440.0
175.90	96440.0
176.90	5958.0
177.80	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079