


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040424\
Data File : VU058370.D
Acq On : 04 Apr 2024 13:29
Operator : MD/SY
Sample : BFB136
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB136

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Apr 05 00:02:56 2024

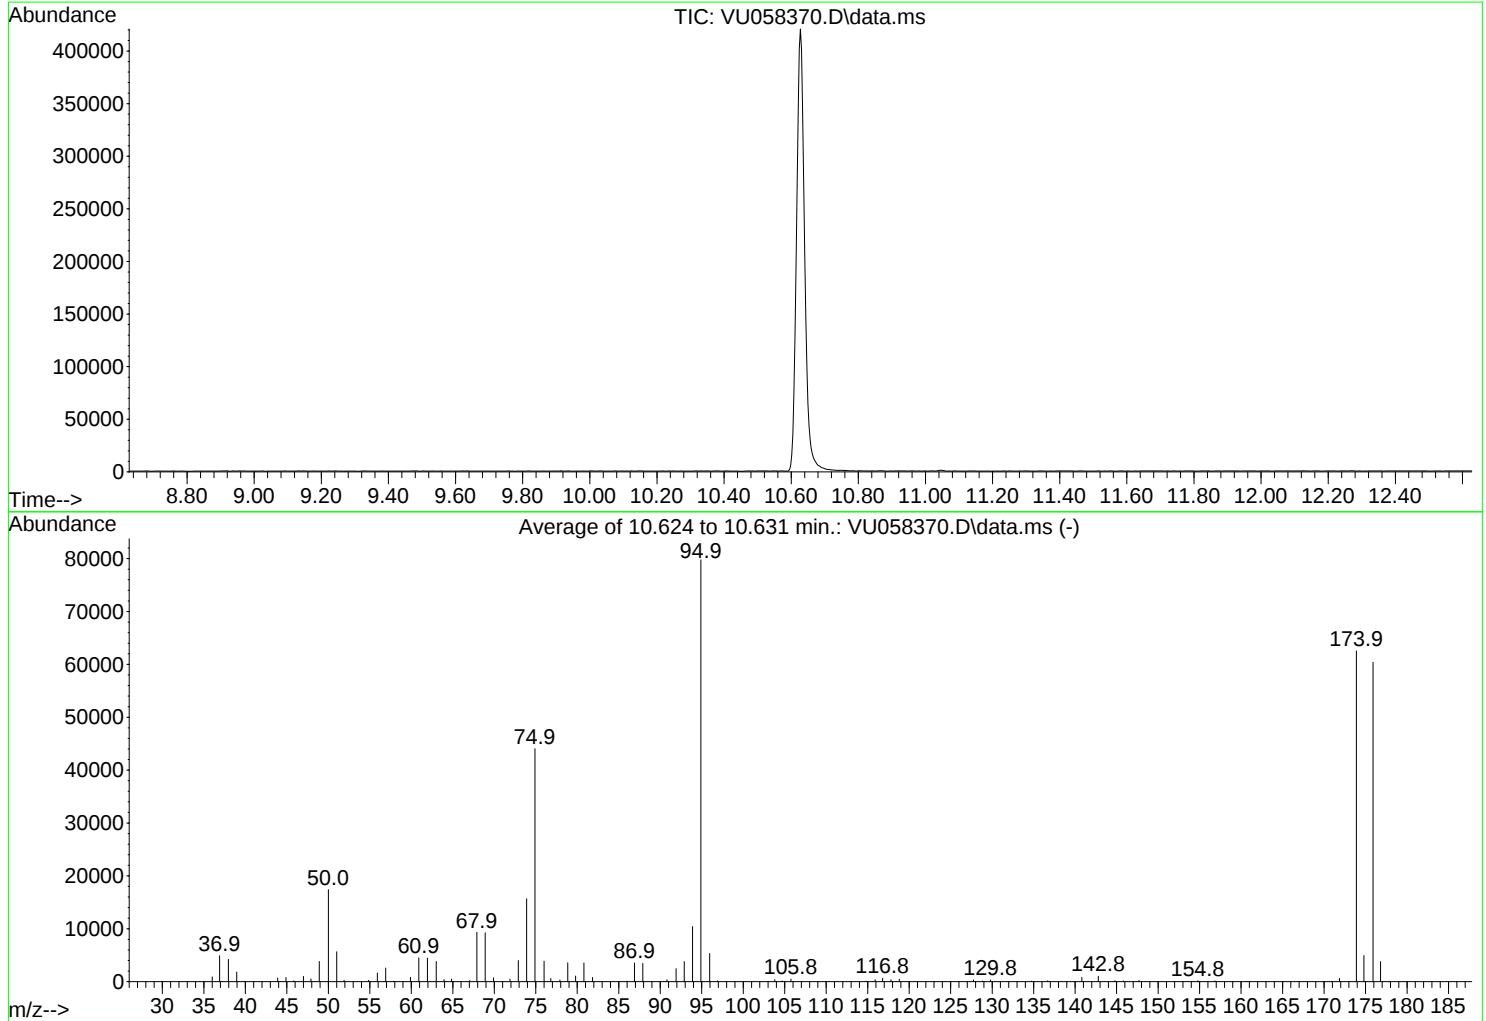

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	17408	PASS
75	95	30	80	55.2	44056	PASS
95	95	100	100	100.0	79768	PASS
96	95	5	9	6.7	5326	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.4	62544	PASS
175	174	5	9	7.9	4932	PASS
176	174	95	101	96.6	60397	PASS
177	176	5	9	6.3	3780	PASS

Scan 2890 (10.582 min): VU058370.D\data.ms
BFB136

m/z	Abundance
39.80	623.0
43.90	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
36.00	911.0
36.90	4952.0
37.90	4255.0
39.00	1907.0
39.90	670.0
43.90	838.0
44.90	785.0
45.90	120.0
47.00	1017.0
47.90	506.0
48.90	3804.0
50.00	17320.0
51.00	5746.0
51.90	228.0
54.90	281.0
55.90	1494.0
56.90	2582.0
57.90	107.0
59.90	843.0
60.90	4533.0
62.00	4647.0
63.00	3782.0
63.90	419.0
64.90	488.0
67.00	240.0
67.90	9400.0
68.90	9157.0
69.90	736.0
71.90	506.0
72.90	3962.0
73.90	15618.0
74.90	43936.0
76.00	3878.0
76.80	604.0
77.90	302.0
78.90	3624.0
79.80	1075.0
80.80	3517.0
81.90	797.0
86.00	115.0
86.90	3531.0
87.90	3296.0
90.80	327.0
91.90	2496.0
92.90	3838.0
93.90	10213.0
94.90	78408.0
96.00	5164.0
96.90	154.0
103.80	358.0
104.70	146.0
105.80	482.0
114.80	149.0
115.90	345.0
116.80	614.0
117.80	393.0
118.80	451.0
127.70	318.0
128.80	120.0
129.80	301.0
134.80	144.0
136.70	180.0
140.80	783.0
142.80	1077.0
144.80	209.0
145.80	137.0
147.70	222.0
154.80	197.0
156.80	123.0
171.80	651.0
173.90	60712.0
174.80	4715.0
175.90	58120.0
176.80	3761.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
36.00	943.0
36.90	5065.0
37.90	4296.0
38.90	1849.0
39.90	702.0
43.90	882.0
44.90	807.0
45.80	154.0
47.00	1026.0
47.90	535.0
48.90	3912.0
50.00	17968.0
51.00	5887.0
51.90	257.0
54.90	260.0
55.90	1721.0
56.90	2641.0
57.80	112.0
59.90	801.0
60.90	4691.0
61.90	4569.0
63.00	3925.0
63.90	426.0
64.80	483.0
67.10	220.0
67.90	9530.0
68.90	9511.0
69.90	748.0
71.90	519.0
72.90	4101.0
73.90	16183.0
74.90	45296.0
76.00	3971.0
76.80	624.0
77.90	315.0
78.90	3712.0
79.80	1085.0
80.80	3636.0
81.80	811.0
86.00	109.0
86.90	3623.0
87.90	3553.0
90.80	379.0
91.90	2515.0
92.90	3908.0
93.90	10795.0
94.90	82472.0
95.90	5480.0
96.90	176.0
103.80	393.0
104.70	171.0
105.70	514.0
114.80	123.0
115.90	389.0
116.80	662.0
117.80	391.0
118.80	472.0
127.80	334.0
128.90	132.0
129.80	360.0
134.80	132.0
136.70	183.0
140.80	851.0
142.80	1063.0
144.80	205.0
145.80	152.0
147.70	249.0
154.80	209.0
156.90	155.0
171.80	654.0
173.90	64480.0
174.80	5103.0
175.90	62480.0
176.80	3877.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
36.00	913.0
36.90	4655.0
38.00	4039.0
38.90	1672.0
39.90	708.0
43.90	839.0
44.90	777.0
45.80	150.0
47.00	950.0
47.90	527.0
48.90	3702.0
50.00	16936.0
51.00	5368.0
51.90	249.0
54.80	233.0
55.90	1662.0
56.90	2544.0
57.80	100.0
59.90	772.0
60.90	4354.0
61.90	4178.0
63.00	3747.0
64.00	381.0
64.90	448.0
67.10	188.0
67.90	9020.0
68.90	9060.0
69.90	670.0
71.90	470.0
72.90	3942.0
73.90	15252.0
74.90	42936.0
76.00	3746.0
76.80	577.0
77.90	336.0
78.80	3352.0
79.80	1001.0
80.80	3451.0
81.80	722.0
86.00	103.0
86.90	3434.0
87.90	3509.0
90.80	368.0
91.90	2386.0
92.90	3588.0
93.90	10252.0
94.90	78424.0
95.90	5335.0
96.90	159.0
103.80	391.0
104.70	172.0
105.70	481.0
115.90	371.0
116.80	624.0
117.80	347.0
118.80	442.0
127.80	318.0
128.90	130.0
129.80	346.0
134.60	112.0
136.70	163.0
140.80	822.0
142.80	983.0
144.80	167.0
145.80	139.0
147.70	250.0
154.80	175.0
156.80	169.0
160.70	111.0
170.90	101.0
171.90	631.0
173.90	62440.0
174.80	4977.0
175.90	60592.0
176.80	3703.0
177.80	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136