
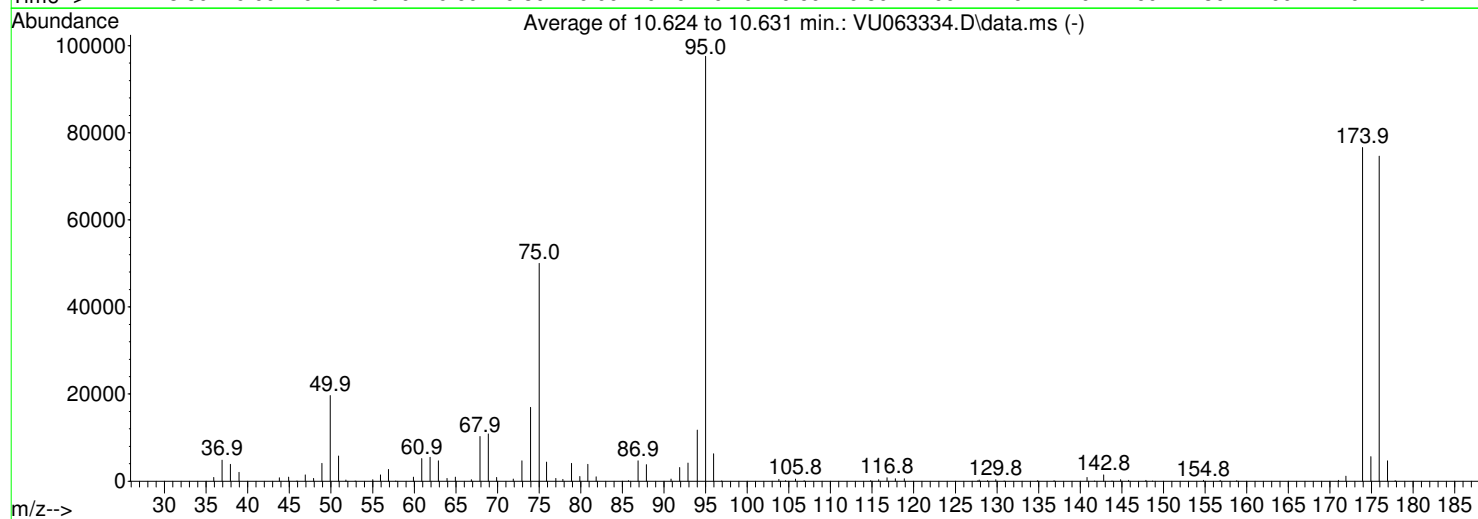


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040425\
Data File : VU063334.D
Acq On : 04 Apr 2025 09:18
Operator : MD/SY
Sample : BFB080
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB080

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040325WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Apr 07 09:46:31 2025

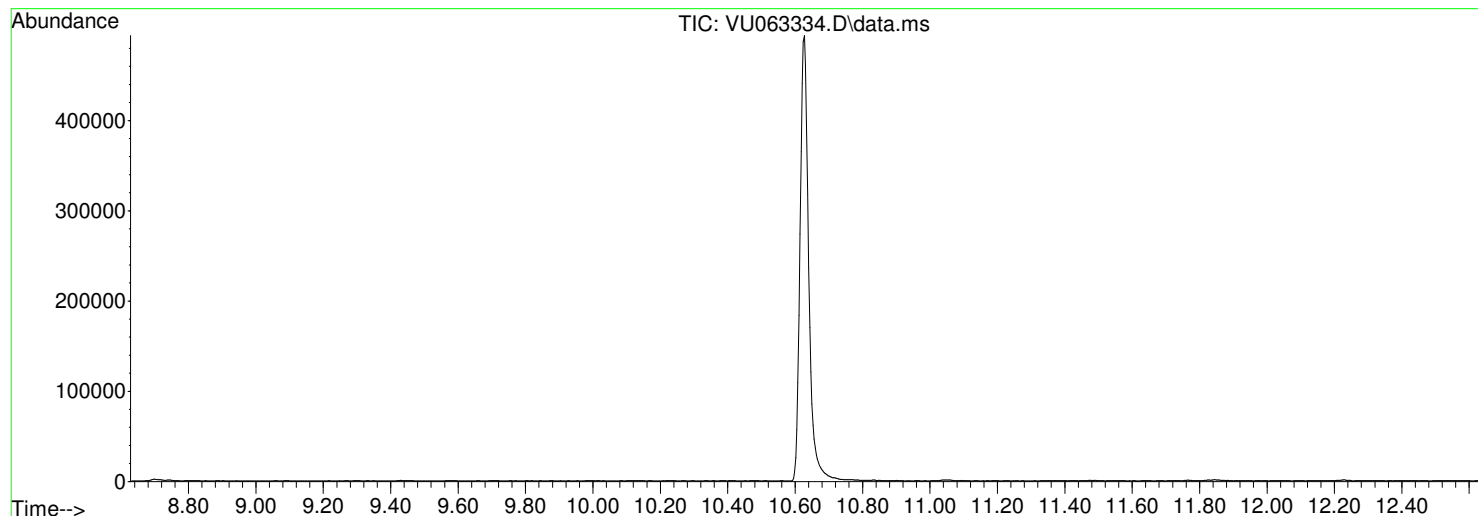

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	19675	PASS
75	95	30	80	51.2	49984	PASS
95	95	100	100	100.0	97581	PASS
96	95	5	9	6.5	6300	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.6	76653	PASS
175	174	5	9	7.4	5641	PASS
176	174	95	101	97.3	74616	PASS
177	176	5	9	6.2	4644	PASS

m/z	Abundance
39.80	348.0
43.80	298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080

m/z	Abundance
35.90	918.0
36.90	4990.0
37.90	4138.0
38.90	2140.0
39.80	367.0
43.90	1108.0
44.90	1014.0
46.90	1374.0
47.90	607.0
48.90	4382.0
49.90	20216.0
50.90	6073.0
51.80	281.0
52.90	124.0
55.00	338.0
56.00	1565.0
56.90	2696.0
59.90	998.0
60.90	5186.0
61.90	5446.0
62.90	4599.0
64.00	710.0
65.00	866.0
66.80	362.0
67.90	10654.0
68.90	11326.0
69.90	848.0
71.90	544.0
72.90	4551.0
73.90	17096.0
75.00	50880.0
75.90	4460.0
77.00	653.0
77.80	441.0
78.90	4107.0
79.90	1050.0
80.90	3858.0
81.90	1066.0
85.80	167.0
86.90	4967.0
87.90	3895.0
90.80	476.0
91.90	3155.0
92.90	4350.0
94.00	12034.0
95.00	99616.0
96.00	6447.0
96.90	124.0
103.80	406.0
105.80	455.0
106.80	132.0
115.80	352.0
116.80	779.0
117.80	547.0
118.90	588.0
127.70	345.0
128.90	155.0
129.80	300.0
130.80	103.0
134.80	121.0
136.90	131.0
140.80	827.0
142.80	1416.0
144.90	374.0
145.70	208.0
147.90	183.0
154.80	191.0
156.80	183.0
158.80	148.0
171.10	226.0
171.90	1123.0
173.90	76624.0
174.90	5737.0
175.90	73624.0
176.90	4683.0
177.90	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080

m/z	Abundance
35.90	881.0
36.90	4896.0
37.90	3946.0
39.00	2120.0
39.90	354.0
43.90	1130.0
44.90	914.0
46.90	1555.0
47.90	615.0
48.90	4186.0
49.90	20208.0
50.90	5905.0
51.80	273.0
55.00	335.0
56.00	1484.0
56.90	2763.0
57.80	106.0
59.90	961.0
60.90	5314.0
61.90	5702.0
62.90	4827.0
64.00	613.0
64.90	924.0
66.90	317.0
67.90	10601.0
68.90	11214.0
69.90	842.0
71.90	512.0
73.00	4831.0
73.90	17432.0
75.00	51144.0
75.90	4525.0
77.00	621.0
77.80	376.0
78.90	4303.0
79.90	1103.0
80.80	3904.0
81.90	1069.0
85.70	138.0
86.90	4800.0
87.90	3889.0
90.80	476.0
91.90	3248.0
92.90	4208.0
94.00	11994.0
95.00	100104.0
95.90	6455.0
103.80	443.0
104.60	140.0
105.80	499.0
106.90	122.0
114.80	114.0
115.80	303.0
116.80	745.0
117.80	596.0
118.90	575.0
127.90	366.0
128.80	141.0
129.90	321.0
134.90	108.0
136.90	124.0
140.80	861.0
141.70	101.0
142.80	1457.0
143.80	109.0
144.90	370.0
145.80	144.0
147.90	186.0
154.80	208.0
156.80	217.0
158.80	115.0
171.10	196.0
171.90	1190.0
173.90	78992.0
174.90	5850.0
175.90	76640.0
176.90	4810.0
177.80	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080

m/z	Abundance
35.90	779.0
36.90	4477.0
37.90	3572.0
38.90	1921.0
39.90	318.0
43.80	1016.0
44.90	785.0
45.90	135.0
46.90	1490.0
47.90	593.0
48.90	3666.0
49.90	18600.0
50.90	5413.0
51.80	267.0
55.00	306.0
55.90	1343.0
56.90	2560.0
57.80	112.0
59.90	817.0
60.90	4996.0
61.90	5320.0
62.90	4503.0
63.90	510.0
64.90	919.0
66.90	290.0
67.90	9510.0
68.90	9942.0
69.90	751.0
71.90	421.0
73.00	4564.0
74.00	16339.0
75.00	47928.0
75.90	4214.0
77.00	570.0
77.90	371.0
78.90	3905.0
79.90	1100.0
80.80	3872.0
81.80	954.0
85.70	143.0
86.90	4175.0
87.90	3648.0
90.90	404.0
91.90	2924.0
92.90	3870.0
94.00	11124.0
95.00	93024.0
95.90	5999.0
103.80	421.0
104.60	156.0
105.80	541.0
114.90	179.0
115.80	317.0
116.80	735.0
117.80	534.0
118.80	546.0
127.80	403.0
128.80	126.0
129.90	351.0
130.90	110.0
136.80	111.0
140.80	829.0
141.80	114.0
142.80	1365.0
143.80	100.0
144.80	355.0
145.90	160.0
147.90	153.0
148.70	101.0
154.80	228.0
156.80	225.0
171.00	173.0
171.90	1176.0
173.90	74344.0
174.90	5335.0
175.90	73584.0
176.90	4438.0
177.80	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB080