




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058450.D
Acq On : 06 Apr 2024 03:42
Operator : MD/SY
Sample : P1948-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK5

Manual IntegrationsAPPROVED

Quant Time: Apr 06 06:02:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 06 00:37:11 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

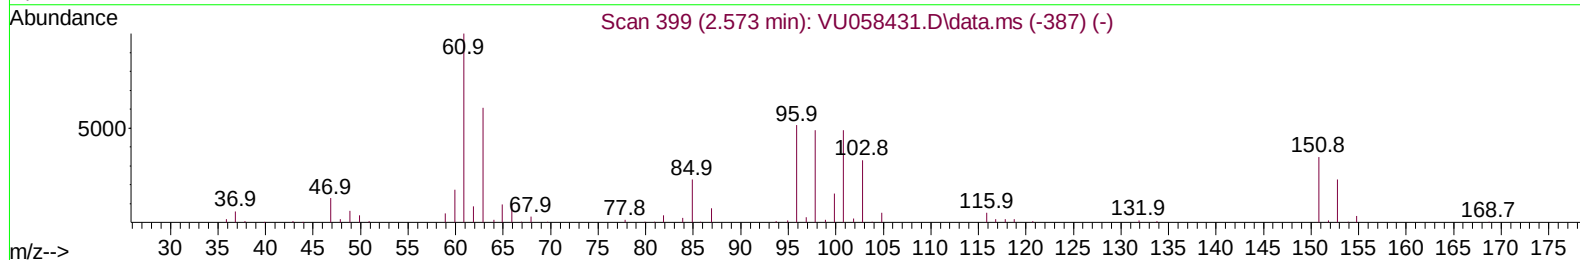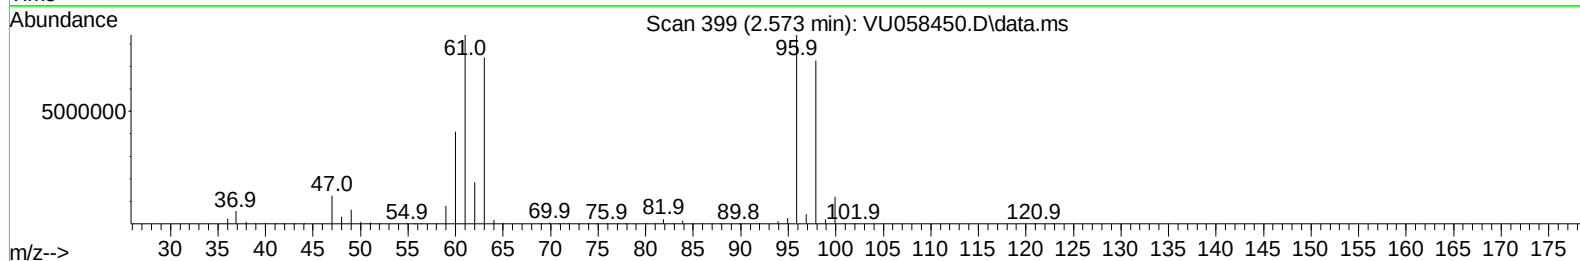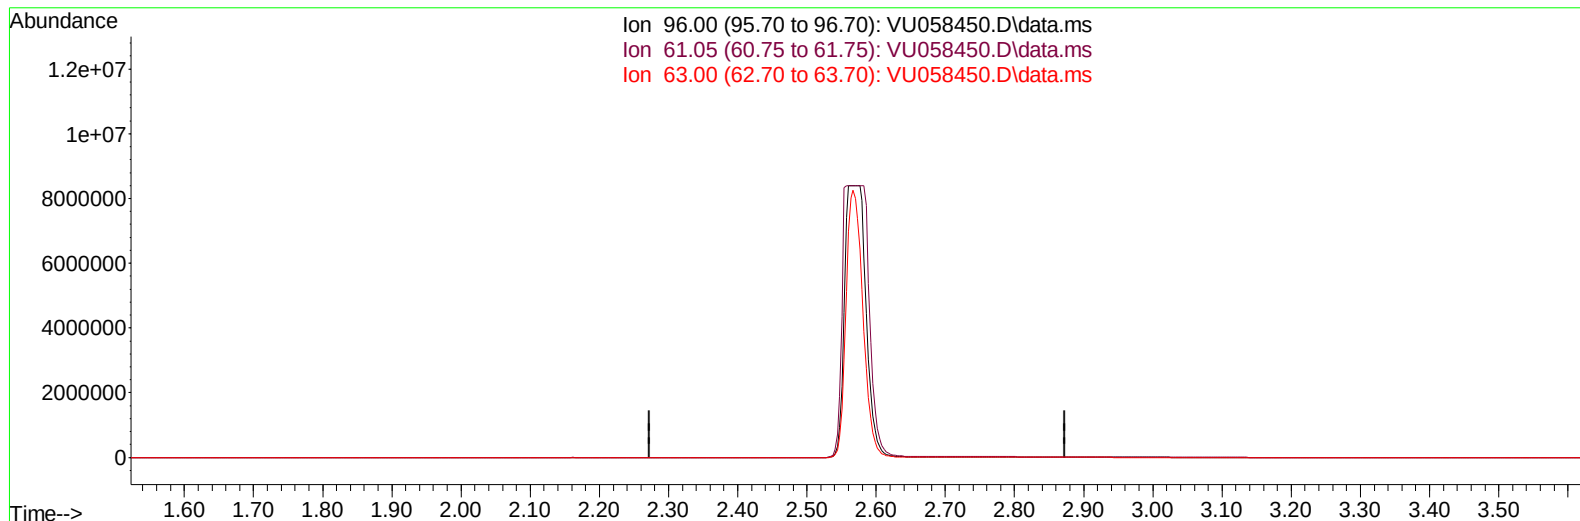

TIC: VU058450.D\data.ms

(12) 1,1-Dichloroethene (T)

2.573min (-2.573) 0.00 ug/L

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
61.05	189.30	0.00#
63.00	125.30	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058450.D
Acq On : 06 Apr 2024 03:42
Operator : MD/SY
Sample : P1948-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK5

Manual IntegrationsAPPROVED

Quant Time: Apr 06 06:02:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 06 00:37:11 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

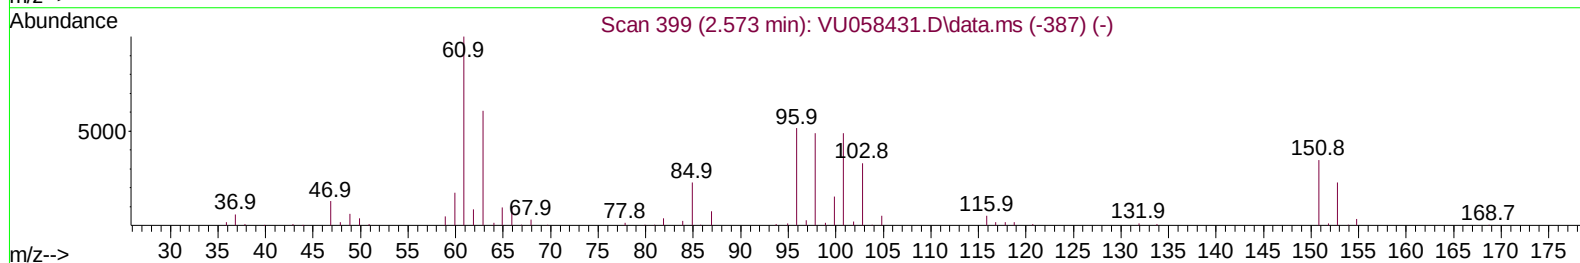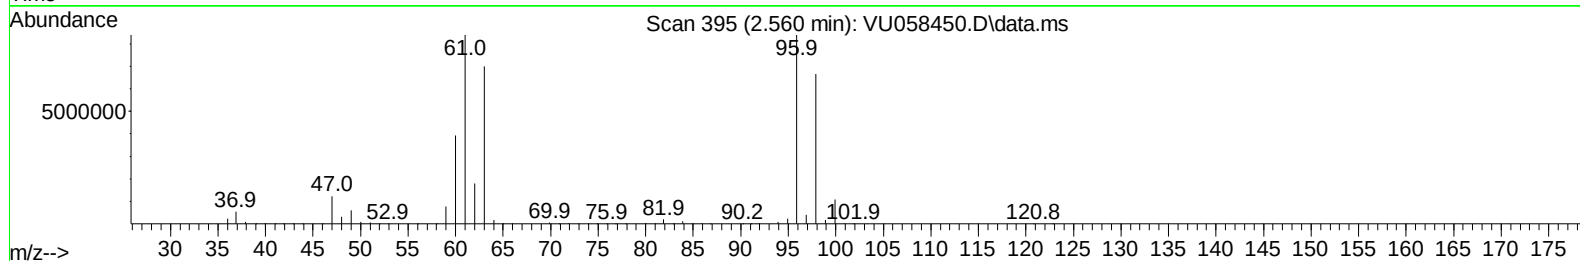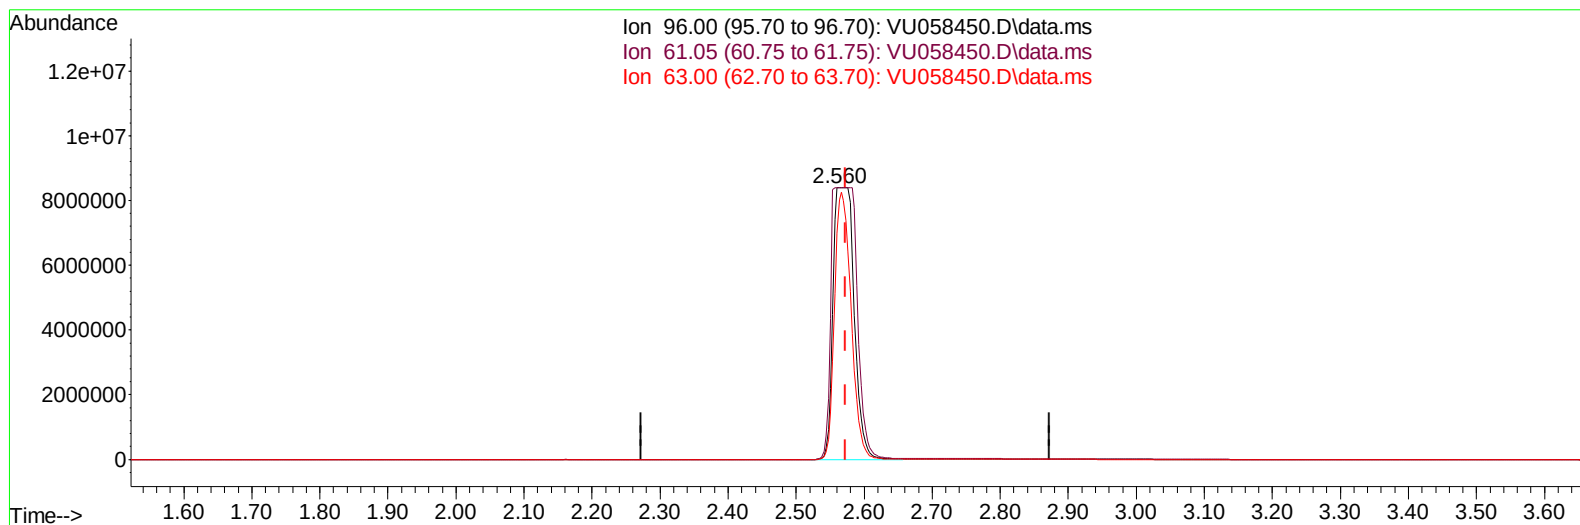

TIC: VU058450.D\data.ms

(12) 1,1-Dichloroethene (T)

2.560min (-0.013) 3013.09 ug/L m

response 17978545

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	189.30	100.00#
63.00	125.30	83.35#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058450.D
Acq On : 06 Apr 2024 03:42
Operator : MD/SY
Sample : P1948-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK5

Manual IntegrationsAPPROVED

Quant Time: Apr 06 06:02:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 06 00:37:11 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

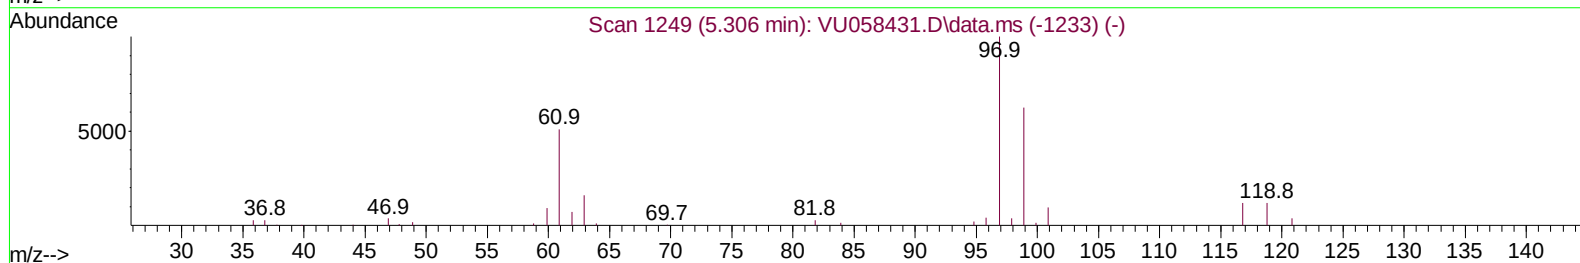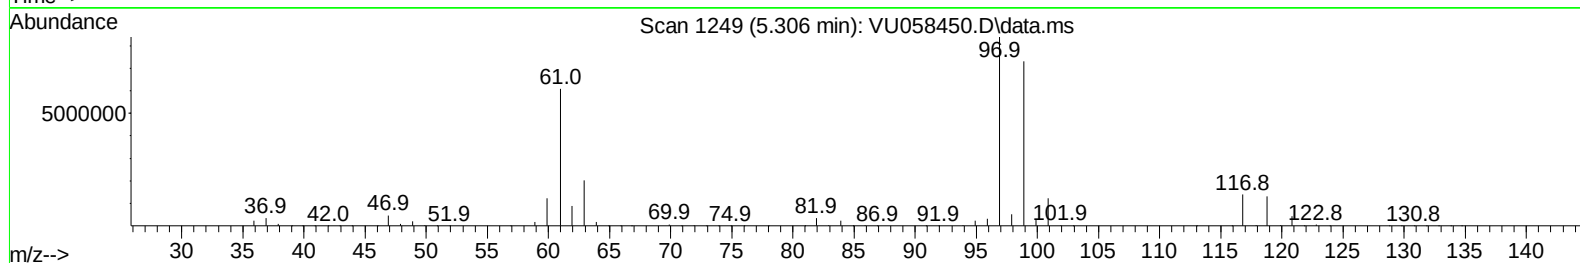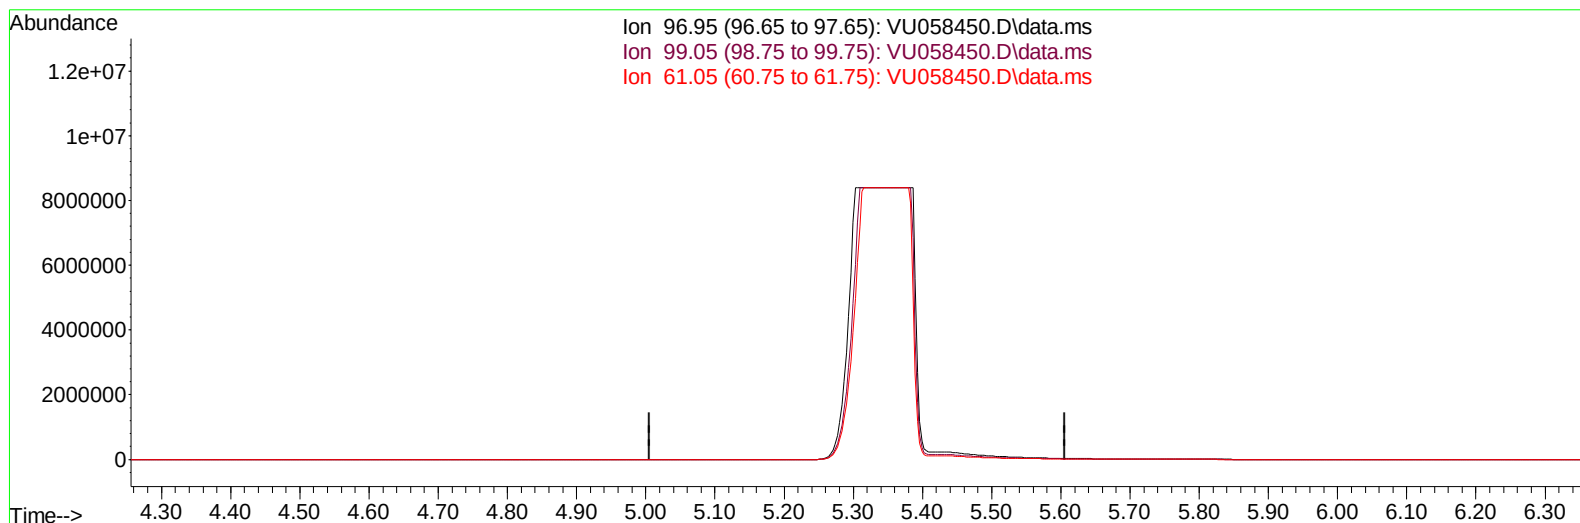

TIC: VU058450.D\data.ms

(29) 1,1,1-Trichloroethane (T)

5.306min (-5.306) 0.00 ug/L

response 0

Ion	Exp%	Act%
96.95	100.00	0.00
99.05	63.00	0.00#
61.05	49.20	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058450.D
Acq On : 06 Apr 2024 03:42
Operator : MD/SY
Sample : P1948-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK5

Manual IntegrationsAPPROVED

Quant Time: Apr 06 06:02:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 06 00:37:11 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
Supervised By :Semsettin Yesilyurt 04/08/2024

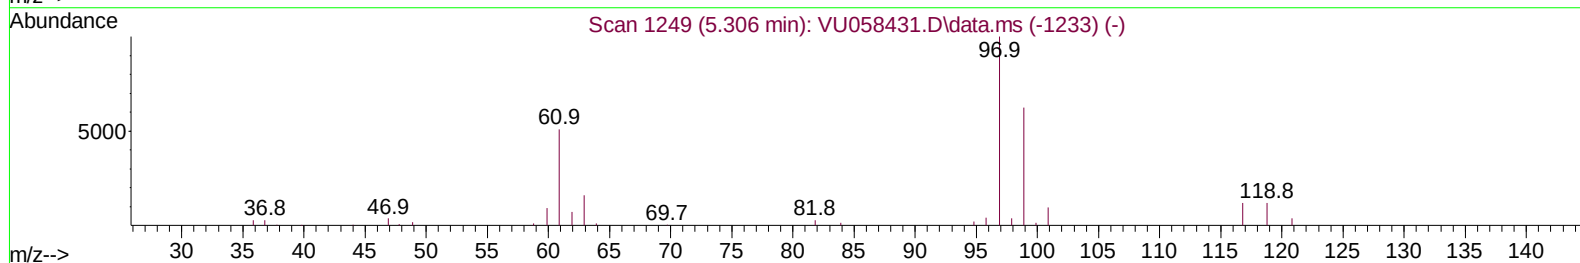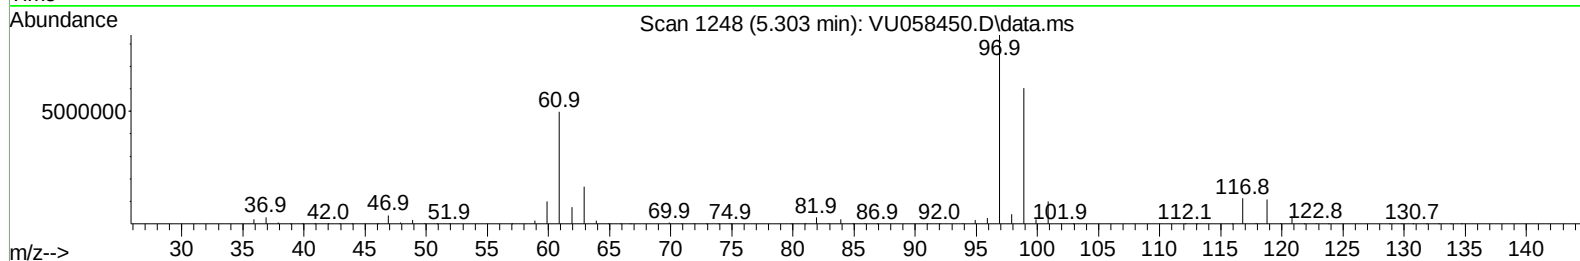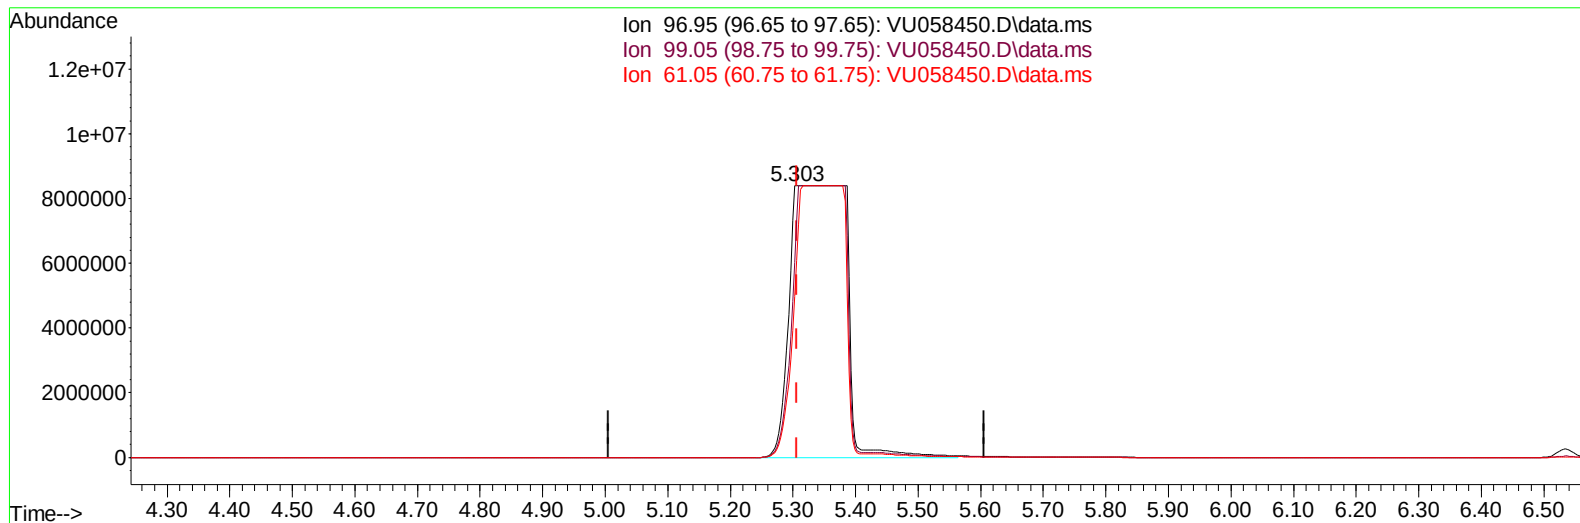

TIC: VU058450.D\data.ms

(29) 1,1,1-Trichloroethane (T)

5.303min (-0.003) 4988.54 ug/L m

response 52437601

Ion	Exp%	Act%
96.95	100.00	100.00
99.05	63.00	0.00#
61.05	49.20	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
 Data File : VU058450.D
 Acq On : 06 Apr 2024 03:42
 Operator : MD/SY
 Sample : P1948-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK5

Manual IntegrationsAPPROVED

Quant Time: Apr 06 06:02:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 06 00:37:11 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/08/2024
 Supervised By :Semsettin Yesilyurt 04/08/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		84194	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		78402	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		33871	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.592	65		22930	4.114	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	82.200%	
7) Chloroethane-d5	1.907	69		20945	4.324	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	86.400%	
11) 1,1-Dichloroethene-d2	2.557	65		16084	6.375	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	127.600%#	
20) 2-Butanone-d5	4.634	46		59443	50.603	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	101.200%	
24) Chloroform-d	5.055	84		52666	4.733	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	94.600%	
26) 1,2-Dichloroethane-d4	5.698	65		24986	4.811	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	96.200%	
32) Benzene-d6	5.724	84		103214	4.890	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	97.800%	
36) 1,2-Dichloropropane-d6	6.682	67		32582	4.922	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	98.400%	
41) Toluene-d8	7.891	98		86534	4.623	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	92.400%	
43) trans-1,3-Dichloroprop...	8.174	79		10389	5.056	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	101.200%	
46) 2-Hexanone-d5	8.631	63		42307	49.919	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	99.840%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		22220	4.755	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	95.000%	
66) 1,2-Dichlorobenzene-d4	12.187	152		26776	4.694	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	93.800%	
Target Compounds							
							Qvalue
5) vinyl chloride	1.599	62		14937	1.741	ug/L	96
8) Chloroethane	1.930	64		4069	0.751	ug/L	94
12) 1,1-Dichloroethene	2.560	96	17978545m	3013.090	ug/L		
16) Methylene chloride	3.039	84		2408	0.304	ug/L	97
19) 1,1-Dichloroethane	3.859	63	7102614	520.353	ug/L		99
22) cis-1,2-Dichloroethene	4.656	96		2431	0.346	ug/L	93
25) Chloroform	5.081	83		31781	2.406	ug/L	100
27) 1,2-Dichloroethane	5.788	62		44668	5.552	ug/L	98
29) 1,1,1-Trichloroethane	5.303	97	52437601m	4988.535	ug/L		
34) Trichloroethene	6.534	95		765295	106.826	ug/L	96
45) 1,1,2-Trichloroethane	8.393	97		2300	0.527	ug/L	94
47) Tetrachloroethene	8.547	164		18645	3.550	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

