

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
 Data File : VU058419.D
 Acq On : 05 Apr 2024 15:13
 Operator : MD/SY
 Sample : P1925-23
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB(20240328)

Quant Time: Apr 05 23:36:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 05 23:33:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.241	114	80617	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	77789	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	33520	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	23610	4.424	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.400%
7) Chloroethane-d5	1.907	69	21679	4.674	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.400%
11) 1,1-Dichloroethene-d2	2.560	65	10969	4.541	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.800%
20) 2-Butanone-d5	4.624	46	53076	47.187	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.380%
24) Chloroform-d	5.052	84	50427	4.733	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
26) 1,2-Dichloroethane-d4	5.695	65	24815	4.991	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.800%
32) Benzene-d6	5.717	84	99296	4.741	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
36) 1,2-Dichloropropane-d6	6.682	67	32163	4.897	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.000%
41) Toluene-d8	7.891	98	82894	4.463	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.200%
43) trans-1,3-Dichloroprop...	8.177	79	8924	4.377	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.600%
46) 2-Hexanone-d5	8.627	63	37125	44.150	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.300%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	19965	4.306	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	26175	4.636	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.800%
Target Compounds						
16) Methylene chloride	3.039	84	4926	0.650	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058419.D
Acq On : 05 Apr 2024 15:13
Operator : MD/SY
Sample : P1925-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB(20240328)


Quant Time: Apr 05 23:36:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 05 23:33:02 2024
Response via : Initial Calibration

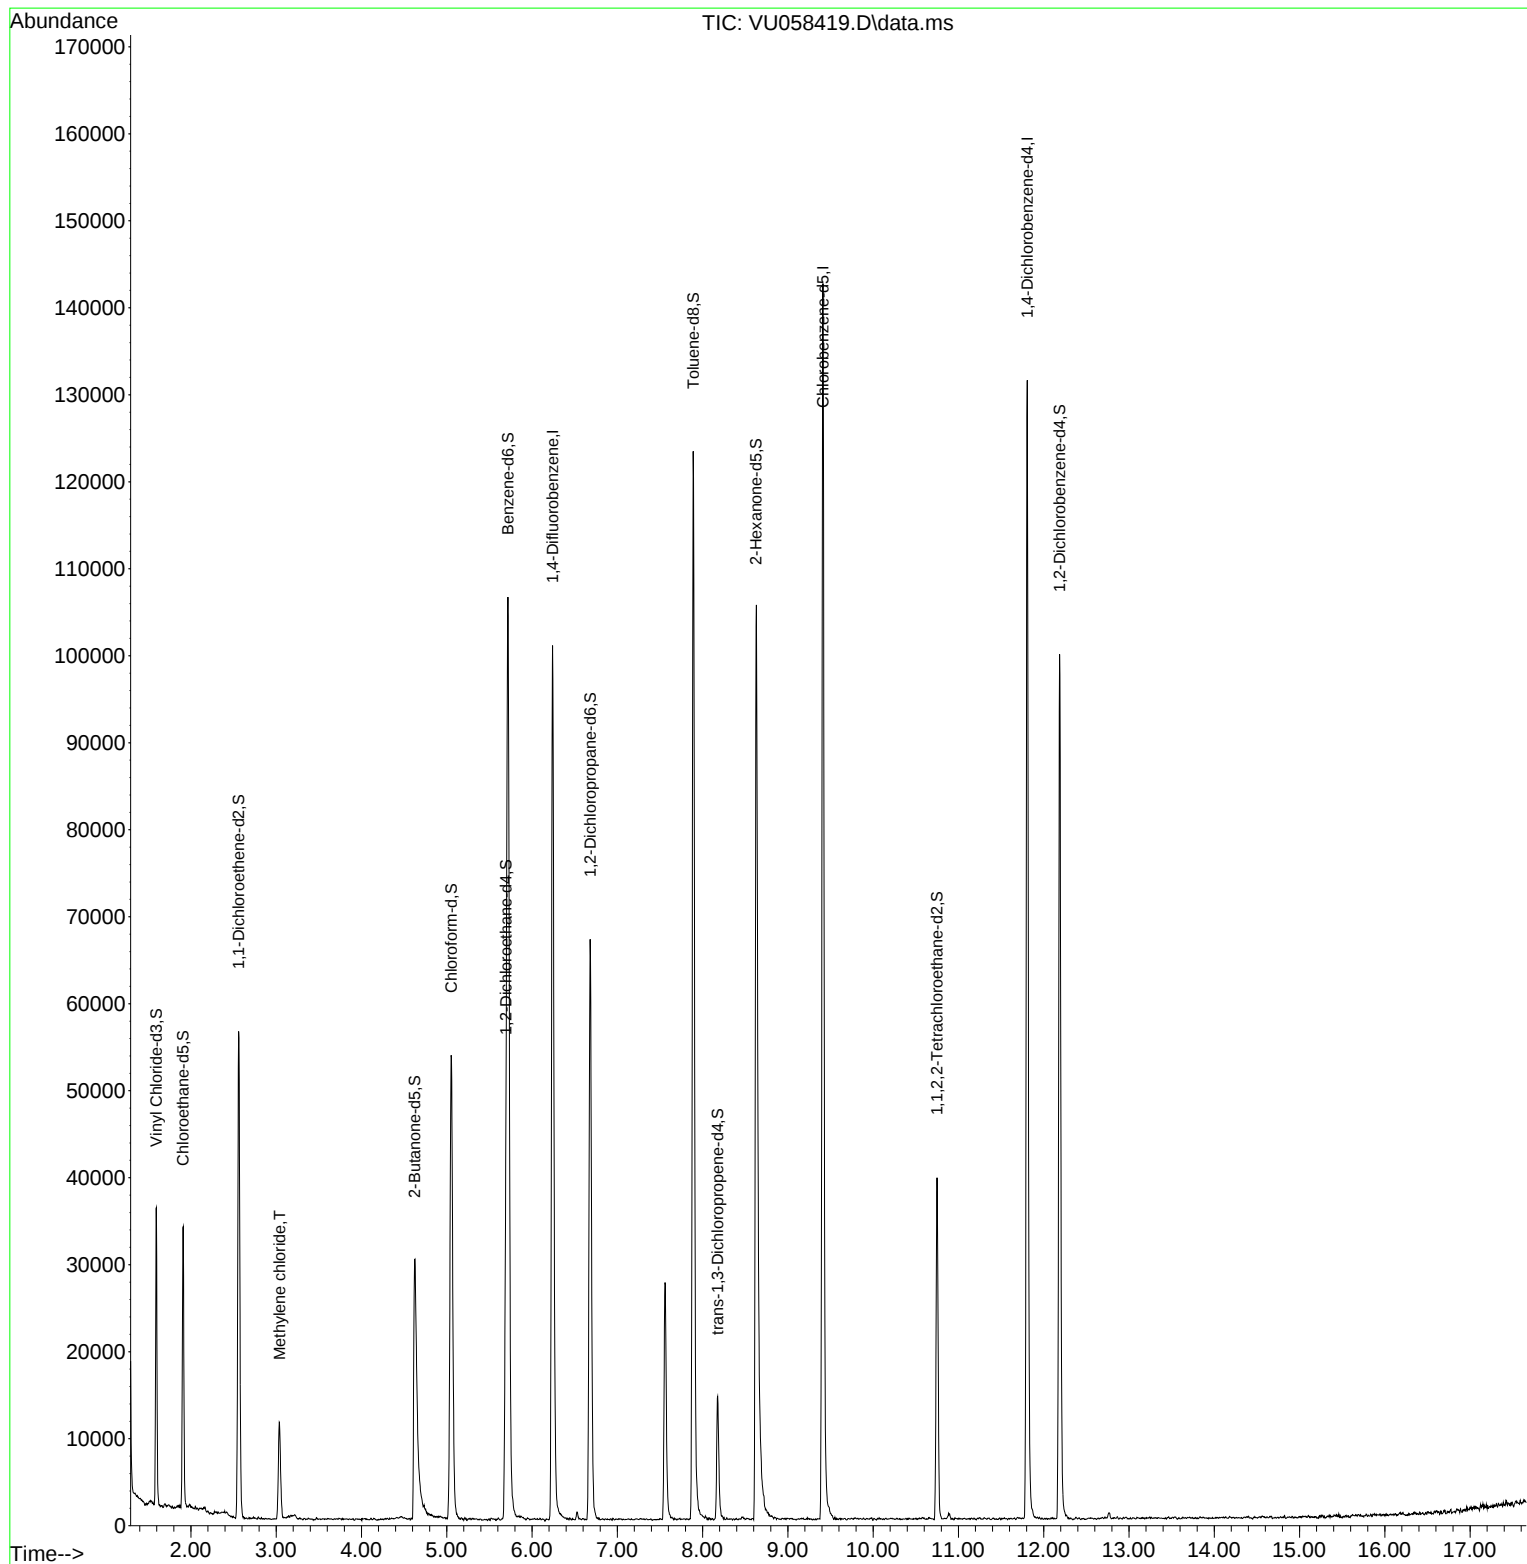

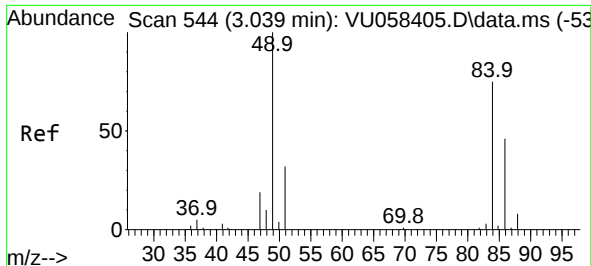

#16
Methylene chloride
Concen: 0.650 ug/L
RT: 3.039 min Scan# 54
Delta R.T. -0.000 min
Lab File: VU058419.D
Acq: 05 Apr 2024 15:13

Instrument :
MSVOA_U
ClientSampleId :
TB(20240328)

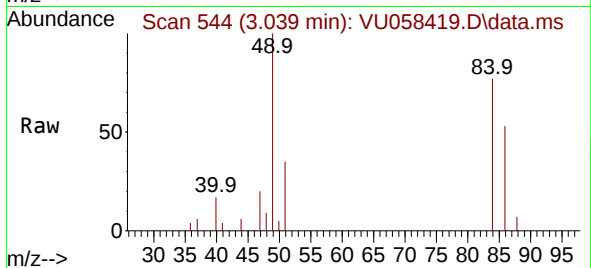

Tgt Ion:	84	Resp:	4926
Ion	Ratio	Lower	Upper
84	100		
86	68.7	44.3	82.3
49	130.4	96.0	178.2

