

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
 Data File : VU058437.D
 Acq On : 05 Apr 2024 22:37
 Operator : MD/SY
 Sample : P1949-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Apr 06 05:58:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 06 00:37:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	79983	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	77172	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	33558	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	22370	4.224	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.400%
7) Chloroethane-d5	1.907	69	20641	4.485	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.800%
11) 1,1-Dichloroethene-d2	2.560	65	10876	4.538	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.800%
20) 2-Butanone-d5	4.628	46	55082	49.359	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.720%
24) Chloroform-d	5.052	84	49458	4.679	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
26) 1,2-Dichloroethane-d4	5.692	65	24174	4.900	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.000%
32) Benzene-d6	5.718	84	97417	4.689	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
36) 1,2-Dichloropropane-d6	6.682	67	31334	4.809	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.200%
41) Toluene-d8	7.891	98	80111	4.348	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.000%
43) trans-1,3-Dichloroprop...	8.177	79	8526	4.216	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.400%
46) 2-Hexanone-d5	8.627	63	38159	45.743	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.480%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	19921	4.331	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	25337	4.483	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.600%
Target Compounds					Qvalue	
16) Methylene chloride	3.039	84	1170	0.156	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058437.D
Acq On : 05 Apr 2024 22:37
Operator : MD/SY
Sample : P1949-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Apr 06 05:58:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 06 00:37:11 2024
Response via : Initial Calibration

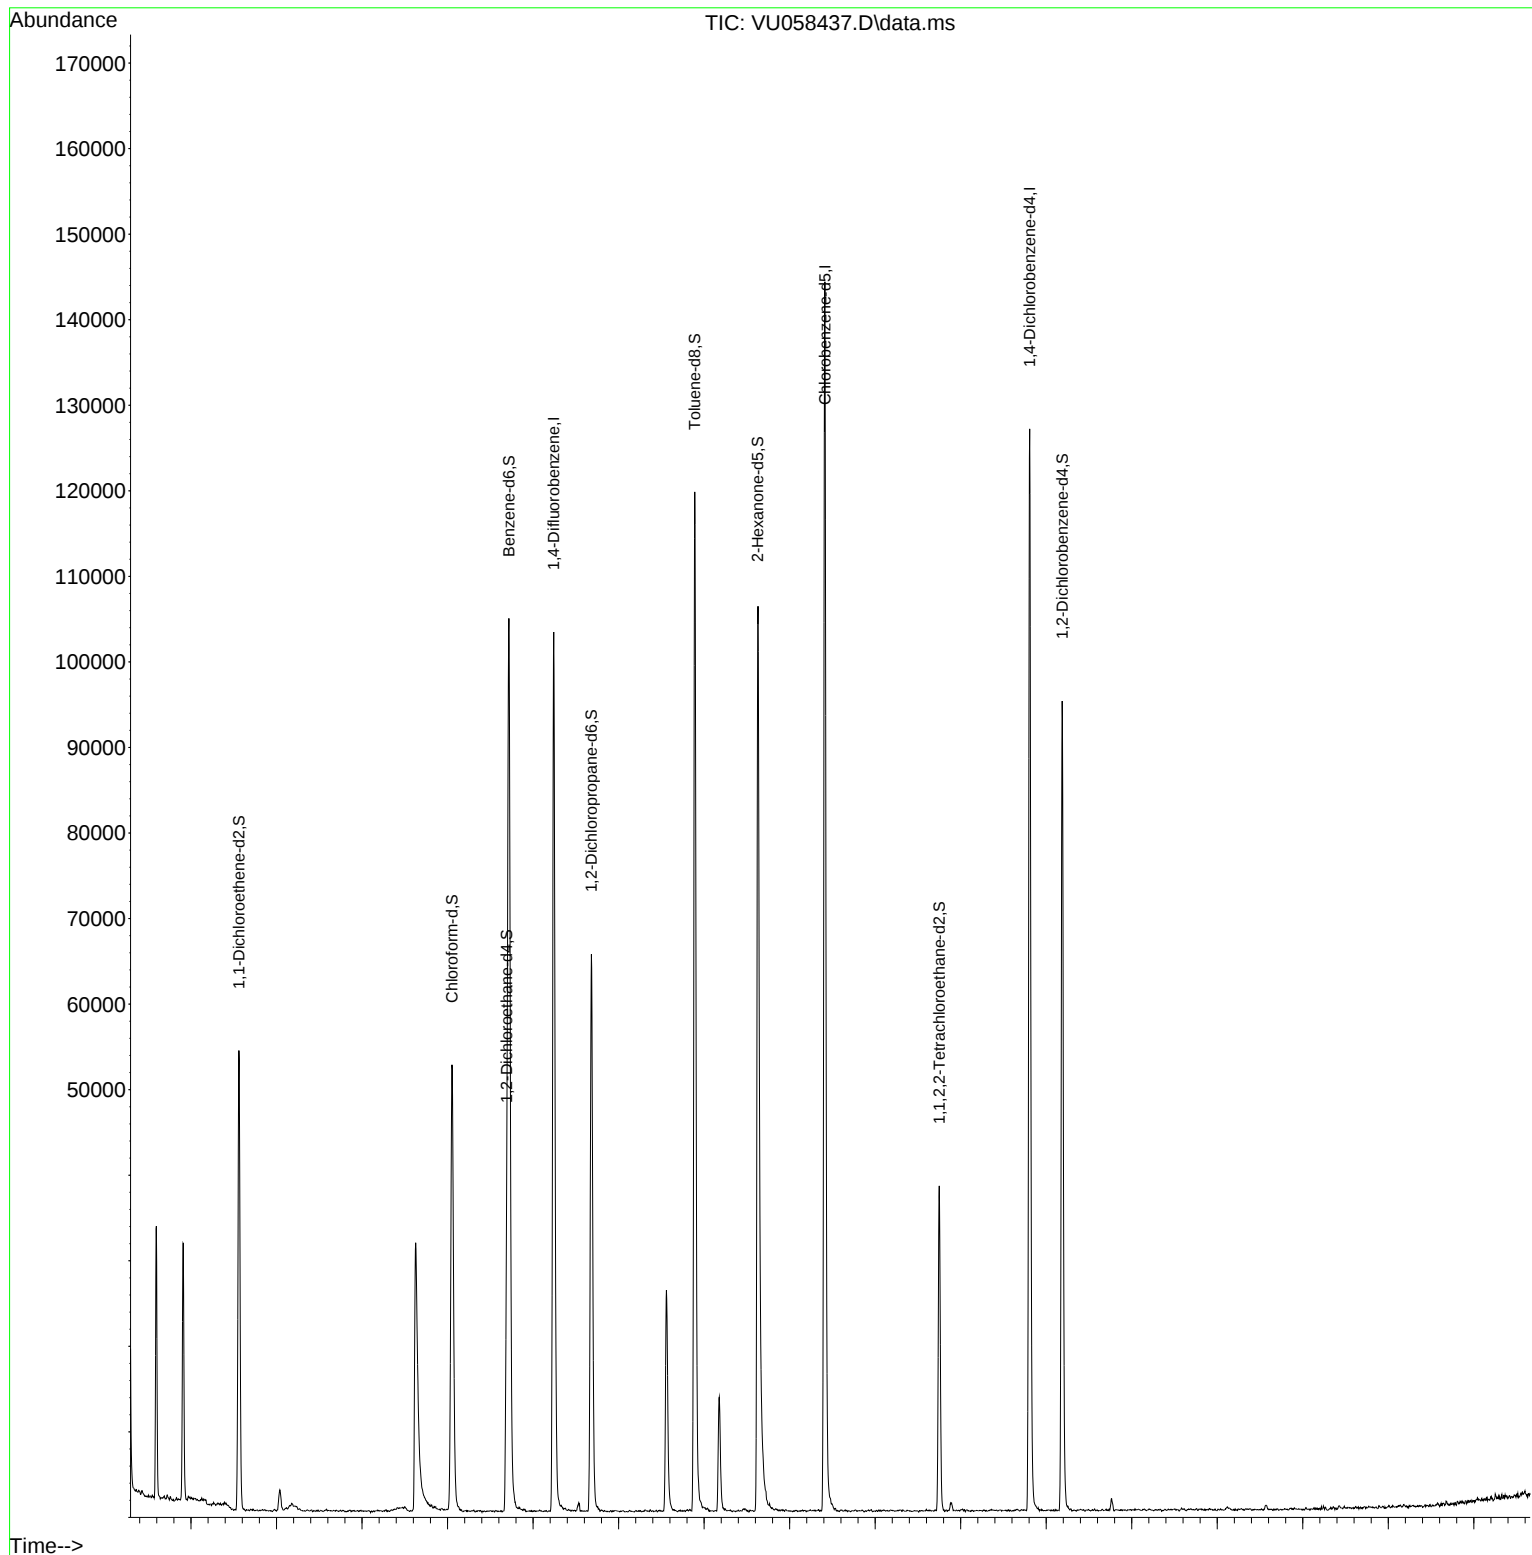

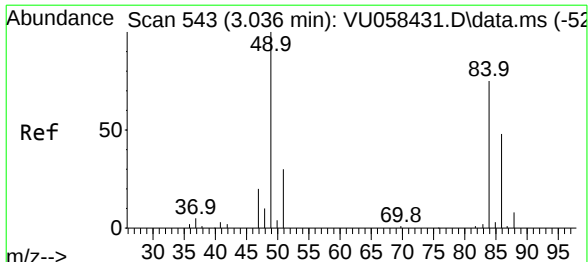

#16
Methylene chloride
Concen: 0.156 ug/L
RT: 3.039 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU058437.D
Acq: 05 Apr 2024 22:37

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Tgt	Ion: 84	Resp:	1170
Ion	Ratio	Lower	Upper
84	100		
86	56.2	44.3	82.3
49	132.6	96.0	178.2

