

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
 Data File : VU058422.D
 Acq On : 05 Apr 2024 16:24
 Operator : MD/SY
 Sample : P1925-15DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-8S(20240328)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU058422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	109	rVB2	36996	43691	4.85%	1.274%
2	1.907	183	192	205	rBV	32103	40251	4.47%	1.174%
3	2.560	382	395	411	rBV2	55961	92831	10.30%	2.707%
4	3.036	531	543	561	rBV	24620	46290	5.14%	1.350%
5	3.351	631	641	654	rBV3	6039	11006	1.22%	0.321%
6	3.859	783	799	820	rVB	11221	26726	2.97%	0.779%
7	4.657	1019	1047	1080	rBV2	120888	354799	39.38%	10.345%
8	5.052	1156	1170	1203	rVB	52063	117695	13.06%	3.432%
9	5.718	1358	1377	1414	rBV2	105454	283224	31.44%	8.258%
10	6.242	1528	1540	1578	rBV	100644	197505	21.92%	5.759%
11	6.682	1665	1677	1697	rBV	64289	126639	14.06%	3.692%
12	7.560	1939	1950	1968	rBV2	26475	47514	5.27%	1.385%
13	7.891	2041	2053	2071	rBV	119064	209637	23.27%	6.112%
14	8.177	2126	2142	2160	rBV3	14122	25202	2.80%	0.735%
15	8.631	2272	2283	2321	rBV2	104318	222420	24.69%	6.485%
16	9.412	2514	2526	2551	rBV2	145969	329551	36.58%	9.609%
17	10.750	2932	2942	2958	rBV	38242	62516	6.94%	1.823%
18	11.740	3239	3250	3260	rBV	68727	108793	12.08%	3.172%
19	11.830	3260	3278	3303	rVB2	426262	900903	100.00%	26.268%
20	12.187	3377	3389	3408	rBV	106331	182527	20.26%	5.322%




Sum of corrected areas: 3429720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058422.D
Acq On : 05 Apr 2024 16:24
Operator : MD/SY
Sample : P1925-15DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-8S(20240328)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

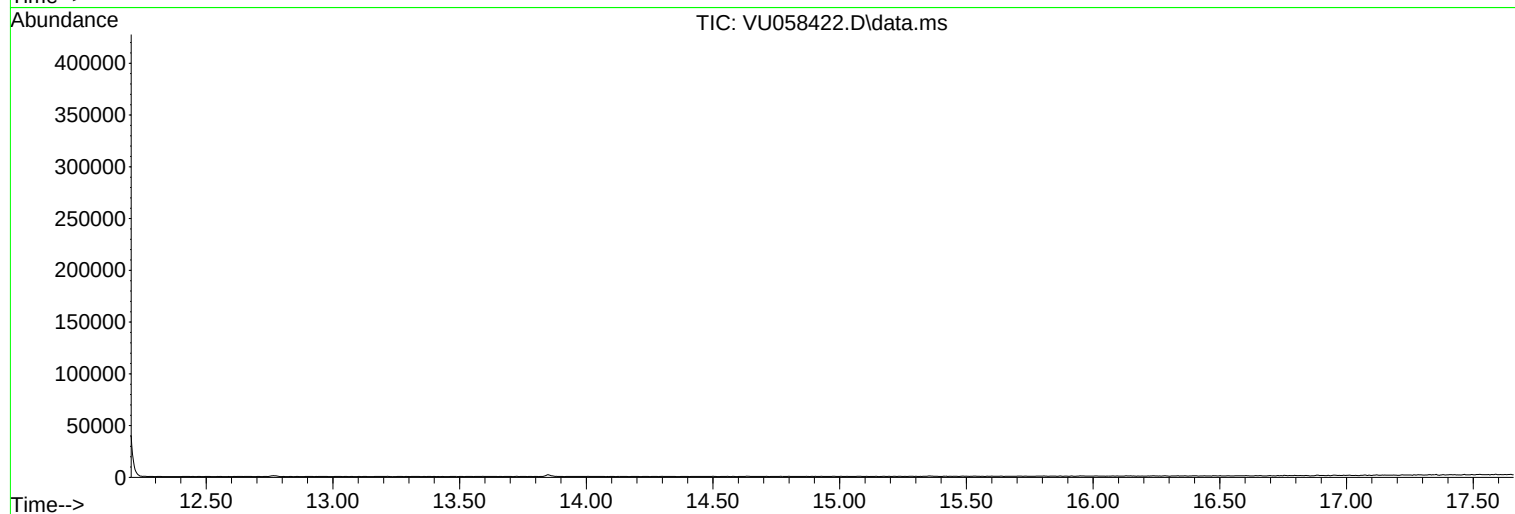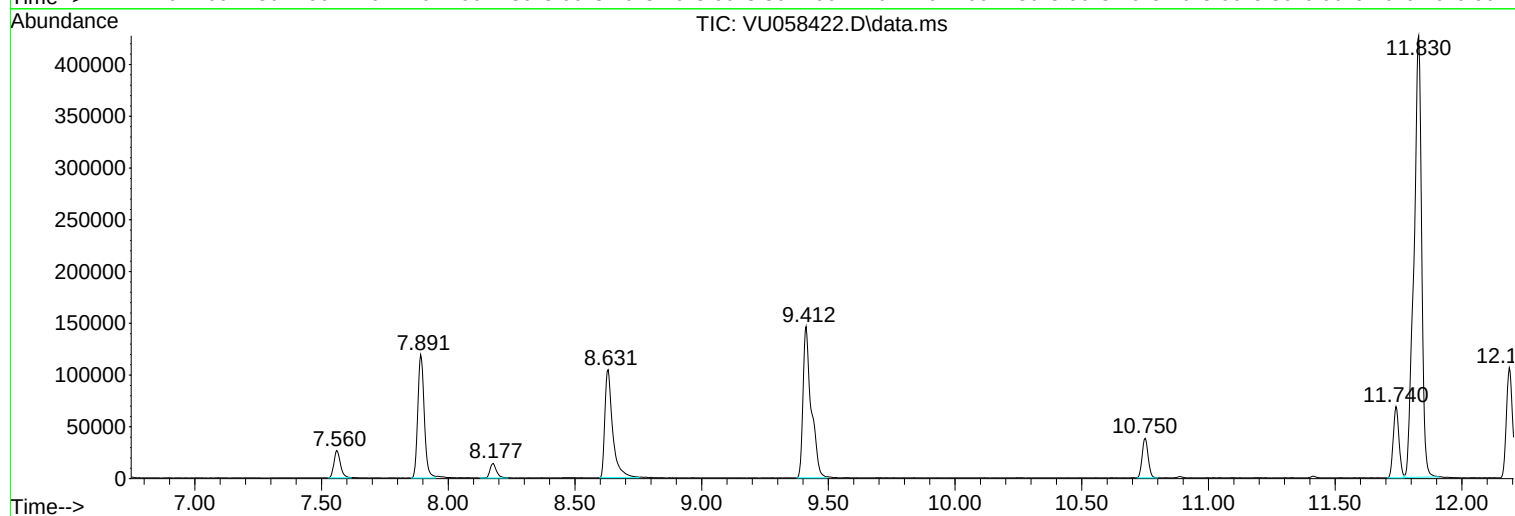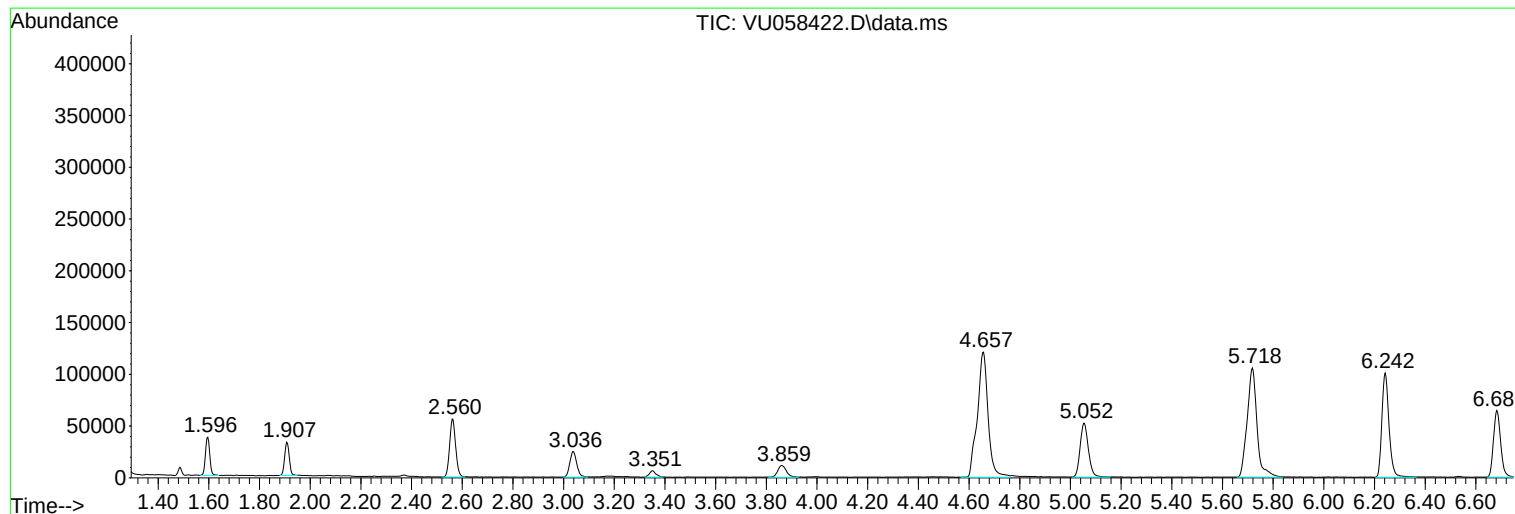

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058422.D
Acq On : 05 Apr 2024 16:24
Operator : MD/SY
Sample : P1925-15DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-8S(20240328)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058422.D
Acq On : 05 Apr 2024 16:24
Operator : MD/SY
Sample : P1925-15DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-8S(20240328)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc