
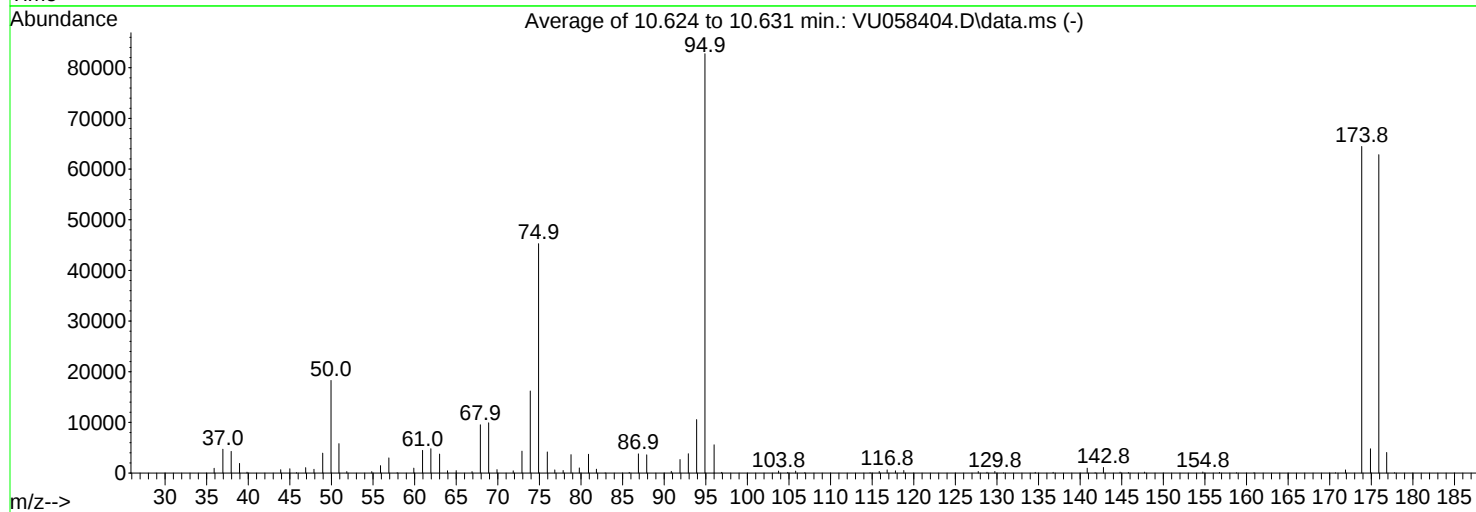


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040524\
Data File : VU058404.D
Acq On : 05 Apr 2024 08:22
Operator : MD/SY
Sample : BFB137
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB137

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Apr 06 00:37:11 2024

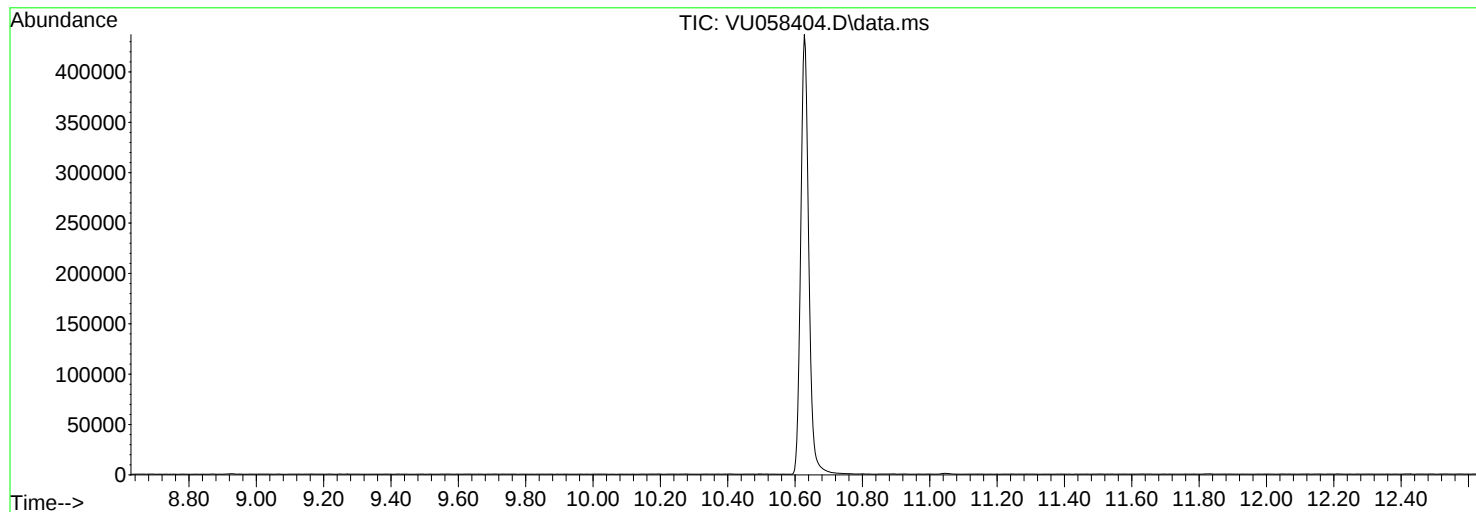

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	18283	PASS
75	95	30	80	54.7	45275	PASS
95	95	100	100	100.0	82765	PASS
96	95	5	9	6.7	5580	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.9	64461	PASS
175	174	5	9	7.4	4793	PASS
176	174	95	101	97.5	62837	PASS
177	176	5	9	6.5	4067	PASS

Scan 2890 (10.582 min): VU058404.D\data.ms
BFB137

m/z	Abundance
39.90	534.0
43.90	174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.90	965.0
36.90	4599.0
38.00	4181.0
38.90	1927.0
39.90	696.0
43.90	835.0
45.00	811.0
45.80	129.0
46.90	1058.0
47.90	757.0
49.00	4004.0
49.90	18368.0
50.90	5665.0
51.90	316.0
54.80	282.0
55.90	1483.0
56.90	2942.0
57.90	126.0
59.90	966.0
60.90	4415.0
62.00	4702.0
63.00	3821.0
63.90	464.0
65.00	464.0
66.90	277.0
67.90	9087.0
68.90	9696.0
69.90	713.0
71.80	458.0
72.90	4306.0
73.90	15871.0
74.90	43992.0
76.00	4203.0
76.90	625.0
77.90	492.0
78.80	3742.0
79.80	987.0
80.90	3591.0
81.90	805.0
85.80	124.0
86.90	3639.0
87.90	3348.0
90.90	349.0
91.90	2591.0
92.90	3780.0
93.90	10308.0
94.90	80656.0
96.00	5563.0
96.90	148.0
103.70	357.0
104.80	144.0
105.80	352.0
106.90	120.0
115.90	307.0
116.80	556.0
117.80	409.0
118.80	519.0
127.70	327.0
128.80	174.0
129.80	321.0
130.80	108.0
134.60	143.0
136.70	167.0
140.90	955.0
142.80	1041.0
144.80	179.0
145.80	114.0
147.70	146.0
154.70	219.0
156.80	131.0
160.90	100.0
170.70	104.0
171.90	614.0
173.80	60752.0
174.90	4618.0
175.90	58880.0
176.90	3905.0
177.80	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.90	990.0
36.90	4866.0
38.00	4420.0
38.90	1965.0
39.80	740.0
43.90	867.0
45.00	874.0
45.80	128.0
46.90	1106.0
47.90	768.0
49.00	4018.0
50.00	18768.0
50.90	6005.0
51.90	305.0
54.90	299.0
55.90	1517.0
56.90	3115.0
57.90	122.0
59.90	999.0
61.00	4647.0
61.90	4986.0
63.00	3876.0
63.90	462.0
65.00	512.0
66.90	294.0
67.90	9857.0
68.90	10240.0
69.90	699.0
71.90	448.0
72.90	4495.0
73.90	16680.0
74.90	46776.0
76.00	4301.0
76.90	657.0
77.80	529.0
78.80	3749.0
79.80	1050.0
80.90	3832.0
81.80	776.0
82.90	103.0
85.80	135.0
86.90	3917.0
87.90	3743.0
90.90	341.0
91.90	2751.0
92.90	3951.0
93.90	10890.0
94.90	85400.0
96.00	5833.0
96.90	146.0
103.80	410.0
104.80	147.0
105.80	399.0
106.90	109.0
114.80	113.0
115.80	337.0
116.80	651.0
117.80	480.0
118.80	527.0
127.70	330.0
128.80	182.0
129.70	335.0
134.60	151.0
136.70	150.0
140.80	1005.0
141.80	112.0
142.80	1152.0
144.80	200.0
145.80	129.0
147.80	197.0
154.70	226.0
156.70	138.0
158.80	110.0
160.90	112.0
170.70	110.0
171.90	630.0
173.90	66512.0
174.90	4945.0
175.90	64872.0
176.80	4199.0
177.80	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.90	911.0
37.00	4676.0
37.90	4252.0
39.00	1815.0
39.80	724.0
43.90	818.0
45.00	877.0
46.90	1054.0
47.90	718.0
48.90	3784.0
50.00	17712.0
50.90	5752.0
51.80	259.0
54.90	291.0
55.90	1421.0
56.90	2923.0
59.90	962.0
60.90	4399.0
61.90	4732.0
63.00	3556.0
64.00	446.0
65.00	480.0
66.90	270.0
67.90	9650.0
68.90	9815.0
69.90	639.0
71.90	437.0
72.90	4205.0
73.90	16053.0
74.90	45056.0
75.90	3992.0
76.80	596.0
77.80	516.0
78.80	3426.0
79.80	1005.0
80.90	3724.0
81.80	717.0
85.80	141.0
86.90	3815.0
87.90	3724.0
90.80	333.0
91.90	2680.0
92.90	3733.0
93.90	10476.0
94.90	82240.0
96.00	5345.0
96.90	128.0
103.70	426.0
104.90	148.0
105.80	425.0
114.70	120.0
115.80	370.0
116.80	710.0
117.80	461.0
118.80	496.0
127.80	287.0
128.80	167.0
129.70	305.0
134.60	142.0
136.80	126.0
140.80	953.0
141.80	112.0
142.80	1122.0
144.80	201.0
145.80	108.0
147.80	240.0
154.80	207.0
156.70	131.0
158.80	118.0
171.90	628.0
173.90	66120.0
174.90	4815.0
175.90	64760.0
176.90	4096.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137