

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041420\
 Data File : VU037704.D
 Acq On : 14 Apr 2020 17:48
 Operator : JC/MD
 Sample : L2275-04
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YAQC2

Quant Time: Apr 15 03:42:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 15 03:02:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	311858	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	298882	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	145783	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	119242	5.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.00%
7) Chloroethane-d5	1.93	69	99220	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.59	63	153410	3.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.20%
20) 2-Butanone-d5	4.66	46	335783	51.81	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.62%
24) Chloroform-d	5.10	84	178992	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.74	65	103767	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.76	84	404562	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
36) 1,2-Dichloropropane-d6	6.72	67	131047	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.92	98	365847	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
43) trans-1,3-Dichloropropene-	8.20	79	56460	4.78	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.60%
46) 2-Hexanone-d5	8.66	63	303345	50.20	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.40%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	101136	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.60%
64) 1,2-Dichlorobenzene-d4	12.20	152	128597	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%


Target Compounds					Ovalue
13) Acetone	2.66	43	16915	3.958 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041420\
Data File : VU037704.D
Acq On : 14 Apr 2020 17:48
Operator : JC/MD
Sample : L2275-04
Misc : 25mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YAQC2

Quant Time: Apr 15 03:42:19 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 15 03:02:33 2020
Response via : Initial Calibration

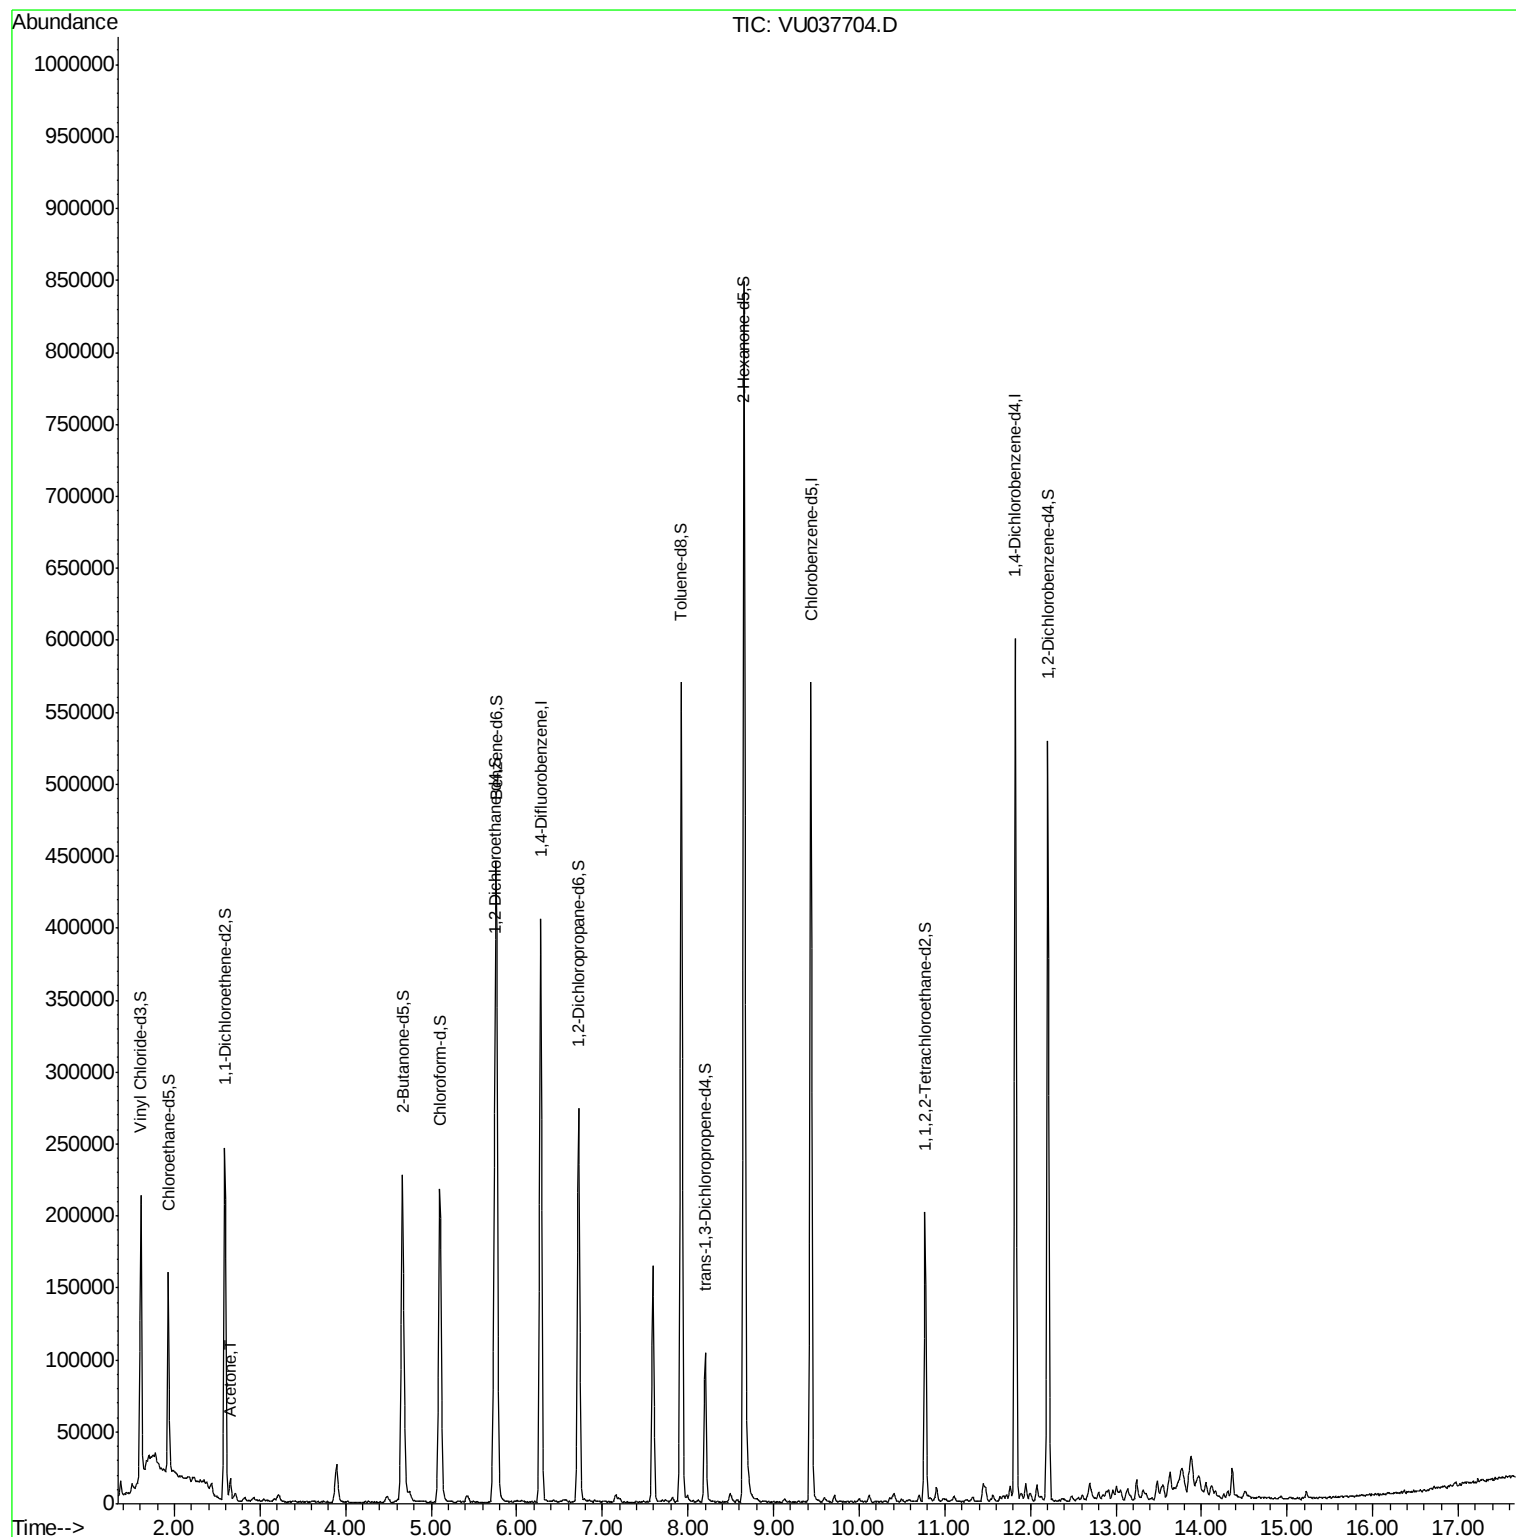

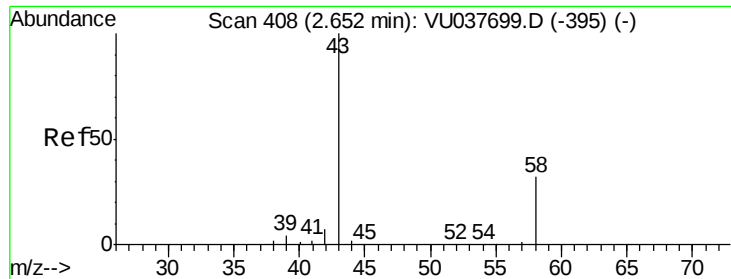

#13

Acetone

Concen: 3.958 ug/L

RT: 2.66 min Scan# 409

Delta R.T. 0.00 min

Lab File: VU037704.D

Acq: 14 Apr 2020 17:48

Instrument :
MSVOA_U
ClientSampleId :
YAQC2

Tot Ion: 43 Resp: 16915

Ion Ratio Lower Upper

43 100

58 29.5 0.0 64.8

