


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041420\
 Data File : VU037692.D
 Acq On : 14 Apr 2020 10:13
 Operator : JC/MD
 Sample : BFB13
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB13

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Apr 15 03:02:33 2020

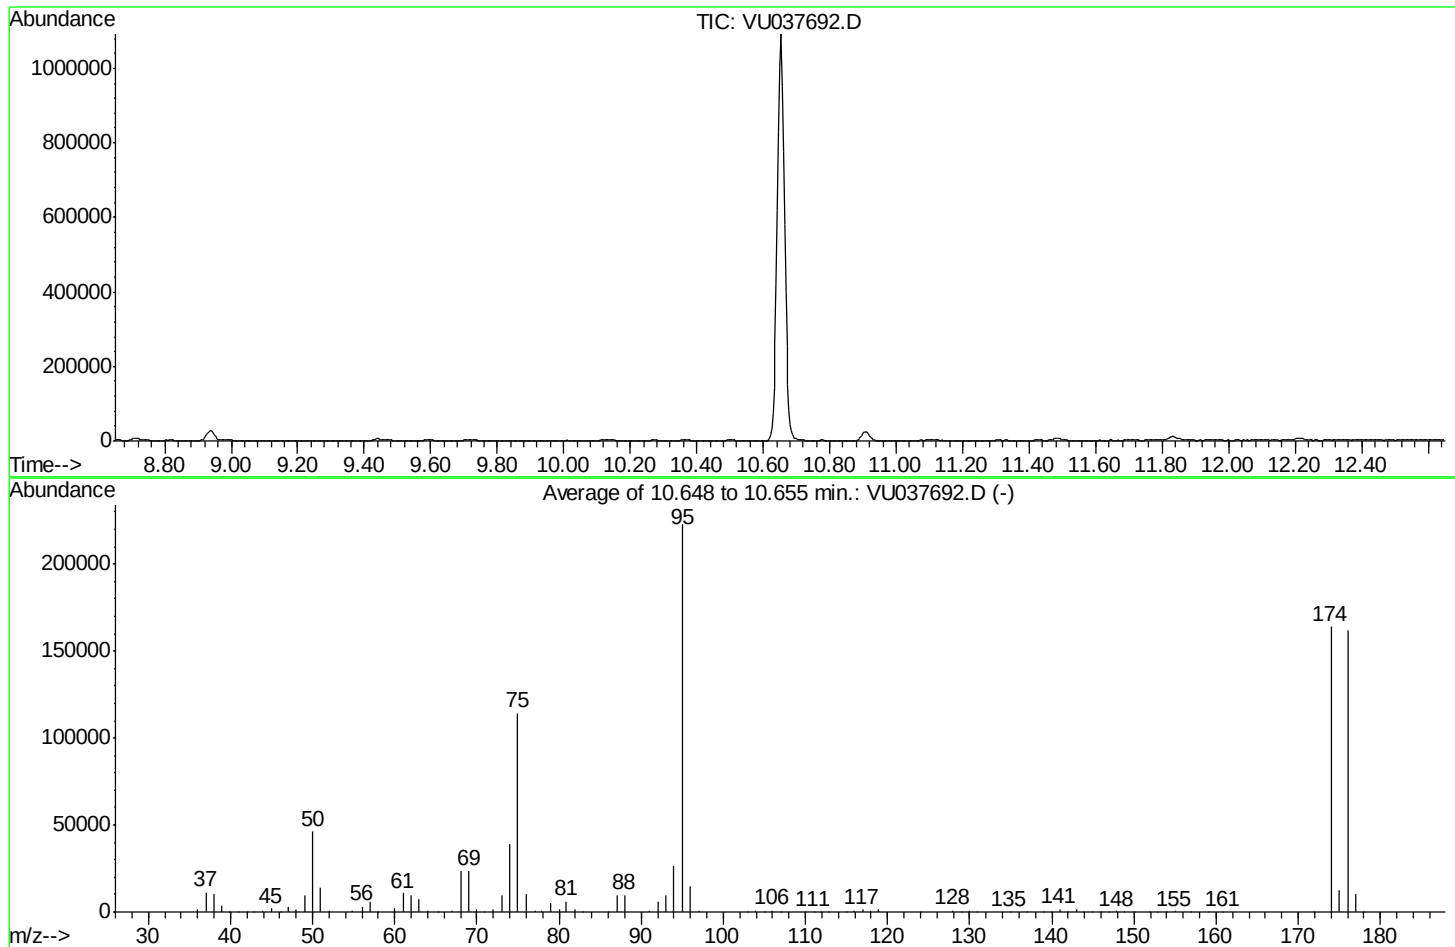

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	46344	PASS
75	95	30	80	51.4	114429	PASS
95	95	100	100	100.0	222826	PASS
96	95	5	9	6.7	14925	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.6	164053	PASS
175	174	5	9	7.8	12752	PASS
176	174	95	101	98.7	161856	PASS
177	176	5	9	6.4	10402	PASS

m/z	Abundance
36.00	1568.0
37.00	10754.0
38.00	9704.0
39.00	4110.0
39.90	347.0
40.90	171.0
42.00	103.0
42.90	254.0
44.00	1846.0
45.00	1898.0
46.10	251.0
47.00	3106.0
48.00	1286.0
49.00	8824.0
50.00	45832.0
51.00	14078.0
52.00	638.0
54.90	440.0
56.00	3256.0
57.00	5954.0
58.00	211.0
60.00	1877.0
61.00	10434.0
62.00	9546.0
63.00	7200.0
64.00	684.0
65.20	149.0
67.00	576.0
68.00	22328.0
69.10	23232.0
70.00	1873.0
71.00	124.0
72.00	1284.0
73.00	9599.0
74.00	37352.0
75.00	110480.0
76.00	9864.0
77.10	1114.0
77.90	889.0
78.90	5007.0
80.00	1601.0
80.90	5582.0
81.90	1332.0
82.90	127.0
86.00	183.0
87.00	8854.0
88.00	9596.0
90.90	782.0
92.00	5686.0
93.00	8703.0
94.00	25600.0
95.10	212608.0
96.00	14025.0
97.00	348.0
103.90	695.0
104.90	280.0
105.90	675.0
106.90	147.0
111.00	190.0
111.80	107.0
114.90	140.0
116.00	627.0
117.00	1149.0
117.90	665.0
118.90	1014.0
123.90	132.0
128.00	849.0
129.00	362.0
129.90	661.0
130.90	332.0
134.90	279.0
136.90	279.0
139.90	140.0
140.90	1746.0
142.00	265.0
143.00	1640.0
143.90	122.0
145.00	159.0
146.00	266.0
146.90	182.0
147.90	324.0
148.80	113.0
150.00	157.0
152.90	146.0
155.00	554.0
156.90	191.0
159.00	163.0
160.90	124.0
171.90	249.0
174.00	152576.0
175.00	11679.0
176.00	150720.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

177.00	9874.0
177.90	317.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
36.00	1671.0
37.00	11533.0
38.00	10277.0
39.00	4223.0
39.90	333.0
40.90	180.0
42.00	124.0
42.90	314.0
44.00	1729.0
45.00	2185.0
46.10	240.0
47.00	3362.0
48.00	1334.0
49.00	9599.0
50.00	47960.0
51.00	14777.0
52.00	677.0
54.90	539.0
56.00	3337.0
57.00	6381.0
58.00	274.0
60.00	2118.0
61.00	11263.0
62.00	10164.0
63.00	7900.0
64.00	773.0
67.00	633.0
68.00	24216.0
69.00	24616.0
70.00	1890.0
70.90	163.0
72.00	1334.0
73.10	9974.0
74.00	40752.0
75.00	118208.0
76.10	10823.0
77.00	1141.0
77.90	846.0
78.90	5420.0
80.00	1709.0
80.90	6172.0
82.00	1443.0
82.80	146.0
87.00	9805.0
88.00	10072.0
90.90	831.0
92.00	5997.0
93.00	9739.0
94.00	27856.0
95.10	230336.0
96.00	15458.0
97.00	518.0
103.90	712.0
105.00	292.0
106.00	786.0
107.00	221.0
111.10	219.0
111.90	131.0
112.70	121.0
114.90	230.0
115.90	670.0
117.00	1297.0
117.90	776.0
118.90	1134.0
124.00	123.0
127.90	875.0
128.90	353.0
129.90	807.0
130.90	323.0
134.90	299.0
136.90	301.0
139.00	104.0
139.80	151.0
140.90	1845.0
142.00	278.0
143.00	1786.0
143.90	113.0
145.00	170.0
145.90	295.0
146.90	170.0
147.90	455.0
148.70	163.0
150.00	162.0
151.80	134.0
152.90	179.0
153.90	100.0
155.00	620.0
156.90	219.0
159.00	162.0
160.90	124.0
171.90	266.0
174.00	169472.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

175.00	13277.0
176.00	167680.0
177.00	10735.0
177.90	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
36.00	1694.0
37.00	11101.0
38.00	10045.0
39.00	3772.0
39.90	304.0
40.90	157.0
42.10	116.0
42.90	327.0
44.00	1706.0
45.00	2160.0
46.10	201.0
47.00	3159.0
48.00	1213.0
49.00	9371.0
50.00	45240.0
51.00	13869.0
52.10	613.0
54.90	609.0
56.00	3214.0
57.00	6342.0
58.00	257.0
60.00	1990.0
61.00	10739.0
62.00	10165.0
63.00	7903.0
64.00	720.0
67.00	643.0
68.00	23960.0
69.00	23256.0
70.00	1761.0
70.90	157.0
72.00	1360.0
73.10	9655.0
74.00	40056.0
75.00	114600.0
76.10	10350.0
77.00	1046.0
77.80	788.0
78.90	5185.0
80.00	1695.0
80.90	6001.0
81.90	1393.0
82.80	199.0
87.00	9653.0
88.00	9481.0
90.90	800.0
92.00	5985.0
93.00	9577.0
94.00	27008.0
95.10	225536.0
96.00	15294.0
97.00	559.0
102.90	100.0
103.90	641.0
105.10	326.0
106.00	854.0
107.00	245.0
110.00	113.0
111.00	182.0
111.90	144.0
112.80	130.0
114.90	281.0
115.90	628.0
117.00	1225.0
117.90	815.0
118.90	1267.0
127.90	792.0
128.90	314.0
129.90	857.0
130.90	292.0
134.90	264.0
136.90	280.0
140.00	148.0
141.00	1742.0
142.00	265.0
142.90	1812.0
143.80	100.0
144.90	140.0
145.90	300.0
146.90	149.0
147.90	532.0
148.70	152.0
150.00	191.0
151.90	161.0
152.90	146.0
153.90	123.0
155.00	608.0
157.00	298.0
159.00	204.0
160.80	133.0
174.00	170112.0
175.00	13301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

176.00	167168.0
177.00	10597.0
177.90	204.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

Scan 2881 (10.603 min): VU037692.D
BFB13

m/z	Abundance
38.90	145.0
39.80	178.0
40.90	135.0
43.90	871.0
55.10	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13