

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041520\
 Data File : VU037736.D
 Acq On : 15 Apr 2020 16:18
 Operator : JC/MD
 Sample : VIBLK21
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK21

Quant Time: Apr 16 10:15:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 16 01:23:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	267376	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	253453	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	125993	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	88527	4.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.40%
7) Chloroethane-d5	1.93	69	76655	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.80%
11) 1,1-Dichloroethene-d2	2.59	63	113514	3.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.20%
20) 2-Butanone-d5	4.67	46	297555	53.55	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.10%
24) Chloroform-d	5.10	84	146934	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.74	65	90941	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
32) Benzene-d6	5.76	84	318587	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
36) 1,2-Dichloropropane-d6	6.72	67	109302	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.92	98	284577	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	8.20	79	46784	4.67	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.40%
46) 2-Hexanone-d5	8.66	63	268943	52.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.96%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	85345	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.00%
64) 1,2-Dichlorobenzene-d4	12.21	152	104900	4.67	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.40%


Target Compounds					Ovalue
3) Chloromethane	1.53	50	4721	0.165 ug/L	95
13) Acetone	2.66	43	4308	1.176 ug/L	74
16) Methylene chloride	3.07	84	4357	0.209 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041520\
Data File : VU037736.D
Acq On : 15 Apr 2020 16:18
Operator : JC/MD
Sample : VIBLK21
Misc : 25mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK21

Quant Time: Apr 16 10:15:32 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 16 01:23:00 2020
Response via : Initial Calibration

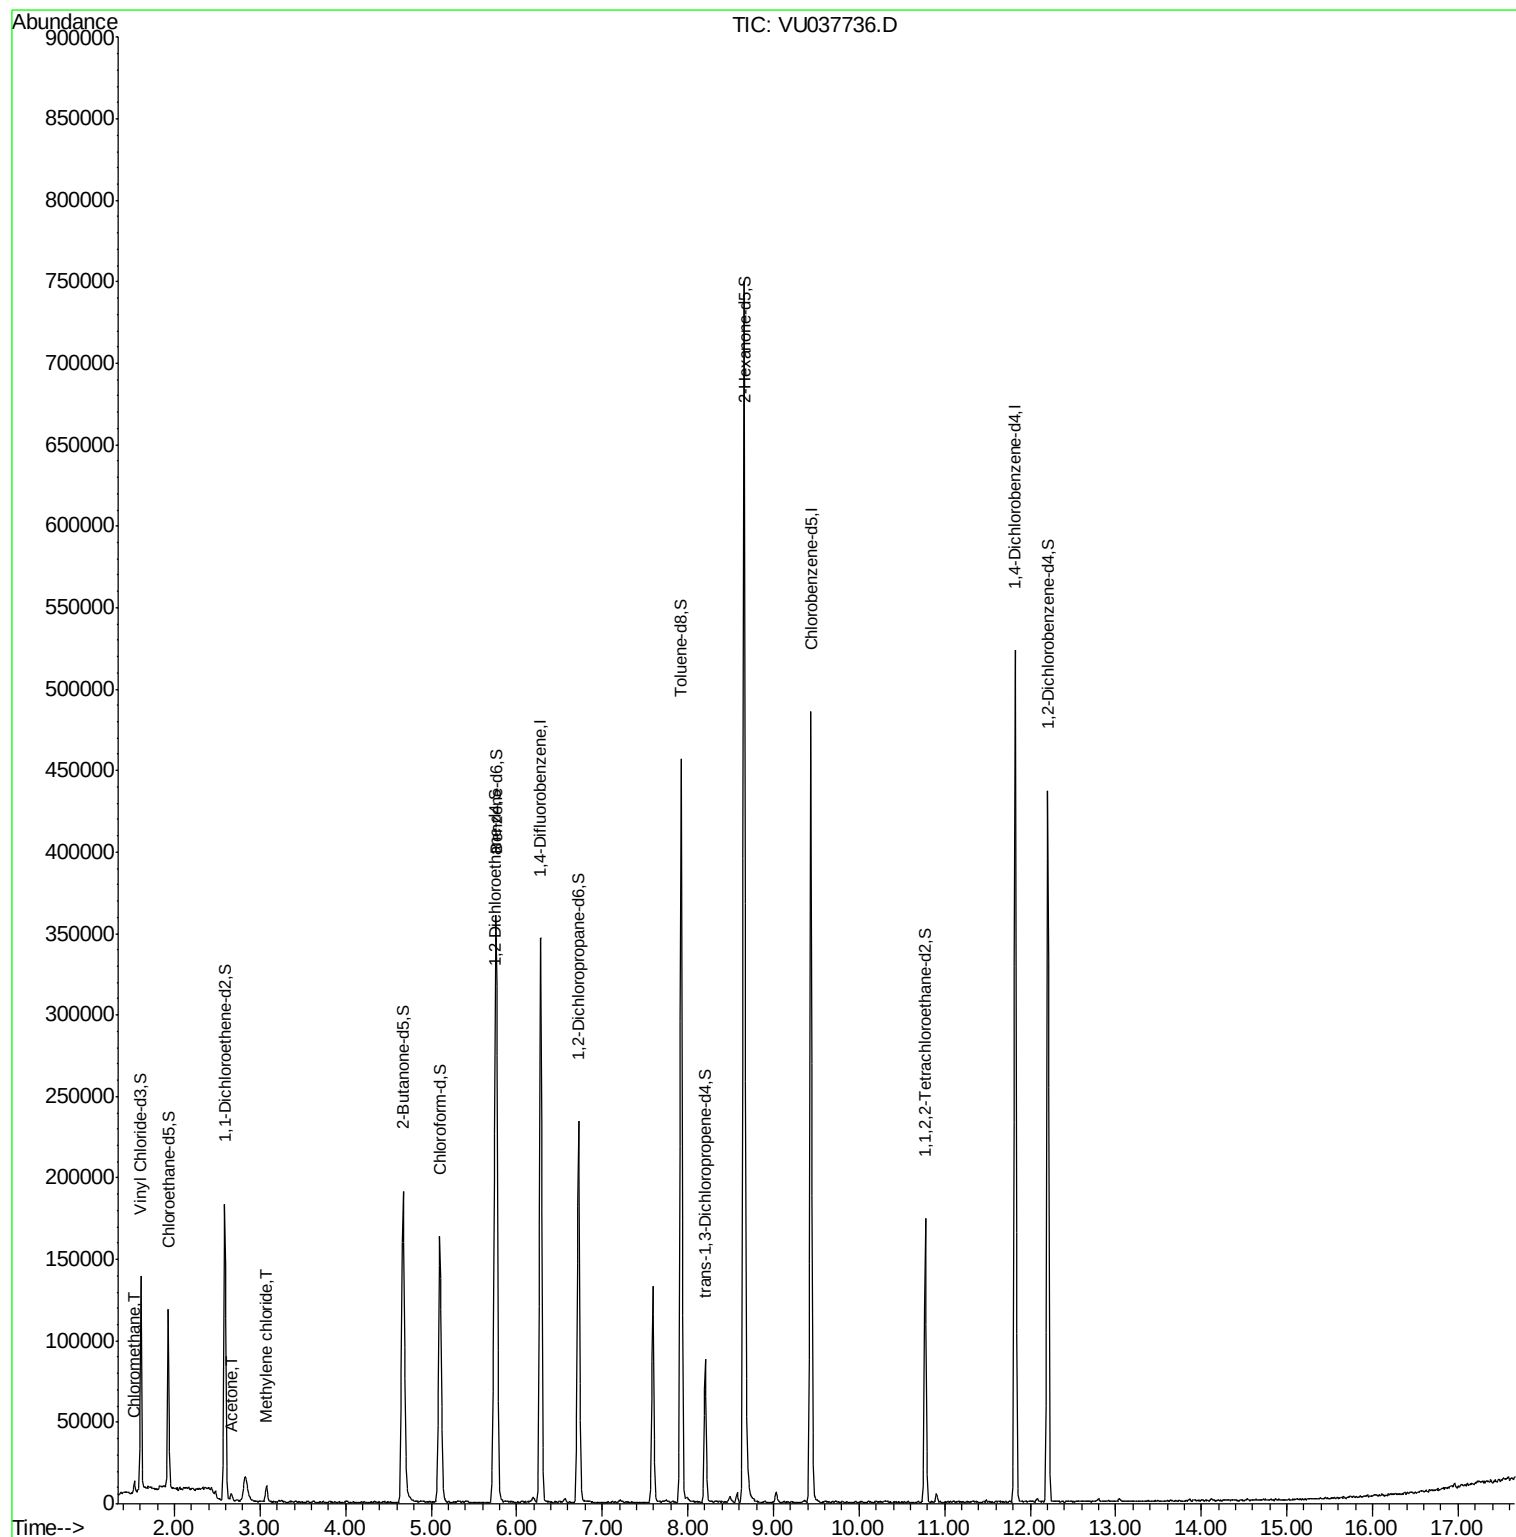

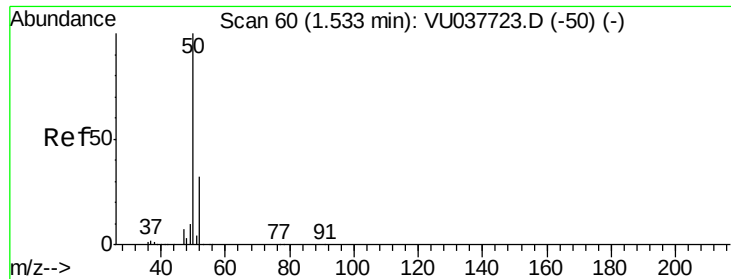

#3

Chloromethane

Concen: 0.165 ug/L

RT: 1.53 min Scan# 59

Delta R.T. -0.00 min

Lab File: VU037736.D

Acq: 15 Apr 2020 16:18

Instrument :

MSVOA_U

ClientSampleId :





VIBLK21

Tot Ion: 50 Resp: 4721

Ion Ratio Lower Upper

50 100

52 29.8 23.0 42.6

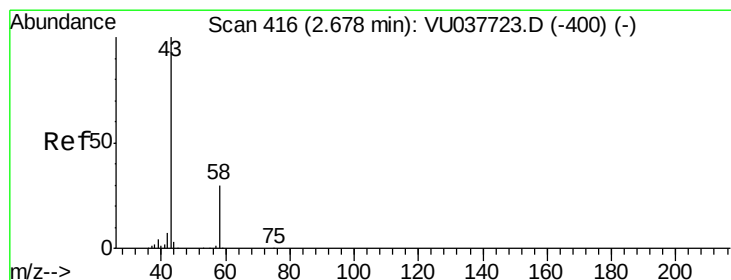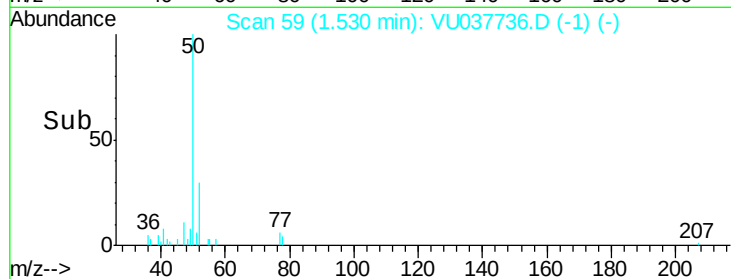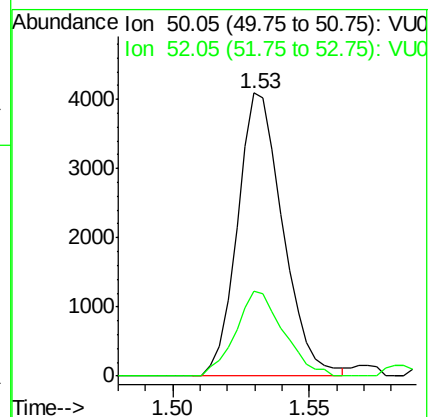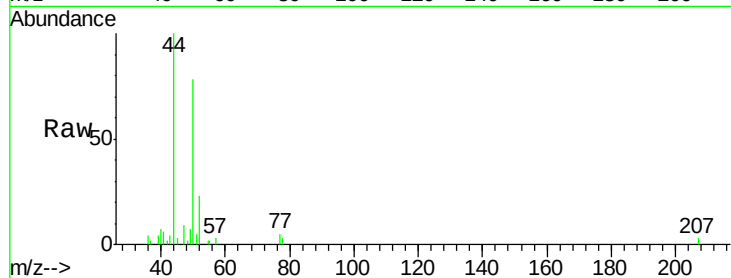

#13

Acetone

Concen: 1.176 ug/L

RT: 2.66 min Scan# 411

Delta R.T. -0.02 min

Lab File: VU037736.D




Acq: 15 Apr 2020 16:18


Tgt Ion: 43 Resp: 4308

Ion Ratio Lower Upper

43 100

58 17.6 0.0 64.8

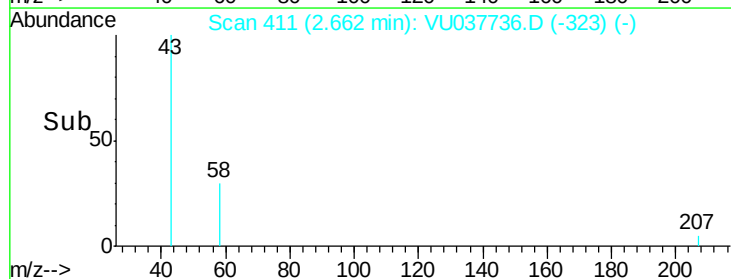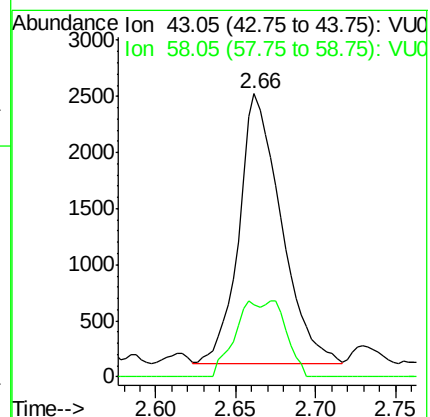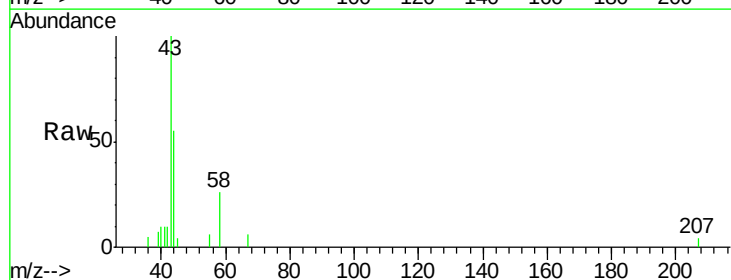

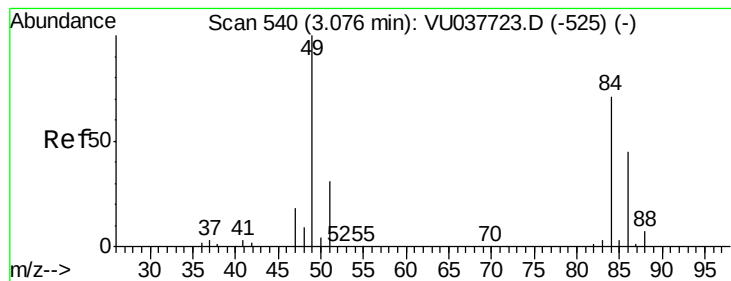

#16
 Methylene chloride
 Concen: 0.209 ug/L
 RT: 3.07 min Scan# 539
 Delta R.T. -0.00 min
 Lab File: VU037736.D
 Acq: 15 Apr 2020 16:18

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK21

Tot Ion:	84	Resp:	4357
Ion	Ratio	Lower	Upper
84	100		
86	54.2	44.2	82.0
49	119.8	92.4	171.6

