


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041520\
 Data File : VU037722.D
 Acq On : 15 Apr 2020 09:20
 Operator : JC/MD
 Sample : BFB14
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB14

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Apr 16 01:23:00 2020

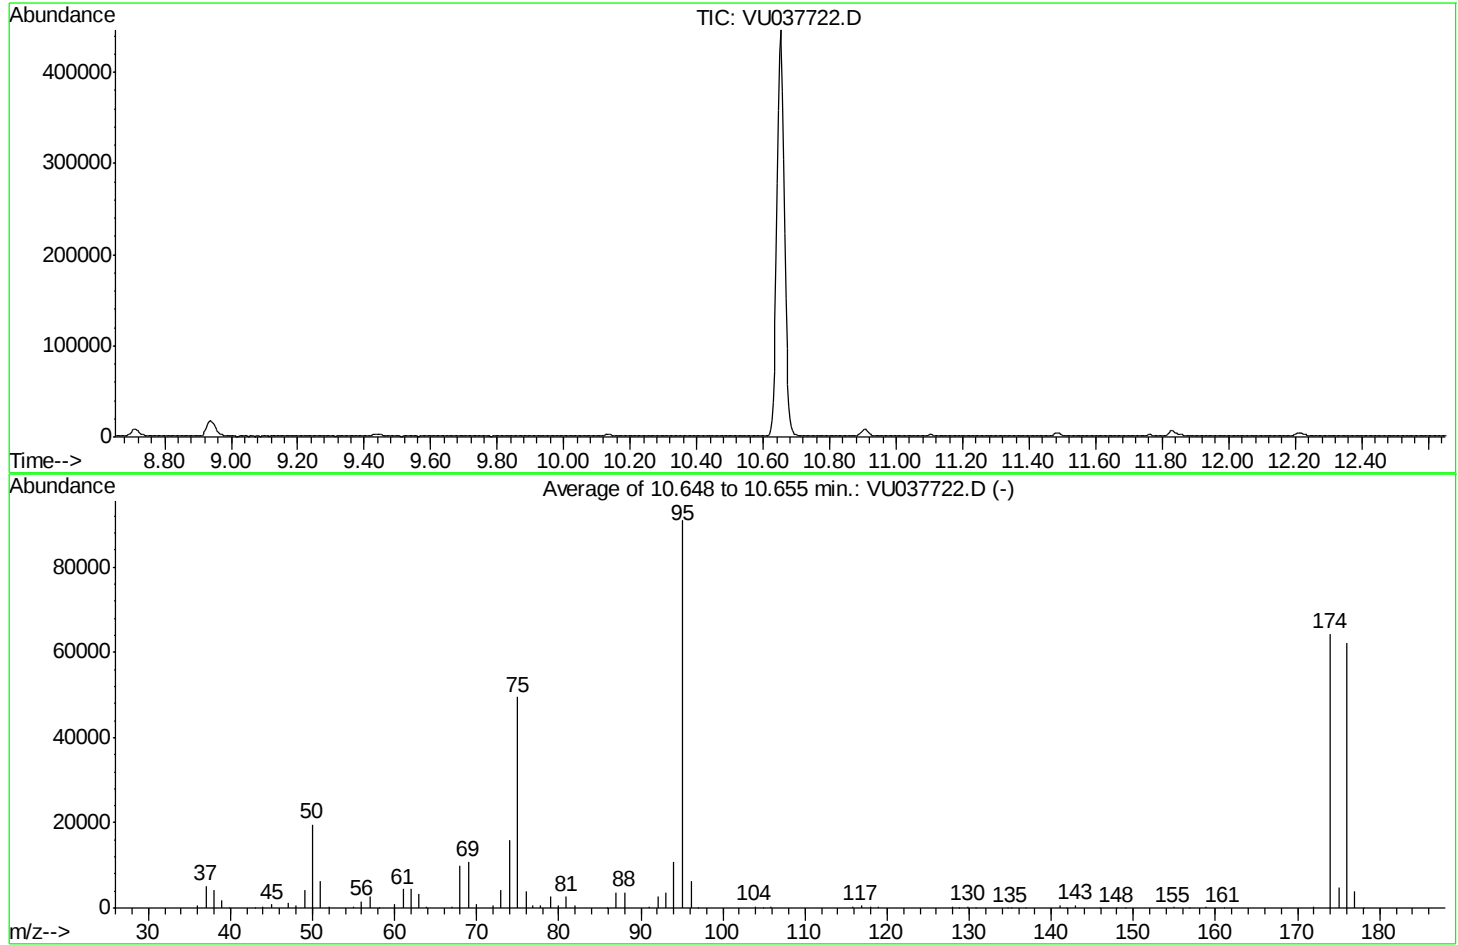

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	19536	PASS
75	95	30	80	54.5	49560	PASS
95	95	100	100	100.0	91002	PASS
96	95	5	9	6.8	6218	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.7	64317	PASS
175	174	5	9	7.6	4876	PASS
176	174	95	101	96.8	62266	PASS
177	176	5	9	6.4	3985	PASS

m/z	Abundance
36.00	642.0
37.00	4977.0
38.00	4433.0
39.00	1891.0
39.90	246.0
41.20	113.0
44.00	982.0
45.10	839.0
47.00	1347.0
48.00	502.0
49.00	4128.0
50.00	19672.0
51.00	6272.0
52.00	336.0
55.00	310.0
56.00	1585.0
57.10	2753.0
60.00	879.0
61.00	4339.0
62.00	4368.0
63.00	3274.0
63.90	453.0
67.00	311.0
68.00	9612.0
69.00	10323.0
70.00	809.0
72.00	481.0
73.00	4362.0
74.00	15744.0
75.00	48584.0
76.00	3906.0
76.90	545.0
77.80	501.0
79.00	2669.0
80.00	726.0
80.90	2425.0
82.00	566.0
87.00	3747.0
88.00	3729.0
90.90	384.0
92.10	2668.0
93.00	3585.0
94.00	10757.0
95.10	89632.0
96.10	6090.0
96.90	143.0
103.90	500.0
105.90	378.0
115.90	270.0
116.90	433.0
118.00	314.0
118.90	348.0
128.00	306.0
128.80	102.0
129.90	365.0
130.80	100.0
134.70	130.0
135.10	115.0
137.00	111.0
141.00	688.0
142.00	158.0
143.00	653.0
145.90	195.0
148.00	119.0
149.00	102.0
154.90	137.0
158.80	153.0
172.00	206.0
174.00	60984.0
175.00	4723.0
176.00	58504.0
177.00	3798.0
178.00	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

m/z	Abundance
36.00	685.0
37.00	5367.0
38.00	4467.0
39.00	2017.0
39.90	242.0
43.90	1096.0
45.10	799.0
47.00	1246.0
48.00	511.0
49.00	4475.0
50.00	19976.0
51.00	6556.0
52.00	324.0
55.00	301.0
56.00	1551.0
57.10	2799.0
58.10	130.0
60.00	909.0
61.00	4616.0
62.00	4669.0
63.00	3385.0
63.90	488.0
67.00	304.0
68.00	10209.0
69.00	11285.0
70.00	826.0
72.00	475.0
73.00	4471.0
74.00	16228.0
75.00	51192.0
76.00	3899.0
76.90	598.0
77.80	502.0
78.90	2875.0
80.00	733.0
80.90	2697.0
81.90	655.0
85.90	132.0
87.00	3743.0
88.00	3754.0
91.00	389.0
92.00	2804.0
93.00	3833.0
94.00	11327.0
95.10	94040.0
96.10	6468.0
96.90	168.0
103.90	416.0
105.90	432.0
115.80	277.0
116.90	511.0
118.00	355.0
118.90	398.0
127.90	346.0
128.70	111.0
129.90	415.0
134.70	123.0
135.10	133.0
141.00	728.0
141.80	145.0
143.00	802.0
145.90	156.0
148.00	144.0
154.90	187.0
156.80	107.0
158.80	192.0
161.00	107.0
172.00	255.0
174.00	66216.0
175.00	5047.0
176.00	64304.0
177.00	4150.0
178.00	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

m/z	Abundance
36.00	754.0
37.00	5119.0
38.00	4118.0
39.00	1832.0
39.90	232.0
43.00	101.0
44.00	1245.0
45.00	804.0
47.00	1108.0
48.00	476.0
49.00	4280.0
50.00	18960.0
51.00	6083.0
52.00	302.0
54.90	318.0
56.00	1419.0
57.10	2587.0
58.10	147.0
60.00	835.0
61.00	4452.0
62.00	4346.0
63.00	3276.0
63.90	396.0
67.00	303.0
68.00	10081.0
69.00	10926.0
70.00	798.0
72.00	437.0
73.00	4076.0
74.00	15542.0
75.00	48904.0
76.00	3592.0
76.90	616.0
77.80	431.0
78.90	2753.0
80.00	708.0
80.90	2736.0
81.90	660.0
85.90	158.0
86.90	3501.0
88.00	3540.0
91.00	345.0
92.00	2631.0
93.00	3621.0
94.00	10798.0
95.10	89336.0
96.10	6096.0
97.00	137.0
103.90	328.0
104.90	115.0
105.90	420.0
115.80	275.0
116.90	532.0
117.90	372.0
118.90	378.0
127.90	302.0
128.70	107.0
129.90	360.0
135.10	145.0
136.80	113.0
141.00	692.0
143.00	795.0
147.90	184.0
154.90	224.0
156.90	126.0
158.80	203.0
160.90	147.0
172.00	267.0
174.00	65752.0
175.00	4859.0
176.00	63992.0
177.00	4008.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

Scan 2882 (10.606 min): VU037722.D
BFB14

m/z	Abundance
39.80	185.0
41.00	124.0
44.00	919.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14