

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041620\
 Data File : VU037749.D
 Acq On : 16 Apr 2020 12:57
 Operator : JC/MD
 Sample : L2296-05
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Apr 17 01:34:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 17 01:29:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	309497	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	299539	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	151775	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	87801	3.75	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.00%
7) Chloroethane-d5	1.93	69	75564	3.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.40%
11) 1,1-Dichloroethene-d2	2.59	63	115469	2.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.40%#
20) 2-Butanone-d5	4.67	46	266881	41.49	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.98%
24) Chloroform-d	5.10	84	148640	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.60%
26) 1,2-Dichloroethane-d4	5.74	65	87591	4.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.60%
32) Benzene-d6	5.76	84	313674	3.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.20%
36) 1,2-Dichloropropane-d6	6.72	67	103929	3.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.00%
41) Toluene-d8	7.92	98	283325	3.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.20%
43) trans-1,3-Dichloropropene-	8.20	79	45447	3.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.80%
46) 2-Hexanone-d5	8.65	63	247280	40.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.66%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	80913	3.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	107489	3.97	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	79.40%#

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl chloride	1.62	62	126216	3.870	ug/L	97
12) 1,1-Dichloroethene	2.60	96	2844	0.133	ug/L #	1
13) Acetone	2.66	43	4192	0.989	ug/L	98
15) Methyl Acetate	3.07	43	4949	0.420	ug/L #	54
17) Methyl tert-butyl Ether	3.41	73	7790	0.126	ug/L #	1
18) trans-1,2-Dichloroethene	3.38	96	3510	0.152	ug/L	95
19) 1,1-Dichloroethane	3.91	63	113922	2.544	ug/L	99
22) cis-1,2-Dichloroethene	4.71	96	96945	3.875	ug/L	92
25) Chloroform	5.13	83	16311	0.383	ug/L	99
27) 1,2-Dichloroethane	5.83	62	18169	0.632	ug/L	98
29) 1,1,1-Trichloroethane	5.36	97	10330	0.284	ug/L	97
30) Cyclohexane	5.42	56	8118	0.180	ug/L	98
33) Benzene	5.81	78	28971	0.293	ug/L	100
34) Trichloroethene	6.57	95	3954	0.163	ug/L	89
35) Methylcyclohexane	6.72	83	23101	0.542	ug/L #	17
37) 1,2-Dichloropropane	6.72	63	11276	0.430	ug/L #	87
45) 1,1,2-Trichloroethane	8.42	97	8401	0.475	ug/L	97

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041620\
 Data File : VU037749.D
 Acq On : 16 Apr 2020 12:57
 Operator : JC/MD
 Sample : L2296-05
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Apr 17 01:34:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 17 01:29:02 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
51) Chlorobenzene	9.47	112	58179	0.920	ug/L	99
54) o-Xylene	10.12	106	5593	0.130	ug/L	89
59) 1,2,3-Trichloropropane	11.83	75	23486	1.367	ug/L	99
62) 1,3-Dichlorobenzene	11.76	146	5575	0.110	ug/L	95
63) 1,4-Dichlorobenzene	11.85	146	9016	0.177	ug/L	96
65) 1,2-Dichlorobenzene	12.22	146	4236	0.089	ug/L	93
68) 1,2,4-trichlorobenzene	13.87	180	2894	0.085	ug/L #	93
69) Naphthalene	14.11	128	7893	0.114	ug/L #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041620\
Data File : VU037749.D
Acq On : 16 Apr 2020 12:57
Operator : JC/MD
Sample : L2296-05
Misc : 25mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Apr 17 01:34:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 17 01:29:02 2020
Response via : Initial Calibration

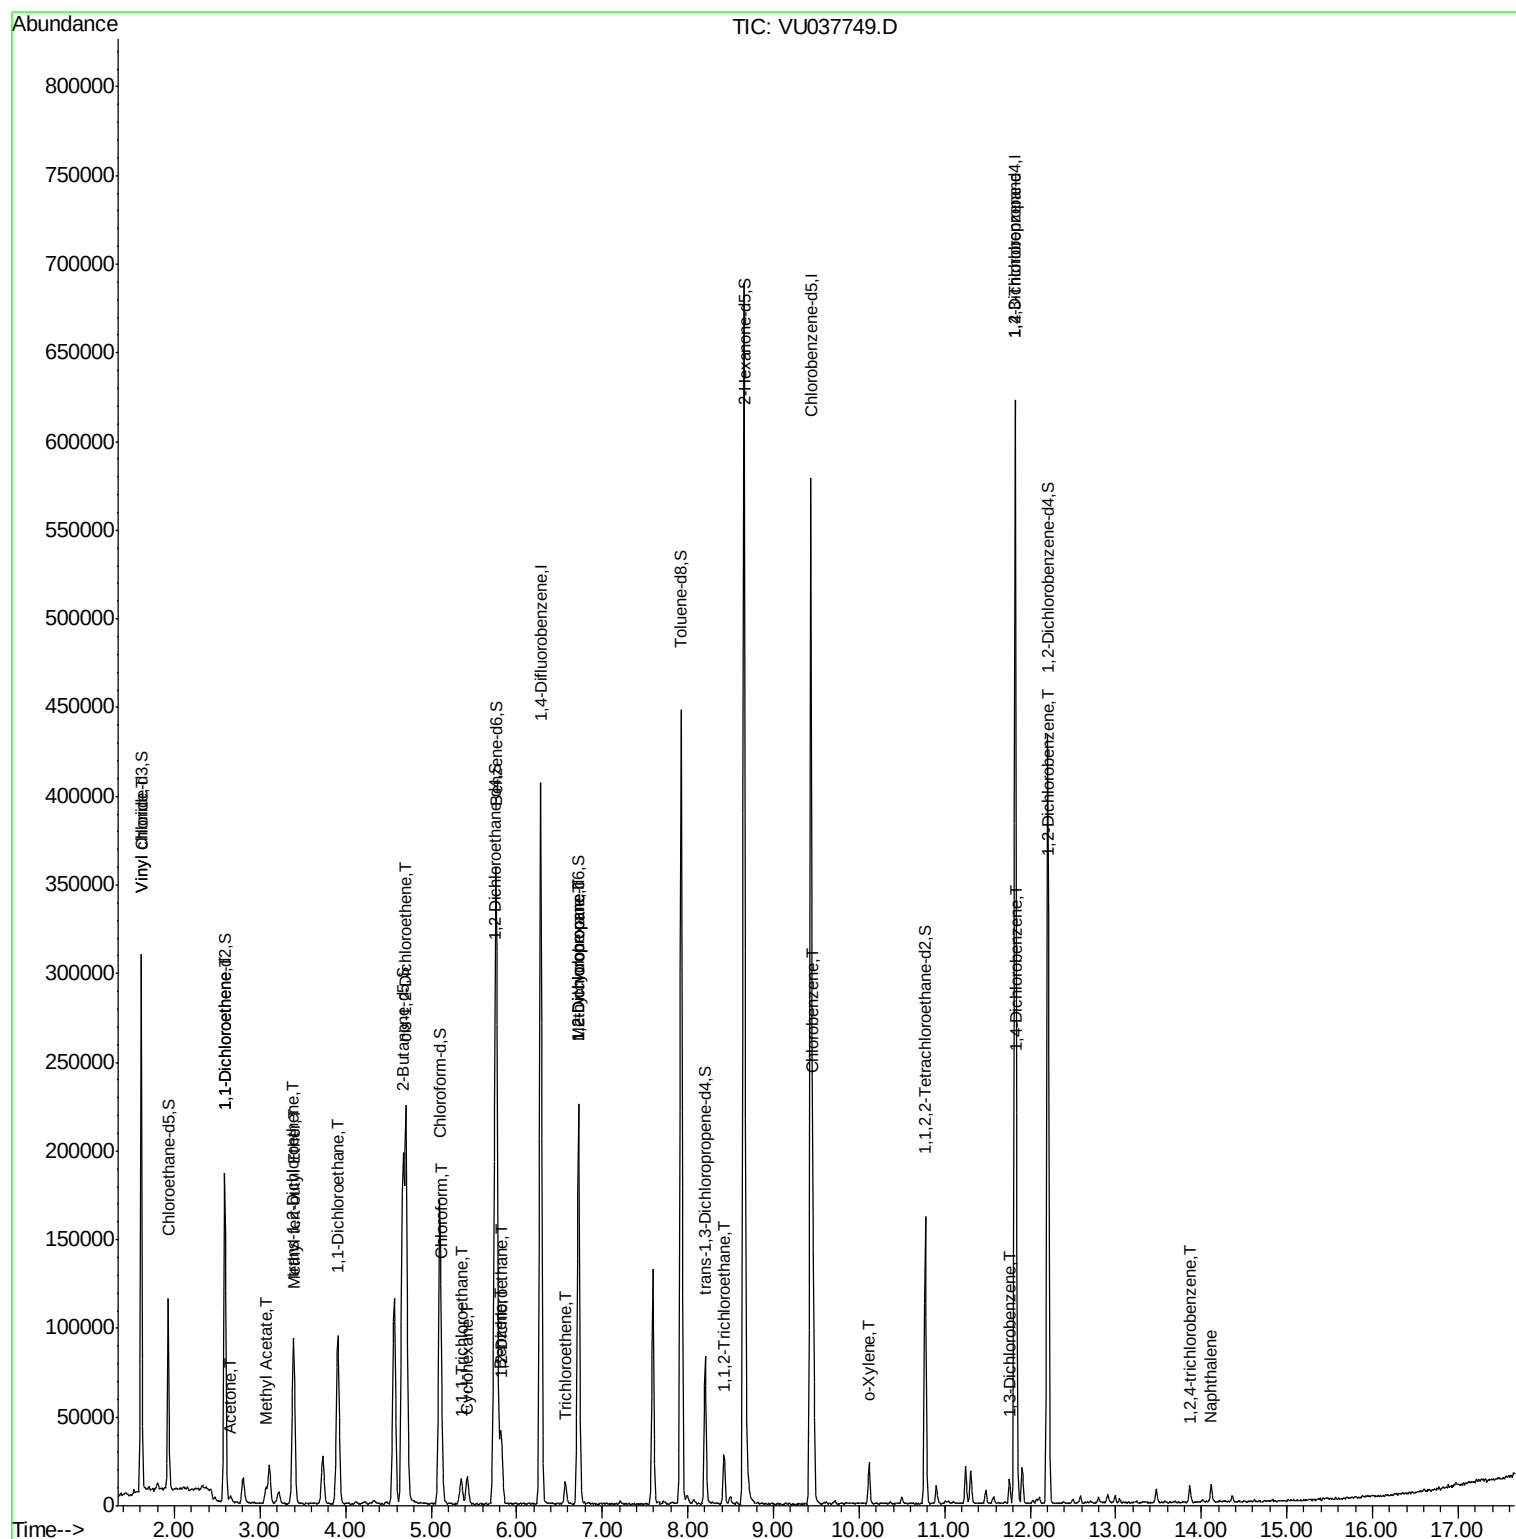



#5

Vinyl chloride

Concen: 3.870 ug/L

RT: 1.62 min Scan# 86

Delta R.T. 0.00 min

Lab File: VU037749.D

Acq: 16 Apr 2020 12:57

Instrument :

MSVOA_U


ClientSampled :

Tot Ion: 62 Resp: 126216

Ion Ratio Lower Upper

62 100

64 33.4 22.1 41.1

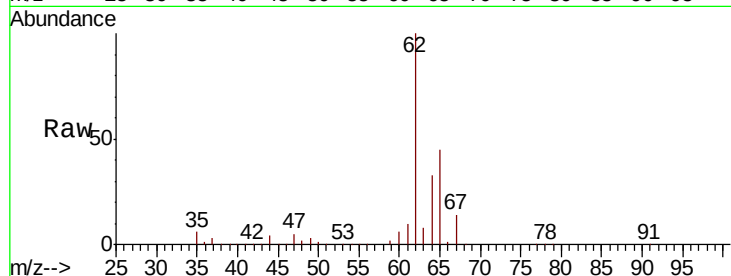

Abundance Ion 62.00 (61.70 to 62.70): VU037749.D (-77) (-)

Ion 64.10 (63.80 to 64.80): VU037749.D (-77) (-)



1.62

100000

50000

0

Time-->



#12

1,1-Dichloroethene

Concen: 0.133 ug/L

RT: 2.60 min Scan# 392

Delta R.T. -0.00 min

Lab File: VU037749.D

Acq: 16 Apr 2020 12:57


Tgt Ion: 96 Resp: 2844

Ion Ratio Lower Upper

96 100

61 473.2 127.7 237.3#

63 2694.3 85.0 157.8#



Abundance Ion 96.00 (95.70 to 96.70): VU037749.D (-380) (-)

Ion 61.05 (60.75 to 61.75): VU037749.D (-380) (-)

Ion 63.00 (62.70 to 63.70): VU037749.D (-380) (-)

80000


60000


40000

20000

0

Time-->



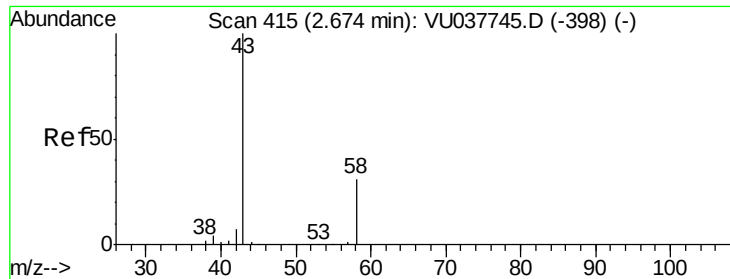

#13

Acetone

Concen: 0.989 ug/L

RT: 2.66 min Scan# 410

Delta R.T. -0.02 min

Lab File: VU037749.D

Acq: 16 Apr 2020 12:57

Instrument :

MSVOA_U


ClientSampleId :

Tot Ion: 43 Resp: 4192

Ion Ratio Lower Upper

43 100

58 31.0 0.0 64.8

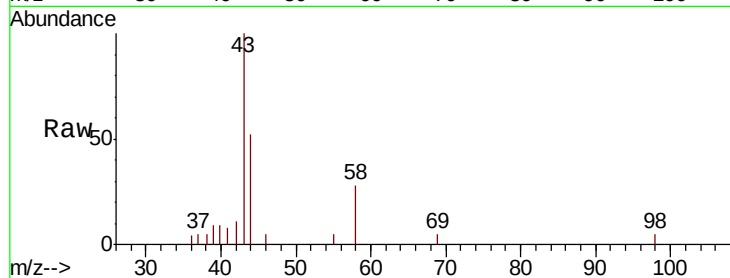

Abundance Ion 43.05 (42.75 to 43.75): VU037749.D (-410) (-)

Ion 58.05 (57.75 to 58.75): VU037749.D (-410) (-)

2500

2000

1500



1000

500

0

2.60 2.65 2.70

Time-->

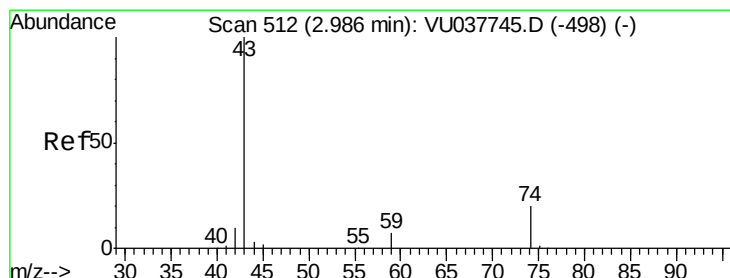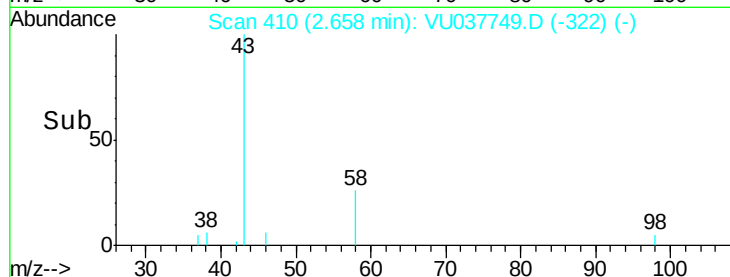

#15

Methyl Acetate

Concen: 0.420 ug/L

RT: 3.07 min Scan# 537

Delta R.T. 0.08 min

Lab File: VU037749.D


Acq: 16 Apr 2020 12:57

Tgt Ion: 43 Resp: 4949

Ion Ratio Lower Upper

43 100

74 0.0 17.2 25.8#

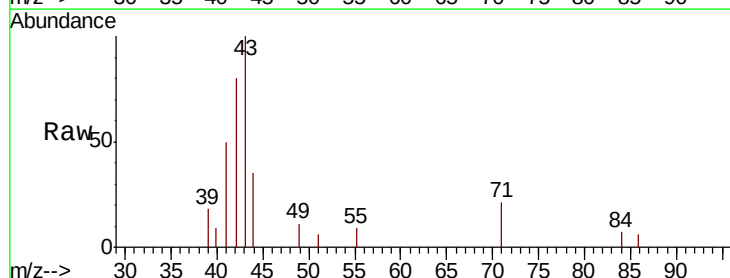

Abundance Ion 43.05 (42.75 to 43.75): VU037749.D (-537) (-)

Ion 74.05 (73.75 to 74.75): VU037749.D (-537) (-)

8000

6000


4000


2000

0

3.02 3.04 3.06 3.08 3.10

Time-->

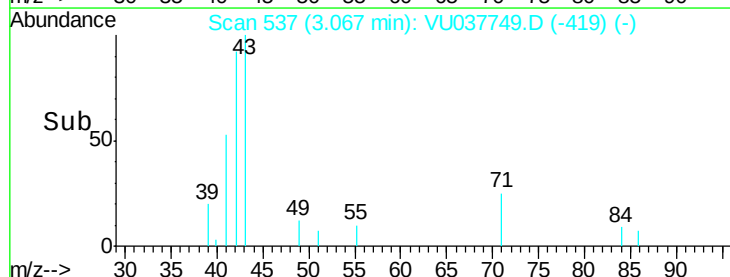


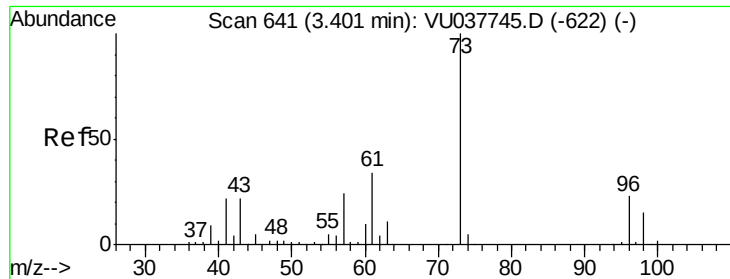




#17
Methyl tert-butyl Ether
Concen: 0.126 ug/L
RT: 3.41 min Scan# 643
Delta R.T. 0.01 min
Lab File: VU037749.D
Acq: 16 Apr 2020 12:57

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion: 73 Resp: 7790
Ion Ratio Lower Upper
73 100
43 191.5 16.4 24.6#
57 702.3 18.4 27.6#

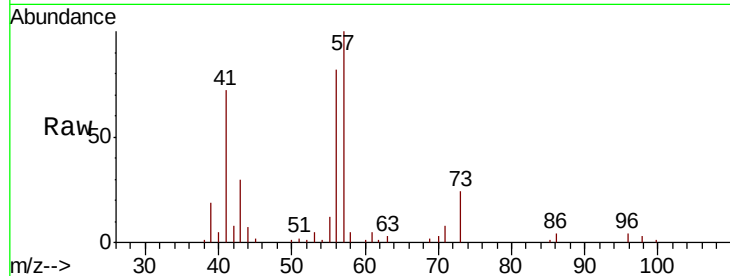


Abundance Ion 73.10 (72.80 to 73.80): VU0
Ion 43.05 (42.75 to 43.75): VU0
Ion 57.10 (56.80 to 57.80): VU0

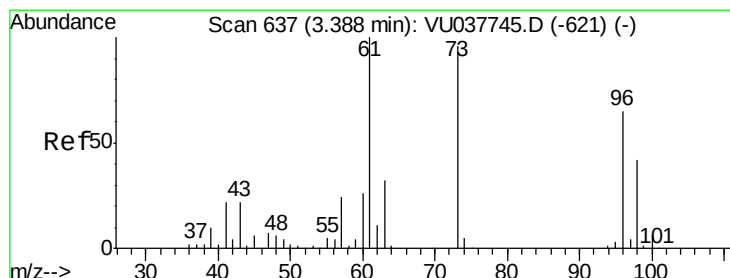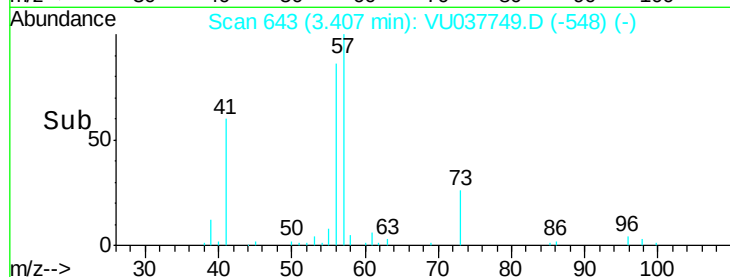
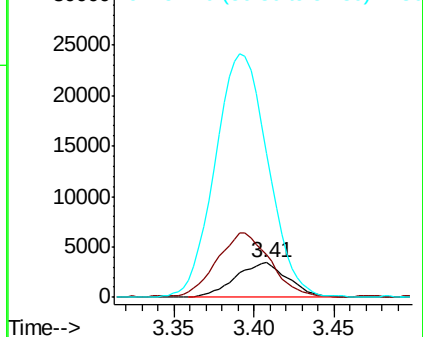



#18
trans-1,2-Dichloroethene
Concen: 0.152 ug/L
RT: 3.38 min Scan# 636
Delta R.T. -0.00 min
Lab File: VU037749.D
Acq: 16 Apr 2020 12:57

Tgt Ion: 96 Resp: 3510
Ion Ratio Lower Upper
96 100
61 160.2 106.7 198.3
98 60.8 44.3 82.3

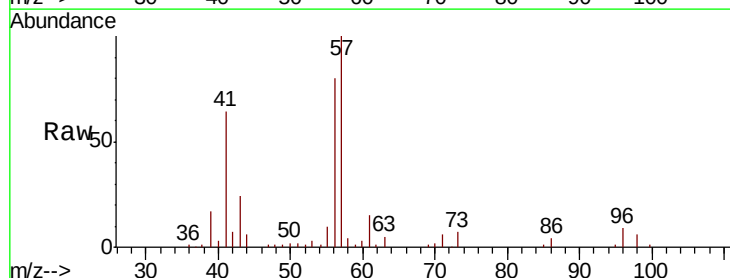

Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.05 (60.75 to 61.75): VU0
Ion 97.95 (97.65 to 98.65): VU0

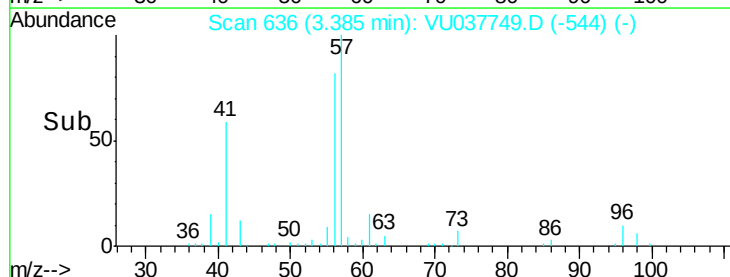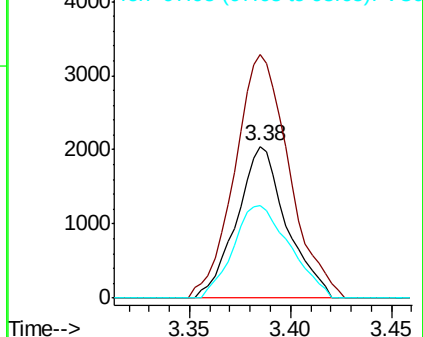

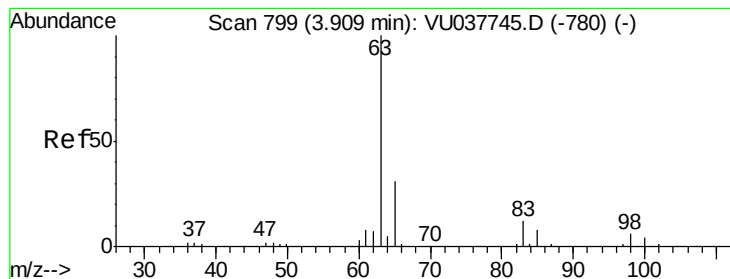

#19

1,1-Dichloroethane

Concen: 2.544 ug/L

RT: 3.91 min Scan# 799

Delta R.T. 0.00 min

Lab File: VU037749.D

Acq: 16 Apr 2020 12:57

Instrument :

MSVOA_U

ClientSampleId :


Tot Ion: 63 Resp: 113922

Ion Ratio Lower Upper

63 100

65 31.2 21.6 40.2




83 12.8 8.6 16.0

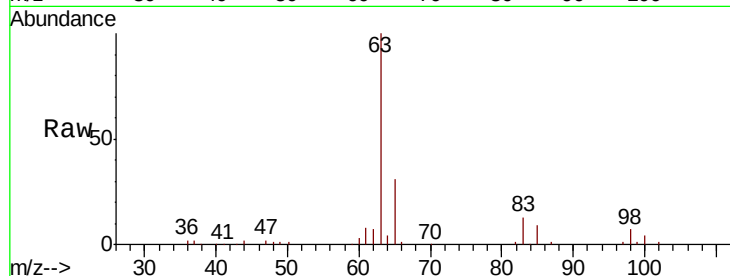

Abundance Ion 63.10 (62.80 to 63.80): VU037749.D (-780) (-)

Ion 65.10 (64.80 to 65.80): VU037749.D (-780) (-)

Ion 83.05 (82.75 to 83.75): VU037749.D (-780) (-)

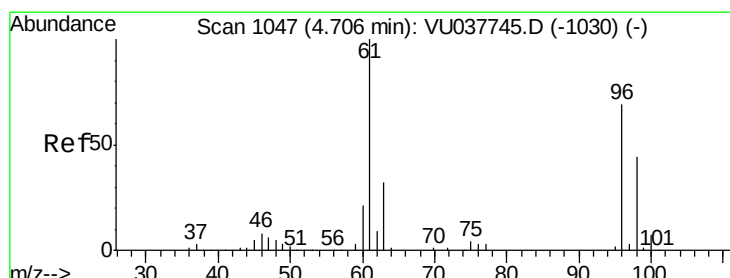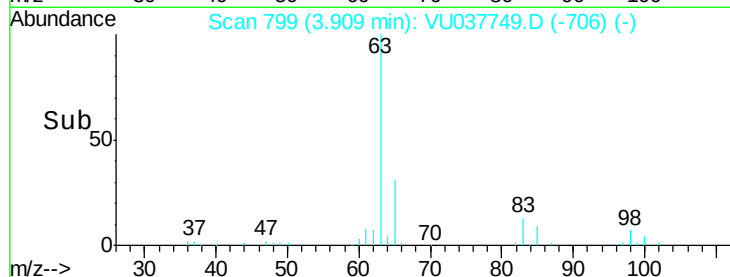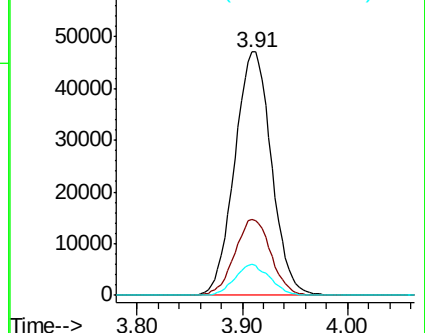

#22

cis-1,2-Dichloroethene

Concen: 3.875 ug/L

RT: 4.71 min Scan# 1047

Delta R.T. -0.00 min

Lab File: VU037749.D

Acq: 16 Apr 2020 12:57


Tgt Ion: 96 Resp: 96945

Ion Ratio Lower Upper

96 100

61 148.2 97.0 180.2



68 0.0 0.0 0.0

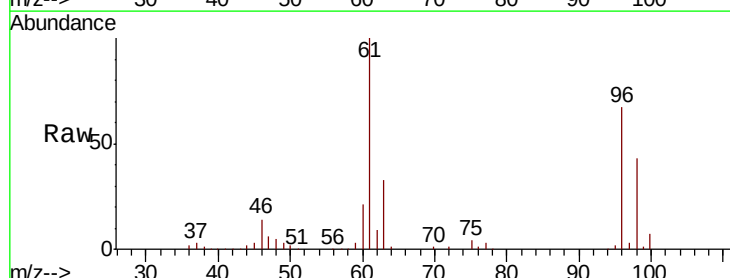


Abundance Ion 96.00 (95.70 to 96.70): VU037749.D (-954) (-)

Ion 61.05 (60.75 to 61.75): VU037749.D (-954) (-)

Ion 68.15 (67.85 to 68.85): VU037749.D (-954) (-)



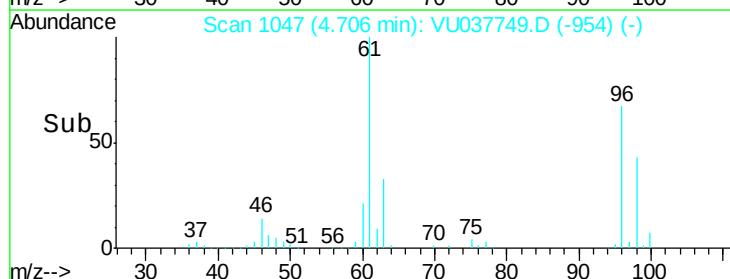
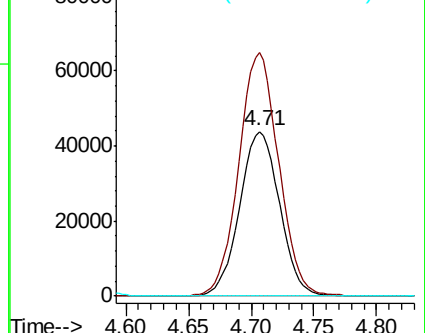


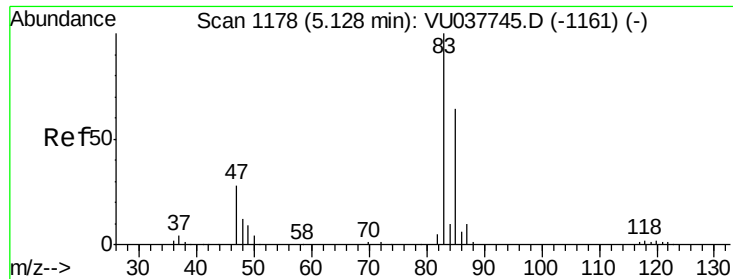

#25
Chloroform
Concen: 0.383 ug/L
RT: 5.13 min Scan# 1178
Delta R.T. 0.00 min
Lab File: VU037749.D
Acq: 16 Apr 2020 12:57




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion: 83 Resp: 16311
Ion Ratio Lower Upper
83 100
85 65.2 44.9 83.3

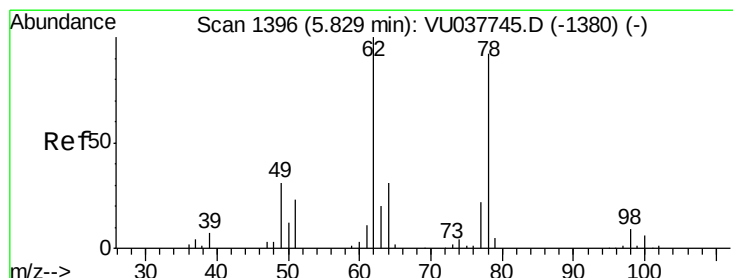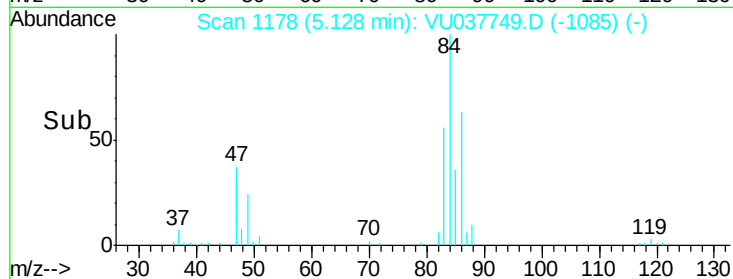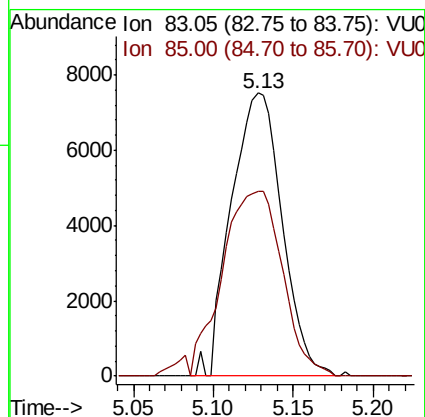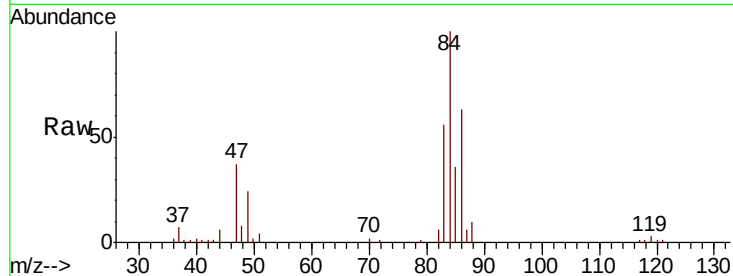

#27
1,2-Dichloroethane
Concen: 0.632 ug/L
RT: 5.83 min Scan# 1397
Delta R.T. 0.00 min
Lab File: VU037749.D
Acq: 16 Apr 2020 12:57

Tgt Ion: 62 Resp: 18169
Ion Ratio Lower Upper
62 100
98 8.8 7.6 11.4


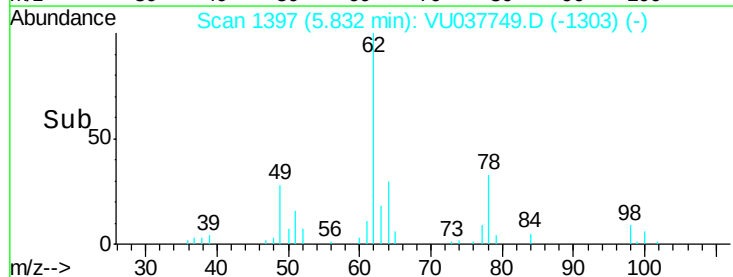
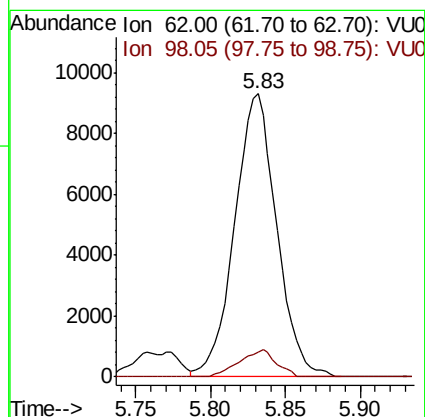
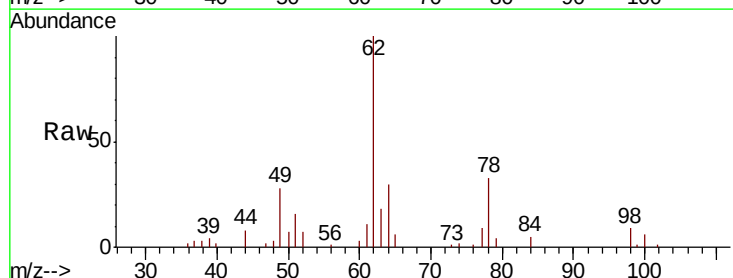


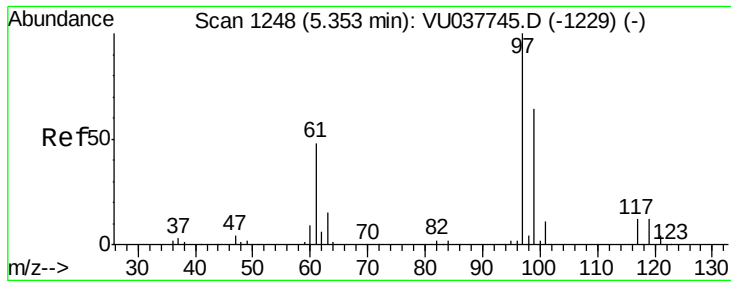

#29
 1,1,1-Trichloroethane
 Concen: 0.284 ug/L
 RT: 5.36 min Scan# 1249
 Delta R.T. 0.00 min
 Lab File: VU037749.D
 Acq: 16 Apr 2020 12:57




Instrument :
 MSVOA_U
 ClientSampleId :


Tot Ion: 97 Resp: 10330
 Ion Ratio Lower Upper
 97 100
 99 63.2 52.0 78.0
 61 50.1 37.8 56.8

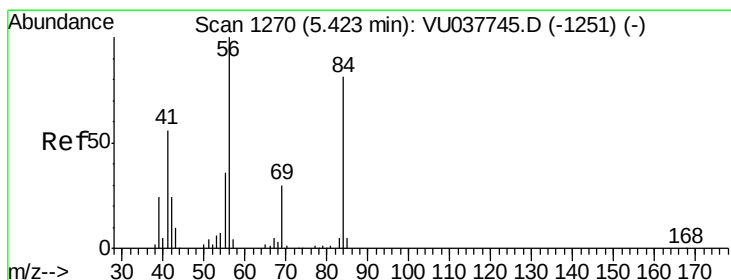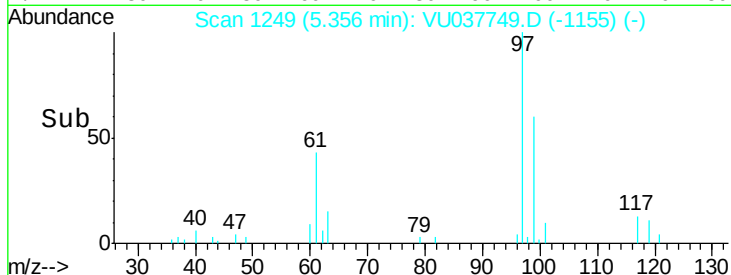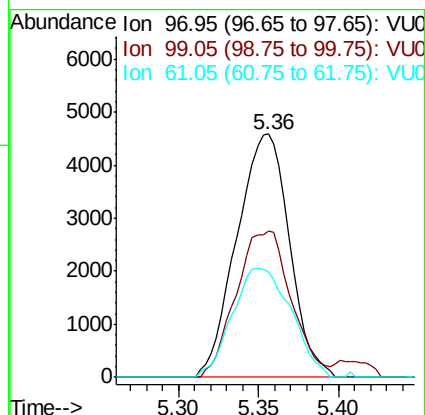

#30
 Cyclohexane
 Concen: 0.180 ug/L
 RT: 5.42 min Scan# 1269
 Delta R.T. -0.00 min
 Lab File: VU037749.D
 Acq: 16 Apr 2020 12:57

Tgt Ion: 56 Resp: 8118
 Ion Ratio Lower Upper
 56 100
 69 25.4 23.9 35.9
 84 82.0 65.6 98.4

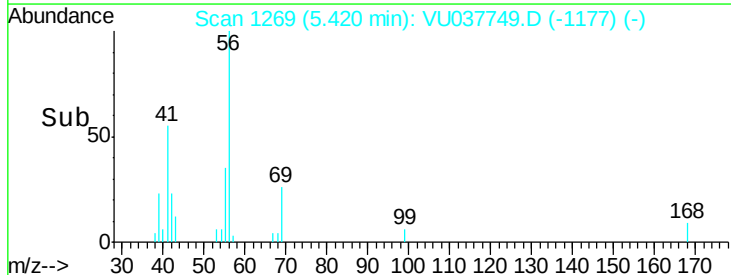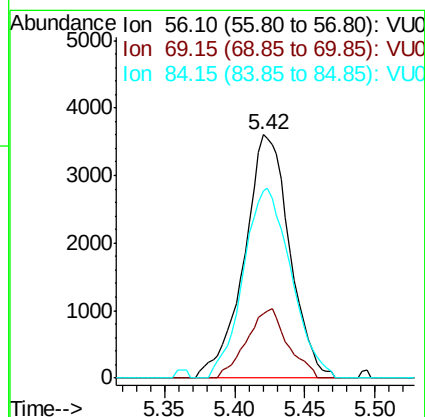

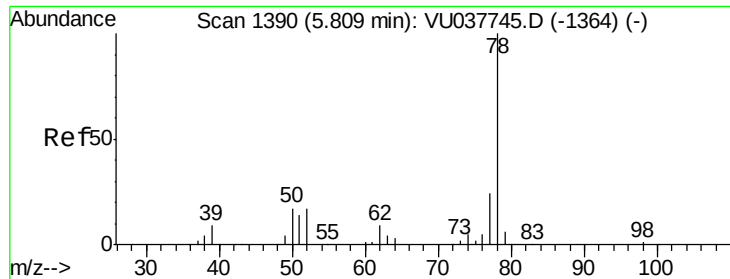

#33

Benzene

Concen: 0.293 ug/L

RT: 5.81 min Scan# 1390


Delta R.T. -0.00 min

Lab File: VU037749.D




Acq: 16 Apr 2020 12:57

Instrument :
MSVOA_U
ClientSampled :

Tgt Ion: 78 Resp: 28971

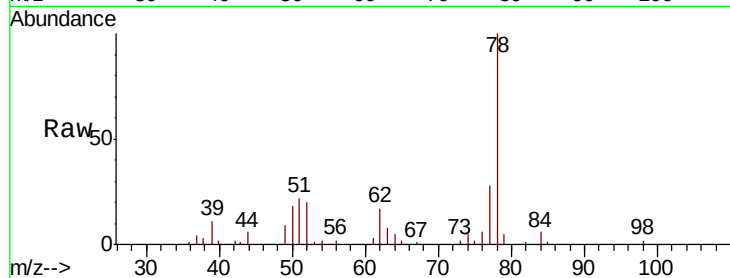

Abundance Ion 78.10 (77.80 to 78.80): VU0

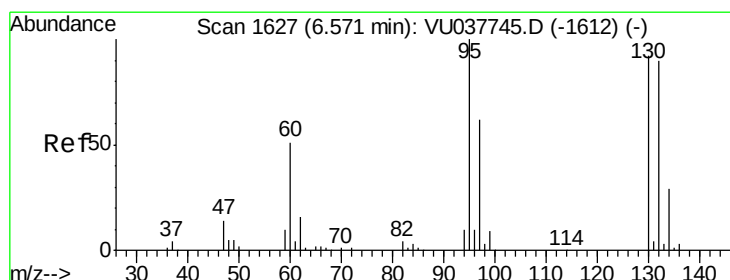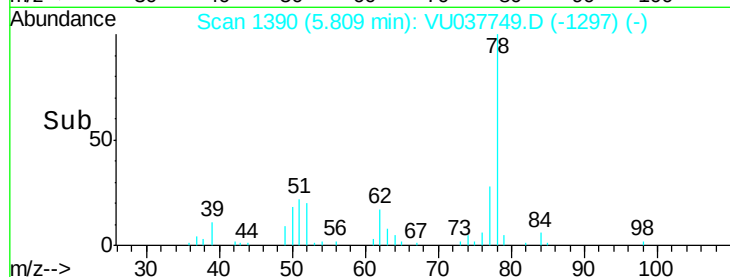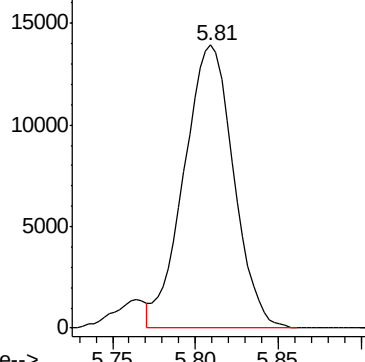

#34

Trichloroethene

Concen: 0.163 ug/L

RT: 6.57 min Scan# 1626

Delta R.T. -0.00 min

Lab File: VU037749.D

Acq: 16 Apr 2020 12:57

Tgt Ion: 95 Resp: 3954

Ion	Ratio	Lower	Upper
95	100		
97	71.7	45.4	84.2
132	100.3	63.7	118.3
130	83.7	68.7	127.5

Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): VU0



Ion 129.95 (129.65 to 130.65): VU0

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): VU0

Ion 129.95 (129.65 to 130.65): VU0

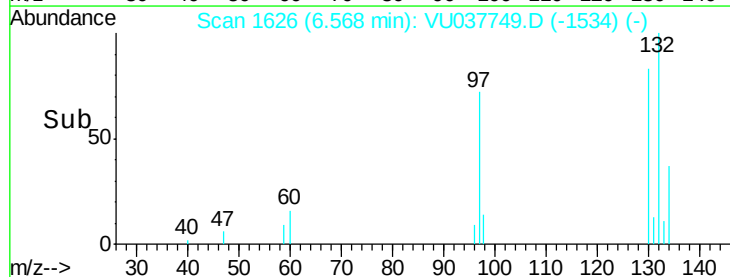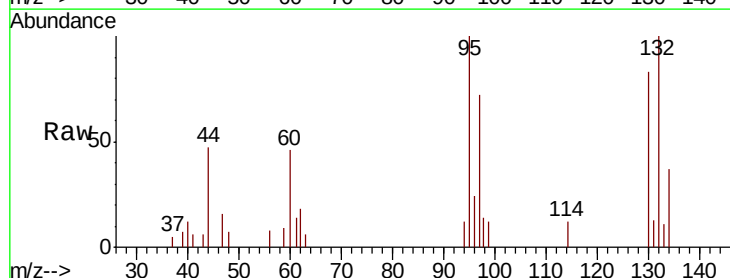

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): VU0

Ion 129.95 (129.65 to 130.65): VU0

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): VU0

Ion 129.95 (129.65 to 130.65): VU0

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): VU0

Ion 129.95 (129.65 to 130.65): VU0

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): VU0

Ion 129.95 (129.65 to 130.65): VU0

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): VU0

Ion 129.95 (129.65 to 130.65): VU0

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): VU0


Ion 129.95 (129.65 to 130.65): VU0

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): VU0


Ion 129.95 (129.65 to 130.65): VU0

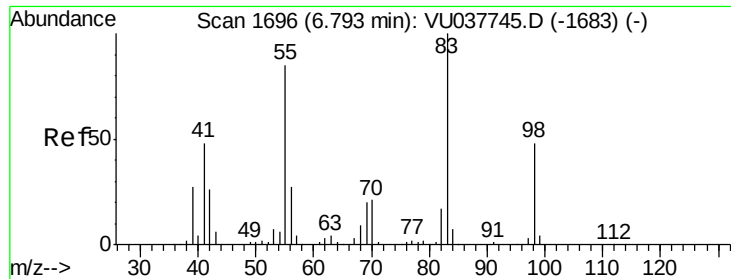




#35
Methylvlcyclohexane
Concen: 0.542 ug/L
RT: 6.72 min Scan# 1674
Delta R.T. -0.07 min
Lab File: VU037749.D
Acq: 16 Apr 2020 12:57

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion: 83 Resp: 23101
Ion Ratio Lower Upper
83 100
55 1.1 65.5 98.3#
98 1.3 38.2 57.4#

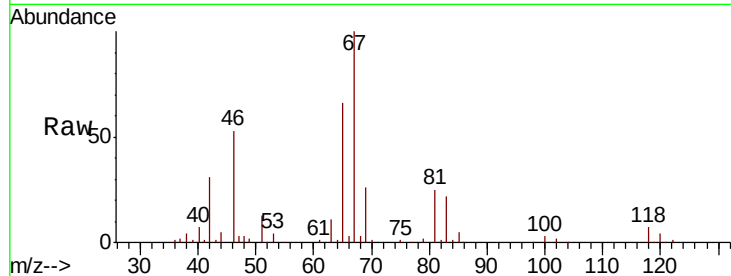


Abundance Ion 83.15 (82.85 to 83.85): VU0
Ion 55.10 (54.80 to 55.80): VU0
Ion 98.15 (97.85 to 98.85): VU0


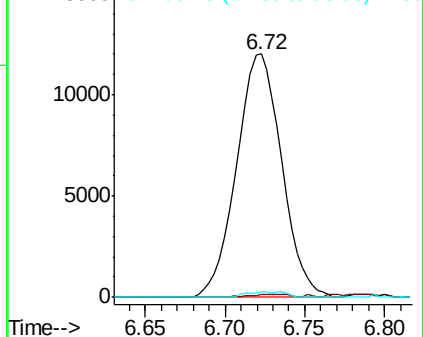



#37
1,2-Dichloropropane
Concen: 0.430 ug/L
RT: 6.72 min Scan# 1674
Delta R.T. -0.10 min
Lab File: VU037749.D
Acq: 16 Apr 2020 12:57

Tgt Ion: 63 Resp: 11276
Ion Ratio Lower Upper
63 100
112 0.0 3.4 5.0#



Abundance Ion 63.10 (62.80 to 63.80): VU0
Ion 112.10 (111.80 to 112.80): V

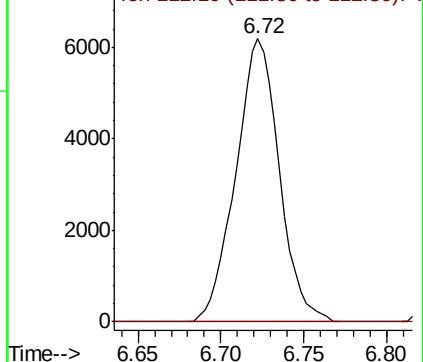







#45
 1,1,2-Trichloroethane
 Concen: 0.475 ug/L
 RT: 8.42 min Scan# 2203
 Delta R.T. -0.00 min
 Lab File: VU037749.D
 Acq: 16 Apr 2020 12:57

Instrument :
 MSVOA_U
 ClientSampleId :

Tot Ion:	97	Resp:	8401
Ion	Ratio	Lower	Upper
97	100		
99	59.4	43.1	80.1
83	87.1	62.4	116.0
85	58.8	39.6	73.6

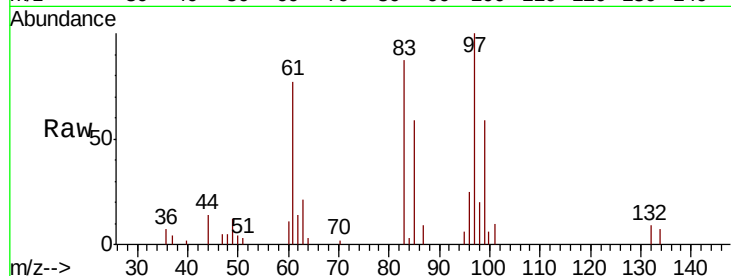


Abundance Ion 96.95 (96.65 to 97.65): VU0
 Ion 99.05 (98.75 to 99.75): VU0
 Ion 82.95 (82.65 to 83.65): VU0
 Ion 85.00 (84.70 to 85.70): VU0


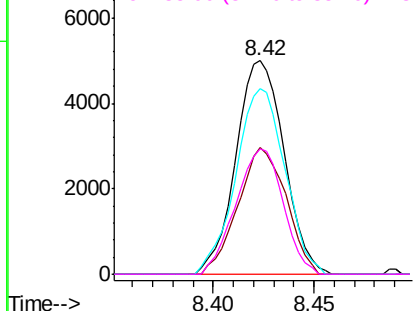



#51
 Chlorobenzene
 Concen: 0.920 ug/L
 RT: 9.47 min Scan# 2527
 Delta R.T. -0.00 min
 Lab File: VU037749.D
 Acq: 16 Apr 2020 12:57

Tgt Ion:	112	Resp:	58179
Ion	Ratio	Lower	Upper
112	100		
114	33.1	22.6	42.0
77	63.4	50.2	75.4



Abundance Ion 112.10 (111.80 to 112.80): V
 Ion 114.05 (113.75 to 114.75): V
 Ion 77.10 (76.80 to 77.80): VU0

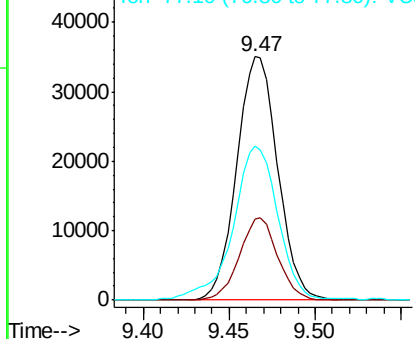


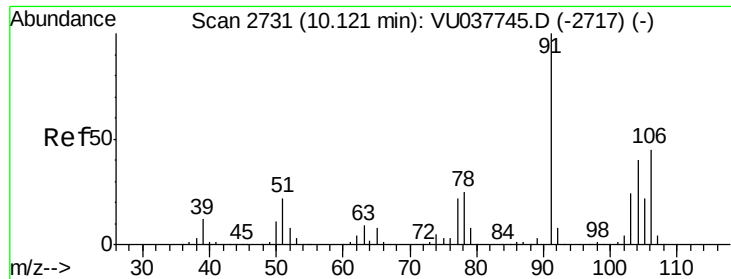




#54
o-Xylene
Concen: 0.130 ug/L
RT: 10.12 min Scan# 2730
Delta R.T. -0.00 min
Lab File: VU037749.D
Acq: 16 Apr 2020 12:57

Instrument :
MSVOA_U
ClientSampled :

Tot Ion:106 Resp: 5593
Ion Ratio Lower Upper
106 100
91 233.8 151.1 280.7

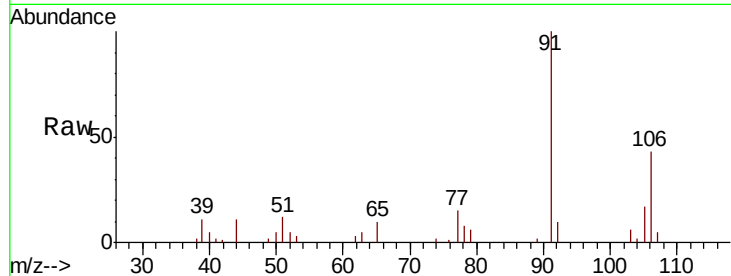


Abundance Ion 106.15 (105.85 to 106.85): VU037749.D (-2638) (-)
Ion 91.15 (90.85 to 91.85): VU037749.D (-2638) (-)


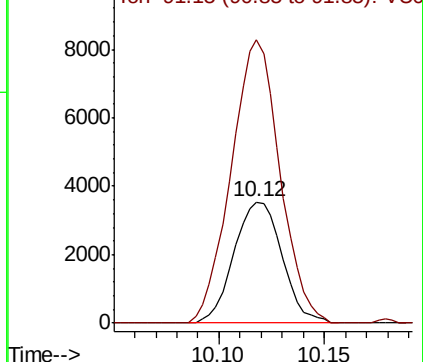



#59
1,2,3-Trichloropropane
Concen: 1.367 ug/L
RT: 11.83 min Scan# 3261
Delta R.T. 0.98 min
Lab File: VU037749.D
Acq: 16 Apr 2020 12:57

Tgt Ion: 75 Resp: 23486
Ion Ratio Lower Upper
75 100
77 32.6 25.4 38.2



Abundance Ion 75.00 (74.70 to 75.70): VU037749.D (-2333) (-)
Ion 77.00 (76.70 to 77.70): VU037749.D (-2333) (-)

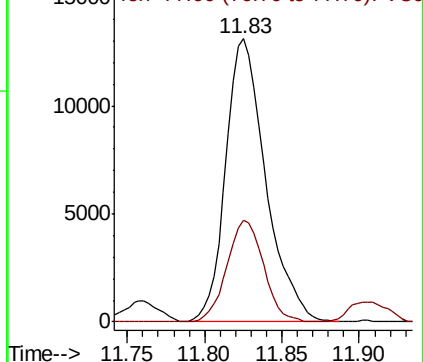


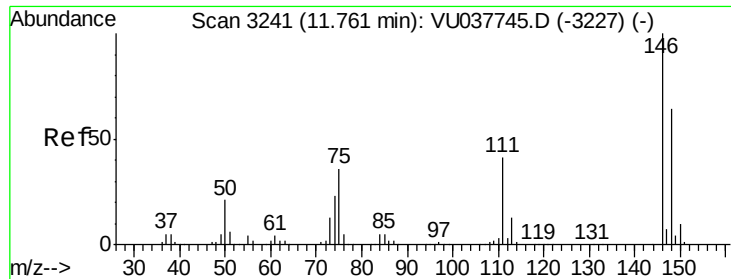




#62
 1,3-Dichlorobenzene
 Concen: 0.110 ug/L
 RT: 11.76 min Scan# 3240
 Delta R.T. -0.00 min
 Lab File: VU037749.D
 Acq: 16 Apr 2020 12:57

Instrument :
 MSVOA_U
 ClientSampled :

Tot Ion:146 Resp: 5575
 Ion Ratio Lower Upper
 146 100
 111 40.6 29.8 55.3
 148 58.4 44.5 82.7

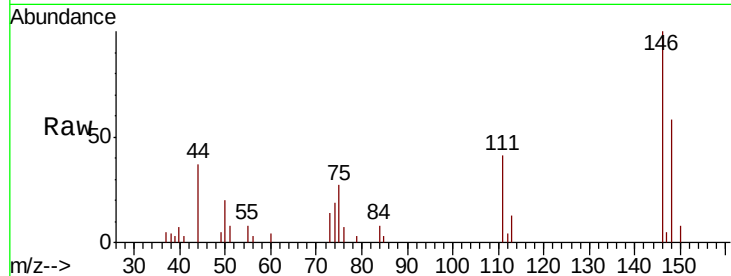


Abundance Ion 145.95 (145.65 to 146.65): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V


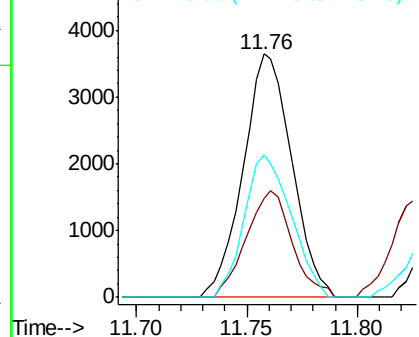



#63
 1,4-Dichlorobenzene
 Concen: 0.177 ug/L
 RT: 11.85 min Scan# 3269
 Delta R.T. 0.00 min
 Lab File: VU037749.D
 Acq: 16 Apr 2020 12:57

Tgt Ion:146 Resp: 9016
 Ion Ratio Lower Upper
 146 100
 111 46.2 28.4 52.8
 148 64.4 44.9 83.3



Abundance Ion 145.95 (145.65 to 146.65): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

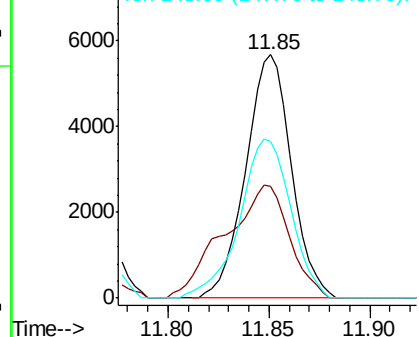



#65

1,2-Dichlorobenzene

Concen: 0.089 ug/L

RT: 12.22 min Scan# 3385

Delta R.T. -0.00 min

Lab File: VU037749.D

Acq: 16 Apr 2020 12:57

Instrument :

MSVOA_U

ClientSampleId :


Tot Ion:146 Resp: 4236

Ion Ratio Lower Upper

146 100

111 52.3 35.0 52.6




148 66.3 51.5 77.3



Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

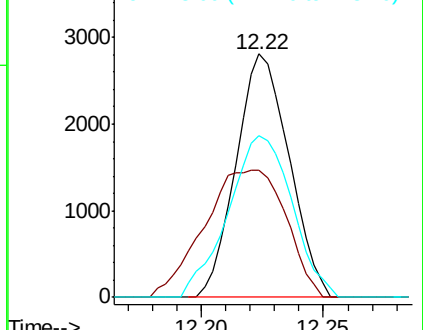

#68

1,2,4-trichlorobenzene

Concen: 0.085 ug/L

RT: 13.87 min Scan# 3896

Delta R.T. -0.01 min

Lab File: VU037749.D

Acq: 16 Apr 2020 12:57


Tgt Ion:180 Resp: 2894

Ion Ratio Lower Upper

180 100

182 100.0 76.4 114.6



145 24.4 25.1 37.7#




Abundance Ion 179.90 (179.60 to 180.60): V

Ion 182.00 (181.70 to 182.70): V

Ion 144.95 (144.65 to 145.65): V

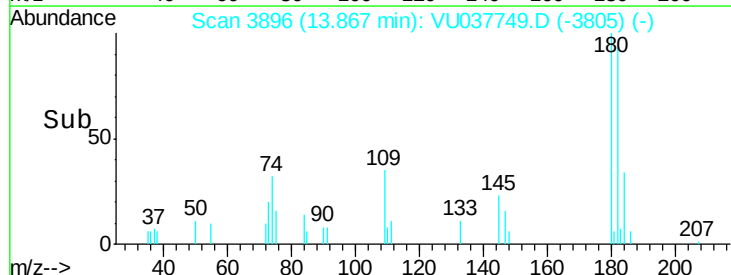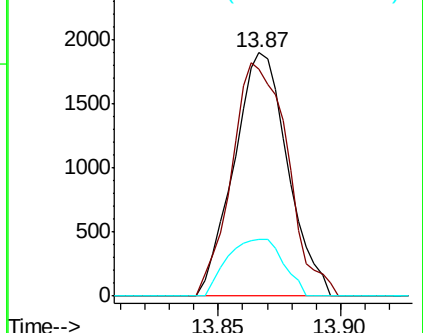

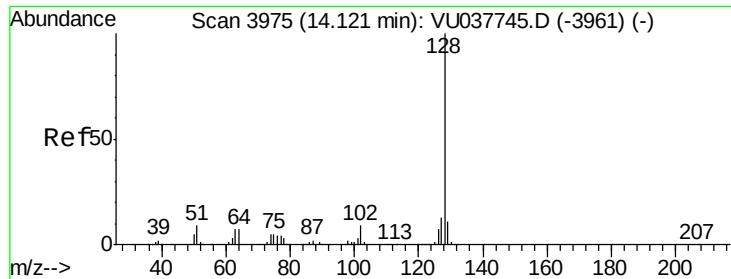

#69

Naphthalene

Concen: 0.114 ug/L

RT: 14.11 min Scan# 3973

Delta R.T. -0.01 min


Lab File: VU037749.D

Acq: 16 Apr 2020 12:57

Instrument :

MSVOA_U

ClientSampleId :




Tot Ion:128 Resp: 7893

Ion Ratio Lower Upper

128 100

129 9.6 8.6 12.8

127 15.8 10.4 15.6#

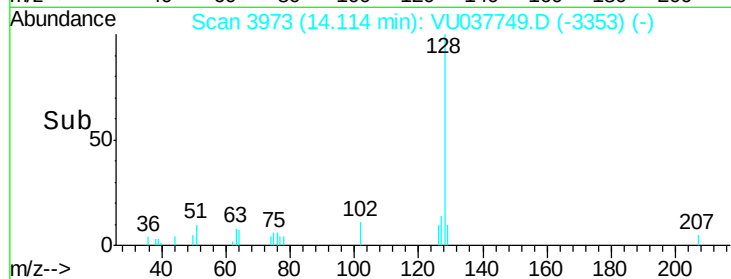

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 129.00 (128.70 to 129.70): V
Ion 127.00 (126.70 to 127.70): V

