


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041620\
 Data File : VU037744.D
 Acq On : 16 Apr 2020 08:40
 Operator : JC/MD
 Sample : BFB15
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB15

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Apr 17 01:29:02 2020

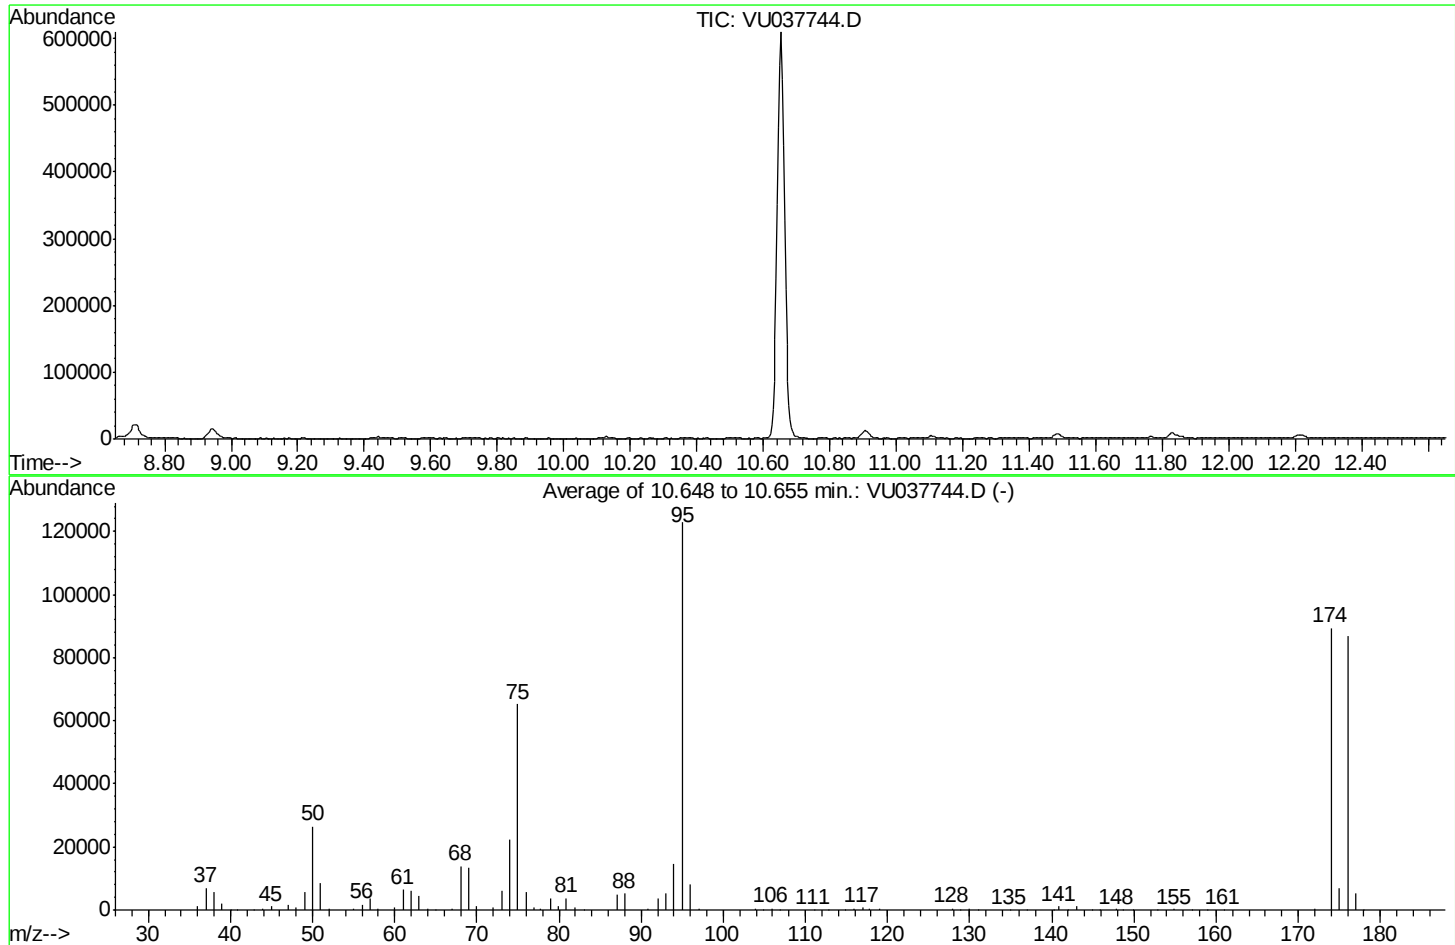

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	26453	PASS
75	95	30	80	53.1	65250	PASS
95	95	100	100	100.0	122877	PASS
96	95	5	9	6.6	8125	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.7	89322	PASS
175	174	5	9	7.6	6821	PASS
176	174	95	101	97.1	86762	PASS
177	176	5	9	6.0	5184	PASS

m/z	Abundance
36.00	1189.0
37.00	6681.0
38.00	5529.0
39.00	1996.0
40.00	246.0
40.80	139.0
42.90	227.0
44.00	1354.0
45.00	1219.0
47.00	1733.0
47.90	699.0
49.00	5826.0
50.00	25392.0
51.00	8147.0
52.00	578.0
54.90	428.0
56.00	1769.0
57.00	3269.0
58.00	217.0
60.00	991.0
61.00	6252.0
62.00	5841.0
63.00	4564.0
64.00	463.0
65.00	106.0
67.00	374.0
68.00	12934.0
69.00	12837.0
70.00	942.0
72.00	843.0
73.00	5966.0
74.00	21488.0
75.00	62080.0
76.00	5531.0
77.00	866.0
77.80	366.0
78.90	3545.0
79.90	1023.0
80.90	3641.0
81.90	719.0
87.00	4557.0
88.00	4763.0
90.80	405.0
92.00	3632.0
93.00	4954.0
94.00	14069.0
95.10	117128.0
96.00	7966.0
97.00	224.0
104.00	576.0
104.90	150.0
105.90	545.0
106.90	127.0
111.00	106.0
112.80	105.0
114.90	173.0
115.80	296.0
117.00	567.0
117.90	330.0
119.00	448.0
127.90	507.0
128.90	166.0
129.90	394.0
130.90	174.0
134.90	188.0
136.90	182.0
140.20	100.0
140.90	1113.0
141.90	165.0
142.90	990.0
145.90	174.0
147.90	272.0
150.00	131.0
154.90	214.0
157.00	171.0
158.90	158.0
160.90	102.0
172.00	246.0
174.00	83416.0
175.00	6482.0
176.00	79904.0
177.00	4859.0
177.90	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	1324.0
37.00	7157.0
38.00	6003.0
39.00	2152.0
40.00	293.0
40.80	163.0
43.00	176.0
43.90	1300.0
45.00	1270.0
47.00	1895.0
47.90	713.0
49.00	6039.0
50.00	27288.0
51.00	8616.0
52.00	492.0
55.00	411.0
56.00	1818.0
57.00	3678.0
58.00	252.0
60.00	1005.0
61.00	6684.0
62.00	6310.0
63.00	4780.0
64.00	514.0
64.90	116.0
67.00	419.0
68.00	14310.0
69.00	13601.0
70.00	1063.0
72.00	792.0
73.00	6203.0
74.00	22880.0
75.00	67352.0
76.00	5739.0
77.00	991.0
77.80	413.0
78.90	3800.0
79.90	1066.0
80.90	3952.0
81.90	800.0
83.00	103.0
87.00	5184.0
88.00	5293.0
90.90	437.0
92.00	3978.0
93.00	5596.0
94.00	15146.0
95.10	127040.0
96.00	8419.0
97.00	300.0
104.00	594.0
104.80	224.0
105.90	649.0
106.90	134.0
112.90	124.0
114.90	182.0
115.80	376.0
117.00	676.0
117.80	348.0
119.00	461.0
127.90	478.0
128.80	185.0
129.90	455.0
131.00	224.0
134.90	202.0
136.90	206.0
140.20	134.0
140.90	1131.0
141.90	152.0
142.90	1128.0
144.90	139.0
145.90	176.0
147.90	355.0
149.90	150.0
154.90	273.0
157.00	183.0
158.90	181.0
160.90	119.0
172.00	250.0
174.00	92408.0
175.00	7056.0
176.00	89808.0
177.00	5293.0
177.90	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	1227.0
37.00	7147.0
38.00	6029.0
39.00	2036.0
40.00	321.0
40.80	134.0
43.00	109.0
43.90	1317.0
45.00	1159.0
47.00	1805.0
47.90	661.0
49.00	5655.0
50.00	26680.0
51.00	8365.0
52.00	345.0
55.00	403.0
56.00	1743.0
57.00	3830.0
57.90	298.0
60.00	1065.0
61.00	6307.0
62.00	6040.0
63.00	4508.0
64.00	517.0
64.90	115.0
67.00	430.0
68.00	14201.0
69.00	13313.0
70.00	1093.0
72.00	744.0
73.00	6011.0
74.00	22280.0
75.00	66320.0
76.00	5462.0
77.00	999.0
77.80	417.0
78.90	3796.0
79.90	1063.0
80.90	3848.0
81.90	742.0
87.00	5371.0
88.00	5328.0
90.90	455.0
92.00	3675.0
93.00	5573.0
94.00	15023.0
95.10	124464.0
96.00	7992.0
97.00	315.0
103.90	648.0
104.80	252.0
105.90	642.0
106.90	105.0
114.80	176.0
115.90	434.0
117.00	678.0
117.80	385.0
119.00	501.0
127.90	434.0
128.90	178.0
129.90	464.0
131.00	242.0
134.90	174.0
136.90	198.0
140.20	124.0
140.90	1065.0
142.00	141.0
143.00	1132.0
144.90	184.0
145.90	141.0
147.90	385.0
148.70	120.0
149.80	127.0
152.80	105.0
154.90	319.0
157.10	198.0
158.90	173.0
160.90	120.0
172.10	313.0
174.00	92144.0
175.00	6927.0
176.00	90576.0
177.00	5400.0
177.90	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

Scan 2882 (10.607 min): VU037744.D
BFB15

m/z	Abundance
38.90	107.0
39.90	188.0
40.90	121.0
42.90	124.0
44.00	733.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15