

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041624\
 Data File : VU058727.D
 Acq On : 16 Apr 2024 19:36
 Operator : MD/SY
 Sample : P2143-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAM8

Quant Time: Apr 17 01:15:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 17 01:09:43 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024
 Supervised By :Semsettin Yesilyurt 04/17/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	75158	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	76541	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	40857	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.589	65	13884	2.790	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.800%
7) Chloroethane-d5	1.905	69	16553	3.828	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.600%
11) 1,1-Dichloroethene-d2	2.557	65	6856	3.044	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.800%
20) 2-Butanone-d5	4.615	46	69521	66.297	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.600%#
24) Chloroform-d	5.062	84	89388	8.999	ug/L	0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	180.000%#
26) 1,2-Dichloroethane-d4	5.692	65	22789	4.916	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
32) Benzene-d6	5.721	84	77300	3.751	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.000%
36) 1,2-Dichloropropane-d6	6.702	67	29055	4.496	ug/L	0.02
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.000%
41) Toluene-d8	7.895	98	62132	3.400	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.000%#
43) trans-1,3-Dichloroprop...	8.174	79	9099	4.536	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.800%
46) 2-Hexanone-d5	8.628	63	51480	62.220	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	124.440%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	22446	4.920	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	25505	3.706	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	74.200%#
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.596	62	7454	0.974	ug/L	92
10) 1,1,2-Trichloro-1,2,2-...	2.570	101	114619	19.078	ug/L	96
12) 1,1-Dichloroethene	2.570	96	854528	160.432	ug/L #	77
13) Acetone	2.622	43	24283	27.132	ug/L	100
16) Methylene chloride	3.027	84	12809928	1812.112	ug/L	86
18) trans-1,2-Dichloroethene	3.342	96	4405	0.789	ug/L	91
19) 1,1-Dichloroethane	3.856	63	61966	5.086	ug/L	98
22) cis-1,2-Dichloroethene	4.650	96	1012172	161.456	ug/L	95
25) Chloroform	5.075	83	1143880	96.995	ug/L	100
27) 1,2-Dichloroethane	5.789	62	7393	1.029	ug/L	97
29) 1,1,1-Trichloroethane	5.310	97	38468	3.749	ug/L	97
30) Cyclohexane	5.380	56	3761	0.347	ug/L #	89
31) Carbon tetrachloride	5.515	117	68575	7.891	ug/L	99
33) Benzene	5.769	78	35900	1.294	ug/L	100
34) Trichloroethene	6.538	95	49758576m	7114.600	ug/L	
38) Bromodichloromethane	7.100	83	31415	3.770	ug/L	100
40) 4-Methyl-2-pentanone	7.792	43	5448	1.586	ug/L #	88
42) Toluene	7.962	91	356225	12.241	ug/L	99
45) 1,1,2-Trichloroethane	8.393	97	17893	4.197	ug/L	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041624\
 Data File : VU058727.D
 Acq On : 16 Apr 2024 19:36
 Operator : MD/SY
 Sample : P2143-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAM8

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024
 Supervised By :Semsettin Yesilyurt 04/17/2024

Quant Time: Apr 17 01:15:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 17 01:09:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

47) Tetrachloroethene	8.551	164	1957568	381.810	ug/L	96
49) Dibromochloromethane	8.805	129	8128m	1.649	ug/L	
52) Ethylbenzene	9.563	91	1044955	33.892	ug/L	100
53) m,p-Xylene	9.686	106	1540403	139.526	ug/L	97
54) o-Xylene	10.094	106	1148408	106.101	ug/L	98
57) 1,1,2,2-Tetrachloroethane	10.776	83	6109	1.162	ug/L	94
59) Bromoform	10.284	173	2025	0.742	ug/L #	94
60) Isopropylbenzene	10.477	105	20725m	0.693	ug/L	
62) 1,3,5-Trimethylbenzene	11.081	105	165404	6.781	ug/L	99
63) 1,2,4-Trimethylbenzene	11.460	105	491639	19.740	ug/L	100
65) 1,4-Dichlorobenzene	11.830	146	8672	0.613	ug/L	98
67) 1,2-Dichlorobenzene	12.203	146	114824	8.688	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041624\
Data File : VU058727.D
Acq On : 16 Apr 2024 19:36
Operator : MD/SY
Sample : P2143-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
C0AM8

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024


Quant Time: Apr 17 01:15:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 17 01:09:43 2024
Response via : Initial Calibration

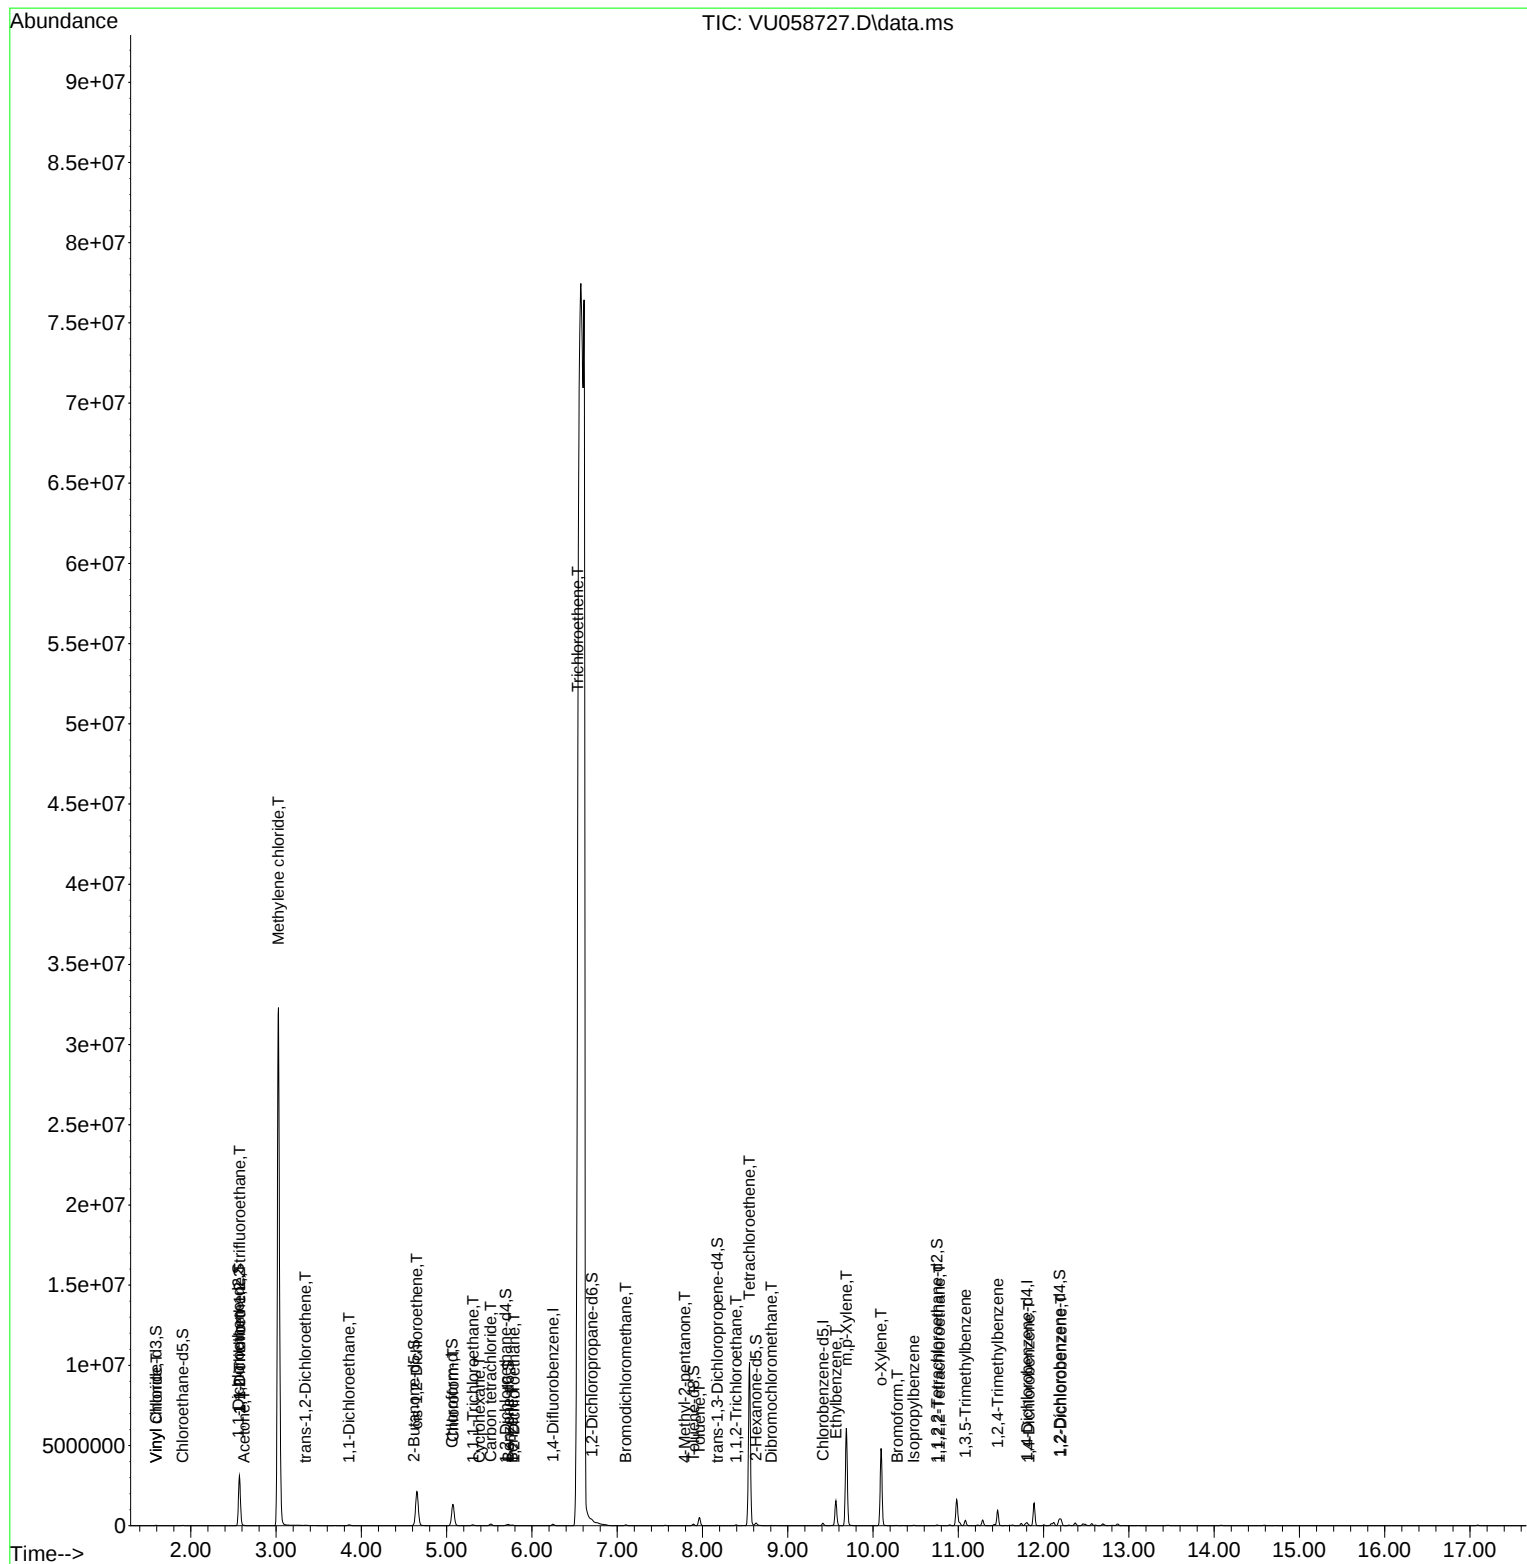

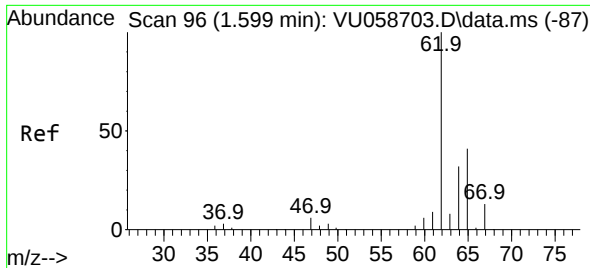

#5
Vinyl chloride
Concen: 0.974 ug/L
RT: 1.596 min Scan# 91
Delta R.T. -0.003 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36




Instrument :
MSVOA_U
ClientSampleId :
COAM8

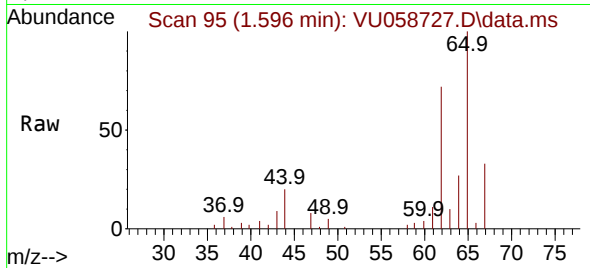

Tgt Ion: 62 Resp: 7454
Ion Ratio Lower Upper
62 100
64 36.8 22.6 42.0




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024

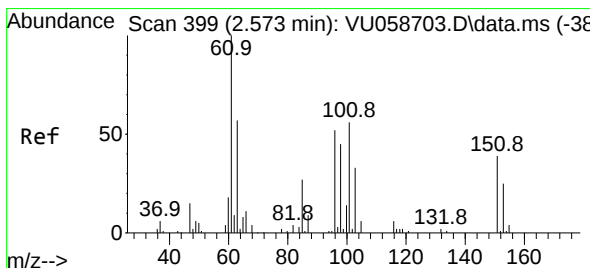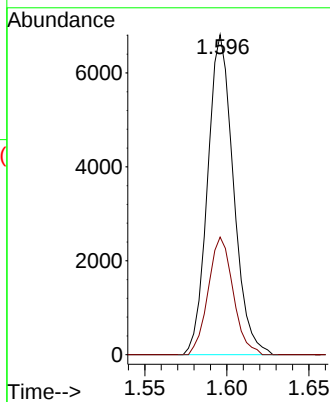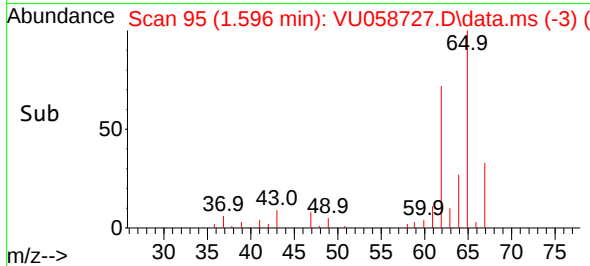

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 19.078 ug/L
RT: 2.570 min Scan# 398
Delta R.T. -0.003 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

Tgt Ion:101 Resp: 114619
Ion Ratio Lower Upper
101 100
85 47.6 36.8 55.2
151 68.9 58.2 87.4

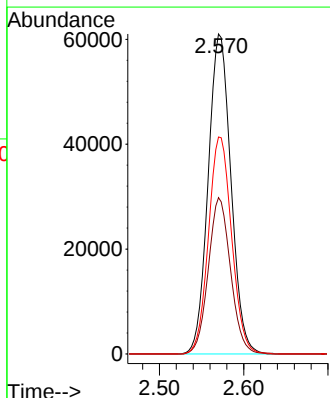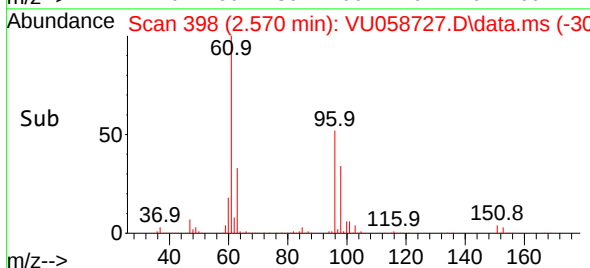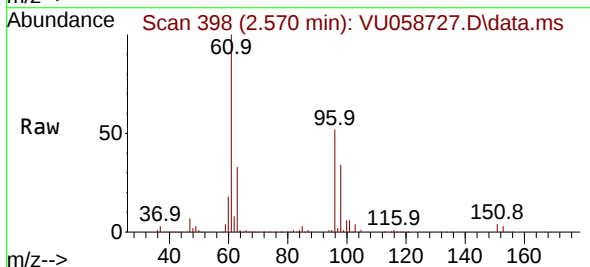



#12

1,1-Dichloroethene

Concen: 160.432 ug/L

RT: 2.570 min Scan# 399

Delta R.T. -0.003 min

Lab File: VU058727.D

Acq: 16 Apr 2024 19:36

Instrument :

MSVOA_U

ClientSampleId :

COAM8

Tgt Ion: 96 Resp: 854528

Ion Ratio Lower Upper

96 100

61 191.5 132.5 246.1





63 63.0 87.7 162.9

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024

Supervised By :Semsettin Yesilyurt 04/17/2024

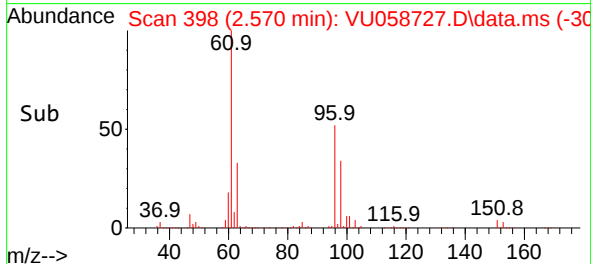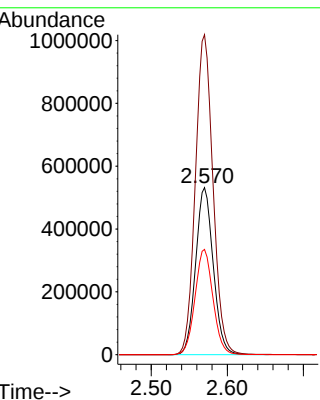

#13

Acetone

Concen: 27.132 ug/L

RT: 2.622 min Scan# 414

Delta R.T. -0.006 min

Lab File: VU058727.D




Acq: 16 Apr 2024 19:36


Tgt Ion: 43 Resp: 24283

Ion Ratio Lower Upper

43 100


58 30.7 0.0 61.4

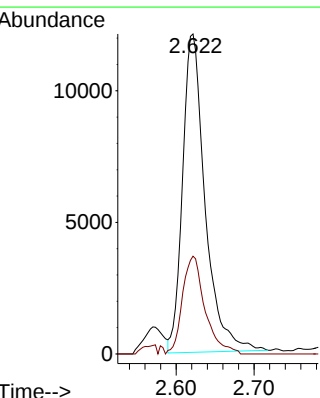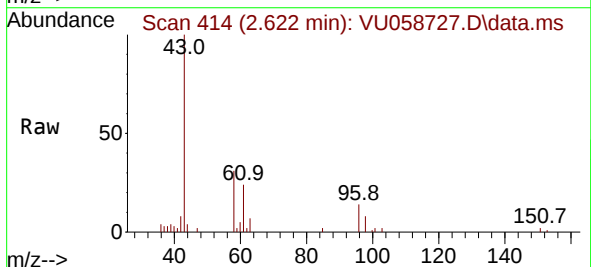



#16
Methylene chloride
Concen: 1812.112 ug/L
RT: 3.027 min Scan# 543
Delta R.T. -0.009 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36




Instrument :
MSVOA_U
ClientSampleId :
COAM8



Tgt Ion: 84 Resp:12809928
Ion Ratio Lower Upper
84 100
86 64.9 44.3 82.3
49 114.4 96.0 178.2




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024

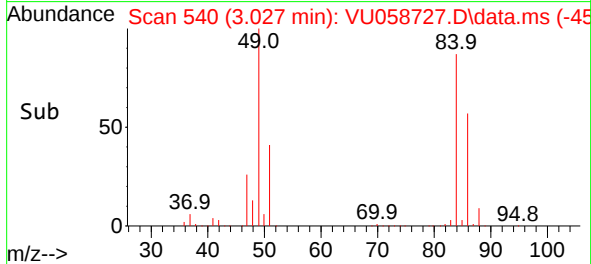

#18
trans-1,2-Dichloroethene
Concen: 0.789 ug/L
RT: 3.342 min Scan# 638
Delta R.T. -0.003 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

Tgt Ion: 96 Resp: 4405
Ion Ratio Lower Upper
96 100
61 166.4 107.6 199.8
98 58.6 45.1 83.7

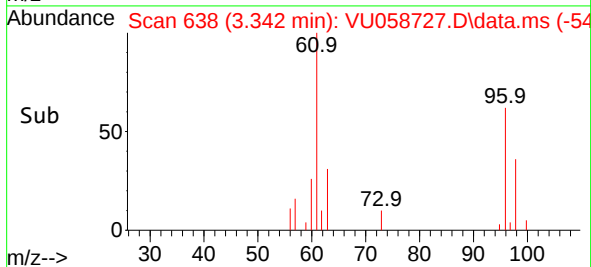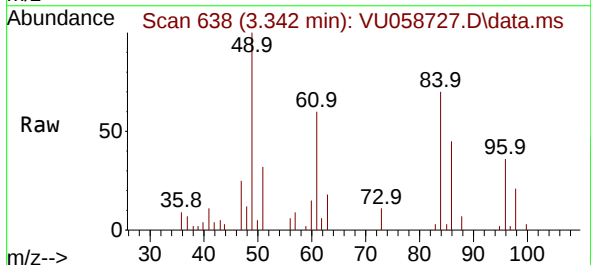



#19

1,1-Dichloroethane

Concen: 5.086 ug/L

RT: 3.856 min Scan# 799

Delta R.T. -0.003 min

Lab File: VU058727.D


Acq: 16 Apr 2024 19:36

Instrument :

MSVOA_U

ClientSampleId :

COAM8

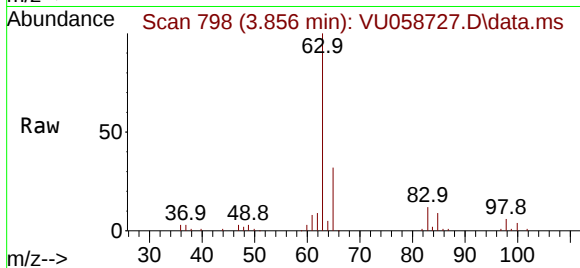

Tgt Ion: 63 Resp: 61960

Ion Ratio Lower Upper

63 100

65 31.7 22.9 42.5




83 12.4 9.6 17.8

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024

Supervised By :Semsettin Yesilyurt 04/17/2024

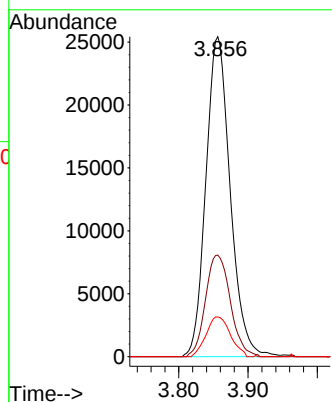

#22

cis-1,2-Dichloroethene

Concen: 161.456 ug/L

RT: 4.650 min Scan# 1045

Delta R.T. -0.006 min

Lab File: VU058727.D

Acq: 16 Apr 2024 19:36




Tgt Ion: 96 Resp: 1012172


Ion Ratio Lower Upper

96 100

61 148.5 98.1 182.3

98 63.5 43.6 81.0

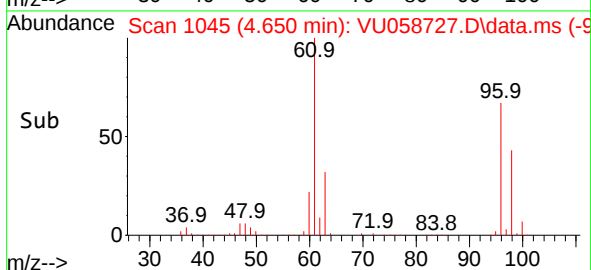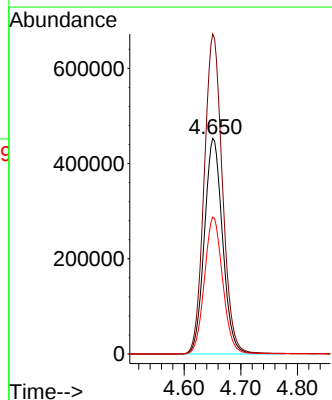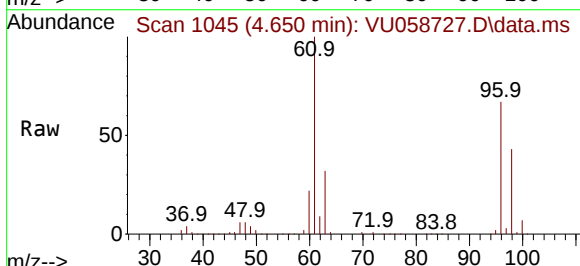

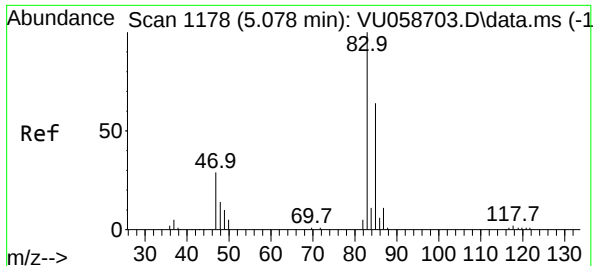

#25

Chloroform

Concen: 96.995 ug/L

RT: 5.075 min Scan# 1178

Delta R.T. -0.003 min

Lab File: VU058727.D

Acq: 16 Apr 2024 19:36

Instrument :

MSVOA_U

ClientSampleId :

COAM8

Tgt Ion: 83 Resp: 114388

Ion Ratio Lower Upper

83 100





85 63.7 44.7 83.1

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024

Supervised By :Semsettin Yesilyurt 04/17/2024

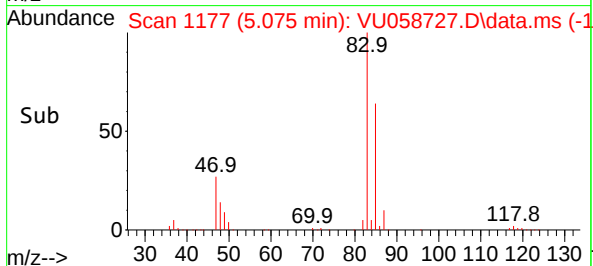

#27

1,2-Dichloroethane

Concen: 1.029 ug/L

RT: 5.789 min Scan# 1399

Delta R.T. 0.004 min

Lab File: VU058727.D




Acq: 16 Apr 2024 19:36


Tgt Ion: 62 Resp: 7393

Ion Ratio Lower Upper

62 100

98 7.7 7.0 10.4

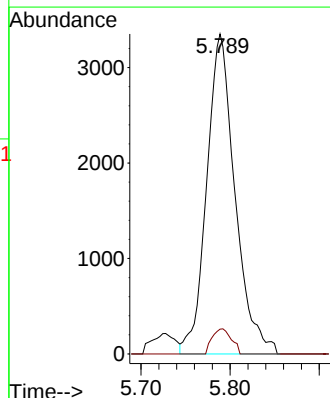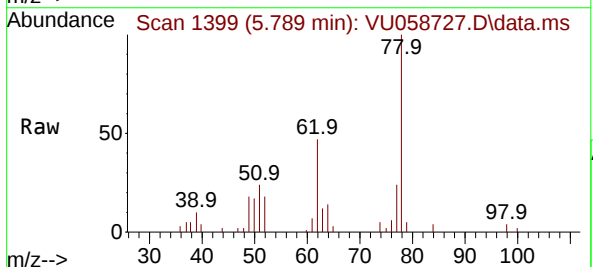



#29

1,1,1-Trichloroethane

Concen: 3.749 ug/L

RT: 5.310 min Scan# 1249

Delta R.T. 0.004 min

Lab File: VU058727.D

Acq: 16 Apr 2024 19:36

Instrument :

MSVOA_U

ClientSampleId :

COAM8

Tgt Ion: 97 Resp: 3846

Ion Ratio Lower Upper

97 100

99 64.9 50.4 75.6





61 52.1 39.4 59.0

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024

Supervised By :Semsettin Yesilyurt 04/17/2024

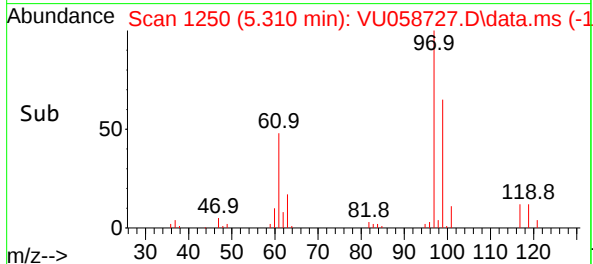

#30

Cyclohexane

Concen: 0.347 ug/L

RT: 5.380 min Scan# 1272

Delta R.T. 0.000 min

Lab File: VU058727.D

Acq: 16 Apr 2024 19:36




Tgt Ion: 56 Resp: 3761


Ion Ratio Lower Upper

56 100

69 19.3 23.2 34.8#


84 86.5 63.3 94.9

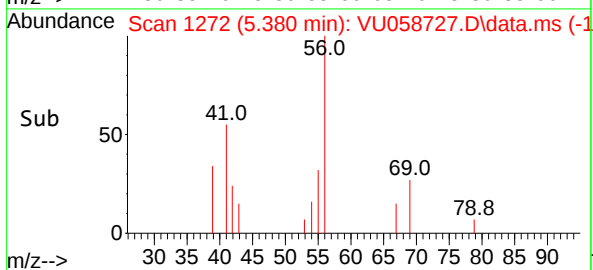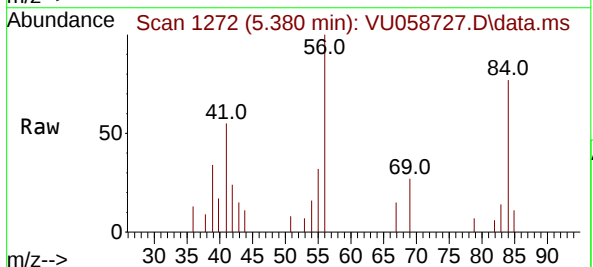



#31
Carbon tetrachloride
Concen: 7.891 ug/L
RT: 5.515 min Scan# 117
Delta R.T. 0.000 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36




Instrument :
MSVOA_U
ClientSampleId :
C0AM8



Tgt Ion:117 Resp: 6857
Ion Ratio Lower Upper
117 100
119 97.1 76.7 115.1




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024

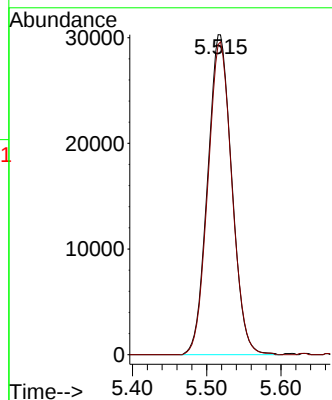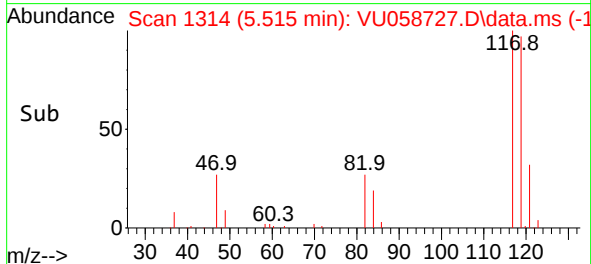

#33
Benzene
Concen: 1.294 ug/L
RT: 5.769 min Scan# 1393
Delta R.T. 0.004 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36


Tgt Ion: 78 Resp: 35900

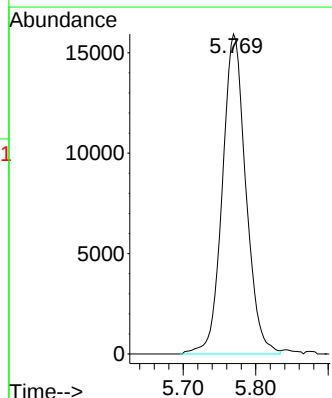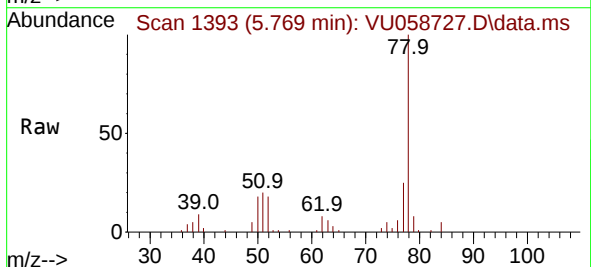



#34
Trichloroethene
Concen: 7114.600 ug/L m
RT: 6.538 min Scan# 1631
Delta R.T. 0.004 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36




Instrument :
MSVOA_U
ClientSampleId :
COAM8




Tgt Ion: 95 Resp: 49758570
Ion Ratio Lower Upper
95 100
97 69.8 45.6 84.6
132 79.9 64.8 120.3
130 86.1 68.0 126.2

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024

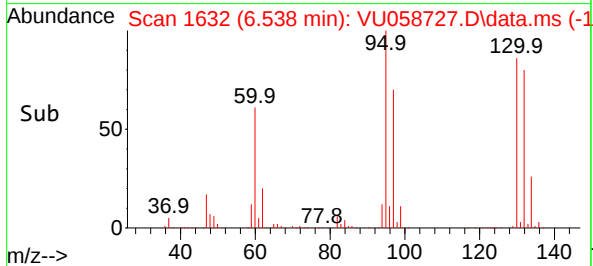


#38
Bromodichloromethane
Concen: 3.770 ug/L
RT: 7.100 min Scan# 1807
Delta R.T. 0.004 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

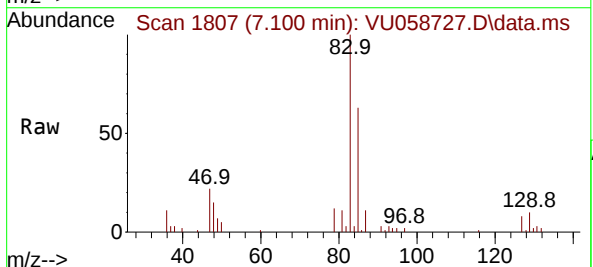

Tgt Ion: 83 Resp: 31415
Ion Ratio Lower Upper
83 100
85 63.2 44.2 82.2
127 8.0 6.5 9.7

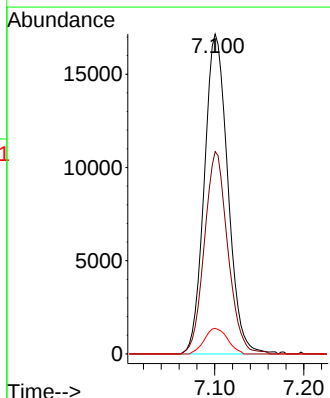



#40

4-Methyl-2-pentanone

Concen: 1.586 ug/L

RT: 7.792 min Scan# 2020

Delta R.T. 0.007 min

Lab File: VU058727.D

Acq: 16 Apr 2024 19:36

Instrument :

MSVOA_U

ClientSampleId :





COAM8

Tgt Ion: 43 Resp: 5448
 Ion Ratio Lower Upper
 43 100
 58 34.7 30.4 45.6
 100 0.0 10.3 15.5

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024
 Supervised By :Semsettin Yesilyurt 04/17/2024

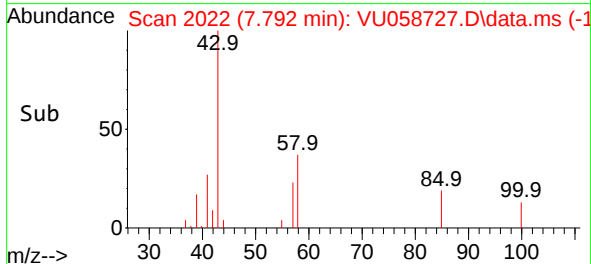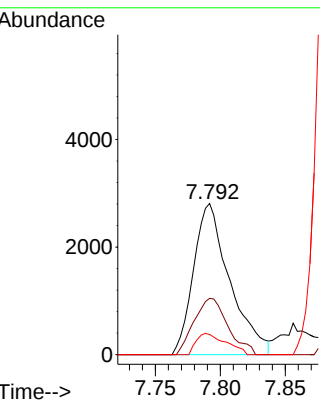

#42

Toluene

Concen: 12.241 ug/L




RT: 7.962 min Scan# 2075


Delta R.T. 0.000 min

Lab File: VU058727.D

Acq: 16 Apr 2024 19:36


Tgt Ion: 91 Resp: 356225
 Ion Ratio Lower Upper
 91 100
 92 56.8 39.5 73.3

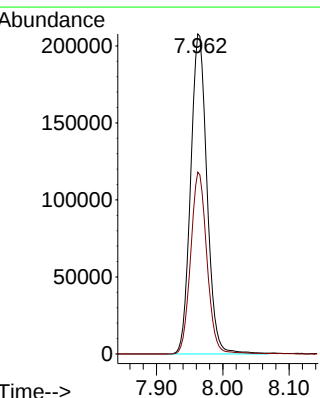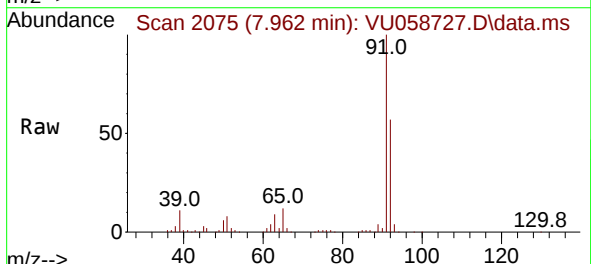



#45
1,1,2-Trichloroethane
Concen: 4.197 ug/L
RT: 8.393 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

Instrument :
MSVOA_U
ClientSampleId :
COAM8






Tgt Ion: 97 Resp: 1789


Ion	Ratio	Lower	Upper
97	100		
99	60.4	43.7	81.1
83	87.0	64.5	119.7
85	56.4	38.1	70.9

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024


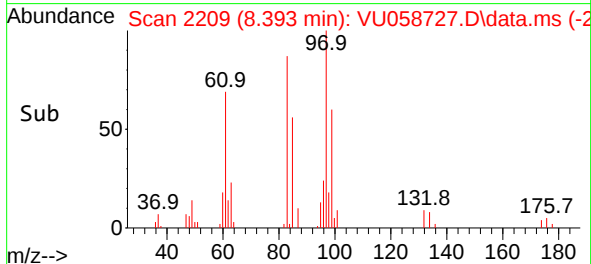



#47
Tetrachloroethene
Concen: 381.810 ug/L
RT: 8.551 min Scan# 2258
Delta R.T. 0.004 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

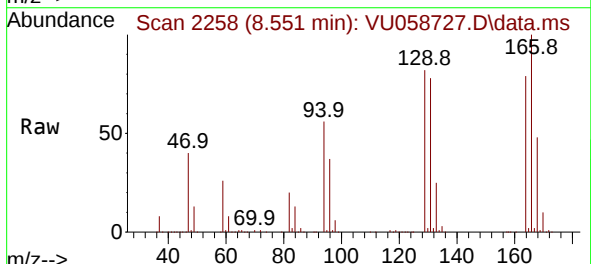

Tgt Ion:164 Resp: 1957568


Ion	Ratio	Lower	Upper
164	100		
129	103.2	67.3	125.1
131	98.6	65.5	121.6
166	126.0	89.5	166.1

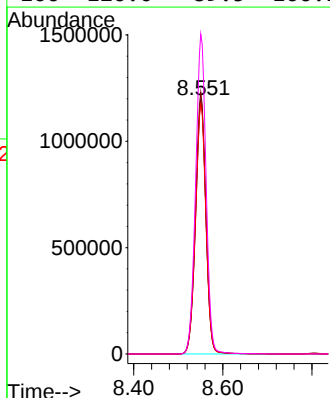



#49
Dibromochloromethane
Concen: 1.649 ug/L m
RT: 8.805 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36




Instrument :
MSVOA_U
ClientSampleId :
COAM8



Tgt Ion:129 Resp: 8128
Ion Ratio Lower Upper
129 100
127 77.7 53.5 99.5




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024

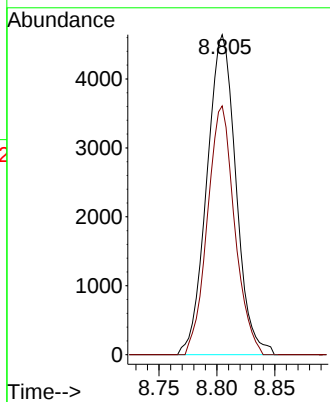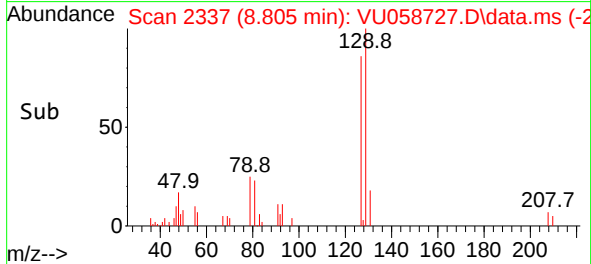

#52
Ethylbenzene
Concen: 33.892 ug/L
RT: 9.563 min Scan# 2573
Delta R.T. -0.003 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

Tgt Ion: 91 Resp: 1044955
Ion Ratio Lower Upper
91 100
106 29.4 20.6 38.4

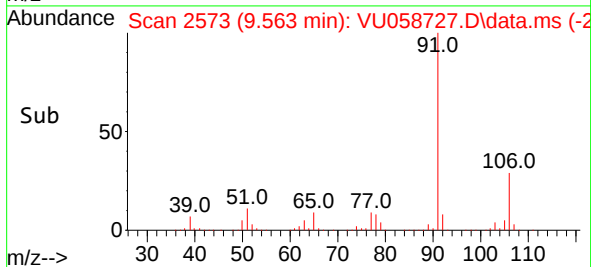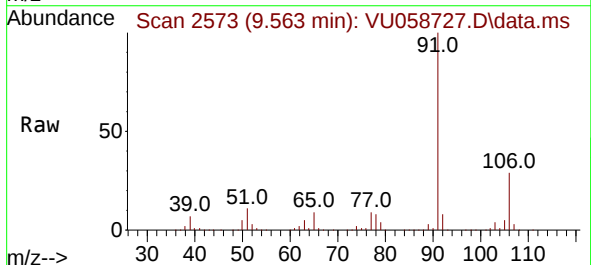







#53
m,p-Xylene
Concen: 139.526 ug/L
RT: 9.686 min Scan# 2612
Delta R.T. -0.003 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

Instrument :
MSVOA_U
ClientSampleId :
C0AM8

Tgt Ion:106 Resp: 1540408
Ion Ratio Lower Upper
106 100
91 215.8 147.8 274.4




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024

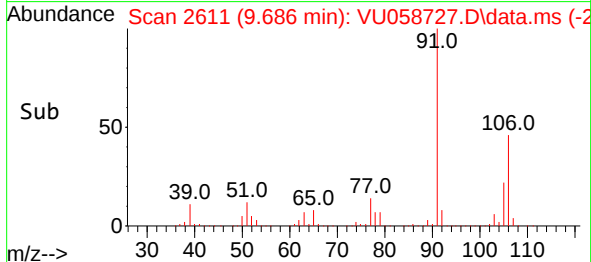

#54
o-Xylene
Concen: 106.101 ug/L
RT: 10.094 min Scan# 2738
Delta R.T. 0.000 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

Tgt Ion:106 Resp: 1148408
Ion Ratio Lower Upper
106 100
91 228.1 156.9 291.5

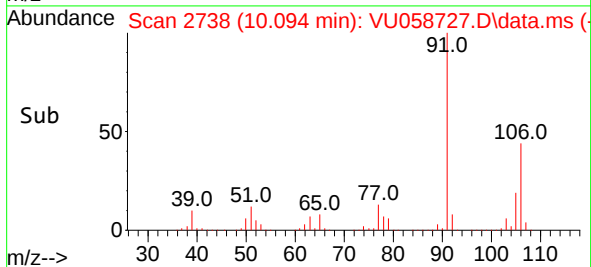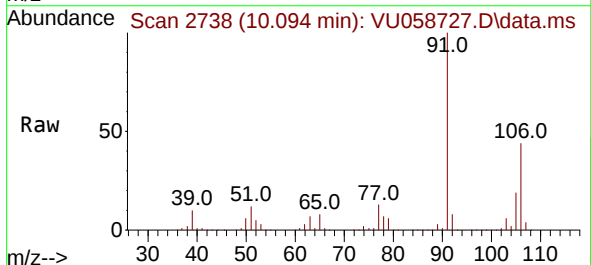







#57
1,1,2,2-Tetrachloroethane
Concen: 1.162 ug/L
RT: 10.776 min Scan# 2950
Delta R.T. 0.000 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

Instrument :
MSVOA_U
ClientSampleId :
COAM8

Tgt Ion: 83 Resp: 6109
Ion Ratio Lower Upper
83 100
85 69.9 45.1 83.7
131 9.2 6.9 10.3




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024

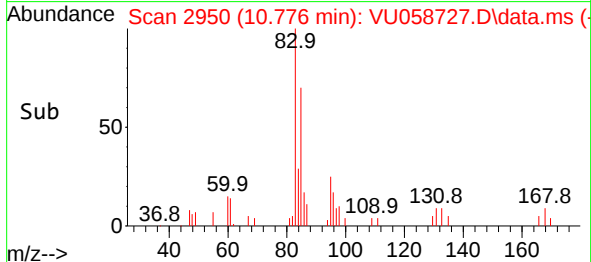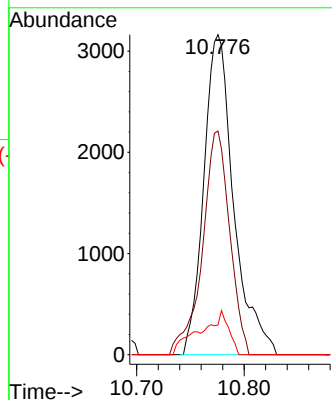

#59
Bromoform
Concen: 0.742 ug/L
RT: 10.284 min Scan# 2797
Delta R.T. 0.000 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36


Tgt Ion:173 Resp: 2025
Ion Ratio Lower Upper
173 100
175 49.8 38.0 57.0
254 3.5 7.5 11.3#

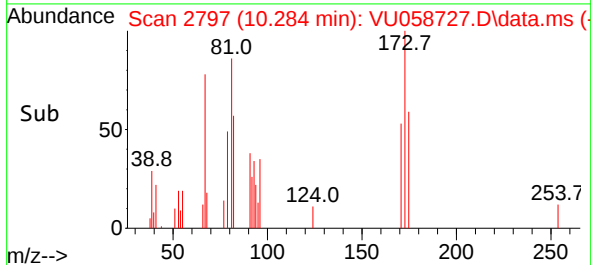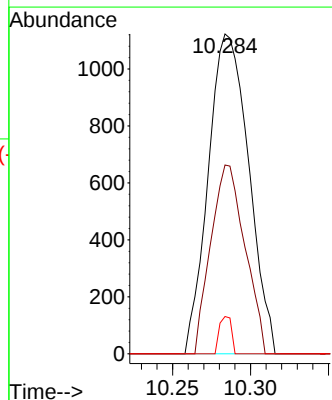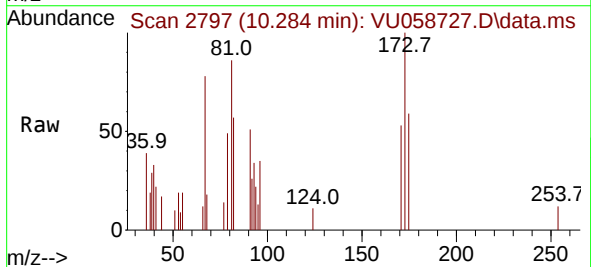

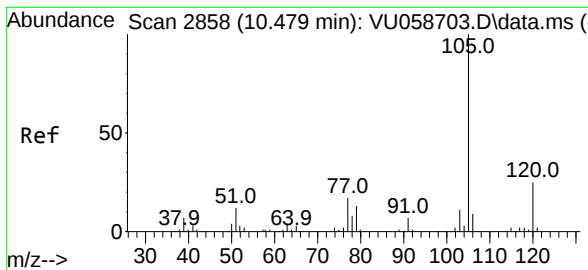

#60
Isopropylbenzene
Concen: 0.693 ug/L m
RT: 10.477 min Scan# 2858
Delta R.T. -0.003 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36




Instrument :
MSVOA_U
ClientSampleId :
C0AM8

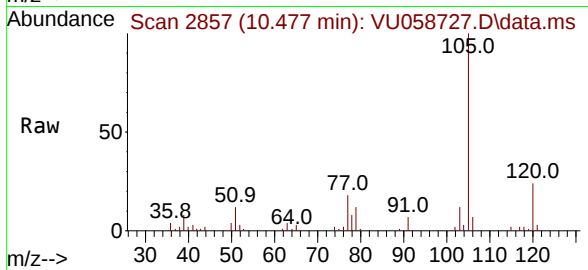


Tgt Ion:105 Resp: 20725
Ion Ratio Lower Upper
105 100
120 421.8 20.2 30.4
77 196.8 13.5 20.3

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024

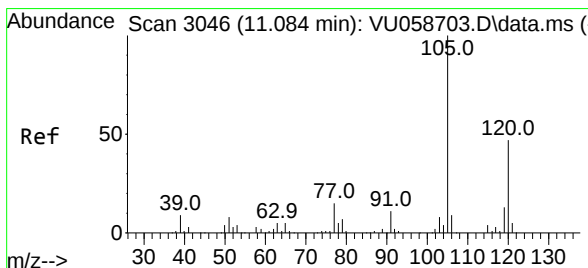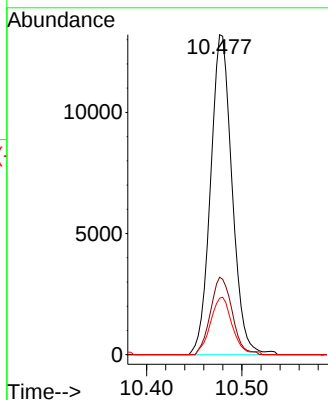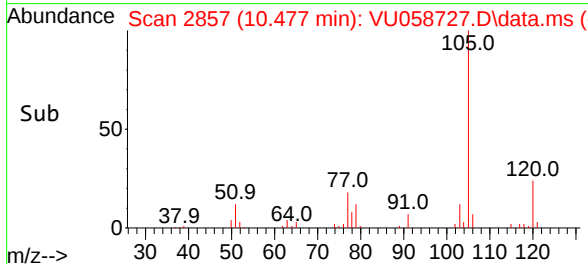


#62
1,3,5-Trimethylbenzene
Concen: 6.781 ug/L
RT: 11.081 min Scan# 3045
Delta R.T. -0.003 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

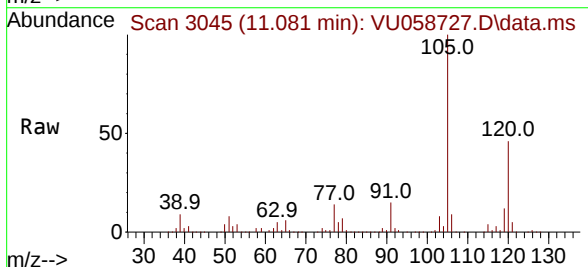

Tgt Ion:105 Resp: 165404
Ion Ratio Lower Upper
105 100
120 46.1 37.2 55.8

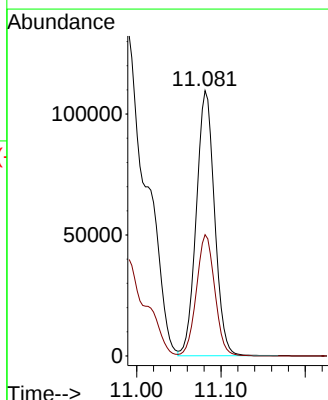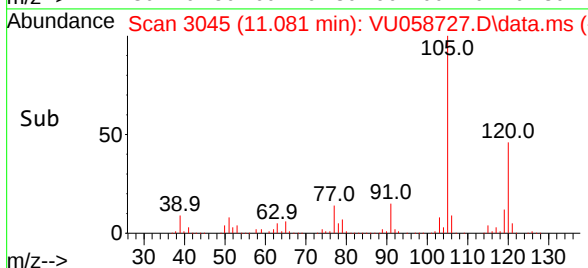

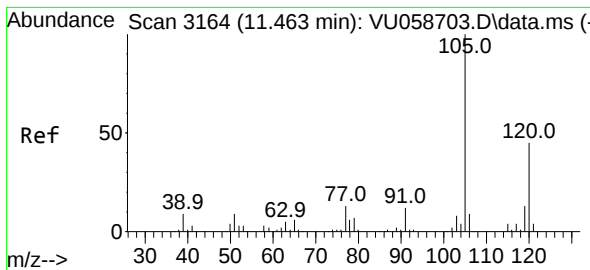

#63

1,2,4-Trimethylbenzene

Concen: 19.740 ug/L

RT: 11.460 min Scan# 3164

Delta R.T. -0.003 min

Lab File: VU058727.D

Acq: 16 Apr 2024 19:36

Instrument :

MSVOA_U

ClientSampleId :

COAM8

Tgt Ion:105 Resp: 491639

Ion Ratio Lower Upper

105 100





120 43.3 34.7 52.1

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024

Supervised By :Semsettin Yesilyurt 04/17/2024

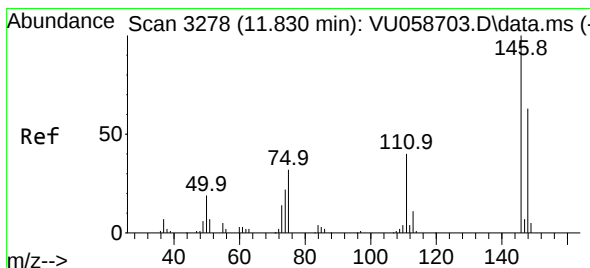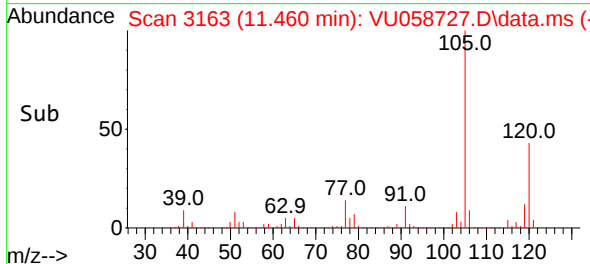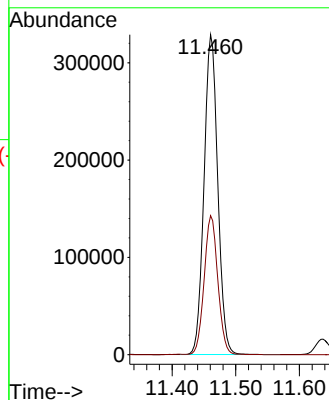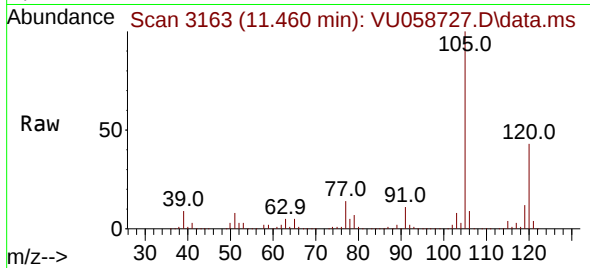

#65

1,4-Dichlorobenzene

Concen: 0.613 ug/L

RT: 11.830 min Scan# 3278

Delta R.T. 0.000 min

Lab File: VU058727.D

Acq: 16 Apr 2024 19:36




Tgt Ion:146 Resp: 8672


Ion Ratio Lower Upper

146 100

111 43.4 28.8 53.6


148 63.2 45.3 84.1

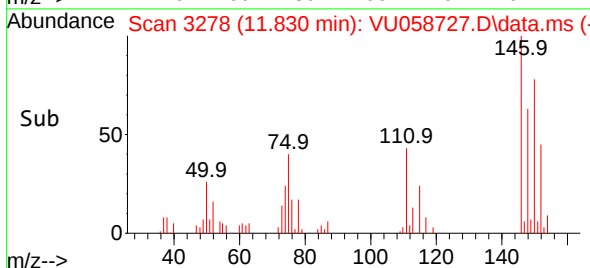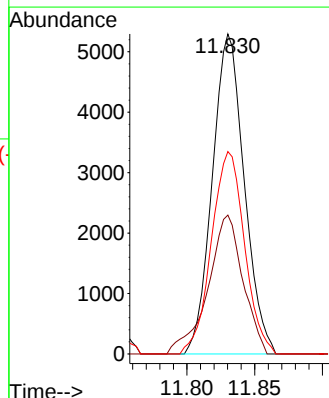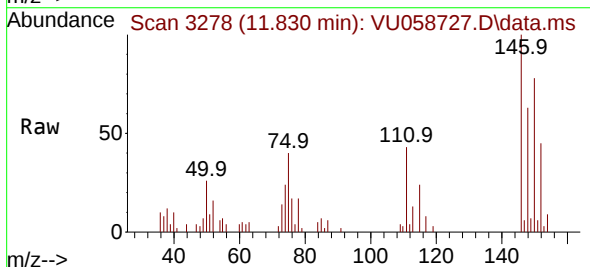



#67
1,2-Dichlorobenzene
Concen: 8.688 ug/L
RT: 12.203 min Scan# 31
Delta R.T. -0.003 min
Lab File: VU058727.D
Acq: 16 Apr 2024 19:36

Instrument :
MSVOA_U
ClientSampleId :
COAM8



Tgt Ion:146 Resp: 114824
Ion Ratio Lower Upper
146 100
111 44.4 35.0 52.4
148 64.4 52.5 78.7

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 04/17/2024
Supervised By :Semsettin Yesilyurt 04/17/2024

