


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041624\
Data File : VU058702.D
Acq On : 16 Apr 2024 08:36
Operator : MD/SY
Sample : BFB144
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB144

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 17 01:09:43 2024

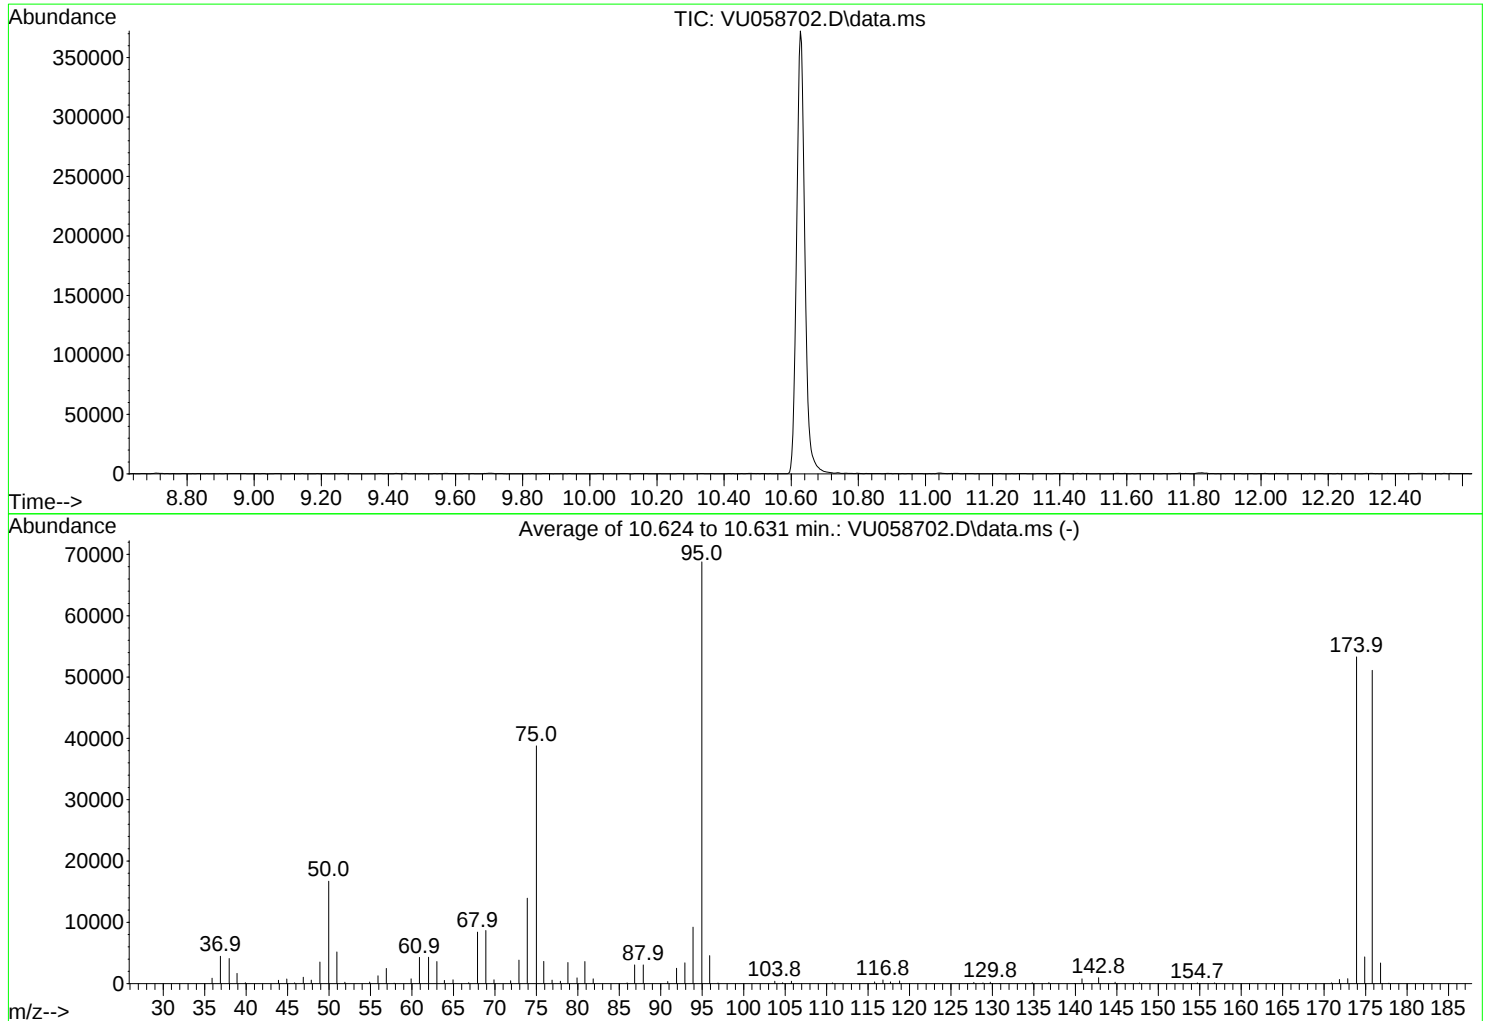

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.3	16688	PASS
75	95	30	80	56.4	38779	PASS
95	95	100	100	100.0	68789	PASS
96	95	5	9	6.6	4559	PASS
173	174	0.00	2	1.5	820	PASS
174	95	50	120	77.4	53272	PASS
175	174	5	9	8.2	4349	PASS
176	174	95	101	95.9	51083	PASS
177	176	5	9	6.6	3356	PASS

m/z	Abundance
43.90	165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

m/z	Abundance
35.90	898.0
36.90	4314.0
37.90	4202.0
38.90	1584.0
40.00	157.0
43.90	792.0
44.90	722.0
45.80	126.0
46.90	1071.0
47.90	555.0
48.90	3582.0
49.90	16592.0
51.00	5032.0
51.90	226.0
54.90	258.0
55.90	1217.0
56.90	2371.0
59.90	820.0
60.90	4109.0
62.00	4111.0
63.00	3686.0
63.90	501.0
64.90	630.0
66.90	157.0
67.90	8090.0
68.90	8549.0
69.90	615.0
71.90	471.0
72.90	3773.0
73.90	13637.0
75.00	37792.0
75.90	3524.0
76.90	582.0
77.90	359.0
78.80	3388.0
79.90	900.0
80.90	3555.0
81.90	760.0
85.90	112.0
86.80	2923.0
87.90	3075.0
90.80	351.0
91.90	2436.0
92.90	3271.0
93.90	9002.0
95.00	67112.0
95.90	4378.0
96.90	114.0
103.80	354.0
104.70	136.0
105.70	369.0
110.70	120.0
115.80	261.0
116.80	587.0
117.70	299.0
118.80	437.0
127.80	204.0
128.80	116.0
129.70	234.0
130.90	108.0
134.80	175.0
136.80	137.0
140.80	758.0
142.80	956.0
144.80	285.0
147.80	129.0
154.70	155.0
156.80	117.0
170.90	136.0
171.90	634.0
172.80	772.0
173.90	50456.0
174.90	4261.0
175.80	48528.0
176.80	3366.0
177.80	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

m/z	Abundance
35.90	945.0
36.90	4530.0
37.90	4188.0
38.90	1677.0
39.90	151.0
43.90	745.0
44.90	793.0
45.80	144.0
46.90	1093.0
47.90	591.0
48.90	3573.0
49.90	17200.0
50.90	5357.0
51.90	258.0
54.90	272.0
55.90	1312.0
56.90	2512.0
57.90	108.0
59.90	803.0
60.90	4402.0
62.00	4482.0
63.00	3676.0
63.90	564.0
65.00	629.0
66.80	169.0
67.90	8697.0
68.90	8964.0
69.90	633.0
71.90	481.0
72.90	3960.0
73.90	14312.0
75.00	39912.0
75.90	3713.0
76.90	594.0
77.90	400.0
78.80	3538.0
79.90	963.0
80.90	3728.0
81.80	819.0
86.00	132.0
86.90	3118.0
87.90	3131.0
90.90	345.0
91.90	2584.0
92.90	3471.0
93.90	9508.0
95.00	70648.0
95.90	4684.0
96.90	120.0
103.70	391.0
104.70	164.0
105.80	394.0
110.70	165.0
115.80	277.0
116.80	632.0
117.70	296.0
118.80	442.0
127.70	219.0
128.90	127.0
129.70	234.0
134.80	173.0
136.80	198.0
140.80	828.0
142.80	1018.0
144.80	258.0
147.70	146.0
154.70	137.0
156.80	137.0
170.90	136.0
171.80	699.0
172.80	846.0
173.90	54920.0
174.90	4472.0
175.80	52744.0
176.80	3463.0
177.80	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

m/z	Abundance
35.90	859.0
36.90	4523.0
38.00	3890.0
38.90	1722.0
39.80	143.0
43.90	645.0
44.90	776.0
45.90	149.0
46.90	968.0
47.80	588.0
48.90	3389.0
50.00	16273.0
50.90	5104.0
51.90	262.0
54.90	249.0
55.90	1339.0
56.90	2528.0
57.80	118.0
59.90	750.0
60.90	4316.0
62.00	4332.0
63.00	3457.0
63.90	533.0
65.00	601.0
66.80	170.0
67.90	8413.0
68.90	8499.0
69.90	609.0
71.90	469.0
72.90	3745.0
73.90	13825.0
75.00	38632.0
75.90	3652.0
76.90	537.0
77.90	392.0
78.80	3423.0
79.90	953.0
80.80	3517.0
81.80	803.0
86.00	132.0
86.90	3098.0
87.90	2974.0
90.90	323.0
91.90	2474.0
92.90	3417.0
93.90	9167.0
94.90	68608.0
95.90	4616.0
96.90	123.0
103.70	415.0
104.70	184.0
105.80	391.0
110.70	143.0
115.80	343.0
116.80	615.0
117.70	282.0
118.80	423.0
127.80	229.0
128.90	146.0
129.80	219.0
134.80	143.0
136.80	196.0
139.90	100.0
140.80	810.0
142.80	937.0
144.80	209.0
145.90	102.0
147.80	164.0
154.70	122.0
156.80	138.0
170.90	117.0
171.80	685.0
172.90	841.0
173.90	54440.0
174.90	4314.0
175.80	51976.0
176.80	3239.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144