

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041720\
 Data File : VU037781.D
 Acq On : 17 Apr 2020 17:34
 Operator : JC/MD
 Sample : L2292-05DL 5X
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF8K9DL

Quant Time: Apr 18 04:36:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 18 01:19:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	265716	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	257572	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	127090	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	84555	4.20	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.00%
7) Chloroethane-d5	1.93	69	76469	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.20%
11) 1,1-Dichloroethene-d2	2.59	63	109088	3.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.00%
20) 2-Butanone-d5	4.66	46	302905	54.85	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.70%
24) Chloroform-d	5.10	84	153858	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.74	65	93678	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.76	84	323186	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
36) 1,2-Dichloropropane-d6	6.72	67	112467	4.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.40%
41) Toluene-d8	7.92	98	287774	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	8.20	79	46077	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
46) 2-Hexanone-d5	8.65	63	265243	50.93	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.86%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	88516	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.00%
64) 1,2-Dichlorobenzene-d4	12.21	152	108548	4.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.80%


Target Compounds					Ovalue
13) Acetone	2.66	43	4571	1.255 ug/L	95
34) Trichloroethene	6.57	95	211545	10.115 ug/L	96
47) Tetrachloroethene	8.57	164	6768	0.450 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041720\
Data File : VU037781.D
Acq On : 17 Apr 2020 17:34
Operator : JC/MD
Sample : L2292-05DL 5X
Misc : 25mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF8K9DL

Quant Time: Apr 18 04:36:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Apr 18 01:19:54 2020
Response via : Initial Calibration

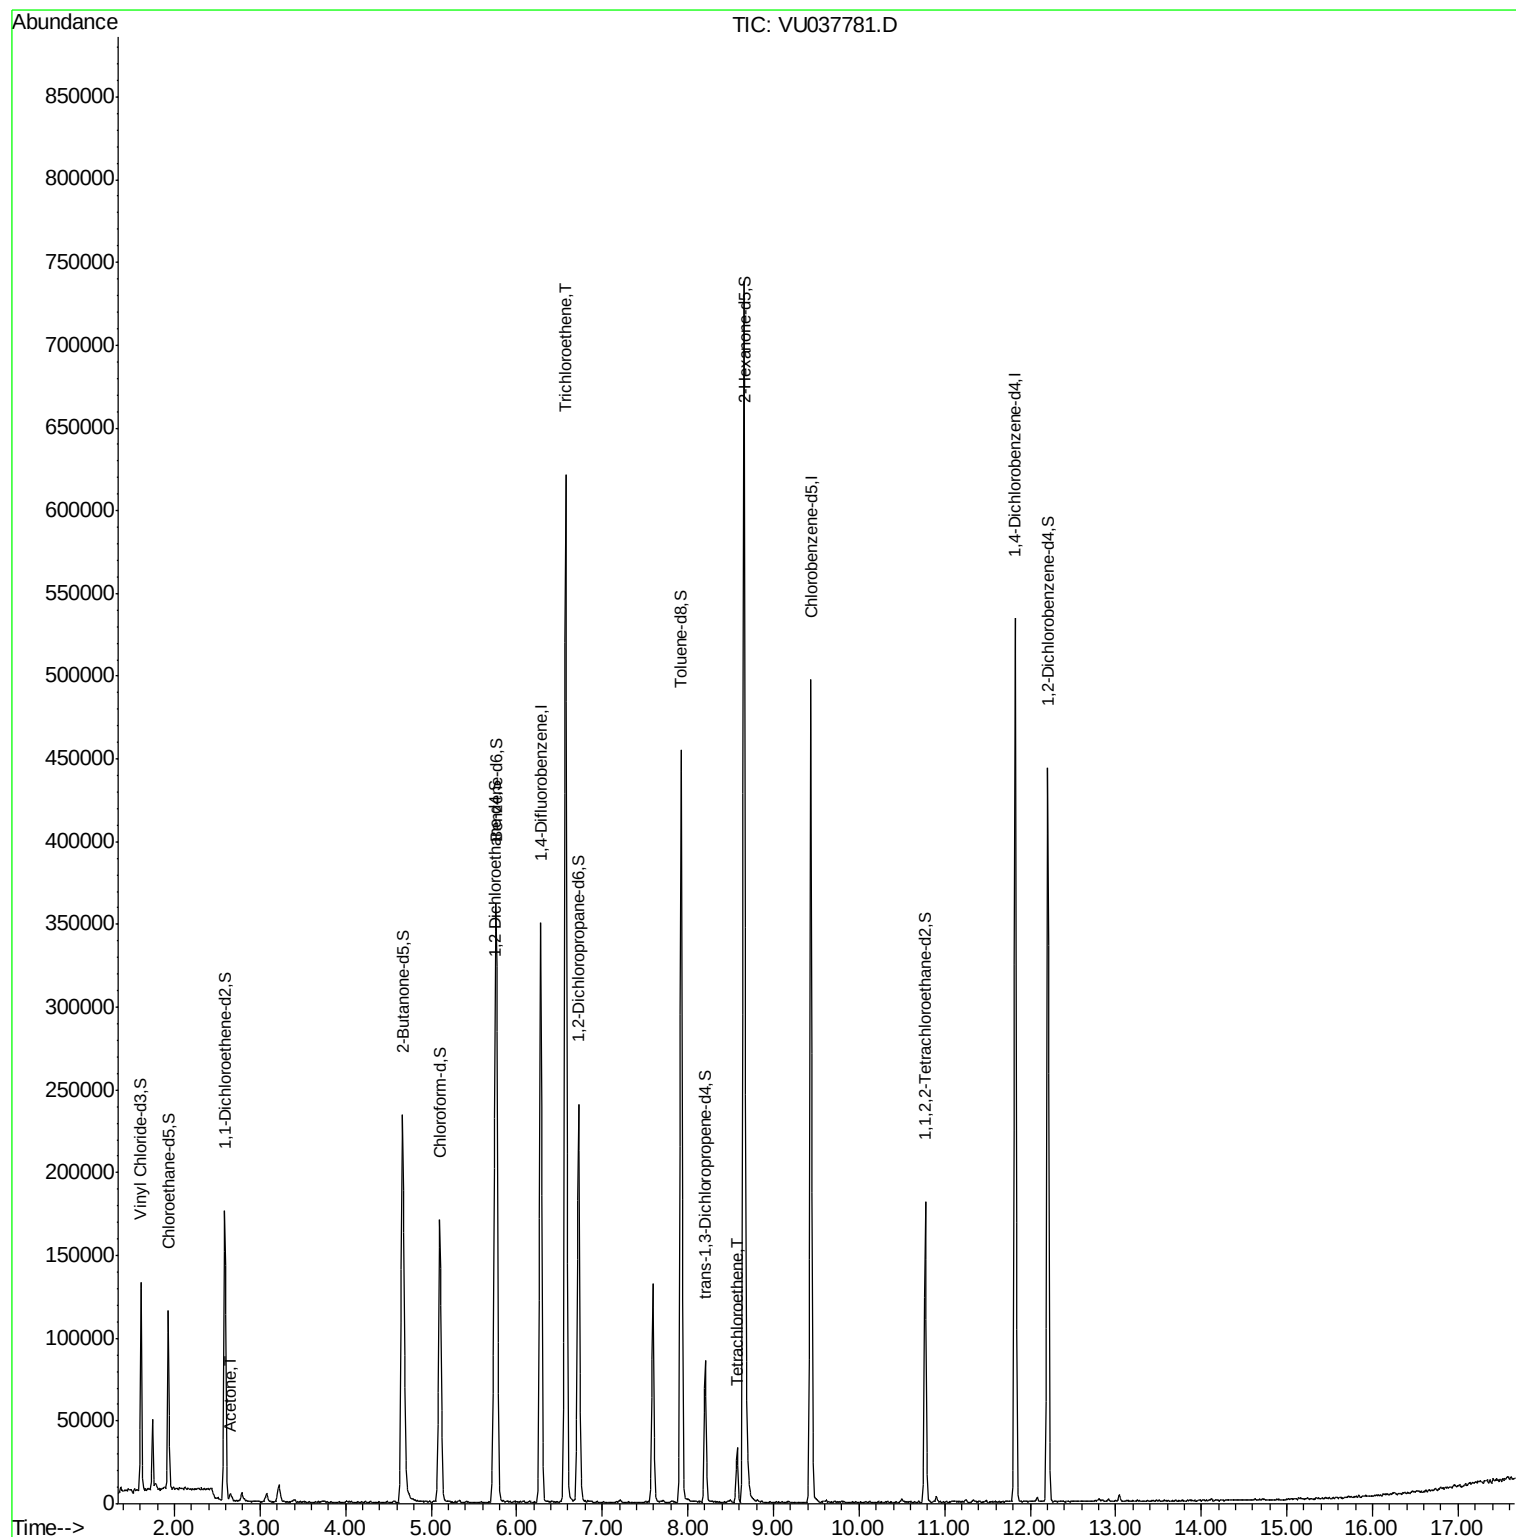

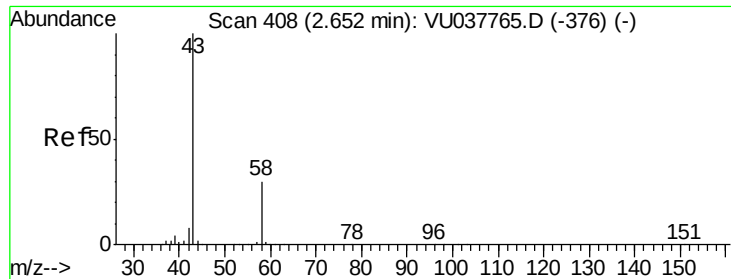

#13

Acetone

Concen: 1.255 ug/L

RT: 2.66 min Scan# 410

Delta R.T. 0.01 min

Lab File: VU037781.D

Acq: 17 Apr 2020 17:34

Instrument :

MSVOA_U

ClientSampleId :


BF8K9DL

Tot Ion: 43 Resp: 4571

Ion Ratio Lower Upper




43 100

58 29.4 0.0 64.8

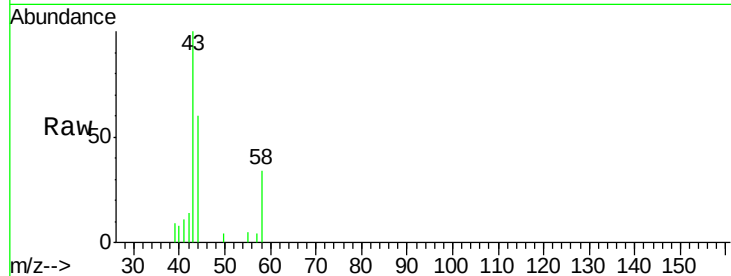

Abundance Ion 43.05 (42.75 to 43.75): VU037781.D (-410) (-)

Ion 58.05 (57.75 to 58.75): VU037781.D (-410) (-)

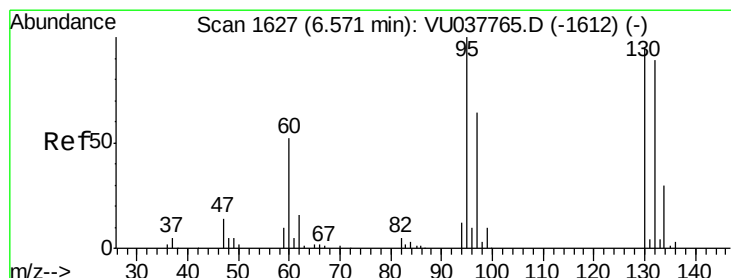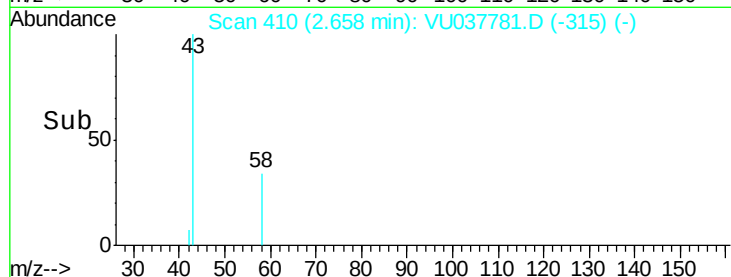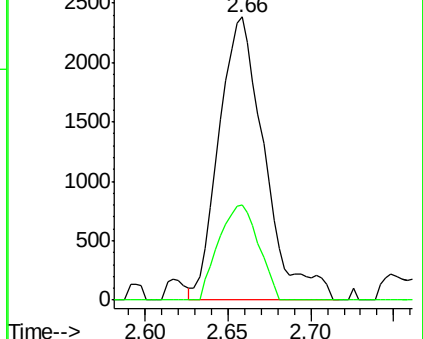

#34

Trichloroethene

Concen: 10.115 ug/L

RT: 6.57 min Scan# 1627

Delta R.T. 0.00 min

Lab File: VU037781.D

Acq: 17 Apr 2020 17:34

Tgt Ion: 95 Resp: 211545


Ion Ratio Lower Upper

95 100

97 64.5 45.4 84.2

132 89.8 63.7 118.3

130 90.4 68.7 127.5


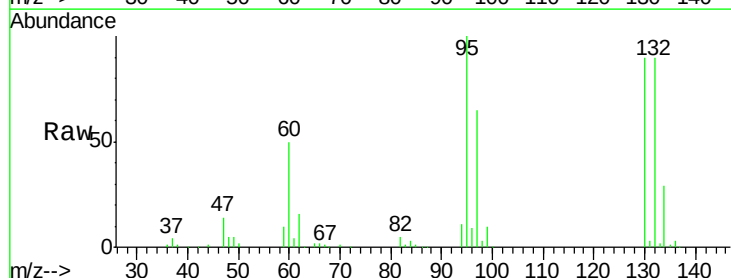



Abundance Ion 95.00 (94.70 to 95.70): VU037781.D (-1627) (-)

Ion 96.95 (96.65 to 97.65): VU037781.D (-1627) (-)

Ion 131.95 (131.65 to 132.65): VU037781.D (-1627) (-)

Ion 129.95 (129.65 to 130.65): VU037781.D (-1627) (-)

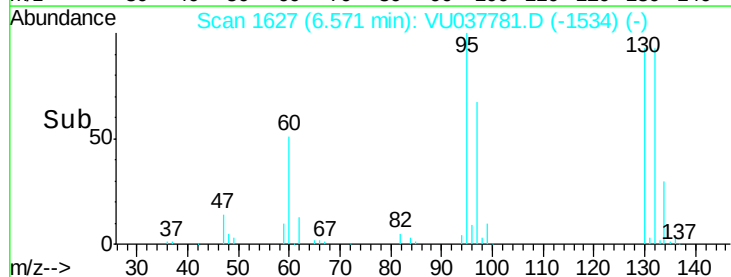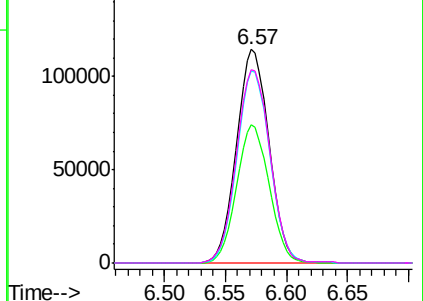

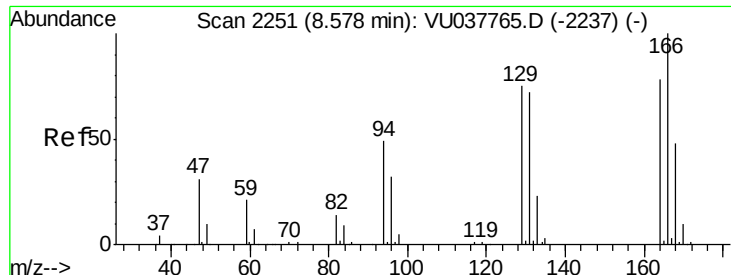

#47

Tetrachloroethene

Concen: 0.450 ug/L

RT: 8.57 min Scan# 2250

Delta R.T. -0.00 min

Lab File: VU037781.D


Acq: 17 Apr 2020 17:34

Instrument :

MSVOA_U

ClientSampleId :

BF8K9DL

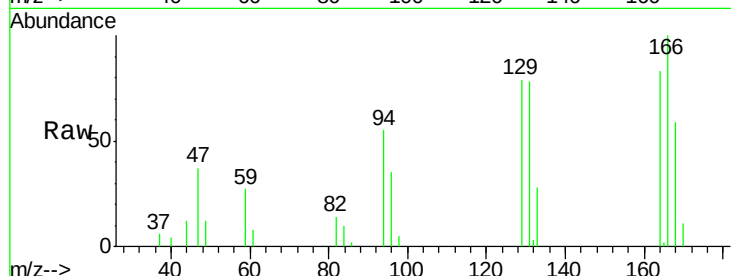

Tot Ion:164 Resp: 6768


Ion Ratio Lower Upper

164 100

129 95.7 68.1 126.5

131 94.7 65.9 122.5

166 120.7 89.7 166.7

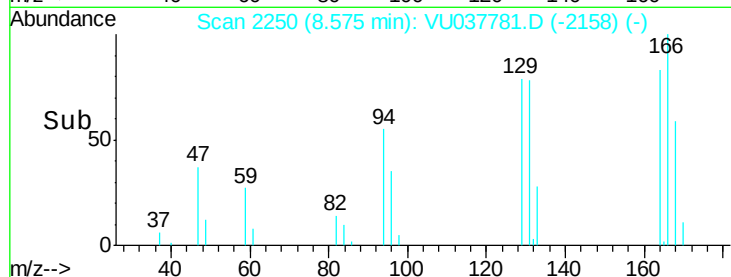

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

