


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041720\
 Data File : VU037764.D
 Acq On : 17 Apr 2020 08:54
 Operator : JC/MD
 Sample : BFB16
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB16

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Apr 18 05:19:30 2020

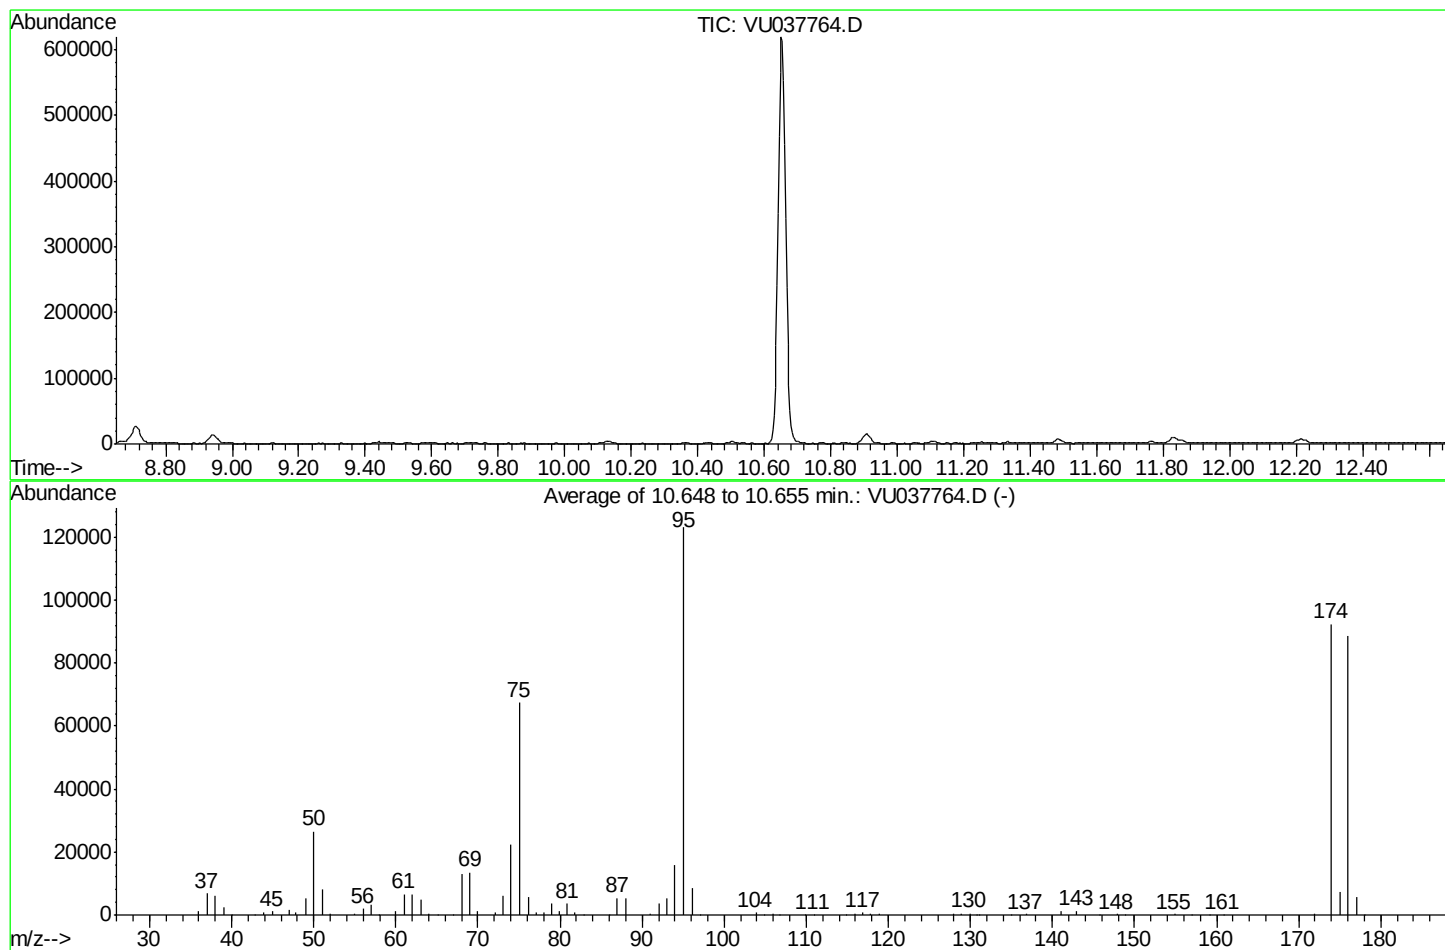

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	26466	PASS
75	95	30	80	54.8	67421	PASS
95	95	100	100	100.0	123061	PASS
96	95	5	9	7.0	8585	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.1	92373	PASS
175	174	5	9	8.2	7531	PASS
176	174	95	101	95.7	88440	PASS
177	176	5	9	6.7	5899	PASS

m/z	Abundance
36.00	1062.0
37.00	6651.0
38.00	5963.0
39.00	2379.0
40.00	255.0
42.80	151.0
44.00	1415.0
45.00	1235.0
47.00	1751.0
47.90	887.0
49.00	5220.0
50.00	25112.0
51.00	7795.0
52.00	422.0
54.90	484.0
56.00	1768.0
57.00	3318.0
58.00	222.0
60.00	1090.0
61.00	6158.0
62.00	6255.0
63.00	4496.0
64.00	463.0
65.10	120.0
66.90	289.0
68.00	12386.0
69.00	12889.0
70.00	1181.0
72.00	739.0
73.00	5524.0
74.00	21008.0
75.00	64816.0
76.10	5646.0
77.10	829.0
78.00	712.0
78.90	3558.0
79.90	983.0
80.90	3365.0
81.80	634.0
82.90	162.0
87.00	5021.0
88.00	5167.0
91.00	437.0
92.00	3308.0
93.00	4977.0
94.00	15458.0
95.10	116184.0
96.10	8251.0
97.10	204.0
103.90	641.0
105.90	420.0
106.80	115.0
109.90	108.0
114.80	141.0
116.00	496.0
116.90	657.0
117.90	369.0
118.80	368.0
127.90	337.0
129.00	172.0
129.90	462.0
130.80	121.0
135.00	129.0
136.80	238.0
141.00	999.0
143.00	1234.0
147.90	220.0
154.90	184.0
157.00	146.0
159.10	108.0
160.80	155.0
172.00	222.0
174.00	85864.0
175.00	7282.0
176.00	80496.0
177.00	5627.0
178.00	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
35.90	1078.0
37.00	7032.0
38.00	6409.0
39.00	2633.0
40.00	226.0
42.80	130.0
44.00	1505.0
45.00	1185.0
47.10	1806.0
47.80	882.0
49.00	5687.0
50.00	27312.0
51.00	8332.0
52.00	458.0
55.00	445.0
56.00	1906.0
57.00	3450.0
57.90	186.0
60.00	1129.0
61.00	6793.0
62.00	6747.0
63.00	4998.0
64.00	469.0
65.10	105.0
66.90	336.0
68.00	13432.0
69.00	14050.0
70.00	1310.0
72.10	700.0
73.00	6050.0
74.00	23088.0
75.00	69456.0
76.10	6169.0
77.10	804.0
78.00	705.0
78.90	3738.0
79.90	1091.0
80.90	3708.0
81.80	688.0
82.90	182.0
86.00	206.0
87.00	5704.0
88.00	5148.0
91.00	486.0
92.00	3522.0
93.00	5291.0
94.00	16448.0
95.10	127088.0
96.10	8901.0
97.10	167.0
103.90	749.0
105.00	123.0
105.90	465.0
110.90	122.0
114.80	155.0
116.00	482.0
116.90	637.0
117.80	394.0
118.90	423.0
127.90	371.0
129.00	225.0
129.90	482.0
131.00	162.0
134.90	138.0
136.80	255.0
141.00	1182.0
143.00	1398.0
145.80	147.0
147.90	233.0
154.90	231.0
157.00	209.0
159.10	115.0
160.80	149.0
171.80	276.0
174.00	95448.0
175.00	7809.0
176.00	91488.0
177.00	6134.0
178.00	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
35.90	1060.0
37.00	6693.0
38.00	6125.0
39.00	2647.0
39.90	207.0
42.90	120.0
44.00	1472.0
44.90	1164.0
47.10	1580.0
47.90	780.0
49.00	5563.0
50.00	26976.0
51.00	8049.0
52.00	446.0
55.00	398.0
56.00	2061.0
57.00	3360.0
57.90	170.0
60.00	1102.0
61.00	6613.0
62.00	6522.0
63.00	5046.0
64.00	425.0
68.00	13278.0
69.00	13827.0
70.00	1239.0
72.10	593.0
73.00	6190.0
74.00	22968.0
75.00	67992.0
76.10	5907.0
77.00	699.0
78.00	602.0
78.90	3545.0
79.90	1110.0
80.90	3714.0
81.80	735.0
82.80	192.0
86.00	182.0
87.00	5671.0
88.00	4973.0
91.00	518.0
92.00	3610.0
93.00	5318.0
94.00	15968.0
95.10	125912.0
96.10	8605.0
97.20	111.0
103.90	730.0
104.80	148.0
106.00	483.0
110.90	144.0
114.80	142.0
115.90	407.0
116.90	662.0
117.80	355.0
118.90	490.0
127.90	349.0
128.90	256.0
129.90	462.0
131.00	174.0
134.80	156.0
136.80	228.0
141.00	1249.0
142.90	1377.0
145.80	176.0
147.90	251.0
148.90	104.0
154.90	256.0
156.90	260.0
160.90	119.0
171.90	283.0
174.00	95808.0
175.10	7504.0
176.00	93336.0
177.00	5936.0
178.00	233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

Scan 2881 (10.603 min): VU037764.D
BFB16

m/z	Abundance
39.00	106.0
40.00	193.0
43.90	659.0
55.20	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16