


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041724\
Data File : VU058730.D
Acq On : 17 Apr 2024 11:39
Operator : MD/SY
Sample : BFB145
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB145

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 18 05:04:53 2024

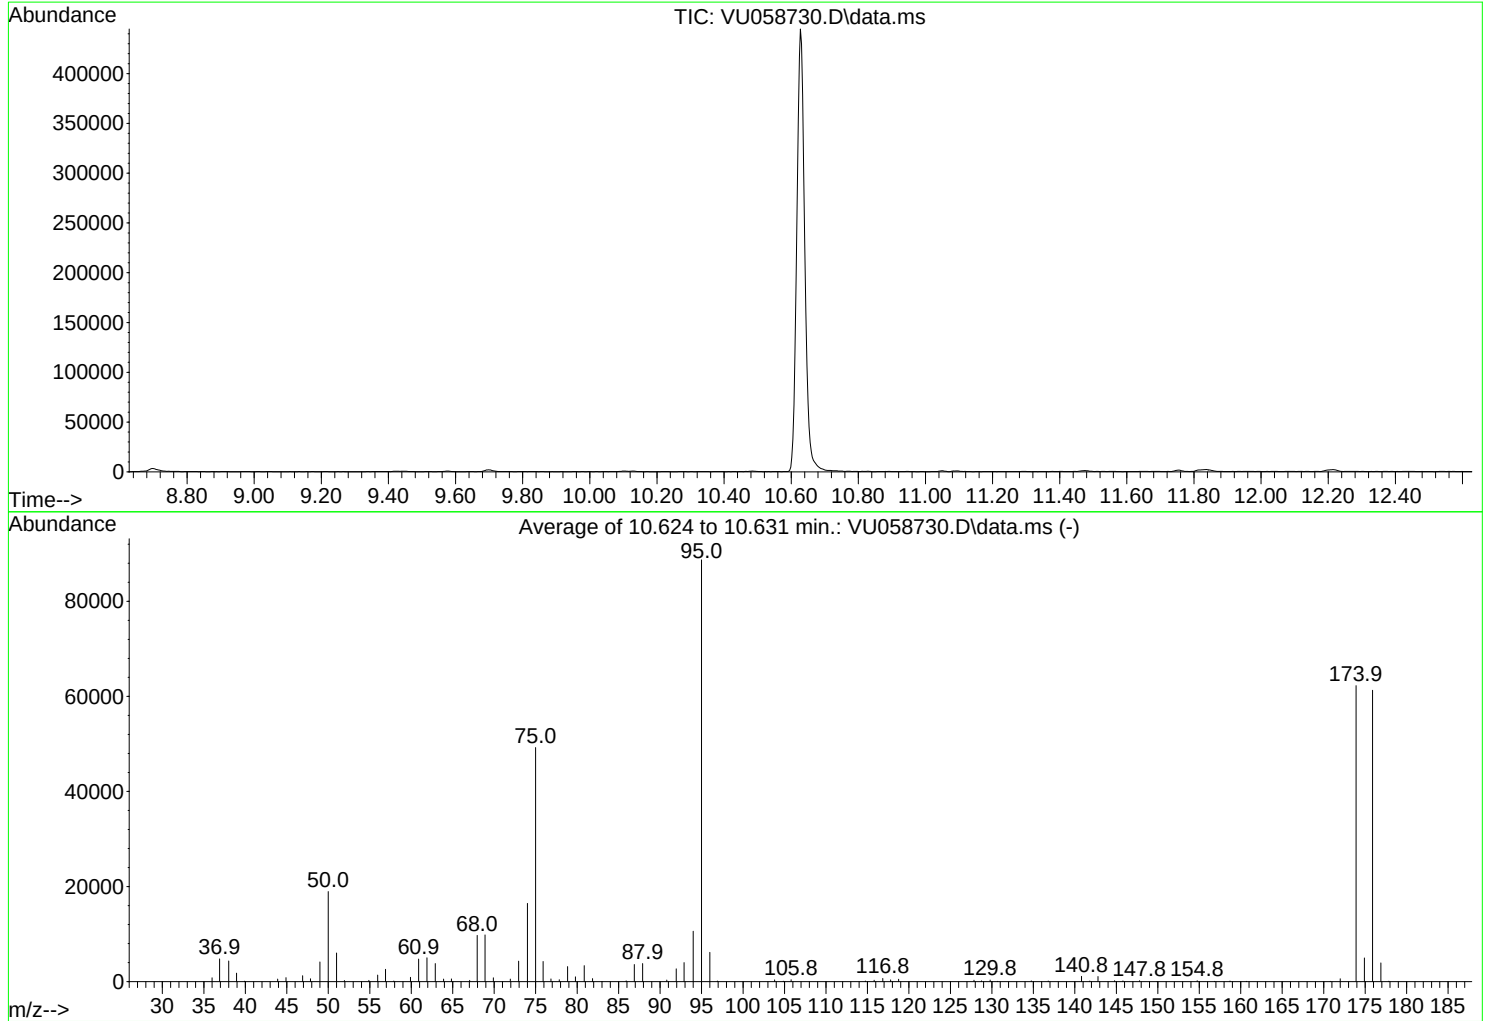

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	18933	PASS
75	95	30	80	55.5	49229	PASS
95	95	100	100	100.0	88720	PASS
96	95	5	9	6.9	6160	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.2	62248	PASS
175	174	5	9	8.0	4981	PASS
176	174	95	101	98.5	61301	PASS
177	176	5	9	6.5	3954	PASS

Scan 2890 (10.582 min): VU058730.D\data.ms
BFB145

m/z	Abundance
39.90	127.0
43.80	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB145

m/z	Abundance
36.00	825.0
36.90	4676.0
38.00	4331.0
39.00	1824.0
39.90	224.0
43.90	758.0
44.90	876.0
46.90	1235.0
47.90	568.0
49.00	4138.0
50.00	18632.0
51.00	5964.0
51.90	254.0
54.90	257.0
55.90	1334.0
56.90	2414.0
57.90	122.0
59.90	930.0
60.90	4710.0
61.90	5042.0
62.90	3773.0
63.90	539.0
64.90	547.0
67.00	251.0
67.90	9451.0
68.90	9453.0
69.90	808.0
71.90	486.0
73.00	4121.0
74.00	15974.0
75.00	48576.0
75.90	4155.0
76.90	547.0
77.80	413.0
78.80	3104.0
79.80	948.0
80.90	3335.0
81.90	622.0
85.90	145.0
86.90	3597.0
87.90	3725.0
90.80	335.0
91.90	2588.0
92.90	3928.0
94.00	10242.0
95.00	86160.0
96.00	5982.0
96.90	124.0
103.80	385.0
104.80	120.0
105.80	413.0
114.70	126.0
115.80	288.0
116.80	637.0
117.80	338.0
118.70	466.0
127.80	305.0
128.90	143.0
129.80	309.0
134.80	181.0
136.80	150.0
140.80	1068.0
141.80	119.0
142.80	1035.0
144.80	202.0
145.80	144.0
147.80	194.0
154.80	214.0
158.70	126.0
170.80	125.0
172.00	615.0
173.90	58760.0
174.90	4829.0
175.90	58688.0
176.90	3794.0
178.00	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB145

m/z	Abundance
36.00	846.0
36.90	4952.0
38.00	4493.0
39.00	1855.0
39.90	223.0
44.00	746.0
44.90	897.0
46.90	1274.0
47.80	619.0
49.00	4226.0
50.00	19544.0
51.00	6214.0
51.90	253.0
54.90	282.0
56.00	1459.0
56.90	2660.0
57.90	127.0
59.90	937.0
60.90	4902.0
61.90	5210.0
62.90	3922.0
63.90	571.0
64.80	607.0
67.10	281.0
67.90	10052.0
68.90	10131.0
69.90	804.0
72.00	571.0
72.90	4432.0
74.00	17040.0
75.00	50832.0
75.90	4346.0
76.80	592.0
77.80	424.0
78.90	3281.0
79.80	1069.0
80.80	3521.0
81.90	651.0
83.00	102.0
85.90	165.0
86.90	3706.0
87.90	3933.0
90.80	368.0
91.90	2761.0
92.90	4121.0
94.00	10916.0
95.00	91640.0
96.00	6337.0
96.90	127.0
103.80	396.0
104.80	117.0
105.80	424.0
114.70	142.0
115.80	316.0
116.80	714.0
117.80	358.0
118.70	531.0
127.80	318.0
128.70	169.0
129.80	354.0
130.70	109.0
134.80	170.0
136.80	150.0
140.80	1136.0
141.80	146.0
142.80	1124.0
144.80	229.0
145.80	170.0
147.80	210.0
149.90	104.0
154.80	219.0
156.90	123.0
158.70	143.0
160.70	115.0
170.80	120.0
172.00	627.0
173.90	64256.0
174.90	5187.0
175.90	63384.0
176.90	4067.0
177.80	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB145

m/z	Abundance
36.00	810.0
36.90	4766.0
38.00	4184.0
38.90	1688.0
39.90	198.0
43.90	666.0
44.90	800.0
46.90	1280.0
47.80	649.0
49.00	4042.0
50.00	18624.0
51.00	5943.0
52.00	247.0
54.90	286.0
56.00	1386.0
56.90	2737.0
57.90	121.0
59.90	888.0
60.90	4660.0
61.90	4840.0
62.90	3691.0
63.90	511.0
64.80	581.0
67.00	256.0
68.00	9659.0
68.90	9936.0
69.90	766.0
72.00	617.0
72.90	4391.0
74.00	16340.0
75.00	48280.0
75.90	4192.0
76.80	571.0
77.90	404.0
78.90	3120.0
79.80	1063.0
80.80	3270.0
81.80	634.0
85.90	164.0
86.90	3484.0
87.90	3749.0
90.80	355.0
92.00	2740.0
92.90	3959.0
94.00	10694.0
95.00	88360.0
96.00	6161.0
96.90	120.0
103.80	380.0
104.90	104.0
105.80	413.0
114.80	137.0
115.80	355.0
116.90	719.0
117.80	371.0
118.80	550.0
127.90	303.0
128.70	185.0
129.80	361.0
130.70	125.0
134.70	145.0
136.80	142.0
140.80	1094.0
141.80	143.0
142.80	1091.0
144.80	218.0
145.80	167.0
147.80	202.0
154.70	196.0
156.80	133.0
158.70	134.0
160.70	118.0
172.00	585.0
173.90	63728.0
174.90	4927.0
175.90	61832.0
176.90	4000.0
177.80	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB145