

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048112.D
 Acq On : 18 Apr 2022 11:49
 Operator : SY/MD
 Sample : N2386-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	97	rBV	157290	187899	15.11%	1.920%
2	1.916	171	179	198	rVB	122655	169883	13.66%	1.736%
3	2.572	370	383	400	rBV	267078	442509	35.59%	4.521%
4	2.687	416	419	425	rVB4	577	434	0.03%	0.004%
5	2.716	425	428	430	rBV3	311	234	0.02%	0.002%
6	2.800	445	454	462	rBV3	652	1295	0.10%	0.013%
7	2.948	496	500	506	rBV2	303	340	0.03%	0.003%
8	3.044	526	530	532	rBV3	621	523	0.04%	0.005%
9	3.157	559	565	568	rBV	208	299	0.02%	0.003%
10	3.189	568	575	586	rVB3	846	1786	0.14%	0.018%
11	3.436	649	652	654	rBV2	223	176	0.01%	0.002%
12	3.514	671	676	678	rBV	191	229	0.02%	0.002%
13	3.588	692	699	701	rBV2	217	274	0.02%	0.003%
14	3.623	708	710	715	rVB2	316	218	0.02%	0.002%
15	3.671	719	725	726	rBV	287	297	0.02%	0.003%
16	3.809	765	768	770	rBV2	203	173	0.01%	0.002%
17	3.983	818	822	826	rBV2	276	245	0.02%	0.003%
18	4.018	831	833	838	rVB2	216	200	0.02%	0.002%
19	4.044	838	841	844	rBV	328	254	0.02%	0.003%
20	4.131	862	868	874	rBV2	199	325	0.03%	0.003%
21	4.289	913	917	921	rBV2	254	292	0.02%	0.003%
22	4.379	939	945	948	rBV2	310	385	0.03%	0.004%
23	4.626	1007	1022	1049	rBV	130572	329063	26.46%	3.362%
24	5.067	1143	1159	1181	rVV	224638	496250	39.91%	5.070%
25	5.234	1207	1211	1215	rVB3	410	349	0.03%	0.004%
26	5.292	1222	1229	1232	rBV2	496	587	0.05%	0.006%
27	5.398	1255	1262	1264	rBV	304	260	0.02%	0.003%
28	5.514	1293	1298	1306	rBV2	213	294	0.02%	0.003%
29	5.552	1306	1310	1312	rBV	204	161	0.01%	0.002%
30	5.645	1333	1339	1340	rBV	252	268	0.02%	0.003%
31	5.729	1343	1365	1402	rVV2	460683	1243448	100.00%	12.704%
32	5.973	1437	1441	1446	rBV3	431	448	0.04%	0.005%
33	6.044	1459	1463	1467	rBV3	419	444	0.04%	0.005%
34	6.073	1467	1472	1473	rBV2	240	193	0.02%	0.002%
35	6.083	1473	1475	1480	rVB2	344	248	0.02%	0.003%
36	6.108	1480	1483	1486	rBV2	337	297	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048112.D
 Acq On : 18 Apr 2022 11:49
 Operator : SY/MD
 Sample : N2386-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.147	1493	1495	1498	rVB2	297	159	0.01%	0.002%
38	6.253	1513	1528	1557	rBV	372571	709397	57.05%	7.248%
39	6.536	1607	1616	1625	rBV5	1836	3337	0.27%	0.034%
40	6.613	1637	1640	1643	rBV2	209	171	0.01%	0.002%
41	6.694	1647	1665	1688	rBV	288678	560580	45.08%	5.727%
42	6.800	1695	1698	1699	rBV2	608	324	0.03%	0.003%
43	7.047	1770	1775	1777	rBV2	525	456	0.04%	0.005%
44	7.186	1808	1818	1829	rBV5	2545	4253	0.34%	0.043%
45	7.568	1924	1937	1960	rBV	148720	263468	21.19%	2.692%
46	7.767	1996	1999	2001	rBV	282	164	0.01%	0.002%
47	7.796	2003	2008	2018	rVB5	1167	1605	0.13%	0.016%
48	7.899	2024	2040	2057	rBV	520645	913153	73.44%	9.330%
49	8.182	2115	2128	2143	rBV	103266	175031	14.08%	1.788%
50	8.472	2215	2218	2220	rBV3	341	198	0.02%	0.002%
51	8.562	2243	2246	2249	rVB2	458	297	0.02%	0.003%
52	8.636	2257	2269	2304	rBV	373328	698486	56.17%	7.136%
53	8.838	2330	2332	2335	rVB3	324	191	0.02%	0.002%
54	8.861	2335	2339	2340	rBV2	334	239	0.02%	0.002%
55	9.063	2394	2402	2409	rVB2	369	414	0.03%	0.004%
56	9.099	2409	2413	2414	rBV	246	169	0.01%	0.002%
57	9.169	2431	2435	2438	rBV3	366	296	0.02%	0.003%
58	9.420	2496	2513	2534	rBV	553037	930475	74.83%	9.507%
59	9.648	2578	2584	2590	rVB3	503	490	0.04%	0.005%
60	9.697	2593	2599	2603	rBV2	1054	1118	0.09%	0.011%
61	9.790	2621	2628	2630	rBV2	476	557	0.04%	0.006%
62	9.861	2648	2650	2656	rVB	317	277	0.02%	0.003%
63	9.980	2683	2687	2692	rVV2	201	187	0.02%	0.002%
64	10.099	2719	2724	2726	rVV4	320	236	0.02%	0.002%
65	10.128	2730	2733	2740	rVB2	354	376	0.03%	0.004%
66	10.169	2740	2746	2750	rBV3	336	425	0.03%	0.004%
67	10.250	2768	2771	2775	rBV3	251	183	0.01%	0.002%
68	10.491	2840	2846	2849	rBV2	397	361	0.03%	0.004%
69	10.671	2896	2902	2911	rVB4	2694	3456	0.28%	0.035%
70	10.758	2915	2929	2948	rBV	443465	717970	57.74%	7.335%
71	10.867	2959	2963	2968	rBV3	873	847	0.07%	0.009%
72	10.899	2968	2973	2975	rVV2	449	355	0.03%	0.004%
73	11.121	3038	3042	3047	rVB4	508	446	0.04%	0.005%
74	11.227	3072	3075	3077	rBV2	297	214	0.02%	0.002%
75	11.381	3119	3123	3125	rBV2	254	225	0.02%	0.002%
76	11.394	3125	3127	3130	rVB	409	210	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048112.D
 Acq On : 18 Apr 2022 11:49
 Operator : SY/MD
 Sample : N2386-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.465	3140	3149	3152	rBV6	1891	2616	0.21%	0.027%
78	11.578	3179	3184	3192	rBV4	494	696	0.06%	0.007%
79	11.658	3205	3209	3211	rBV	286	259	0.02%	0.003%
80	11.700	3215	3222	3227	rVV4	1123	1460	0.12%	0.015%
81	11.748	3231	3237	3244	rVB3	636	834	0.07%	0.009%
82	11.816	3244	3258	3280	rBV	592910	951506	76.52%	9.721%
83	12.034	3319	3326	3331	rBV3	406	557	0.04%	0.006%
84	12.195	3357	3376	3397	rBV	574790	940109	75.61%	9.605%
85	12.330	3415	3418	3419	rBV2	456	265	0.02%	0.003%
86	12.404	3438	3441	3447	rBV3	301	338	0.03%	0.003%
87	12.491	3463	3468	3473	rBV2	353	378	0.03%	0.004%
88	12.581	3492	3496	3498	rBV2	256	208	0.02%	0.002%
89	12.629	3509	3511	3513	rBV	255	164	0.01%	0.002%
90	12.645	3513	3516	3521	rVB4	430	357	0.03%	0.004%
91	12.861	3581	3583	3589	rBV3	202	189	0.02%	0.002%
92	12.909	3595	3598	3599	rBV	254	165	0.01%	0.002%
93	13.098	3654	3657	3662	rBV3	406	403	0.03%	0.004%
94	13.433	3758	3761	3763	rBV2	318	227	0.02%	0.002%
95	13.606	3813	3815	3826	rVB2	401	653	0.05%	0.007%
96	13.651	3826	3829	3832	rBV	377	261	0.02%	0.003%
97	13.754	3858	3861	3865	rBV2	446	347	0.03%	0.004%
98	13.848	3883	3890	3898	rVB5	2970	4285	0.34%	0.044%
99	14.095	3959	3967	3978	rVB2	4092	6275	0.50%	0.064%
100	14.336	4034	4042	4051	rBV3	2250	3820	0.31%	0.039%




Sum of corrected areas: 9787748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048112.D
Acq On : 18 Apr 2022 11:49
Operator : SY/MD
Sample : N2386-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

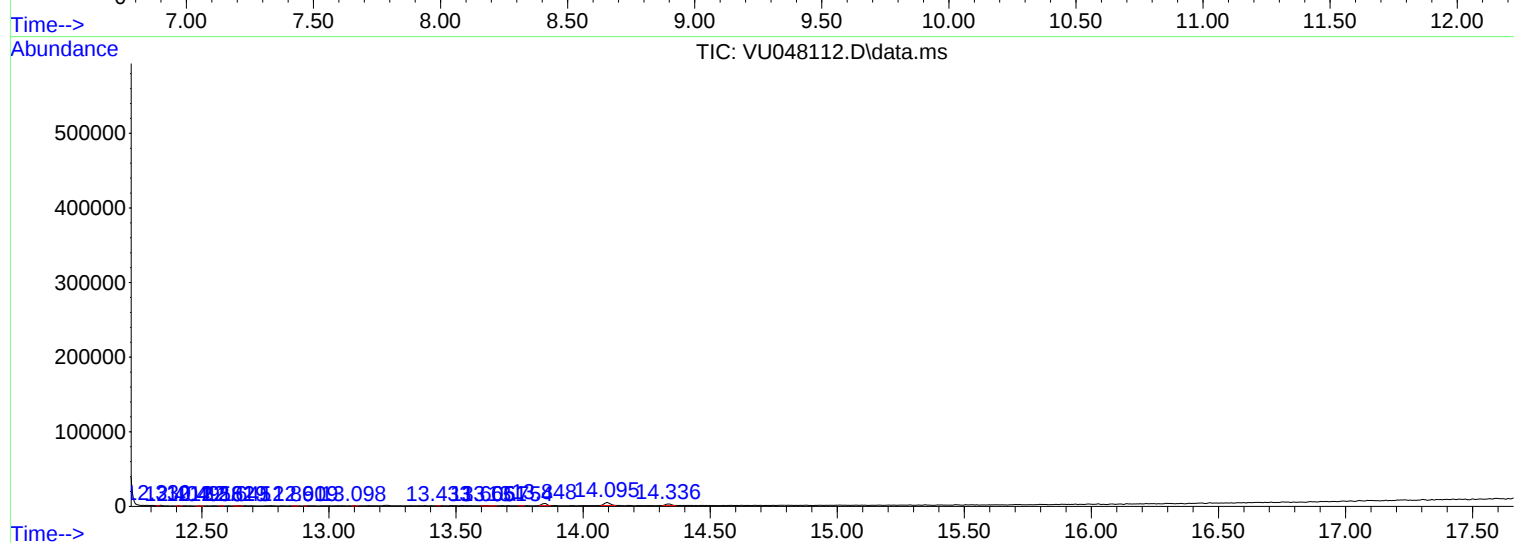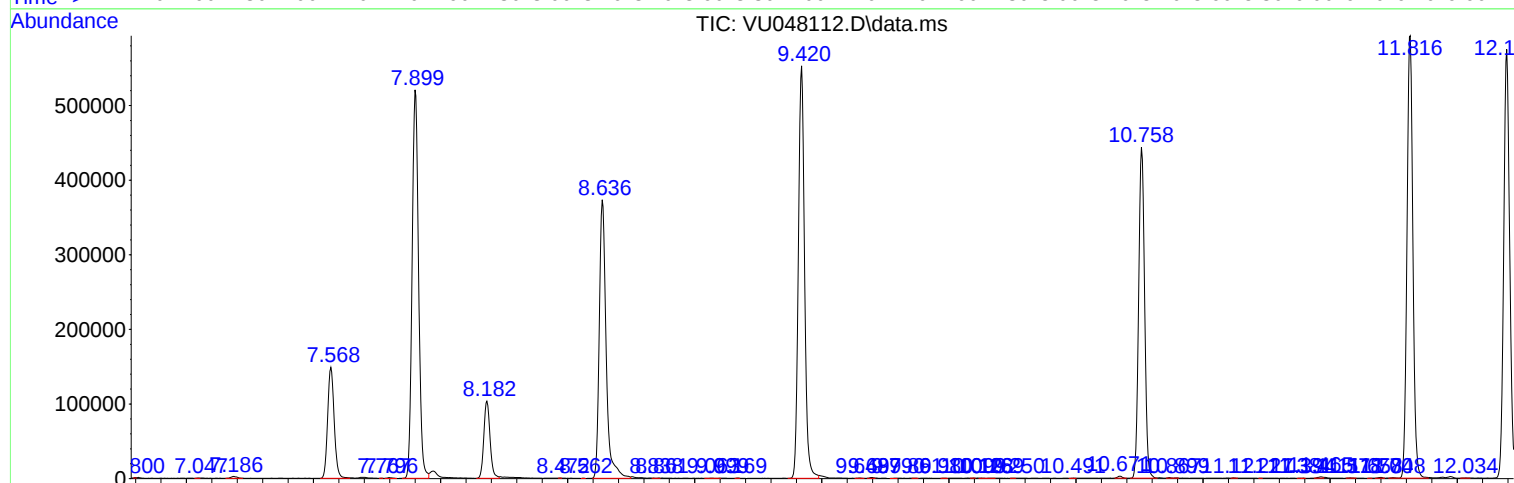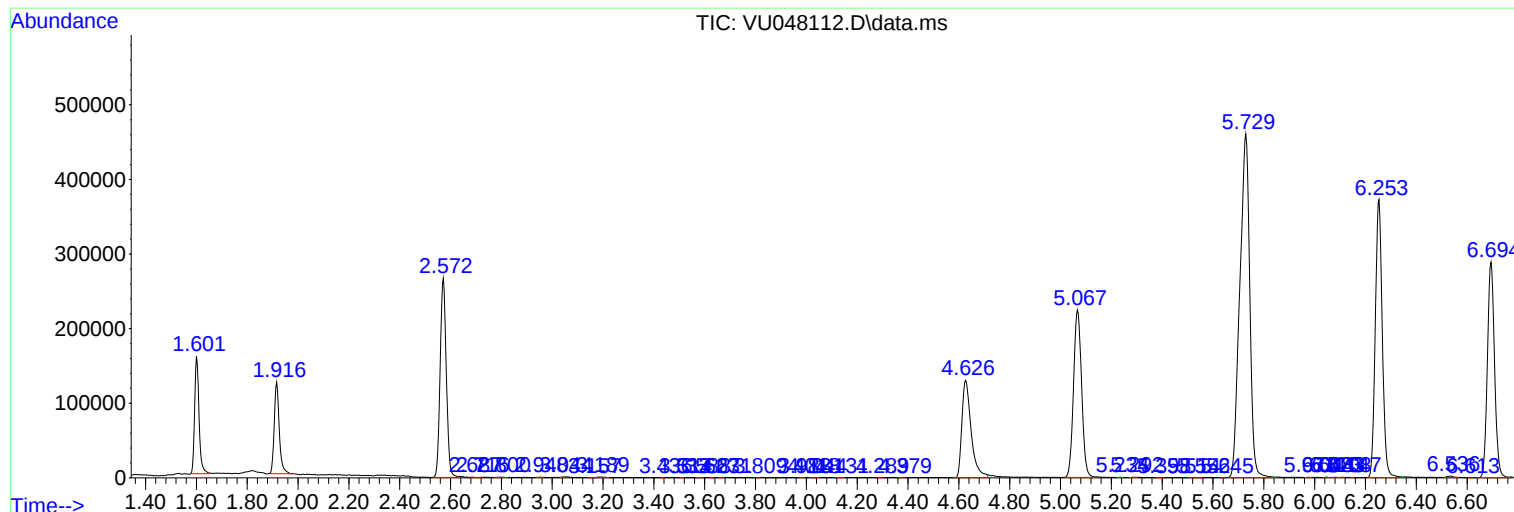

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048112.D
Acq On : 18 Apr 2022 11:49
Operator : SY/MD
Sample : N2386-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048112.D
Acq On : 18 Apr 2022 11:49
Operator : SY/MD
Sample : N2386-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------